

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081721\
 Data File : P0080608.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Aug 2021 12:28
 Operator : DD\AJ
 Sample : M3437-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VERTICAL-EXPAND

Manual Integrations
 APPROVED

mohammad
 8/18/2021 3:42:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 14:13:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 11 05:48:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.990	4.105	1470782	522032	21.240	20.945
2) SA Decachlor...	11.101	9.505	1879028	118889	36.301m	5.242m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081721\
Data File : PO080608.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Aug 2021 12:28
Operator : DD\AJ
Sample : M3437-02
Misc :
ALS Vial : 63 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VERTICAL-EXPAND


Manual Integrations
APPROVED

mohammad
8/18/2021 3:42:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 14:13:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 11 05:48:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

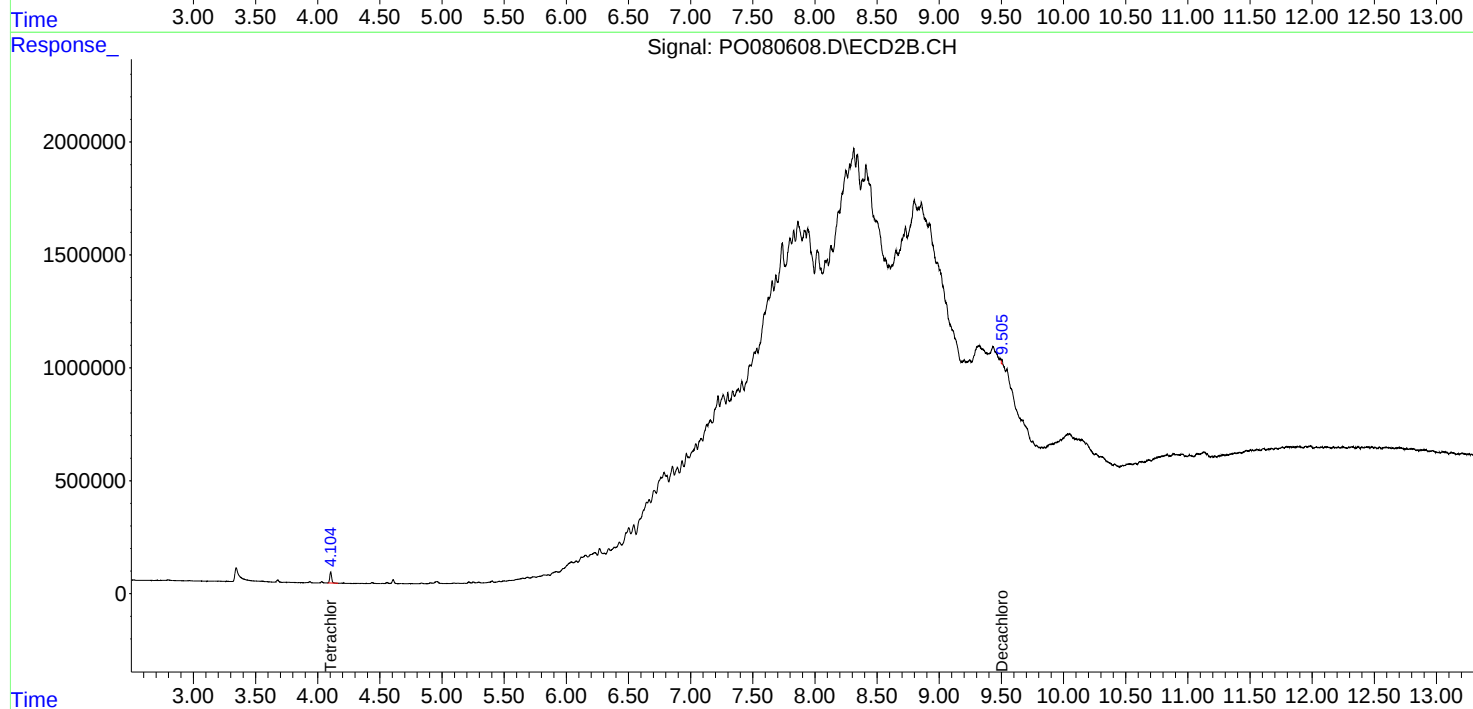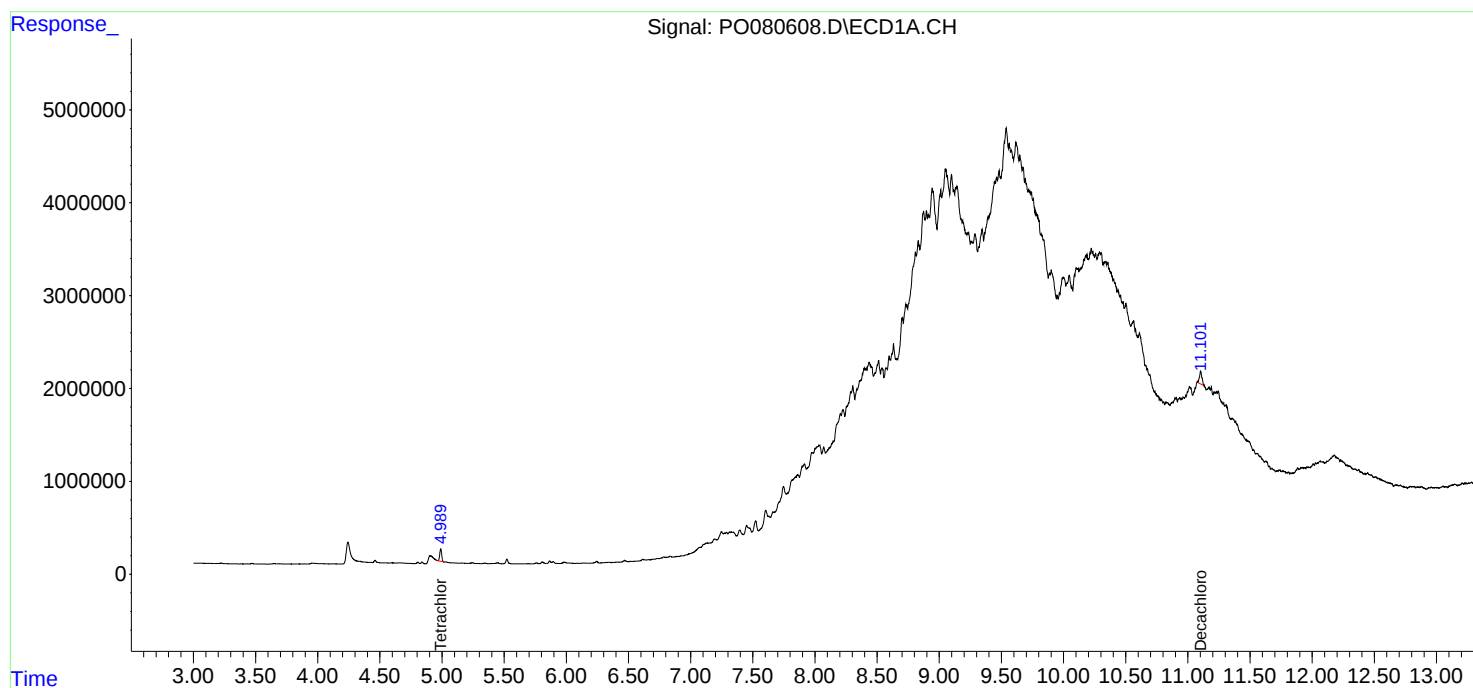

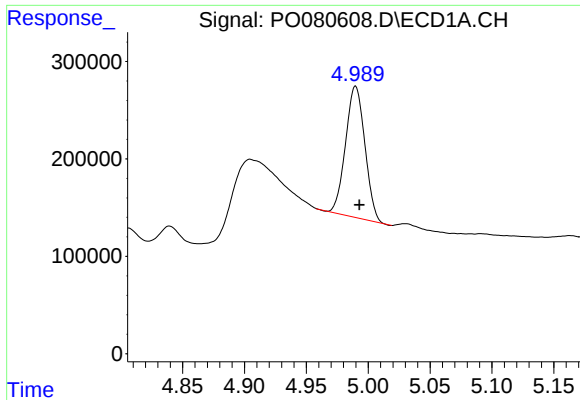


#1 Tetrachloro-m-xylene

R.T.: 4.990 min
Delta R.T.: -0.003 min
Response: 1470782
Conc: 21.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
VERTICAL-EXPAND


Manual Integrations
APPROVED

mohammad
8/18/2021 3:42:35 PM

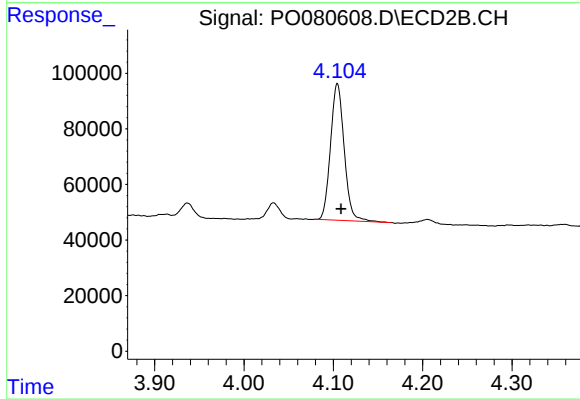


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: -0.004 min
Response: 522032
Conc: 20.95 ng/ml

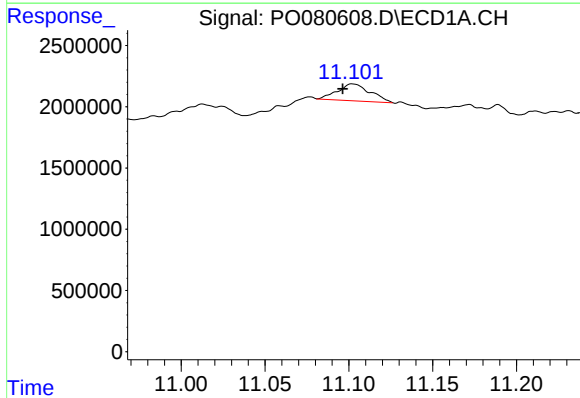

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: 0.005 min
Response: 1879028
Conc: 36.30 ng/ml m

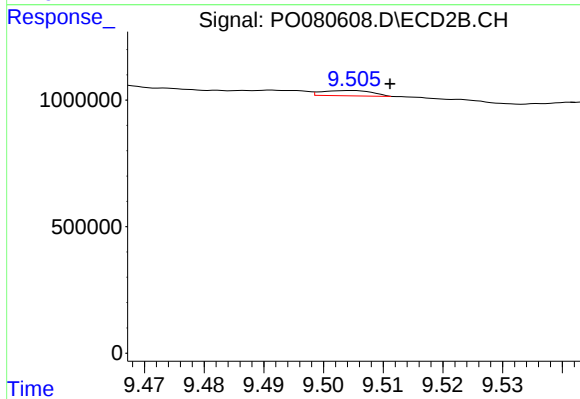

#2 Decachlorobiphenyl

R.T.: 9.505 min
Delta R.T.: -0.006 min
Response: 118889
Conc: 5.24 ng/ml m