

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081723\
 Data File : P0097206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 18:15
 Operator : YP/AJ
 Sample : 04047-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NEVINS-SB05-Z60-61

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:22:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.615	38969487	15431976	11.773	11.657
2) SA Decachlor...	10.350	8.629	31358808	22083675	14.331	19.088m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081723\
Data File : PO097206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 18:15
Operator : YP/AJ
Sample : 04047-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NEVINS-SB05-Z60-61


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:22:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

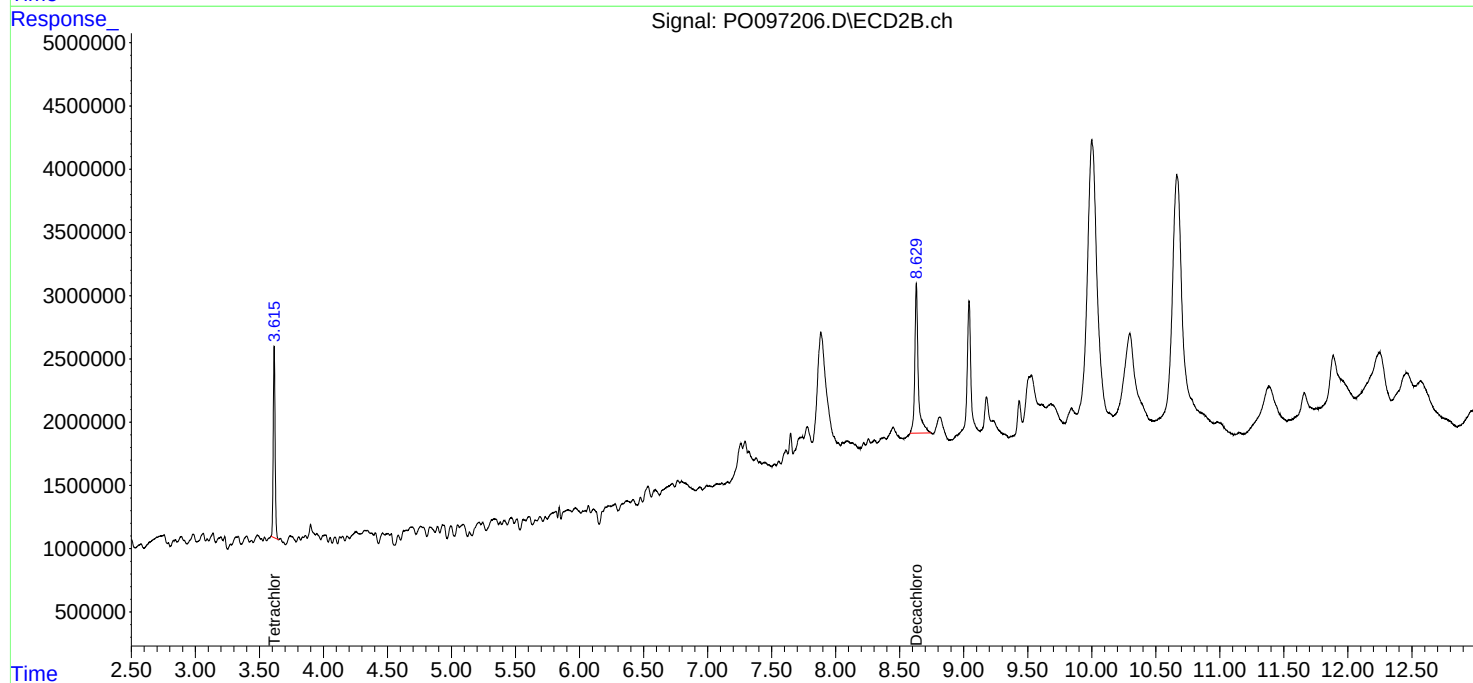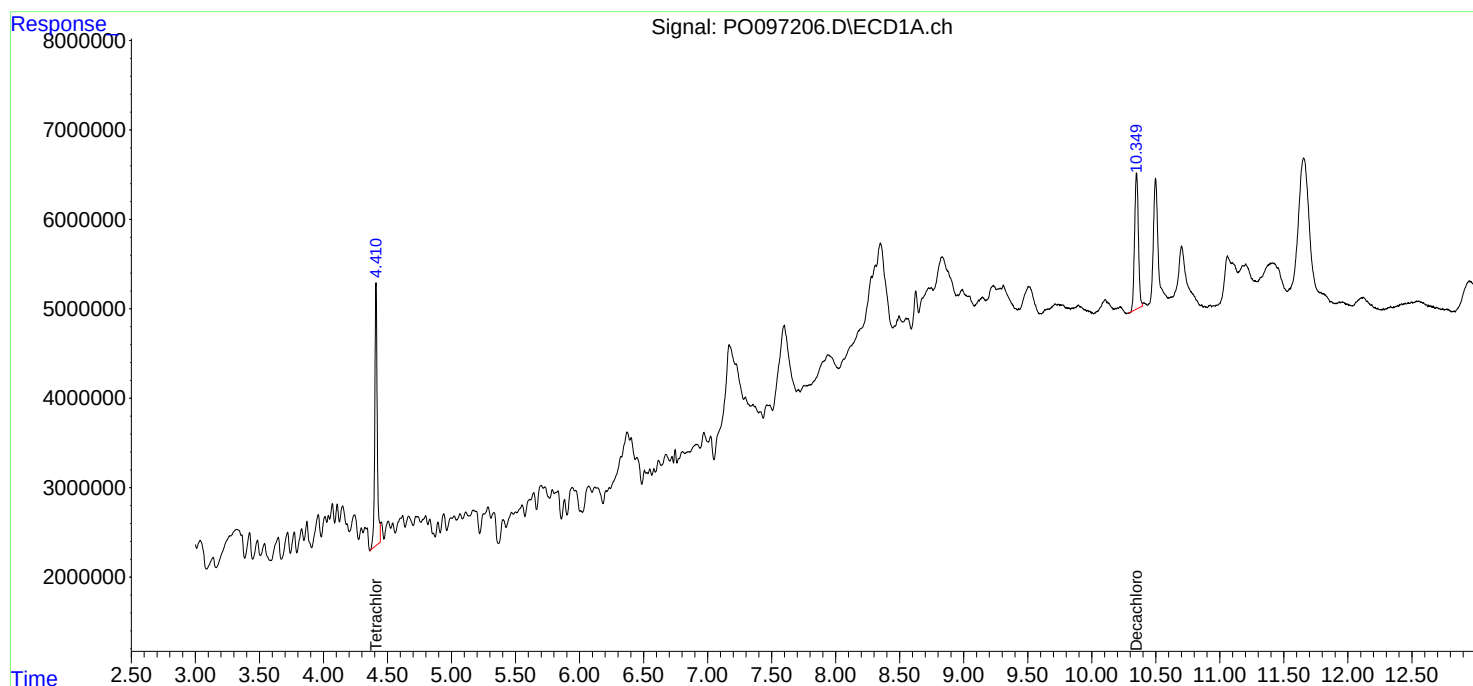

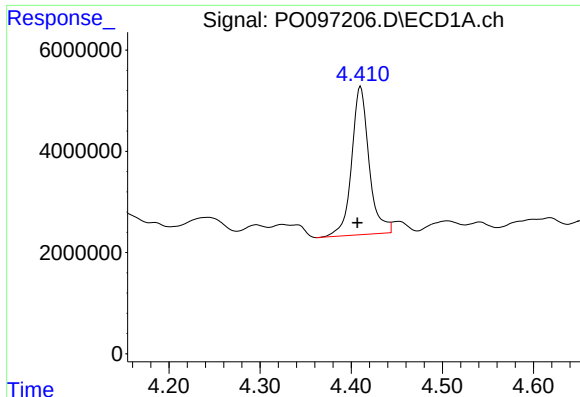


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: 0.003 min
Response: 38969487
Conc: 11.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
NEVINS-SB05-Z60-61


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

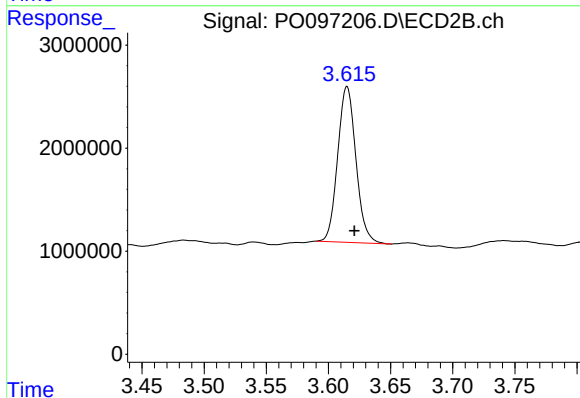


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: -0.006 min
Response: 15431976
Conc: 11.66 ng/ml

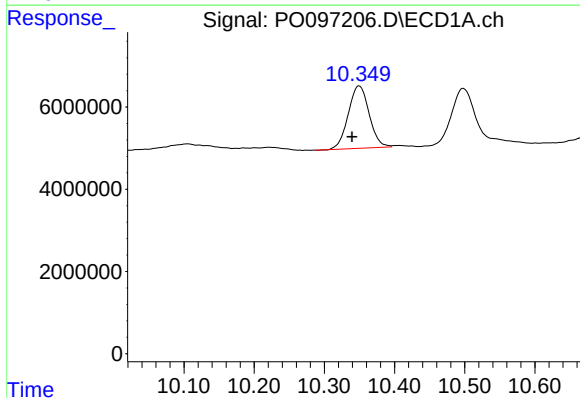

#2 Decachlorobiphenyl

R.T.: 10.350 min
Delta R.T.: 0.010 min
Response: 31358808
Conc: 14.33 ng/ml

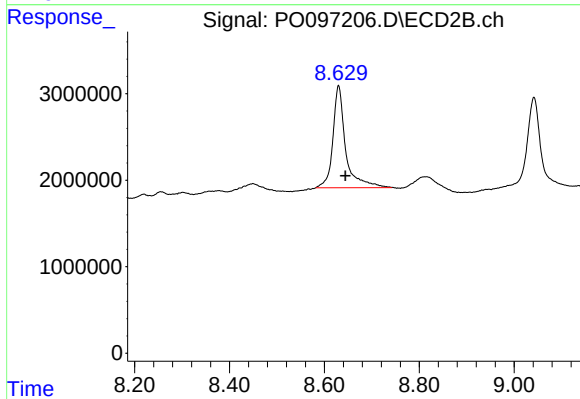

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.015 min
Response: 22083675
Conc: 19.09 ng/ml m