

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081723\
 Data File : P0097207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 18:32
 Operator : YP/AJ
 Sample : 04047-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NEVINS-SB05-Z60-61-Q

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:22:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.615	40771342	16552620	12.317	12.504
2) SA Decachlor...	10.349	8.629	32014745	14514028	14.631	12.545m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081723\
Data File : PO097207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 18:32
Operator : YP/AJ
Sample : 04047-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NEVINS-SB05-Z60-61-Q


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:22:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

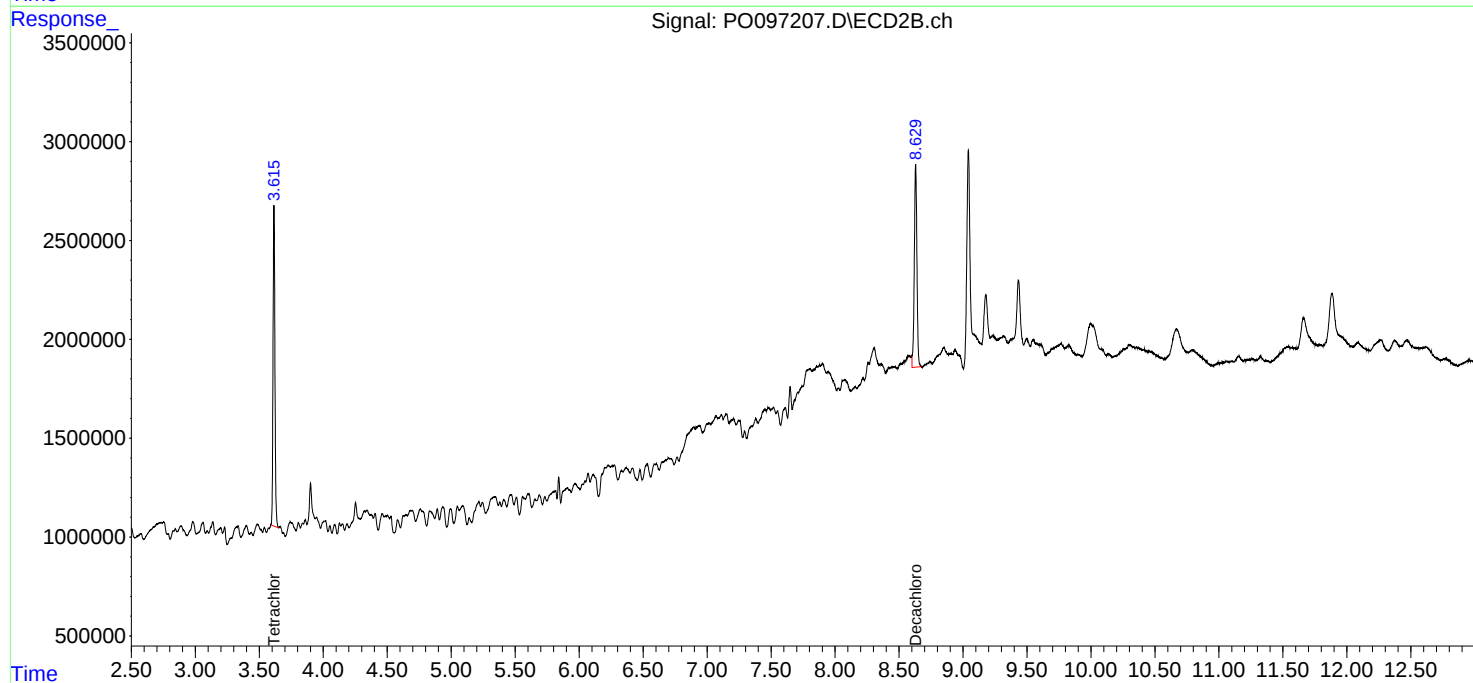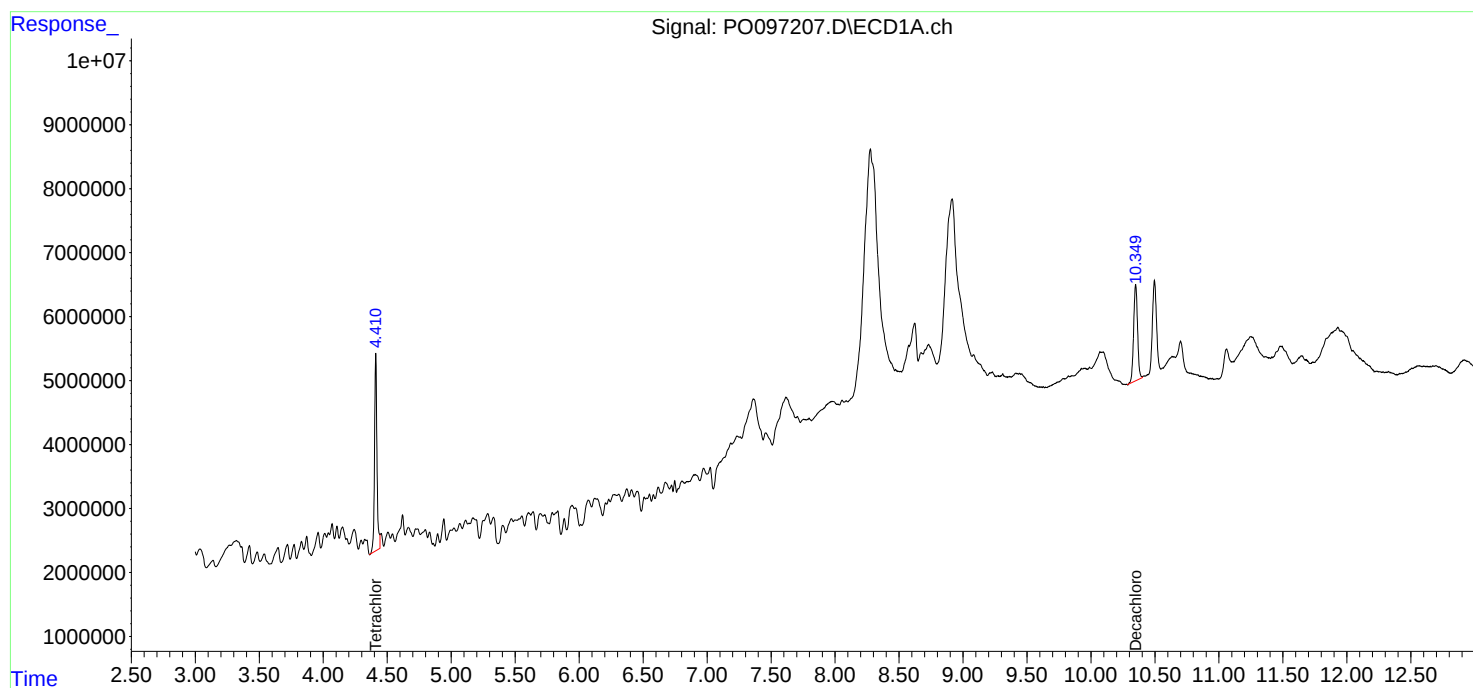

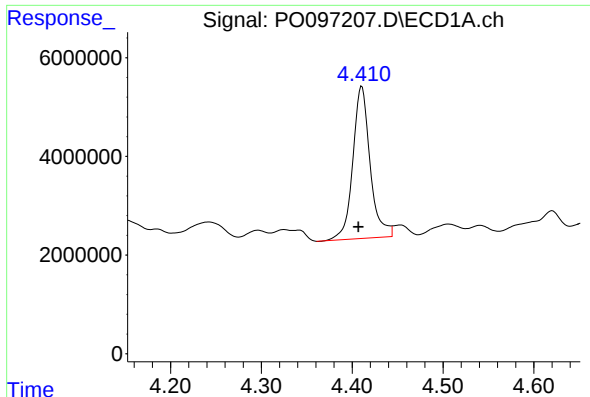


#1 Tetrachloro-m-xylene

R.T.: 4.411 min
Delta R.T.: 0.004 min
Response: 40771342
Conc: 12.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
NEVINS-SB05-Z60-61-Q


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

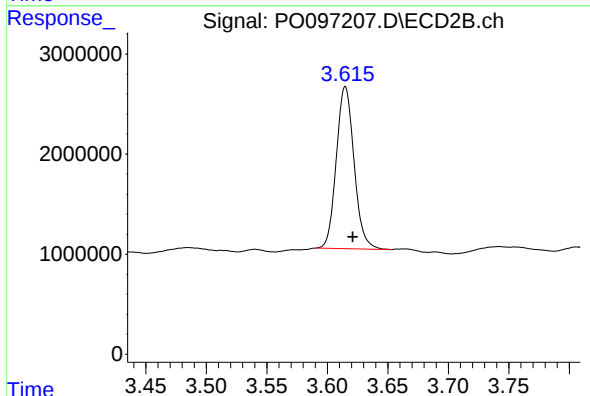


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: -0.006 min
Response: 16552620
Conc: 12.50 ng/ml

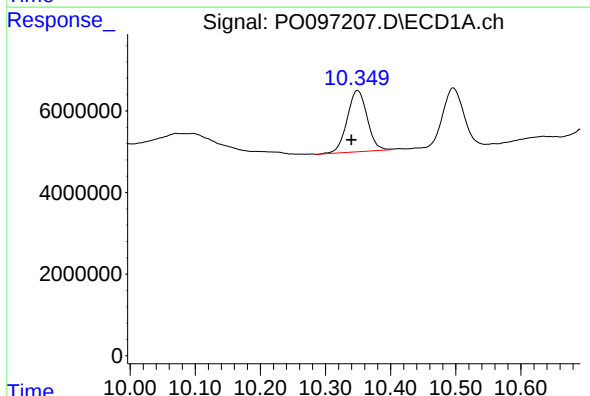

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: 0.010 min
Response: 32014745
Conc: 14.63 ng/ml

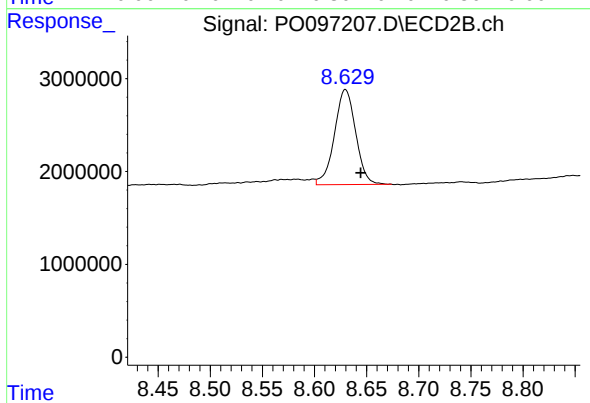

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.015 min
Response: 14514028
Conc: 12.55 ng/ml m