

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081723\
 Data File : P0097222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 23:15
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:27:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.614	71047879	27465538	21.463	20.748
2) SA Decachlor...	10.346	8.628	52183590	25438127	23.848	21.988m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081723\
Data File : PO097222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 23:15
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:27:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

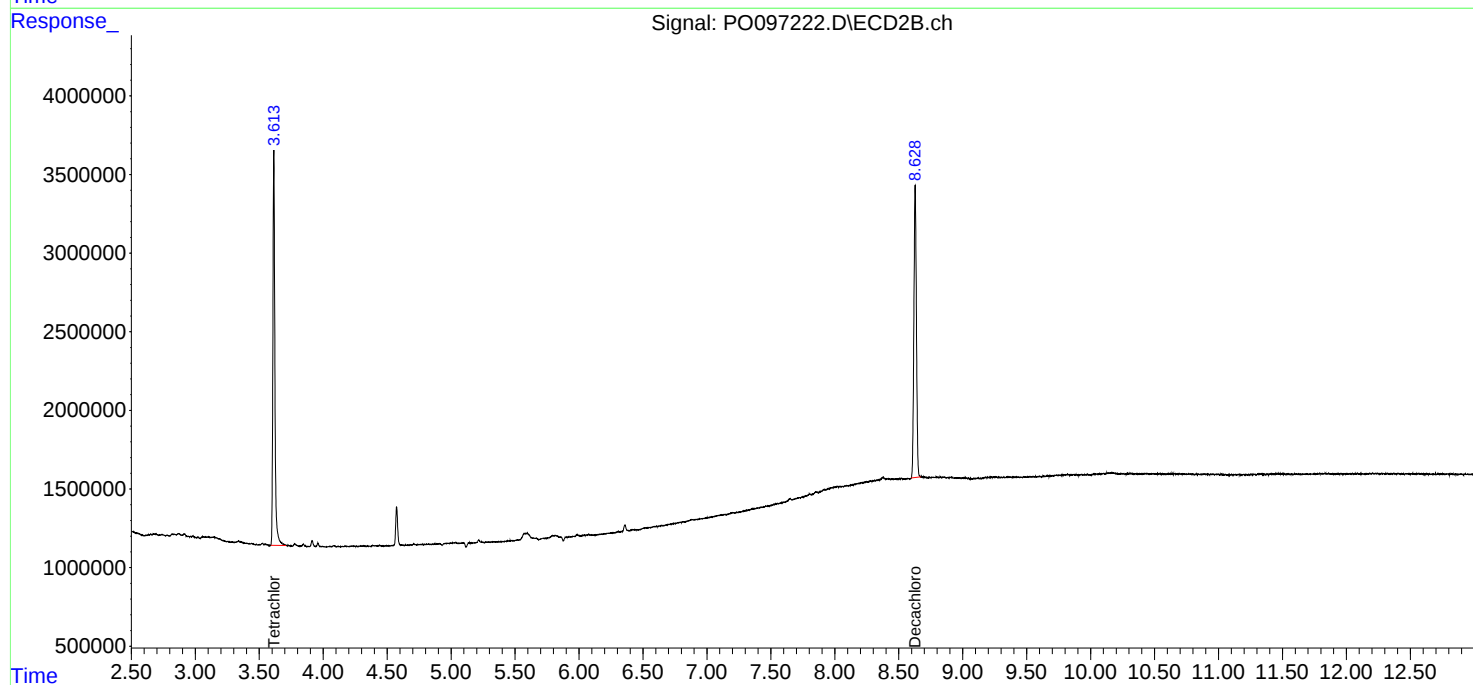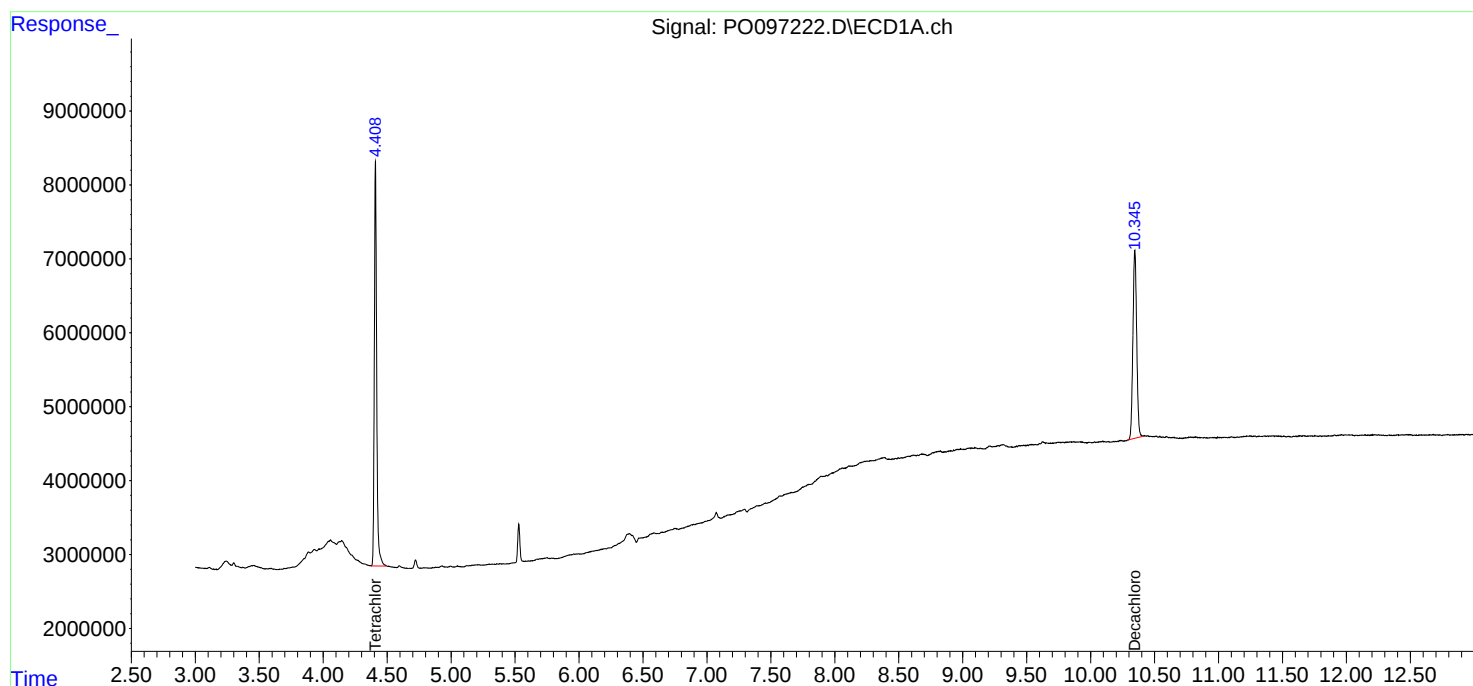

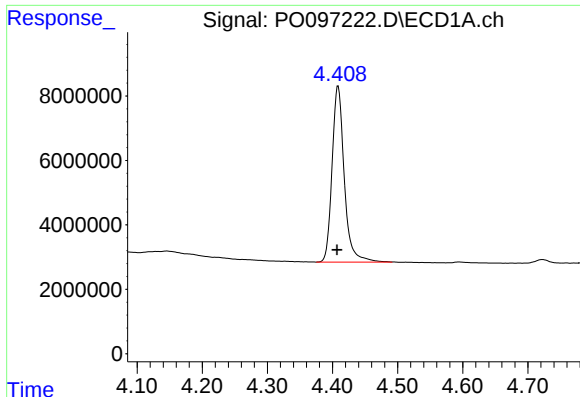

#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: 0.002 min
Response: 71047879
Conc: 21.46 ng/ml

Instrument :

ECD_O


ClientSampleId :

I.BLK

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

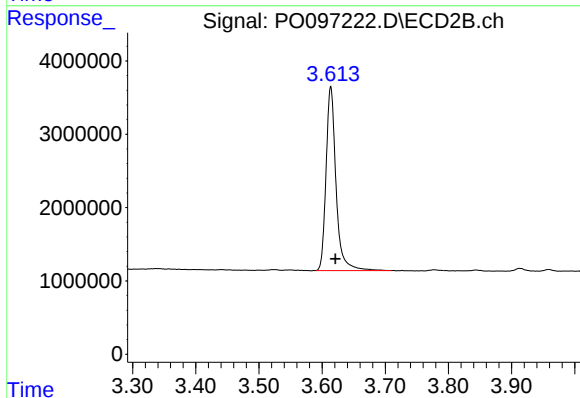


#1 Tetrachloro-m-xylene

R.T.: 3.614 min
Delta R.T.: -0.007 min
Response: 27465538
Conc: 20.75 ng/ml

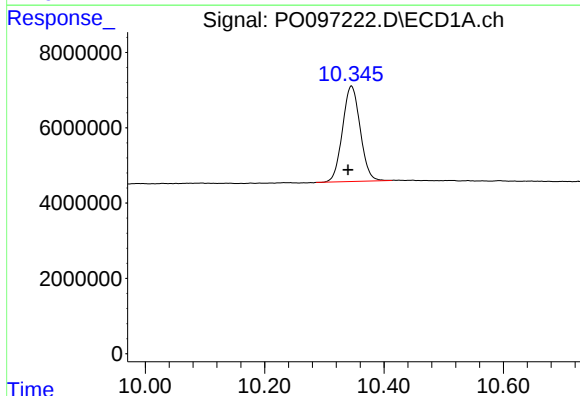

#2 Decachlorobiphenyl

R.T.: 10.346 min
Delta R.T.: 0.006 min
Response: 52183590
Conc: 23.85 ng/ml

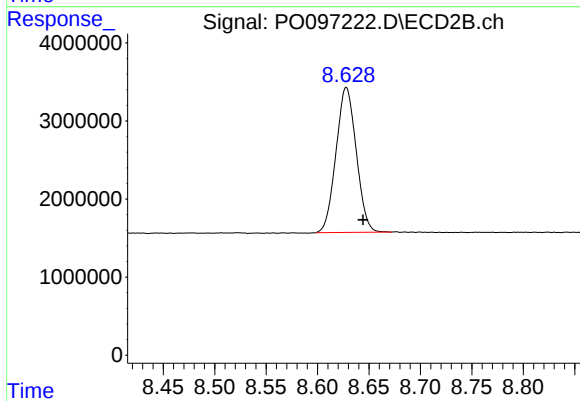

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.017 min
Response: 25438127
Conc: 21.99 ng/ml m