

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081820\
 Data File : P0070652.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Aug 2020 18:42
 Operator : DD\AJ
 Sample : L3712-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-26572

Manual Integrations
 APPROVED

Ankita
 8/20/2020 2:08:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:13:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.366	3.551	1876147	1050890	28.372	23.852
2)	SA Decachlor...	9.996	8.741	1982644	1327506	23.155	23.916
Target Compounds							
26)	L6 AR-1254-1	6.570	5.634	354059	378187	99.498m	107.992
27)	L6 AR-1254-2	6.792	5.796	743089	258690	133.459	83.065 #
28)	L6 AR-1254-3	7.166	6.205	863341	577712	149.914	117.188
29)	L6 AR-1254-4	7.462	6.446	441754	271822	84.685	75.524
30)	L6 AR-1254-5	7.883	6.869	1018840	681368	192.855	148.140

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081820\
Data File : PO070652.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Aug 2020 18:42
Operator : DD\AJ
Sample : L3712-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Ankita
8/20/2020 2:08:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:13:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

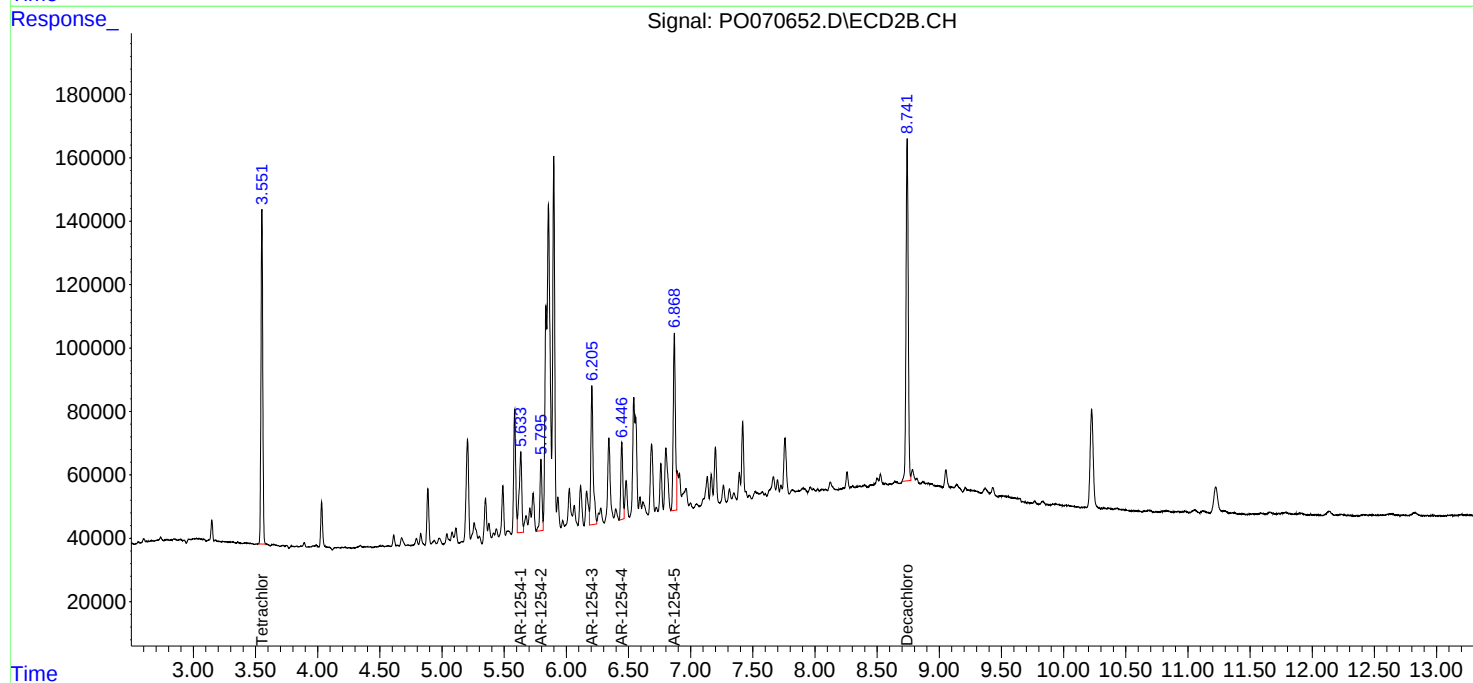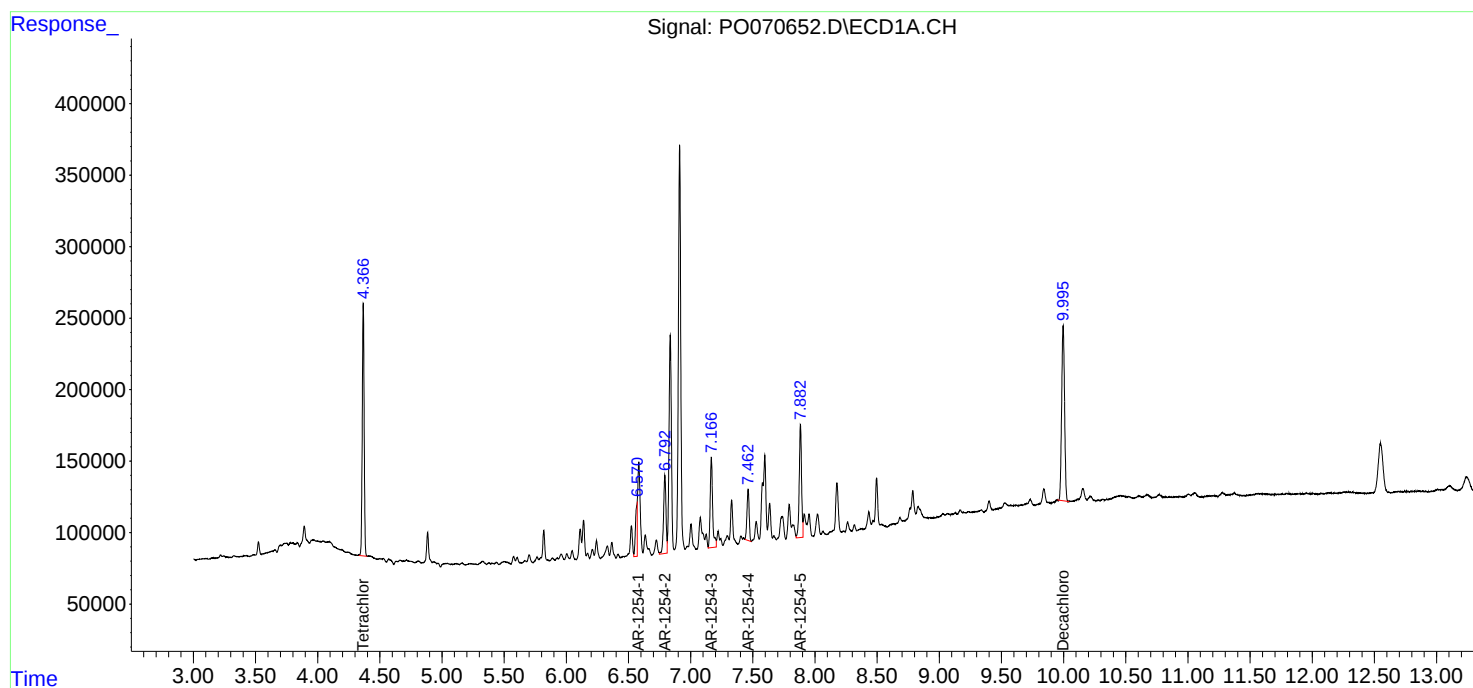

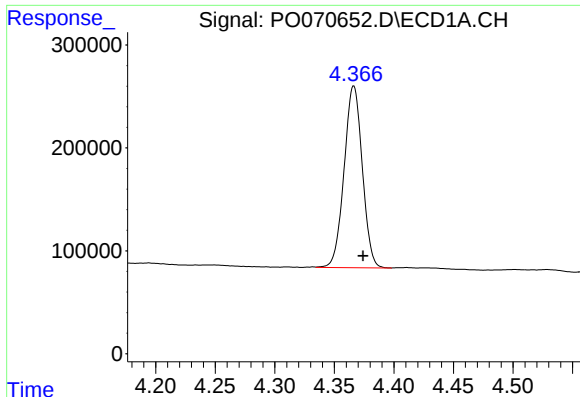


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.008 min
Response: 1876147
Conc: 28.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Ankita
8/20/2020 2:08:42 PM

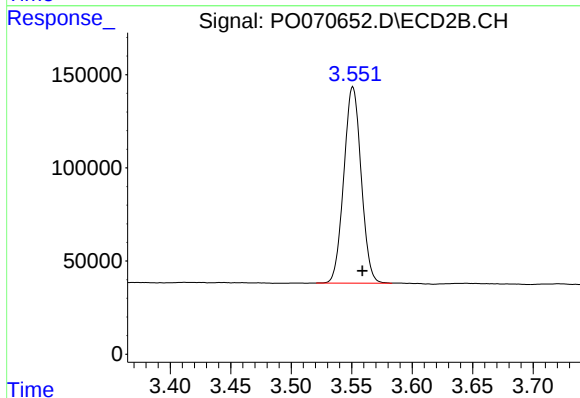


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.008 min
Response: 1050890
Conc: 23.85 ng/ml

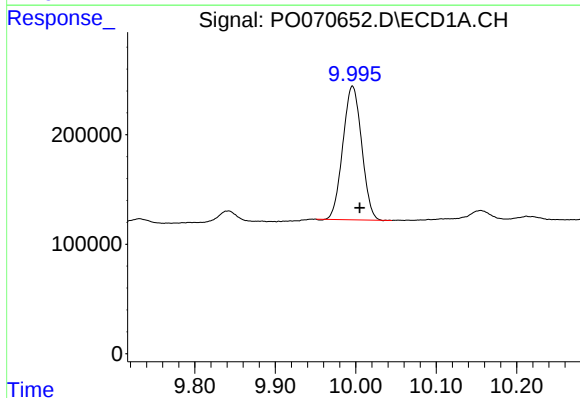


#2 Decachlorobiphenyl

R.T.: 9.996 min
Delta R.T.: -0.009 min
Response: 1982644
Conc: 23.16 ng/ml

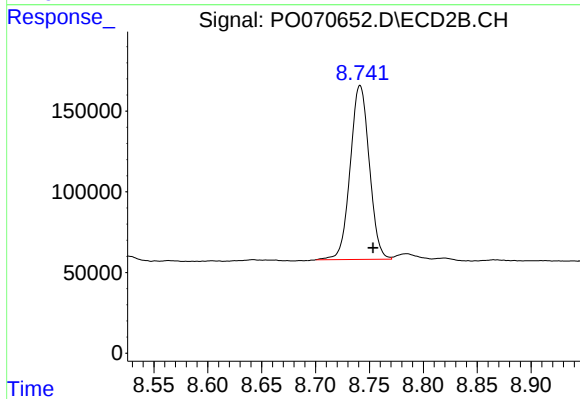

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.012 min
Response: 1327506
Conc: 23.92 ng/ml

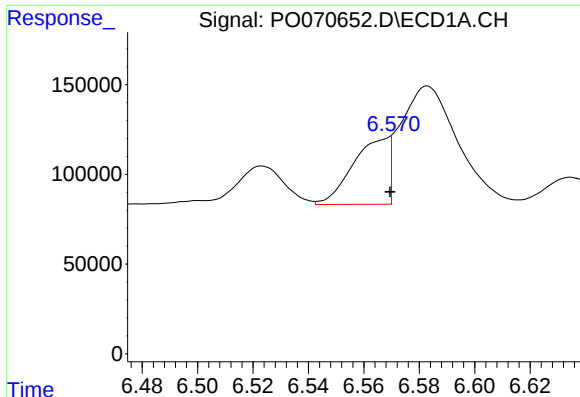


#26 AR-1254-1

R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 354059
Conc: 99.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Ankita
8/20/2020 2:08:42 PM

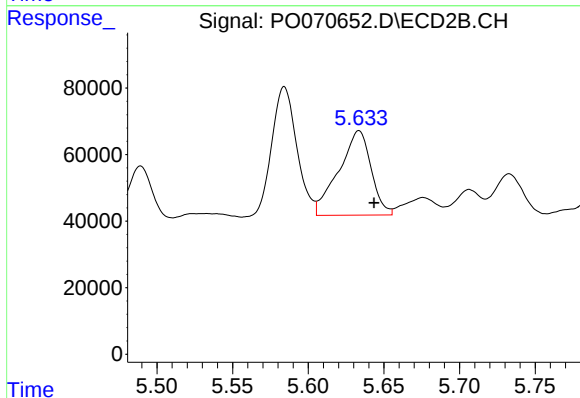


#26 AR-1254-1

R.T.: 5.634 min
Delta R.T.: -0.010 min
Response: 378187
Conc: 107.99 ng/ml

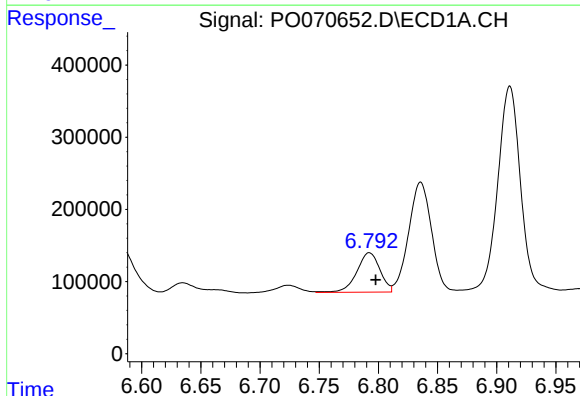


#27 AR-1254-2

R.T.: 6.792 min
Delta R.T.: -0.005 min
Response: 743089
Conc: 133.46 ng/ml

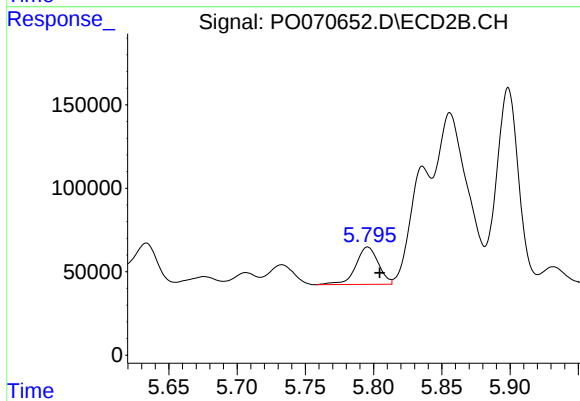

#27 AR-1254-2

R.T.: 5.796 min
Delta R.T.: -0.009 min
Response: 258690
Conc: 83.06 ng/ml

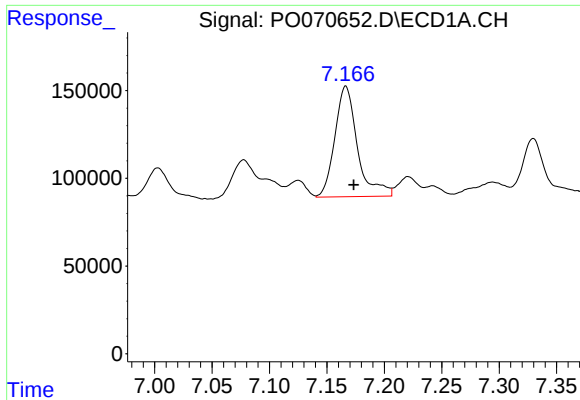


#28 AR-1254-3

R.T.: 7.166 min
Delta R.T.: -0.007 min
Response: 863341
Conc: 149.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26572


Manual Integrations
APPROVED

Ankita
8/20/2020 2:08:42 PM

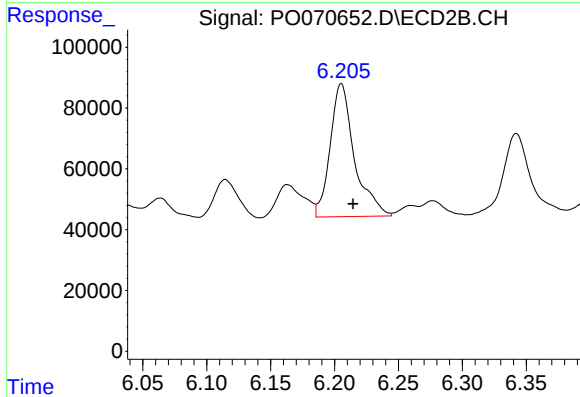


#28 AR-1254-3

R.T.: 6.205 min
Delta R.T.: -0.009 min
Response: 577712
Conc: 117.19 ng/ml

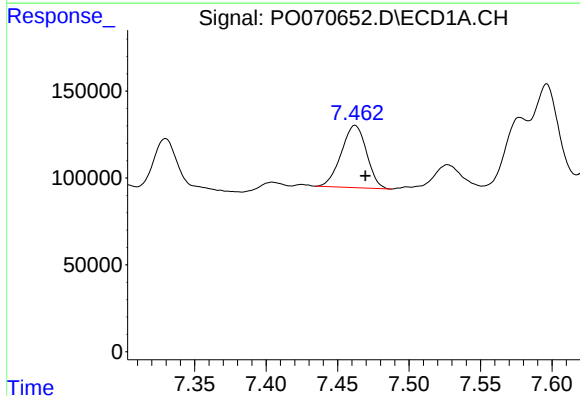


#29 AR-1254-4

R.T.: 7.462 min
Delta R.T.: -0.007 min
Response: 441754
Conc: 84.69 ng/ml

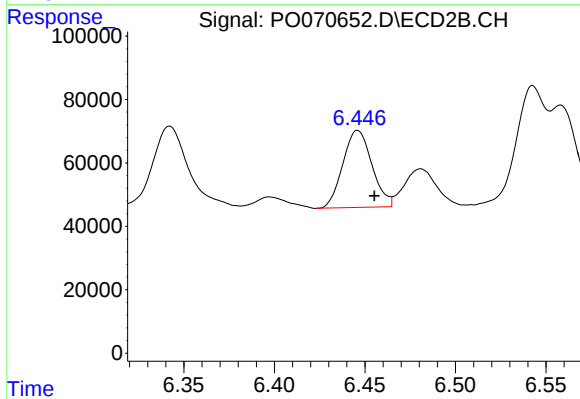

#29 AR-1254-4

R.T.: 6.446 min
Delta R.T.: -0.009 min
Response: 271822
Conc: 75.52 ng/ml

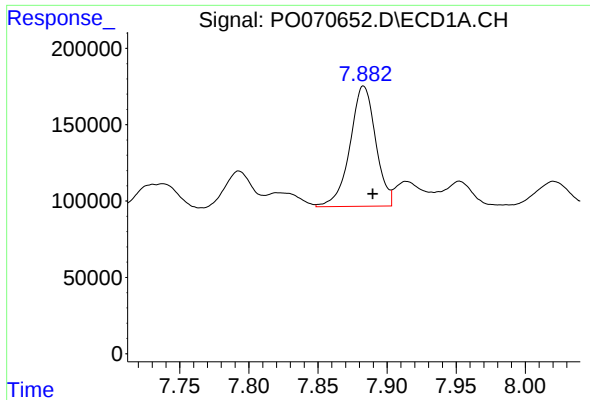


#30 AR-1254-5

R.T.: 7.883 min
Delta R.T.: -0.007 min
Response: 1018840
Conc: 192.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-26572

Manual Integrations
APPROVED

Ankita
8/20/2020 2:08:42 PM

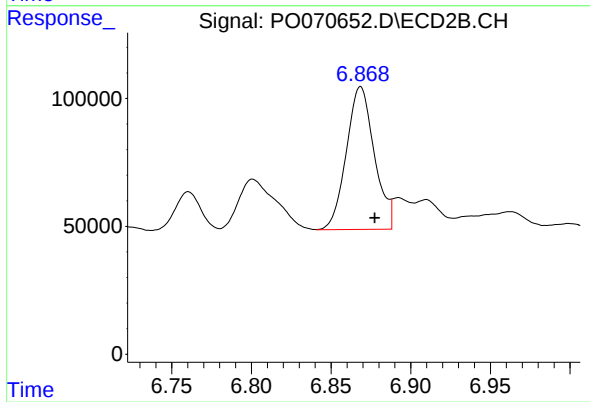

#30 AR-1254-5

R.T.: 6.869 min
Delta R.T.: -0.009 min
Response: 681368
Conc: 148.14 ng/ml