

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081823\
 Data File : P0097278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2023 22:46
 Operator : YP/AJ
 Sample : 04029-01 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEE806M-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 00:14:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 08 04:34:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.613	5766768	2187612	1.742	1.653
2) SA Decachlor...	10.349	8.628	4528858	2259472	2.070m	1.953
Target Compounds						
26) L6 AR-1254-1	6.470	5.501	5272283	3982585	48.241	53.967
27) L6 AR-1254-2	6.695	5.650	8521148	3313170	52.852	50.291
28) L6 AR-1254-3	7.071	6.053	7071943	4025217	45.131	39.829
29) L6 AR-1254-4	7.364	6.283	5217934	2564338	51.756	44.308
30) L6 AR-1254-5	7.796	6.702	4630092	2988097	41.261	33.988

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081823\
Data File : PO097278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2023 22:46
Operator : YP/AJ
Sample : 04029-01 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEE806M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 00:14:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 08 04:34:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

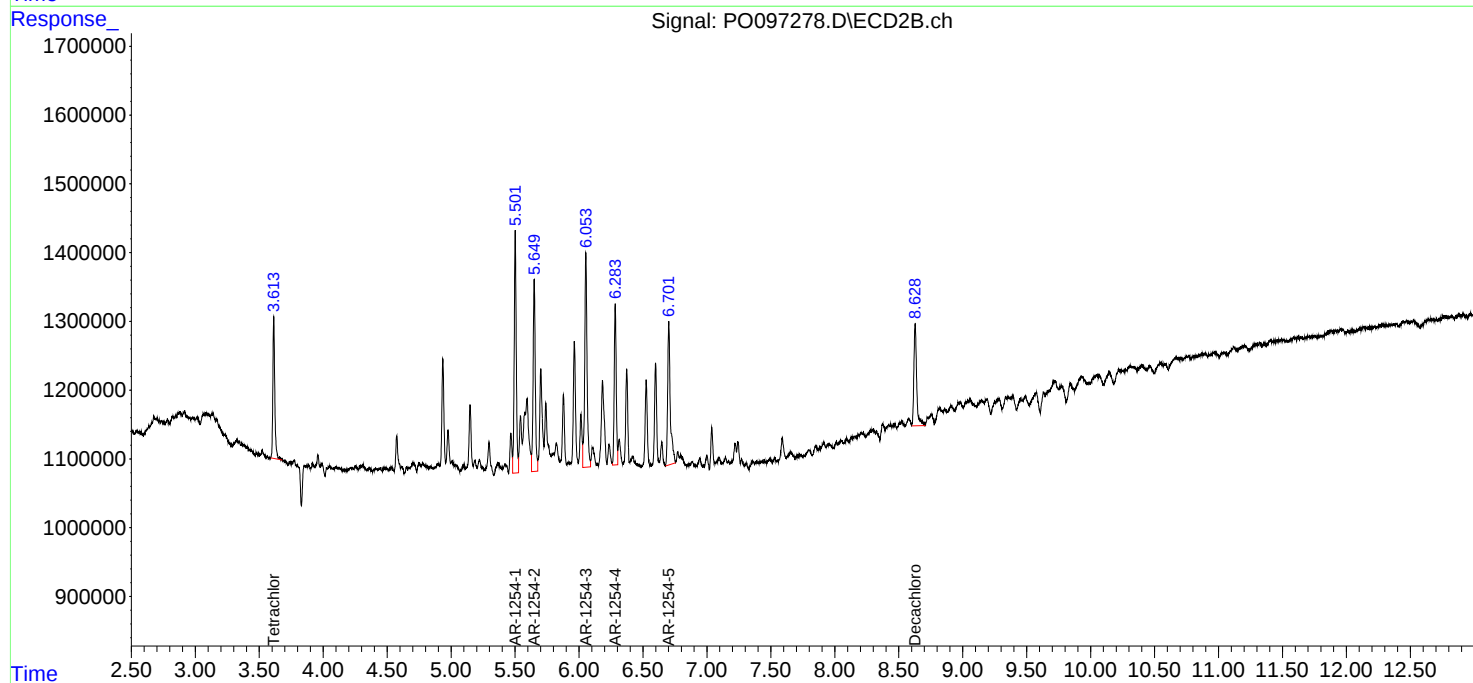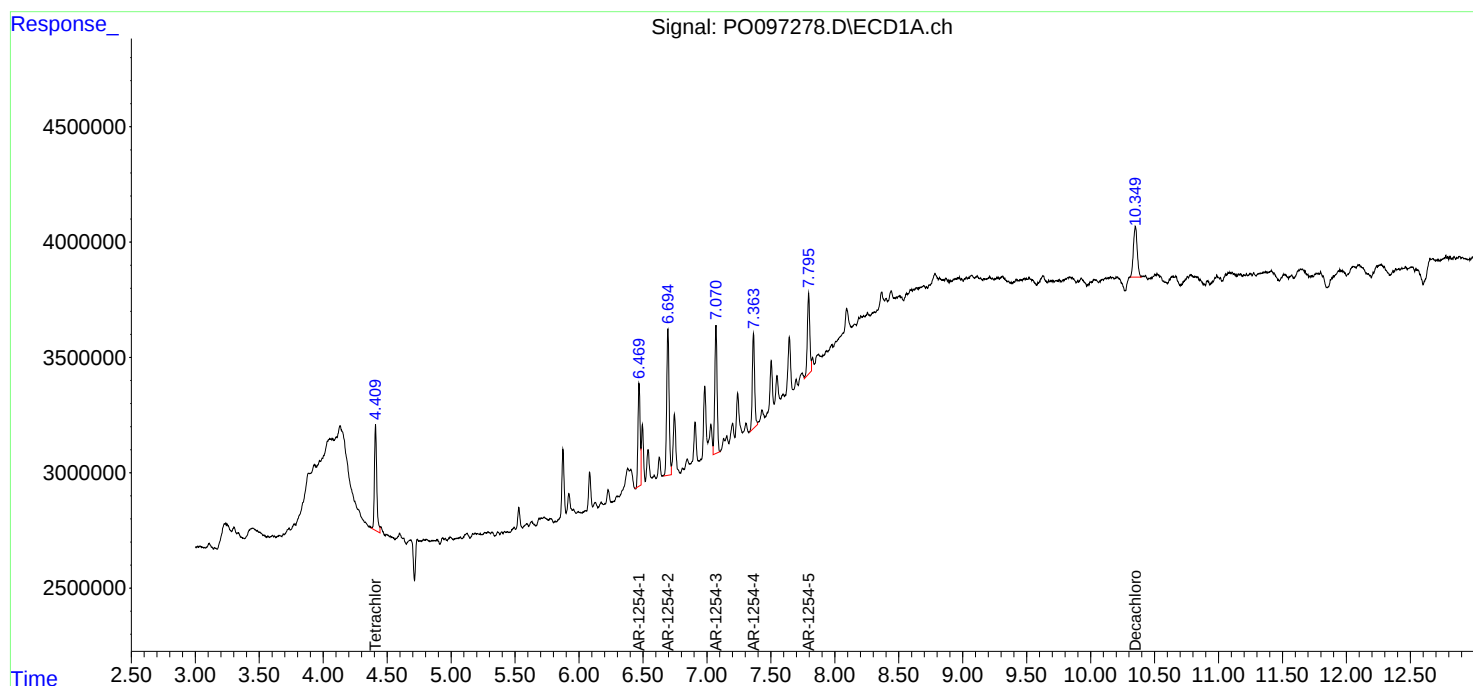

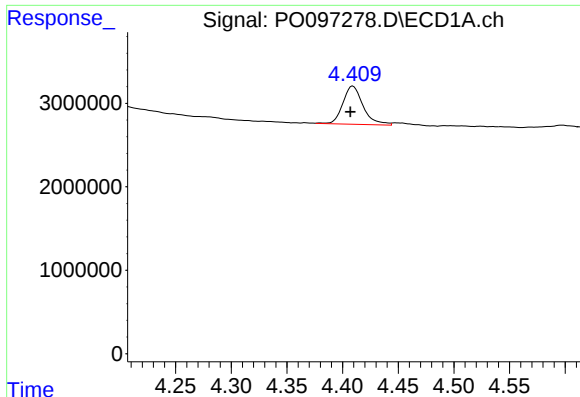


#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: 0.002 min
Response: 5766768
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE806M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

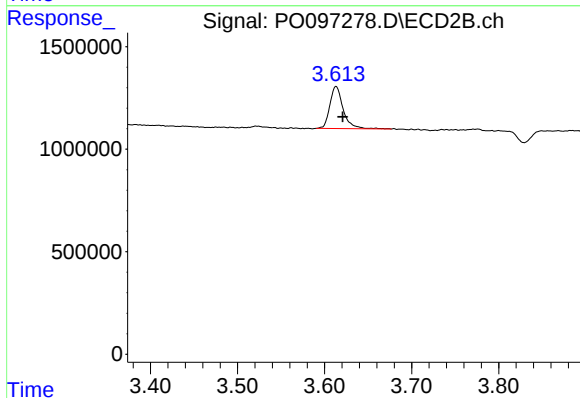


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: -0.008 min
Response: 2187612
Conc: 1.65 ng/ml

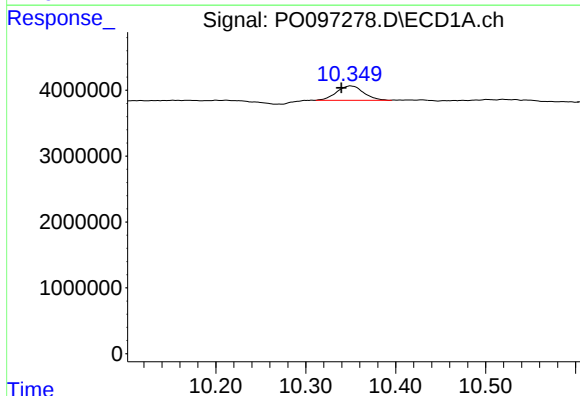


#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: 0.009 min
Response: 4528858
Conc: 2.07 ng/ml m

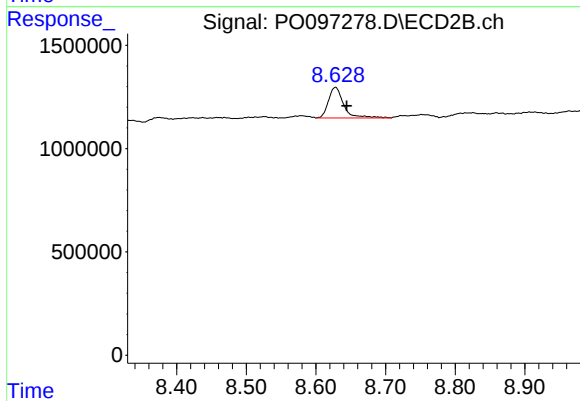

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.016 min
Response: 2259472
Conc: 1.95 ng/ml

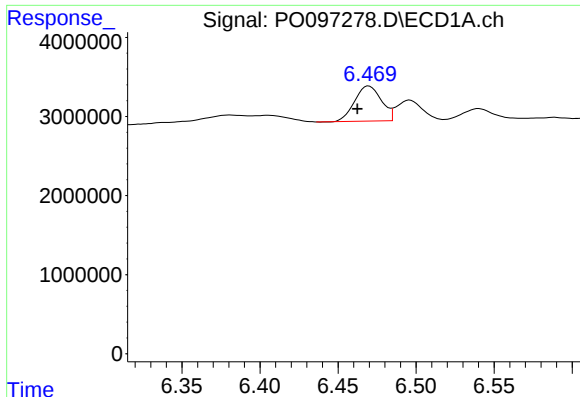


#26 AR-1254-1

R.T.: 6.470 min
Delta R.T.: 0.007 min
Response: 5272283
Conc: 48.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE806M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

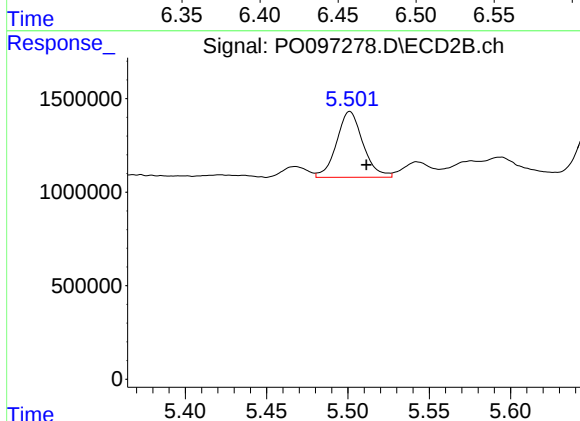


#26 AR-1254-1

R.T.: 5.501 min
Delta R.T.: -0.010 min
Response: 3982585
Conc: 53.97 ng/ml

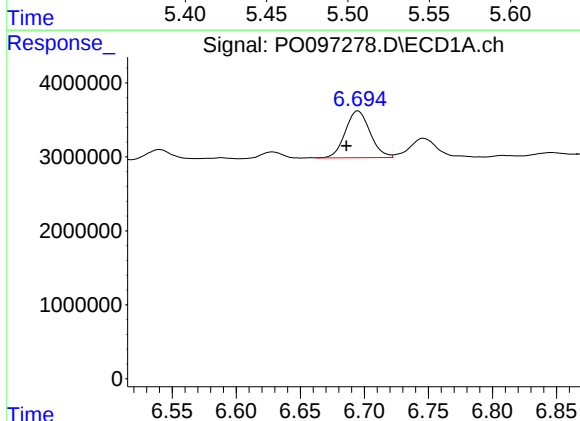


#27 AR-1254-2

R.T.: 6.695 min
Delta R.T.: 0.009 min
Response: 8521148
Conc: 52.85 ng/ml

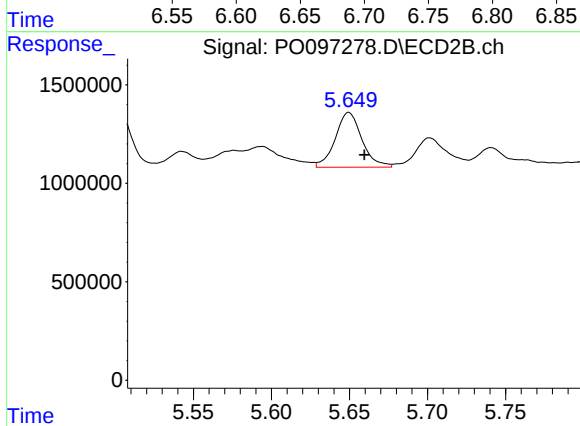

#27 AR-1254-2

R.T.: 5.650 min
Delta R.T.: -0.010 min
Response: 3313170
Conc: 50.29 ng/ml

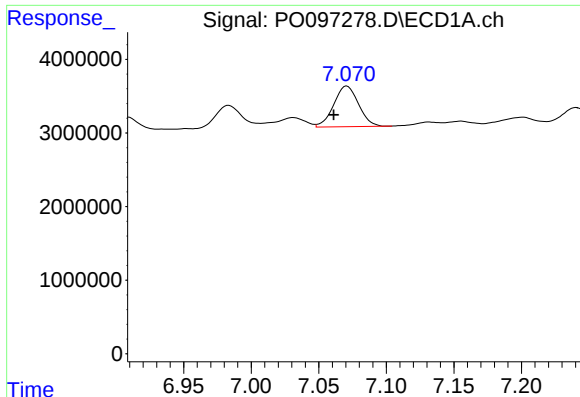


#28 AR-1254-3

R.T.: 7.071 min
Delta R.T.: 0.010 min
Response: 7071943
Conc: 45.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE806M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

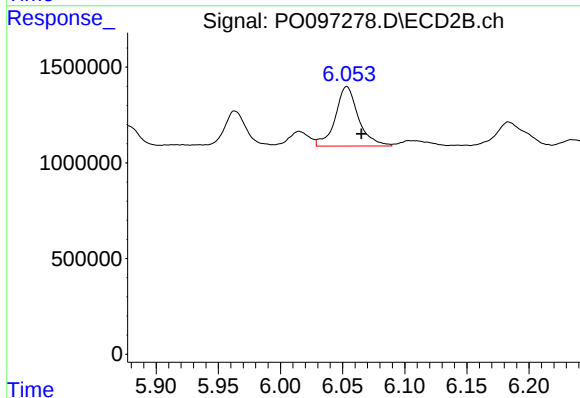


#28 AR-1254-3

R.T.: 6.053 min
Delta R.T.: -0.012 min
Response: 4025217
Conc: 39.83 ng/ml

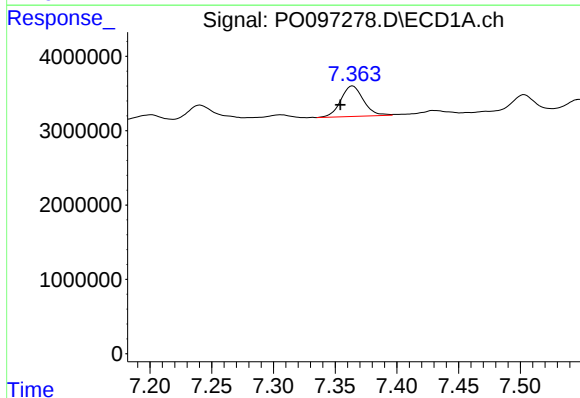


#29 AR-1254-4

R.T.: 7.364 min
Delta R.T.: 0.010 min
Response: 5217934
Conc: 51.76 ng/ml

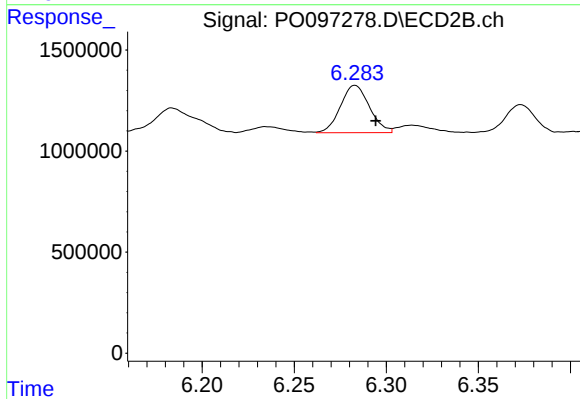

#29 AR-1254-4

R.T.: 6.283 min
Delta R.T.: -0.011 min
Response: 2564338
Conc: 44.31 ng/ml

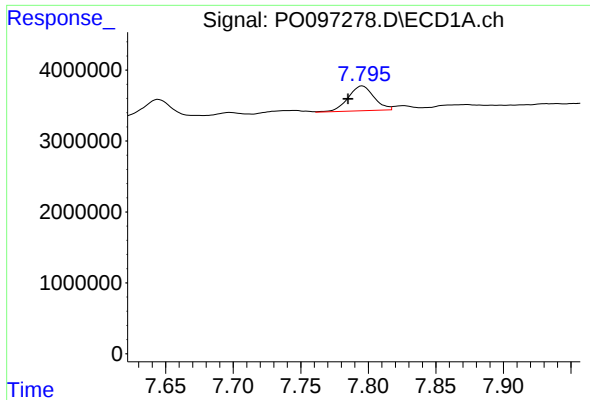


#30 AR-1254-5

R.T.: 7.796 min
Delta R.T.: 0.011 min
Response: 4630092
Conc: 41.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE806M-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

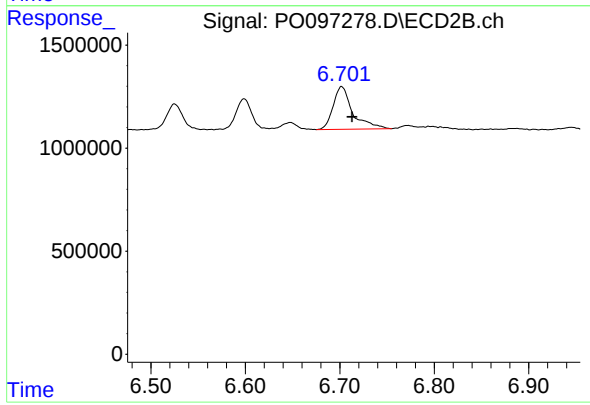

#30 AR-1254-5

R.T.: 6.702 min
Delta R.T.: -0.011 min
Response: 2988097
Conc: 33.99 ng/ml