

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 21:44
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:14:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.649	0	43015	N.D.	0.008 #
2)	SA Decachlor...	8.686	8.618	214730	616876	0.031	0.326 #
Target Compounds							
3)	L1 AR-1016-1	4.739	4.734	168963	188118	0.633	1.103 #
4)	L1 AR-1016-2	4.768	4.752	565172	94729	1.408	0.368 #
5)	L1 AR-1016-3	4.840	4.931	1035592	593416	4.061	4.250
6)	L1 AR-1016-4	4.954	4.970	1712265	2054784	7.852	17.608 #
7)	L1 AR-1016-5	5.192	5.180	3198763	1578563	14.433	11.075
8)	L2 AR-1221-1	3.835f	3.872	392404	142509	4.194	2.258 #
9)	L2 AR-1221-2	3.957	3.954	197478	79117	2.923	1.695 #
10)	L2 AR-1221-3	3.973f	4.027	80475	90547	0.364	0.610 #
11)	L3 AR-1232-1	3.973f	4.027	80475	90547	0.462	0.771 #
12)	L3 AR-1232-2	4.524	4.752	1052942	94729	10.545	0.773 #
13)	L3 AR-1232-3	4.768	4.931	565172	593416	2.983	9.368 #
14)	L3 AR-1232-4	4.954	5.007	1712265	252868	18.183	4.498 #
15)	L3 AR-1232-5	4.996	5.180	3904081	1578563	63.027	26.369 #
16)	L4 AR-1242-1	4.739	4.734	168963	188118	0.735	1.302 #
17)	L4 AR-1242-2	4.768	4.752	565172	94729	1.645	0.437 #
18)	L4 AR-1242-3	4.840	4.931	1035592	593416	4.667	5.073
19)	L4 AR-1242-4	4.954	5.007	1712265	252868	9.871	2.150 #
20)	L4 AR-1242-5	5.599	5.528	5896926	770749	29.461	5.168 #
21)	L5 AR-1248-1	4.739	4.734	168963	188118	0.968	1.687 #
22)	L5 AR-1248-2	4.996	4.970	3904081	2054784	16.142	12.787
23)	L5 AR-1248-3	5.192	5.007	3198763	252868	10.032	1.490 #
24)	L5 AR-1248-4	5.553	5.180	3277168	1578563	6.560	7.924
25)	L5 AR-1248-5	5.599	5.567	5896926	479887	17.268	2.260 #
26)	L6 AR-1254-1	5.553	5.528	3277168	770749	6.069	2.444 #
27)	L6 AR-1254-2	5.724	5.669	54717939	535915	110.888	1.912 #
28)	L6 AR-1254-3	6.098	6.091	504000	13087478	0.682	31.391 #
29)	L6 AR-1254-4	6.316	6.303	4478351	129854	8.040	0.472 #
30)	L6 AR-1254-5	6.751	6.714	2564.2E6	1246.8E6	3658.113	3487.716
31)	L7 AR-1260-1	6.251	6.201	1118357	1045669	2.508	4.100 #
32)	L7 AR-1260-2	6.429	6.393	25069436	13750672	36.506	39.775
33)	L7 AR-1260-3	6.751f	6.563	2564.2E6	-68001	4152.795	N.D. #
34)	L7 AR-1260-4	7.048	7.009	1204305	172259	2.689	0.831 #
35)	L7 AR-1260-5	7.293	7.255	1157195	206514	0.956	0.441 #
36)	L8 AR-1262-1	6.751f	6.790	2564.2E6	613205	2800.114	1.479 #
37)	L8 AR-1262-2	7.293	7.255	1157195	206514	0.765	0.399 #
38)	L8 AR-1262-3	7.573	7.540	1018381	151680	1.838	0.845 #
39)	L8 AR-1262-4	7.645	7.595	1041931	186362	1.065	0.643 #
40)	L8 AR-1262-5	8.139	8.074	324743	59366	0.779	0.548 #
41)	L9 AR-1268-1	7.573	7.540	1018381	151680	0.592	0.298 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081825\
 Data File : P0113036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 21:44
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:14:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.645	7.606	1041931	167706	0.719	0.404 #
43) L9	AR-1268-3	7.844	7.832	649042	47713	0.538	0.146 #
44) L9	AR-1268-4	8.139	8.074	324743	59366	0.705	0.493 #
45) L9	AR-1268-5	8.433	8.421f	665471	401091	0.209	0.514 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081825\
Data File : PO113036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 21:44
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:14:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

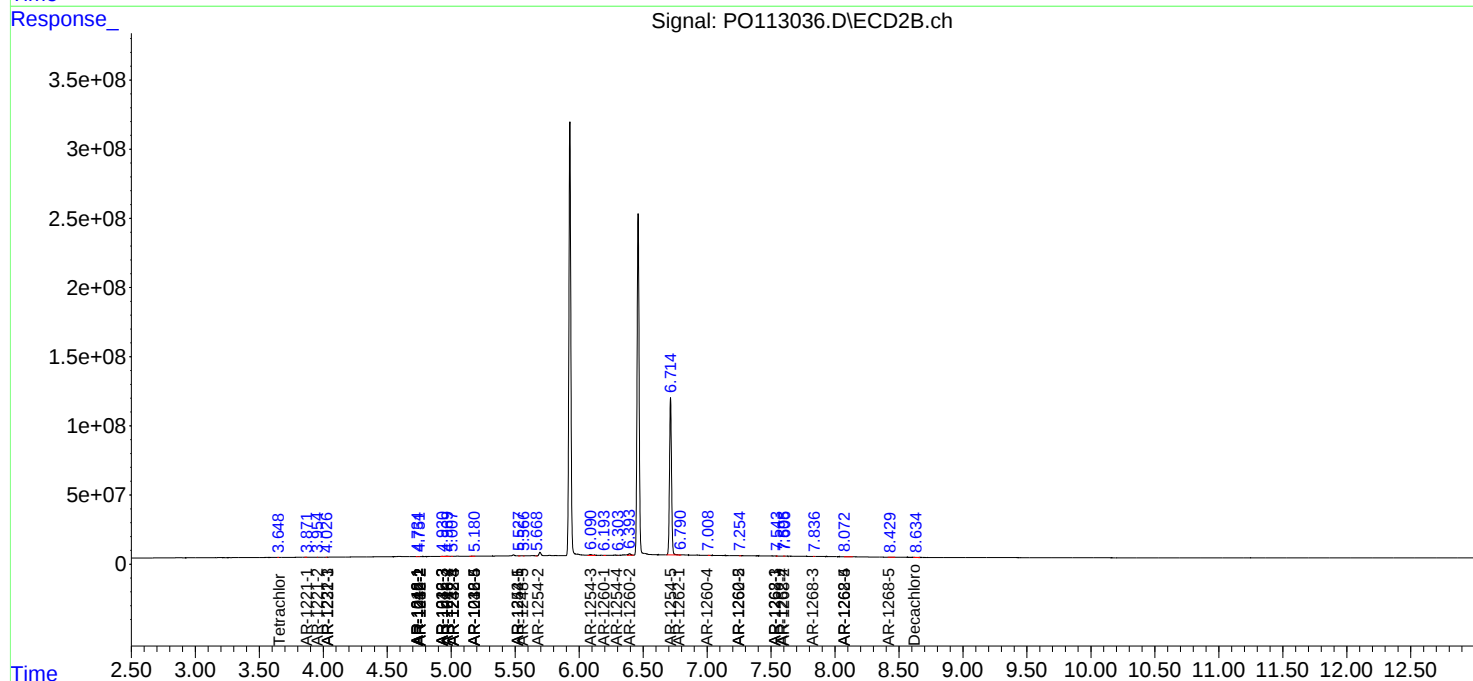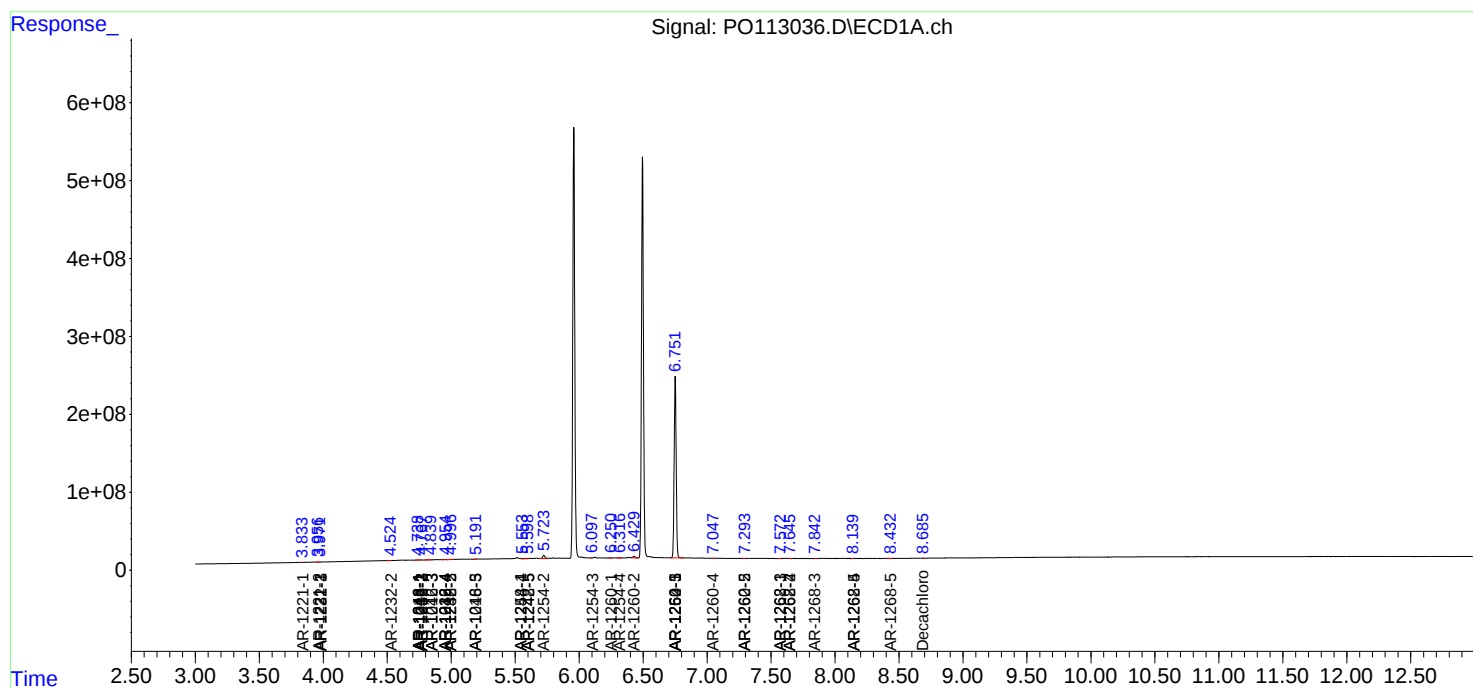


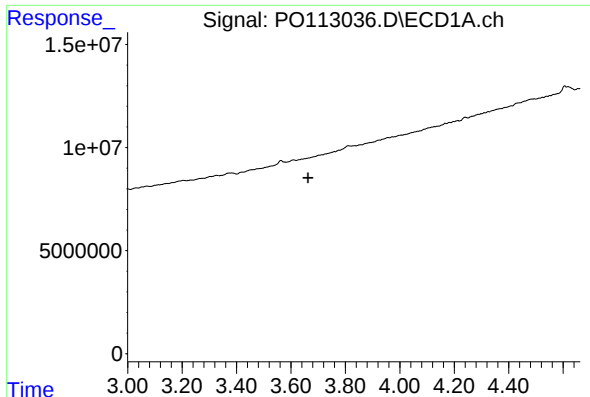

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

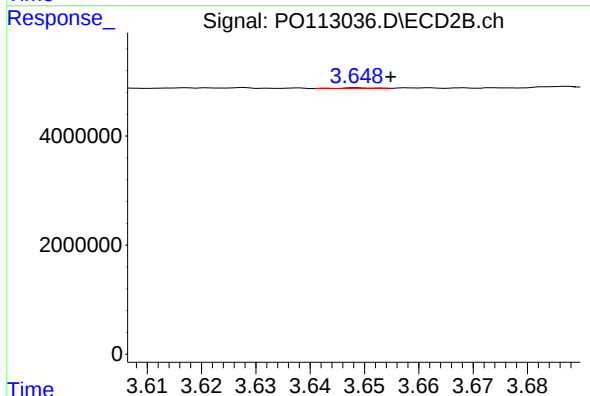


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.006 min
Response: 43015
Conc: 0.01 ng/ml

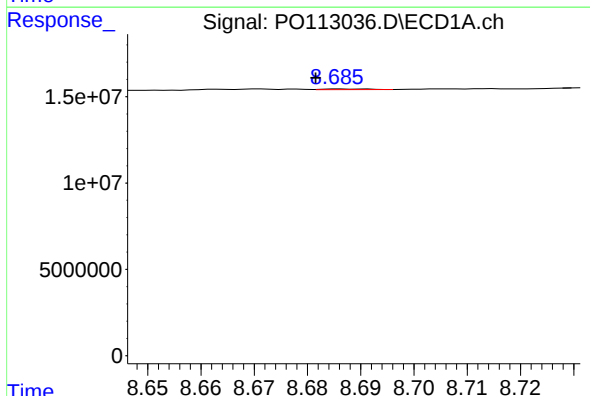


#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: 0.005 min
Response: 214730
Conc: 0.03 ng/ml

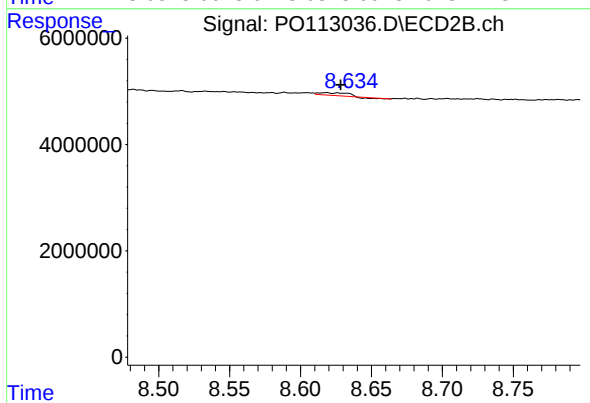

#2 Decachlorobiphenyl


R.T.: 8.618 min
Delta R.T.: -0.010 min
Response: 616876
Conc: 0.33 ng/ml

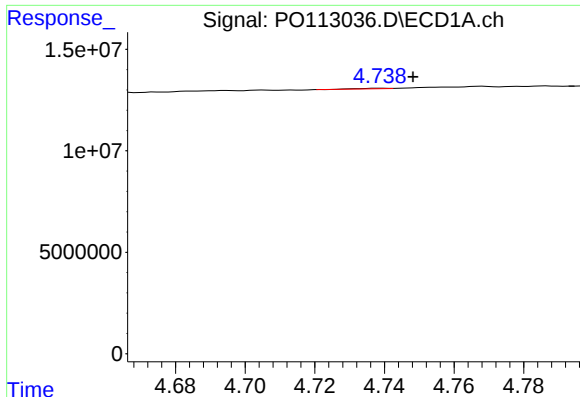

#3 AR-1016-1


R.T.: 4.739 min
Delta R.T.: -0.010 min
Response: 168963
Conc: 0.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

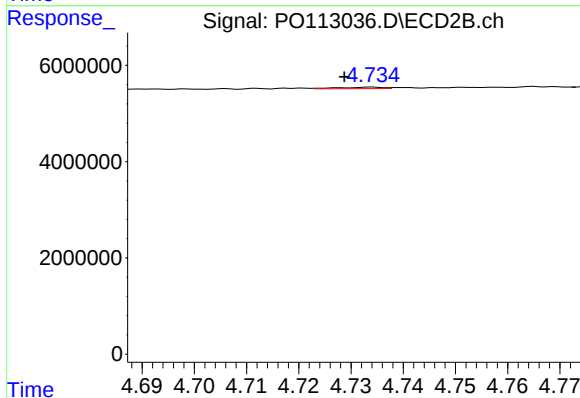


#3 AR-1016-1

R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 188118
Conc: 1.10 ng/ml

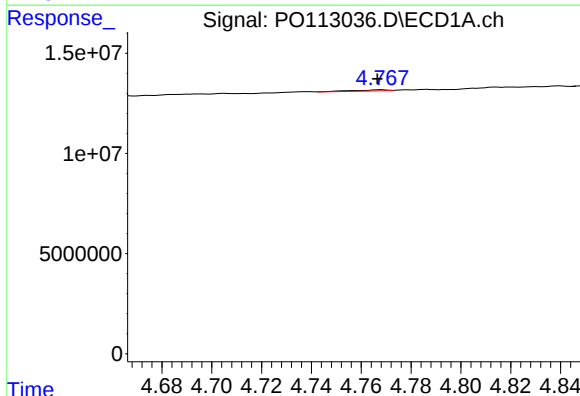


#4 AR-1016-2

R.T.: 4.768 min
Delta R.T.: 0.001 min
Response: 565172
Conc: 1.41 ng/ml

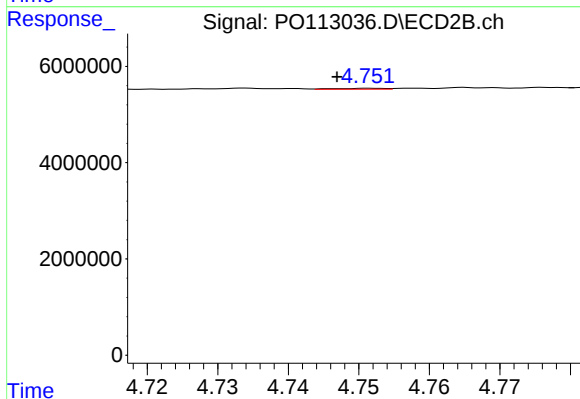

#4 AR-1016-2


R.T.: 4.752 min
Delta R.T.: 0.005 min
Response: 94729
Conc: 0.37 ng/ml

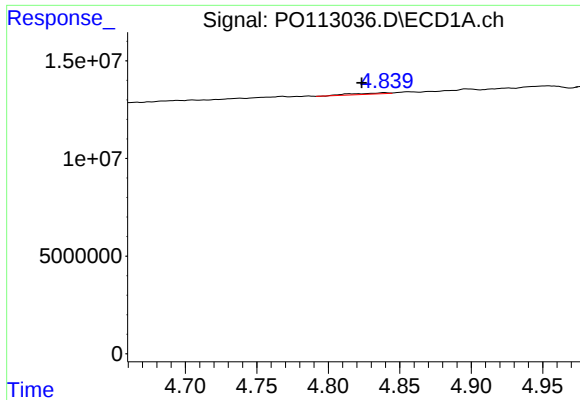

#5 AR-1016-3


R.T.: 4.840 min
Delta R.T.: 0.016 min
Response: 1035592
Conc: 4.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

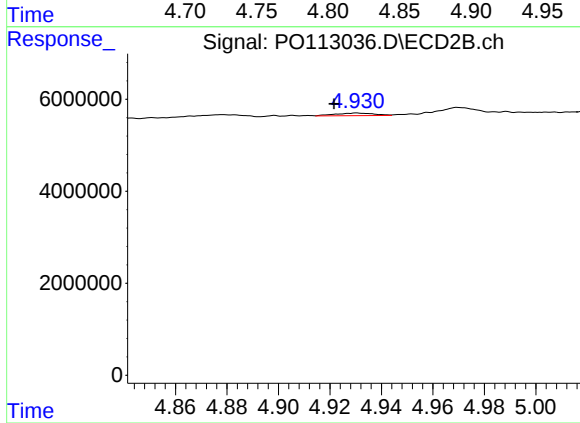


#5 AR-1016-3

R.T.: 4.931 min
Delta R.T.: 0.009 min
Response: 593416
Conc: 4.25 ng/ml

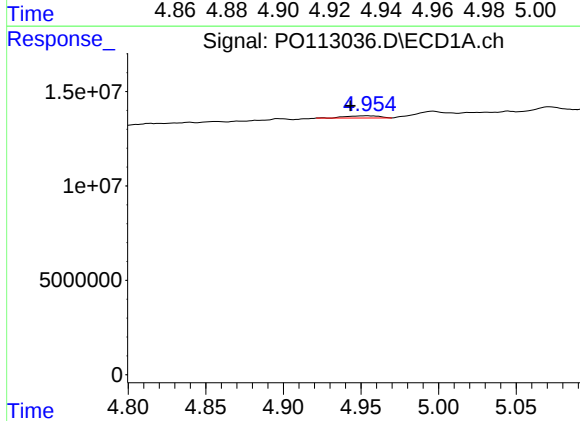


#6 AR-1016-4

R.T.: 4.954 min
Delta R.T.: 0.011 min
Response: 1712265
Conc: 7.85 ng/ml

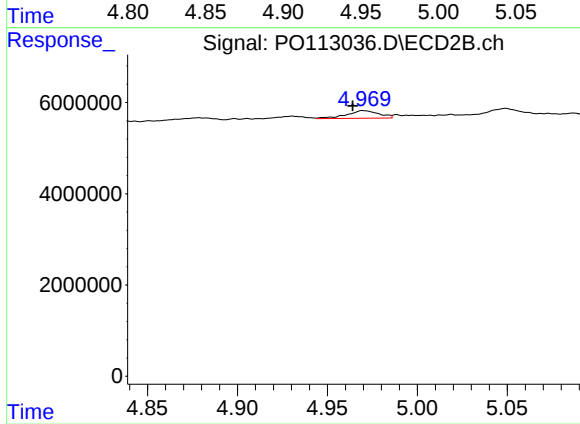

#6 AR-1016-4


R.T.: 4.970 min
Delta R.T.: 0.006 min
Response: 2054784
Conc: 17.61 ng/ml

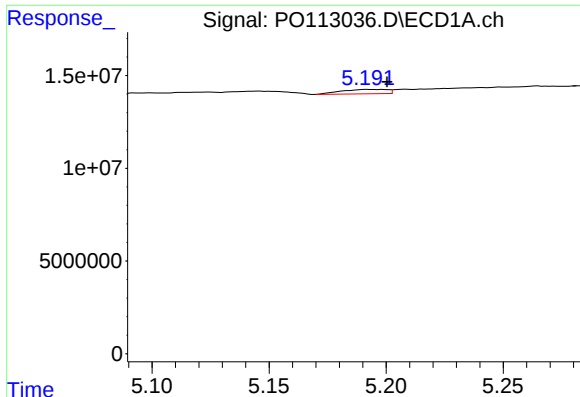

#7 AR-1016-5


R.T.: 5.192 min
Delta R.T.: -0.008 min
Response: 3198763
Conc: 14.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

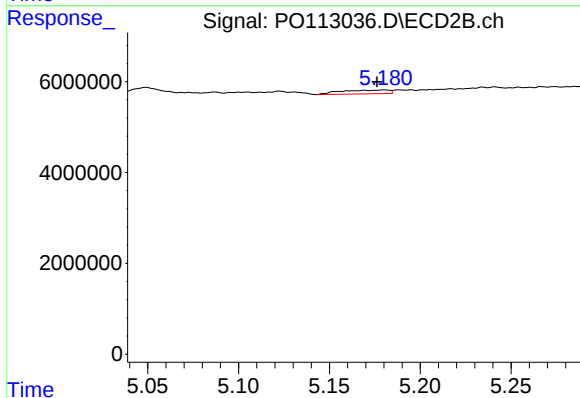


#7 AR-1016-5

R.T.: 5.180 min
Delta R.T.: 0.004 min
Response: 1578563
Conc: 11.08 ng/ml

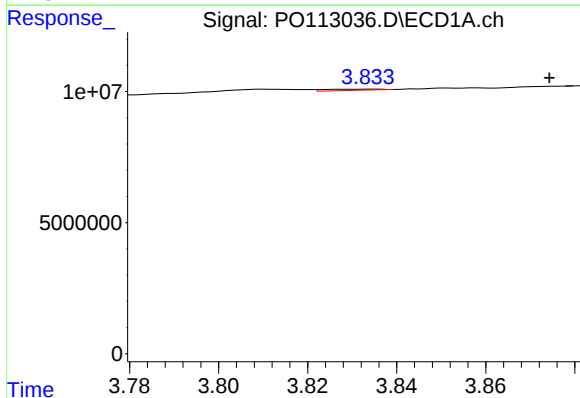


#8 AR-1221-1

R.T.: 3.835 min
Delta R.T.: -0.039 min
Response: 392404
Conc: 4.19 ng/ml

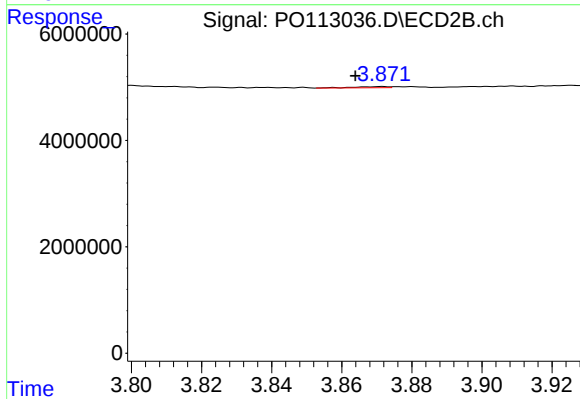

#8 AR-1221-1


R.T.: 3.872 min
Delta R.T.: 0.008 min
Response: 142509
Conc: 2.26 ng/ml

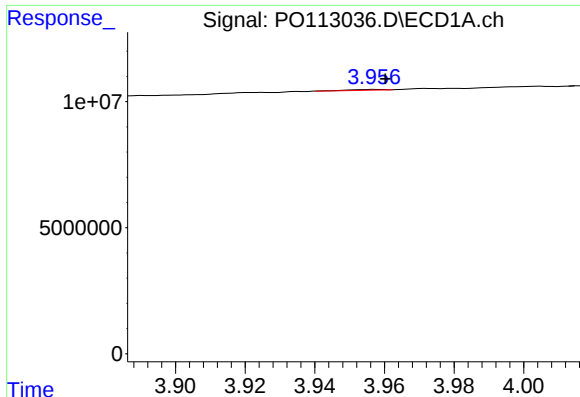

#9 AR-1221-2


R.T.: 3.957 min
Delta R.T.: -0.003 min
Response: 197478
Conc: 2.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

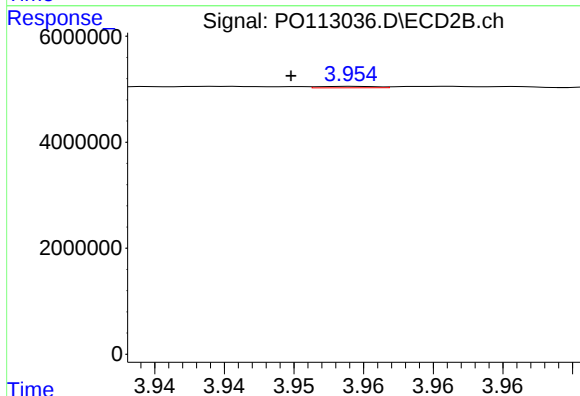


#9 AR-1221-2

R.T.: 3.954 min
Delta R.T.: 0.004 min
Response: 79117
Conc: 1.70 ng/ml

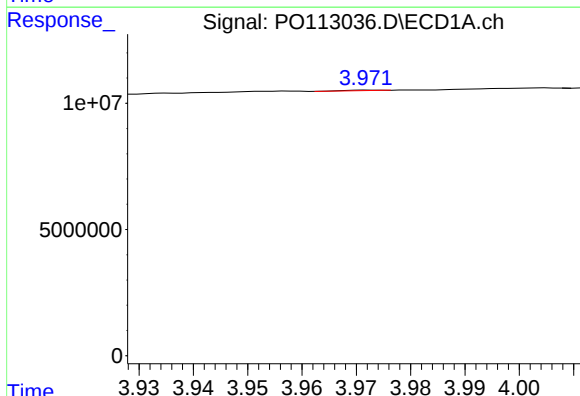


#10 AR-1221-3

R.T.: 3.973 min
Delta R.T.: -0.063 min
Response: 80475
Conc: 0.36 ng/ml

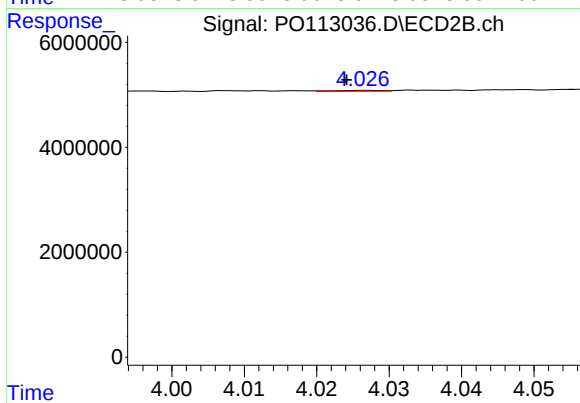

#10 AR-1221-3


R.T.: 4.027 min
Delta R.T.: 0.003 min
Response: 90547
Conc: 0.61 ng/ml

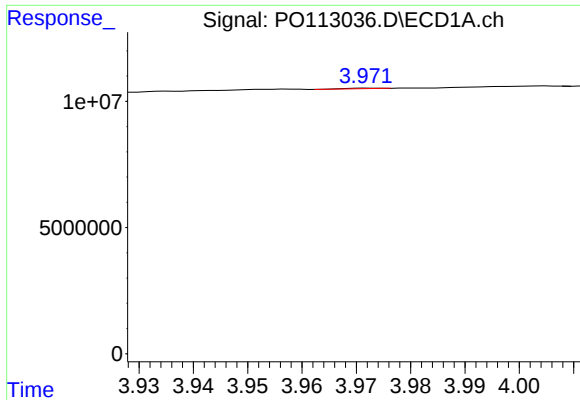

#11 AR-1232-1


R.T.: 3.973 min
Delta R.T.: -0.063 min
Response: 80475
Conc: 0.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

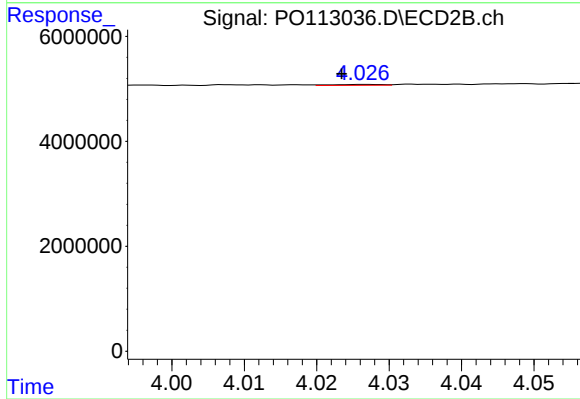


#11 AR-1232-1

R.T.: 4.027 min
Delta R.T.: 0.003 min
Response: 90547
Conc: 0.77 ng/ml

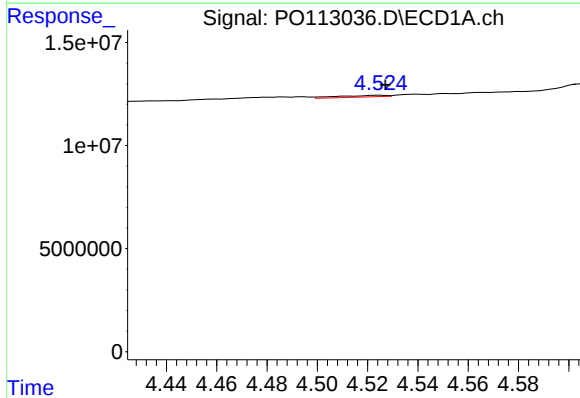


#12 AR-1232-2

R.T.: 4.524 min
Delta R.T.: -0.003 min
Response: 1052942
Conc: 10.54 ng/ml

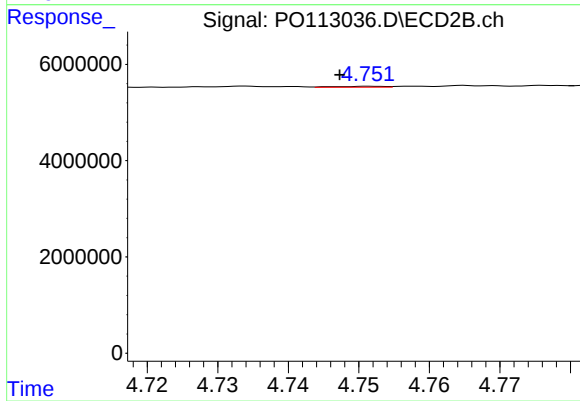

#12 AR-1232-2


R.T.: 4.752 min
Delta R.T.: 0.004 min
Response: 94729
Conc: 0.77 ng/ml

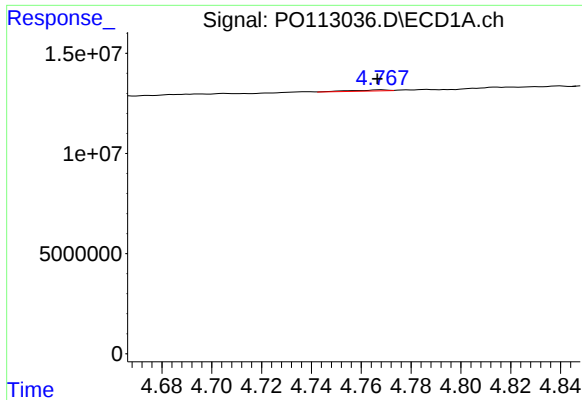

#13 AR-1232-3


R.T.: 4.768 min
Delta R.T.: 0.001 min
Response: 565172
Conc: 2.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

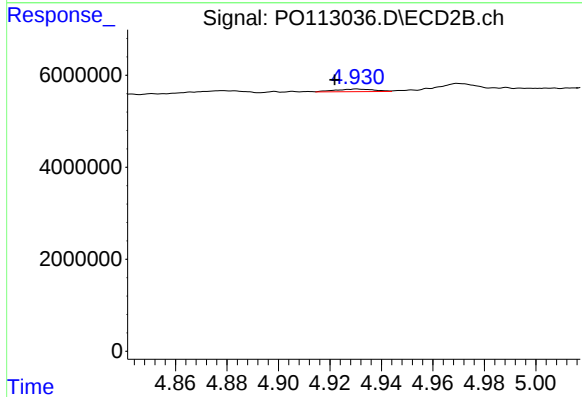


#13 AR-1232-3

R.T.: 4.931 min
Delta R.T.: 0.009 min
Response: 593416
Conc: 9.37 ng/ml

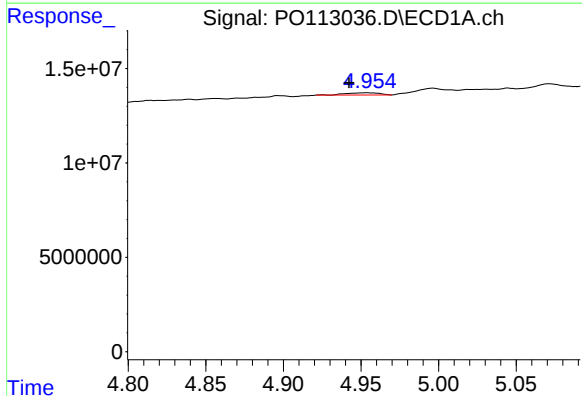


#14 AR-1232-4

R.T.: 4.954 min
Delta R.T.: 0.012 min
Response: 1712265
Conc: 18.18 ng/ml

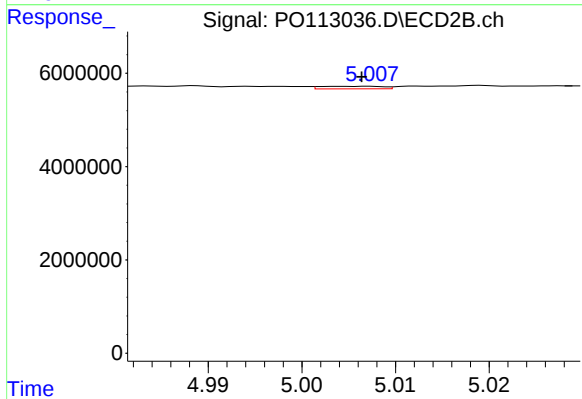

#14 AR-1232-4


R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 252868
Conc: 4.50 ng/ml

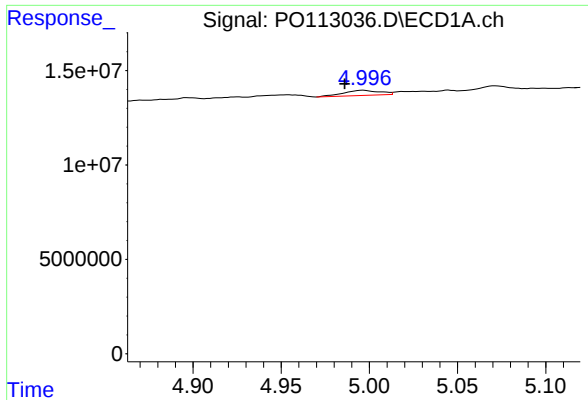

#15 AR-1232-5


R.T.: 4.996 min
Delta R.T.: 0.010 min
Response: 3904081
Conc: 63.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

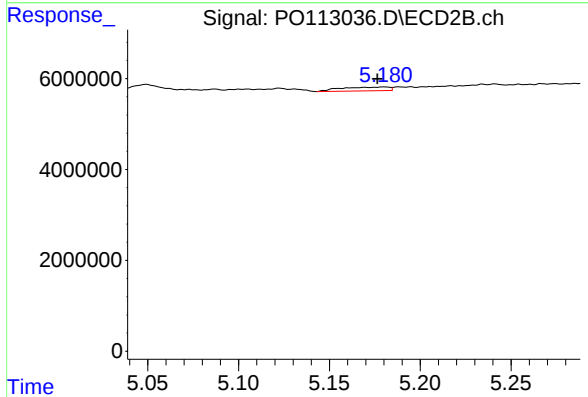


#15 AR-1232-5

R.T.: 5.180 min
Delta R.T.: 0.003 min
Response: 1578563
Conc: 26.37 ng/ml

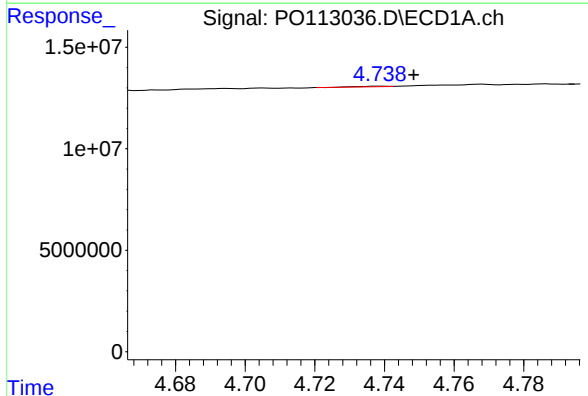


#16 AR-1242-1

R.T.: 4.739 min
Delta R.T.: -0.010 min
Response: 168963
Conc: 0.73 ng/ml

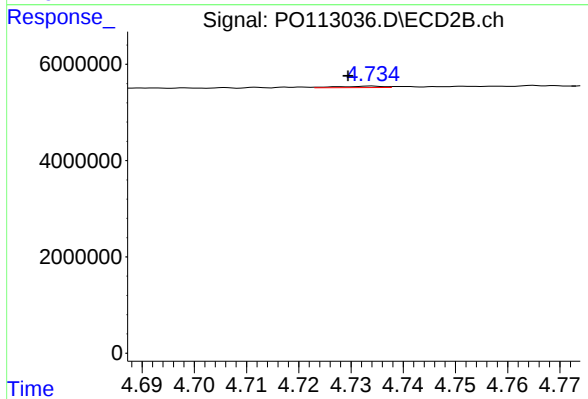

#16 AR-1242-1


R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 188118
Conc: 1.30 ng/ml

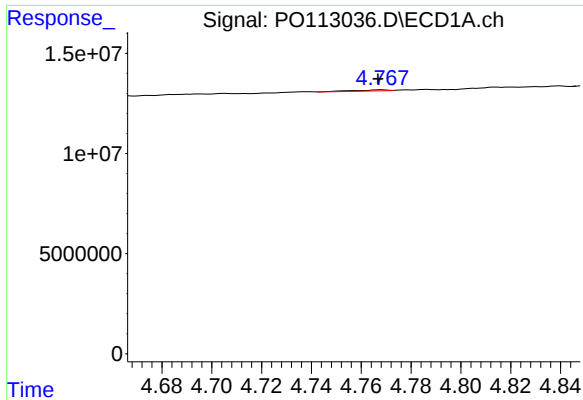

#17 AR-1242-2


R.T.: 4.768 min
Delta R.T.: 0.001 min
Response: 565172
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

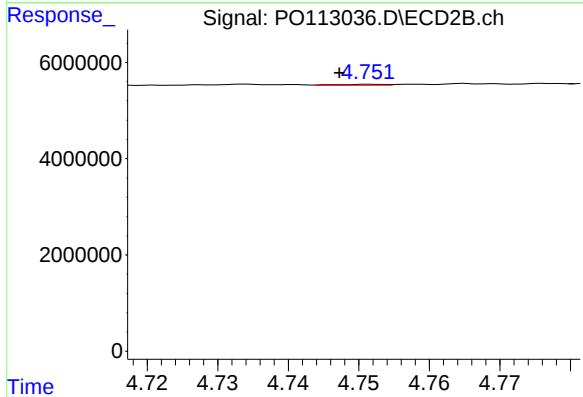


#17 AR-1242-2

R.T.: 4.752 min
Delta R.T.: 0.004 min
Response: 94729
Conc: 0.44 ng/ml

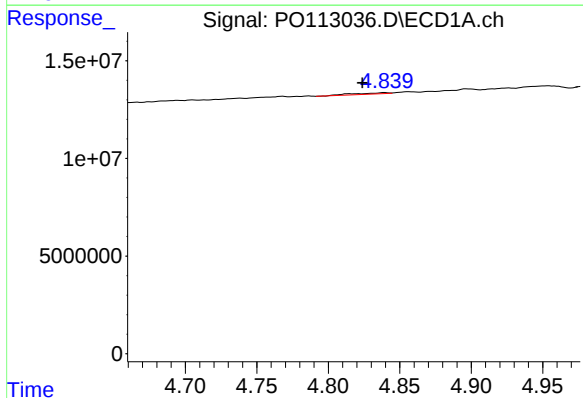


#18 AR-1242-3

R.T.: 4.840 min
Delta R.T.: 0.016 min
Response: 1035592
Conc: 4.67 ng/ml

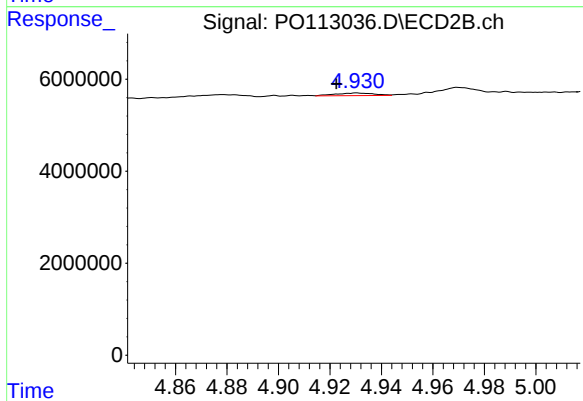

#18 AR-1242-3


R.T.: 4.931 min
Delta R.T.: 0.008 min
Response: 593416
Conc: 5.07 ng/ml

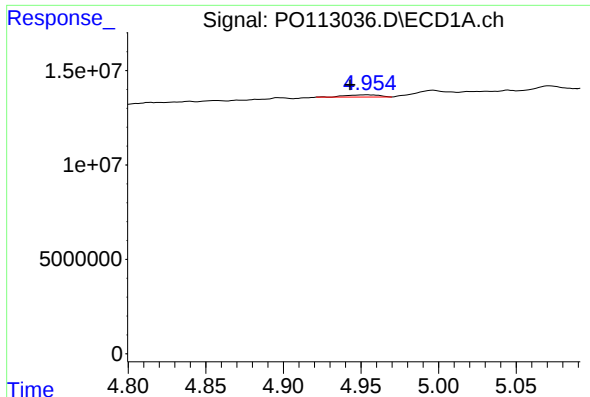

#19 AR-1242-4


R.T.: 4.954 min
Delta R.T.: 0.011 min
Response: 1712265
Conc: 9.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

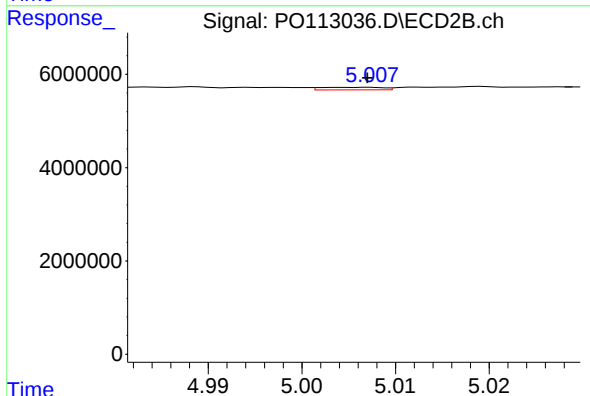


#19 AR-1242-4

R.T.: 5.007 min
Delta R.T.: 0.000 min
Response: 252868
Conc: 2.15 ng/ml

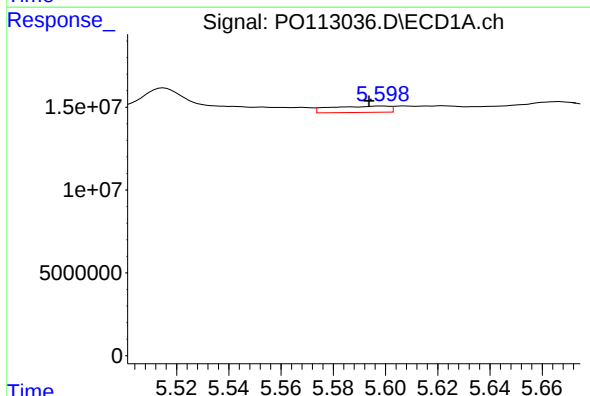


#20 AR-1242-5

R.T.: 5.599 min
Delta R.T.: 0.005 min
Response: 5896926
Conc: 29.46 ng/ml

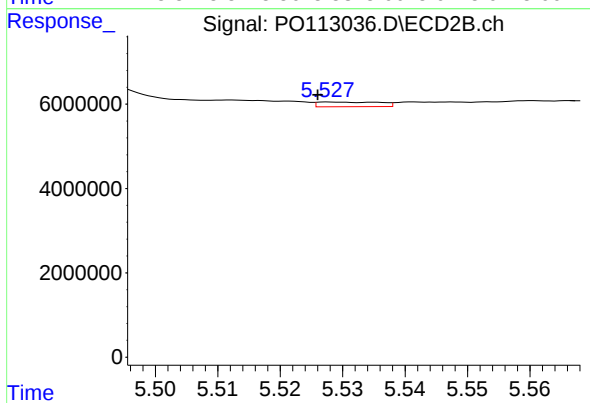

#20 AR-1242-5


R.T.: 5.528 min
Delta R.T.: 0.002 min
Response: 770749
Conc: 5.17 ng/ml

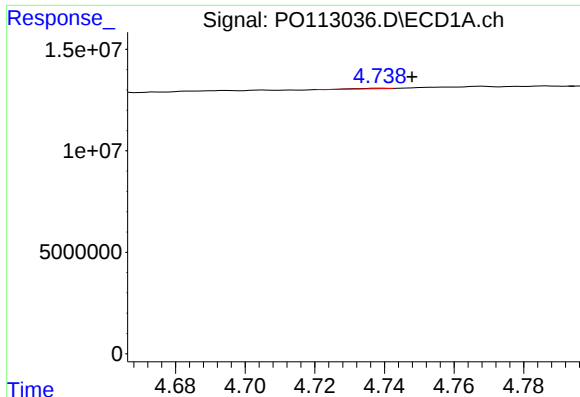

#21 AR-1248-1


R.T.: 4.739 min
Delta R.T.: -0.009 min
Response: 168963
Conc: 0.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

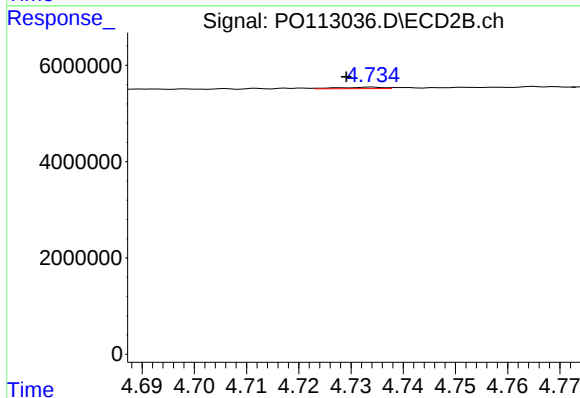


#21 AR-1248-1

R.T.: 4.734 min
Delta R.T.: 0.005 min
Response: 188118
Conc: 1.69 ng/ml

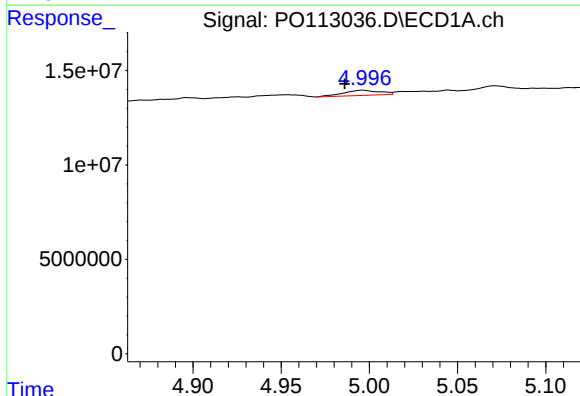


#22 AR-1248-2

R.T.: 4.996 min
Delta R.T.: 0.010 min
Response: 3904081
Conc: 16.14 ng/ml

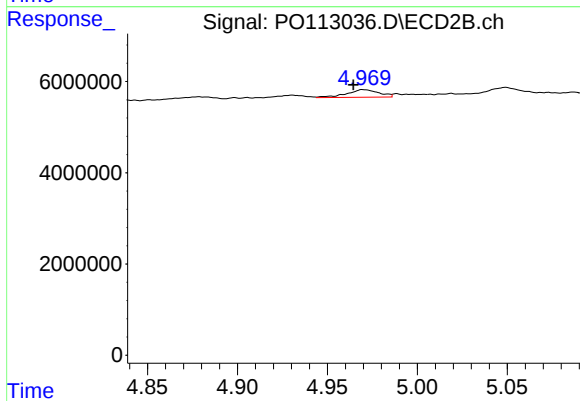

#22 AR-1248-2


R.T.: 4.970 min
Delta R.T.: 0.005 min
Response: 2054784
Conc: 12.79 ng/ml

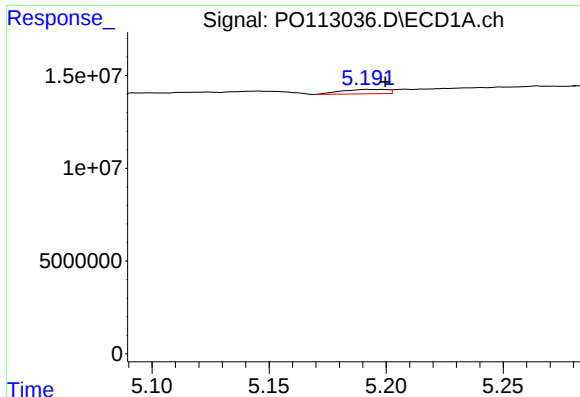

#23 AR-1248-3


R.T.: 5.192 min
Delta R.T.: -0.007 min
Response: 3198763
Conc: 10.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

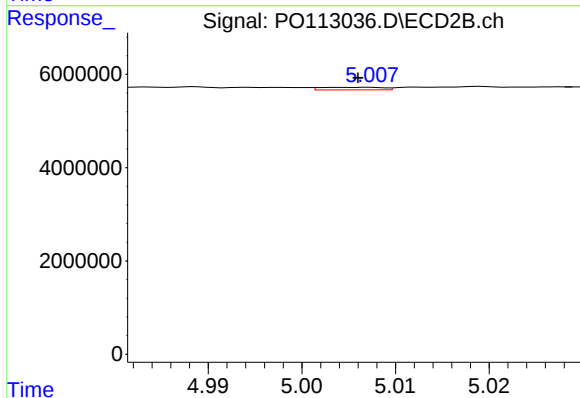


#23 AR-1248-3

R.T.: 5.007 min
Delta R.T.: 0.001 min
Response: 252868
Conc: 1.49 ng/ml

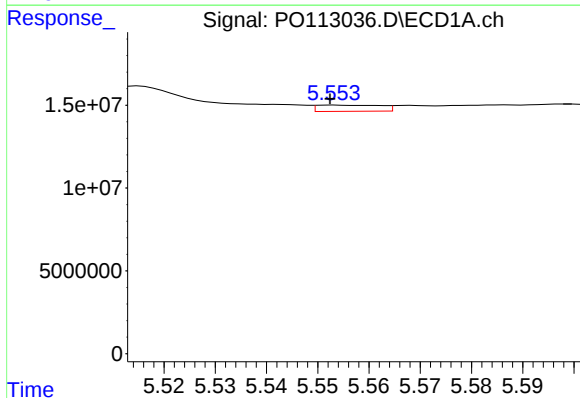


#24 AR-1248-4

R.T.: 5.553 min
Delta R.T.: 0.000 min
Response: 3277168
Conc: 6.56 ng/ml

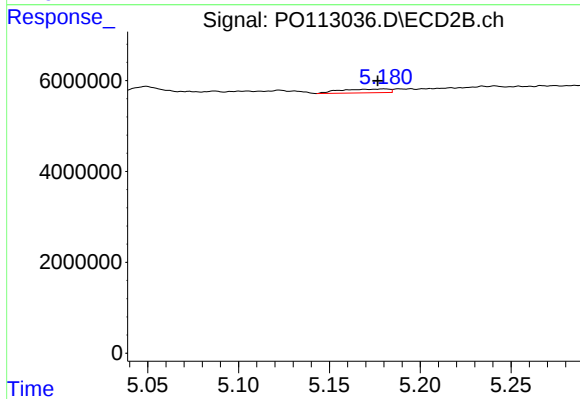

#24 AR-1248-4


R.T.: 5.180 min
Delta R.T.: 0.003 min
Response: 1578563
Conc: 7.92 ng/ml

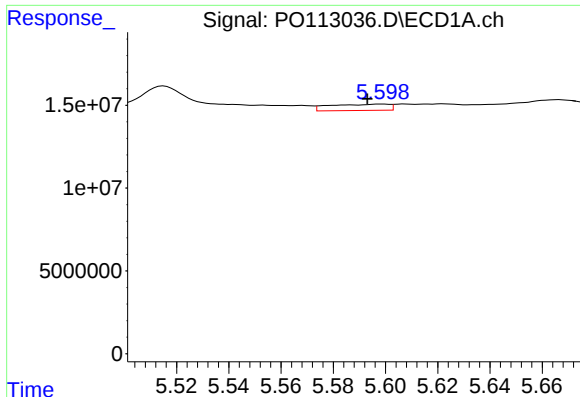

#25 AR-1248-5


R.T.: 5.599 min
Delta R.T.: 0.006 min
Response: 5896926
Conc: 17.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

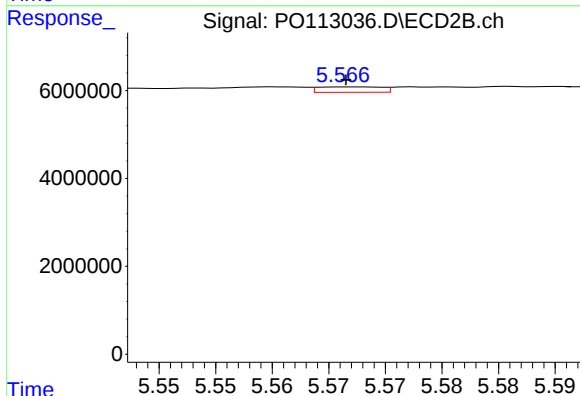


#25 AR-1248-5

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 479887
Conc: 2.26 ng/ml

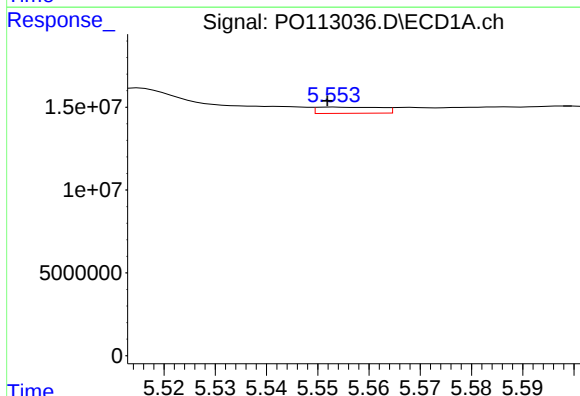


#26 AR-1254-1

R.T.: 5.553 min
Delta R.T.: 0.001 min
Response: 3277168
Conc: 6.07 ng/ml

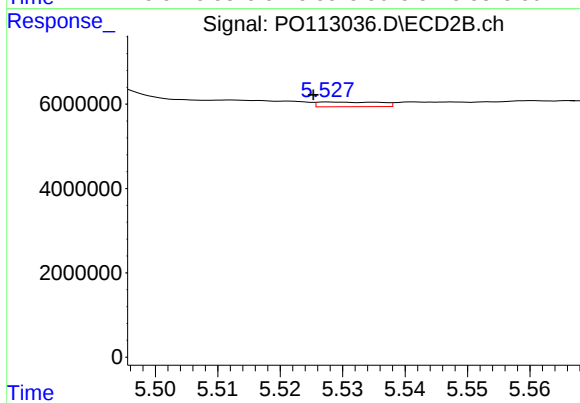

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: 0.002 min
Response: 770749
Conc: 2.44 ng/ml

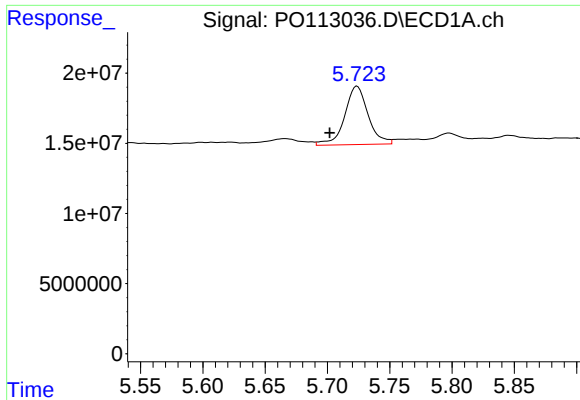

#27 AR-1254-2


R.T.: 5.724 min
Delta R.T.: 0.022 min
Response: 54717939
Conc: 110.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

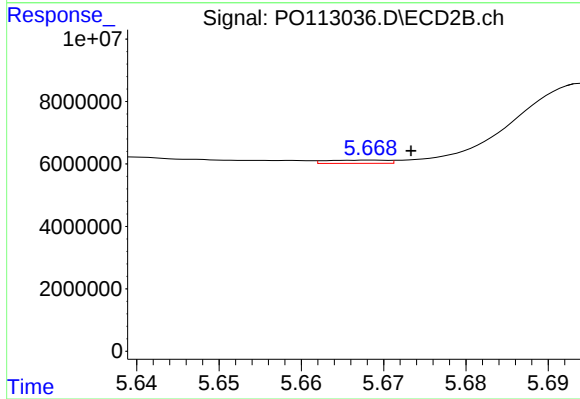


#27 AR-1254-2

R.T.: 5.669 min
Delta R.T.: -0.005 min
Response: 535915
Conc: 1.91 ng/ml

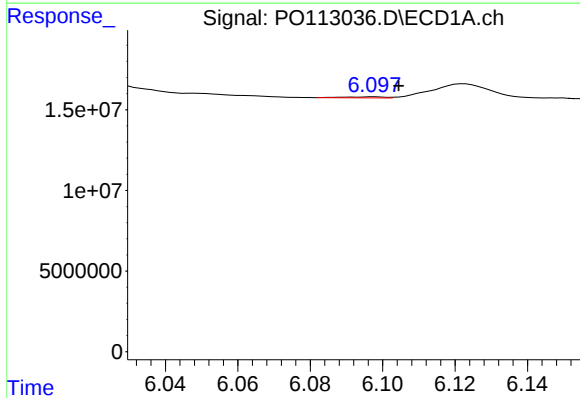


#28 AR-1254-3

R.T.: 6.098 min
Delta R.T.: -0.007 min
Response: 504000
Conc: 0.68 ng/ml

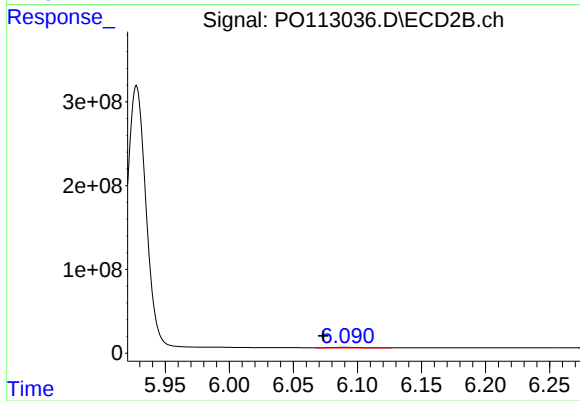

#28 AR-1254-3


R.T.: 6.091 min
Delta R.T.: 0.017 min
Response: 13087478
Conc: 31.39 ng/ml

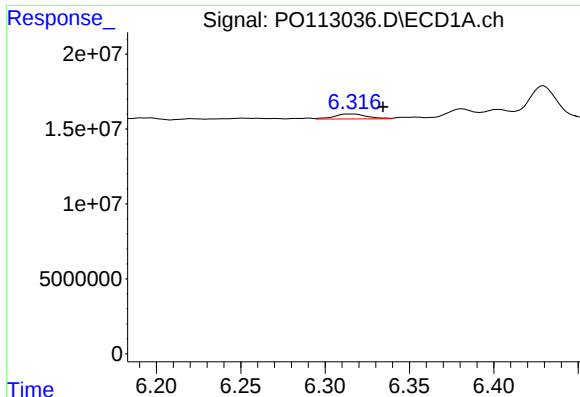

#29 AR-1254-4


R.T.: 6.316 min
Delta R.T.: -0.019 min
Response: 4478351
Conc: 8.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

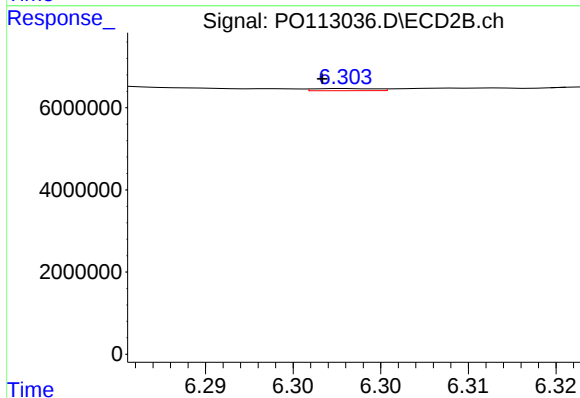


#29 AR-1254-4

R.T.: 6.303 min
Delta R.T.: 0.002 min
Response: 129854
Conc: 0.47 ng/ml

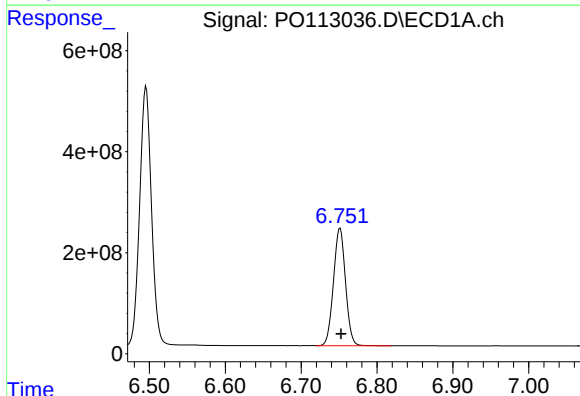


#30 AR-1254-5

R.T.: 6.751 min
Delta R.T.: -0.001 min
Response: 2564241036
Conc: 3658.11 ng/ml

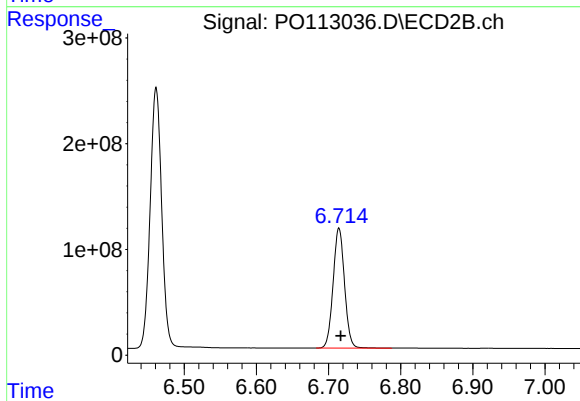

#30 AR-1254-5


R.T.: 6.714 min
Delta R.T.: -0.002 min
Response: 1246825700
Conc: 3487.72 ng/ml

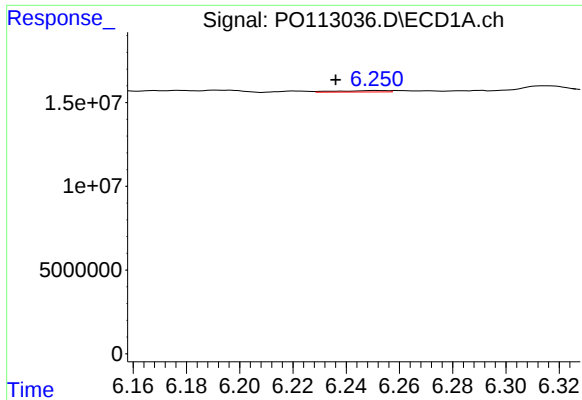

#31 AR-1260-1


R.T.: 6.251 min
Delta R.T.: 0.015 min
Response: 1118357
Conc: 2.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

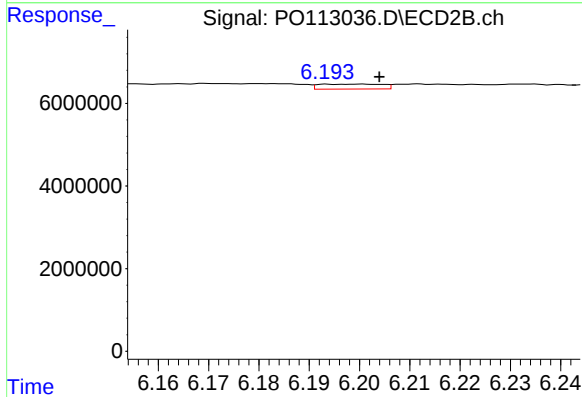


#31 AR-1260-1

R.T.: 6.201 min
Delta R.T.: -0.003 min
Response: 1045669
Conc: 4.10 ng/ml

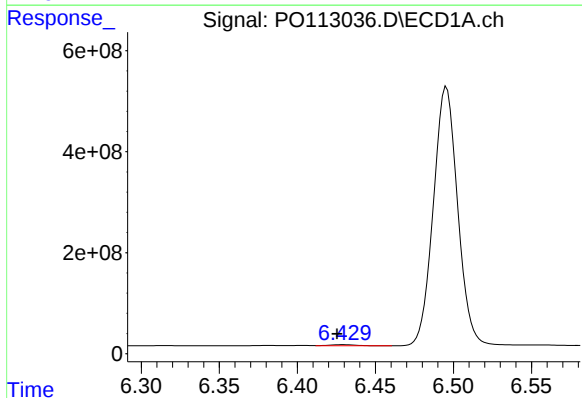


#32 AR-1260-2

R.T.: 6.429 min
Delta R.T.: 0.004 min
Response: 25069436
Conc: 36.51 ng/ml

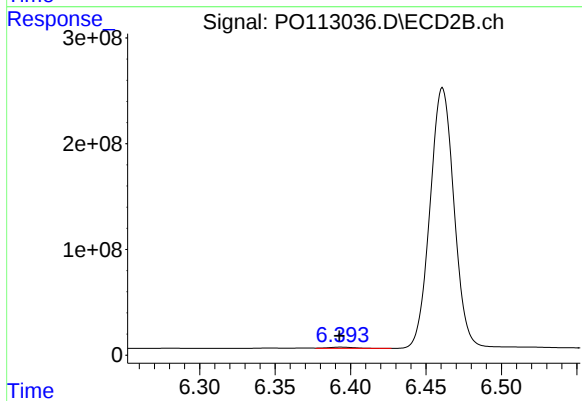

#32 AR-1260-2


R.T.: 6.393 min
Delta R.T.: 0.000 min
Response: 13750672
Conc: 39.77 ng/ml

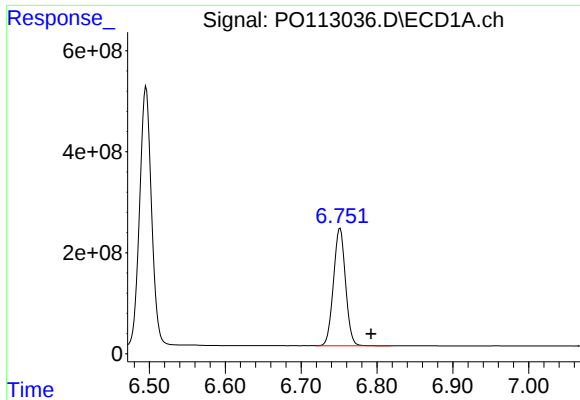

#33 AR-1260-3


R.T.: 6.751 min
Delta R.T.: -0.041 min
Response: 2564241036
Conc: 4152.79 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

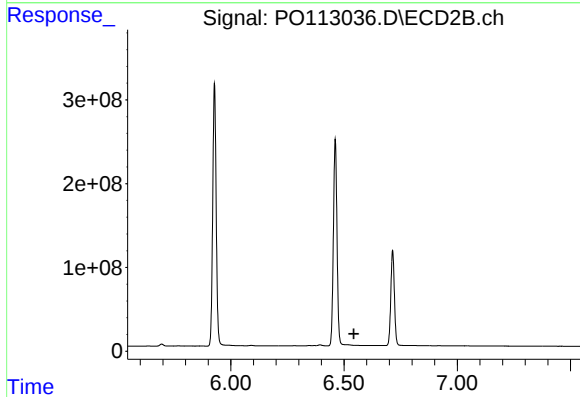


#33 AR-1260-3

R.T.: 6.563 min
Delta R.T.: 0.019 min
Response: -68001
Conc: N.D.

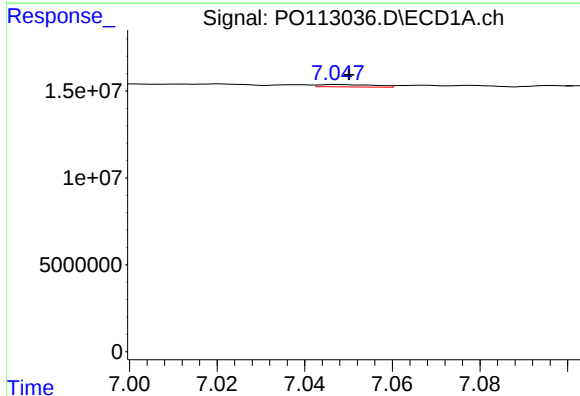


#34 AR-1260-4

R.T.: 7.048 min
Delta R.T.: -0.002 min
Response: 1204305
Conc: 2.69 ng/ml

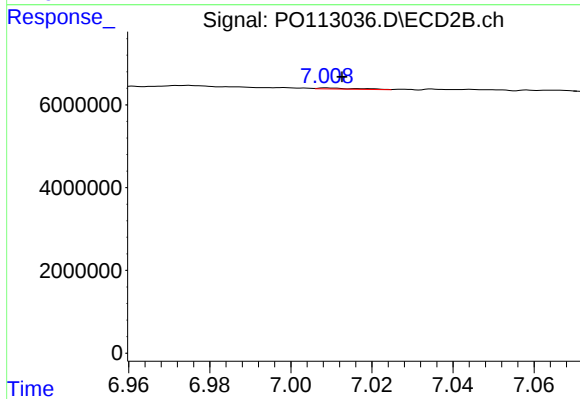

#34 AR-1260-4


R.T.: 7.009 min
Delta R.T.: -0.004 min
Response: 172259
Conc: 0.83 ng/ml

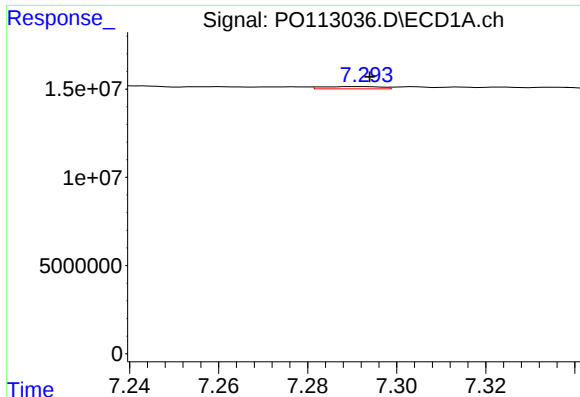

#35 AR-1260-5


R.T.: 7.293 min
Delta R.T.: -0.001 min
Response: 1157195
Conc: 0.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

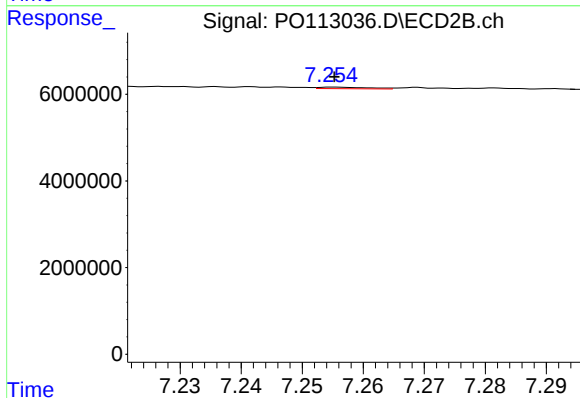


#35 AR-1260-5

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 206514
Conc: 0.44 ng/ml

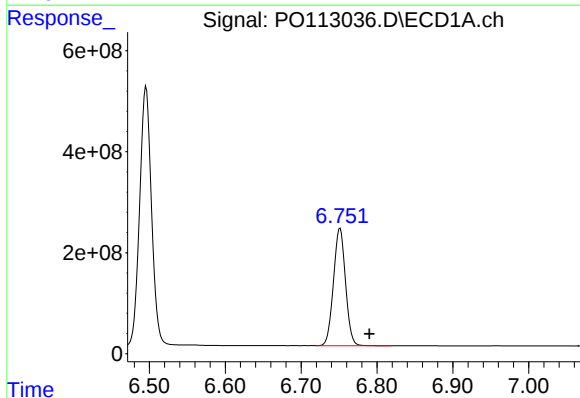


#36 AR-1262-1

R.T.: 6.751 min
Delta R.T.: -0.039 min
Response: 2564241036
Conc: 2800.11 ng/ml

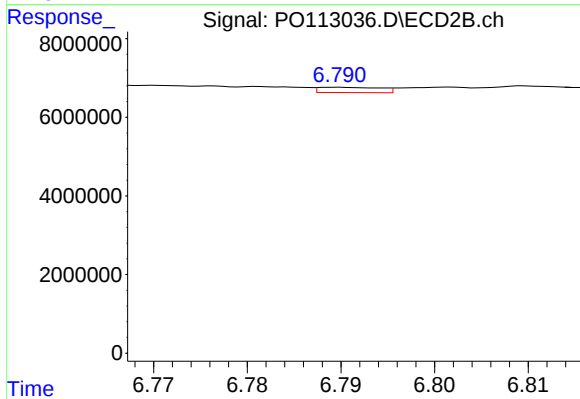

#36 AR-1262-1


R.T.: 6.790 min
Delta R.T.: 0.034 min
Response: 613205
Conc: 1.48 ng/ml

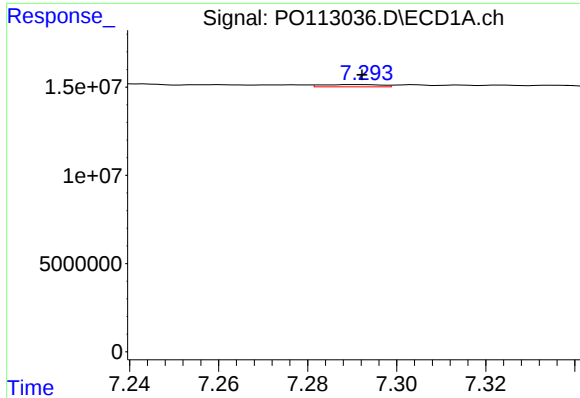

#37 AR-1262-2


R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 1157195
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

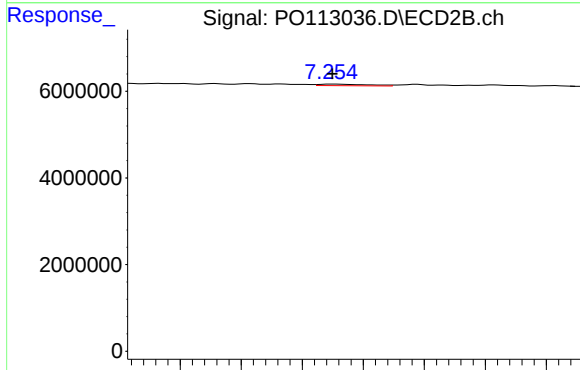


#37 AR-1262-2

R.T.: 7.255 min
Delta R.T.: 0.000 min
Response: 206514
Conc: 0.40 ng/ml

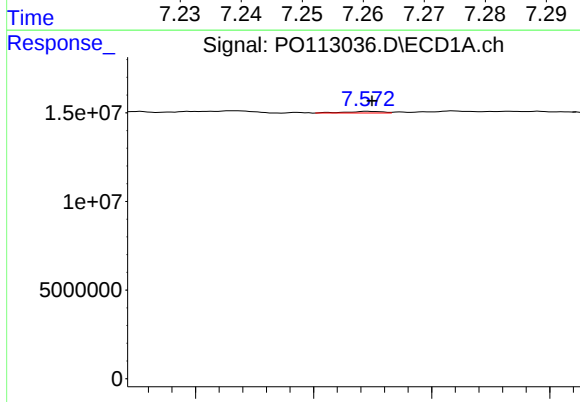


#38 AR-1262-3

R.T.: 7.573 min
Delta R.T.: -0.002 min
Response: 1018381
Conc: 1.84 ng/ml

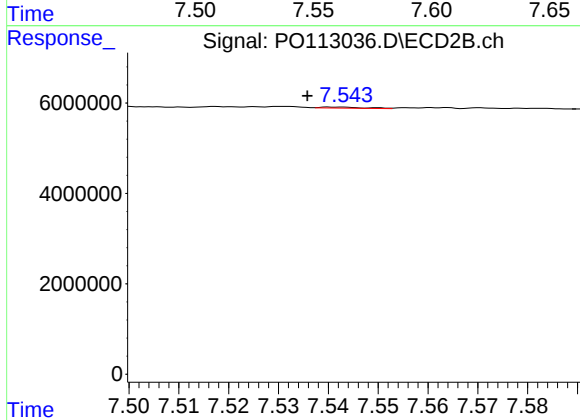

#38 AR-1262-3


R.T.: 7.540 min
Delta R.T.: 0.004 min
Response: 151680
Conc: 0.84 ng/ml

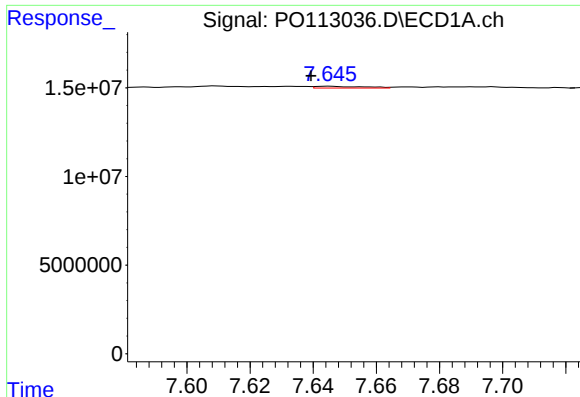

#39 AR-1262-4


R.T.: 7.645 min
Delta R.T.: 0.006 min
Response: 1041931
Conc: 1.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

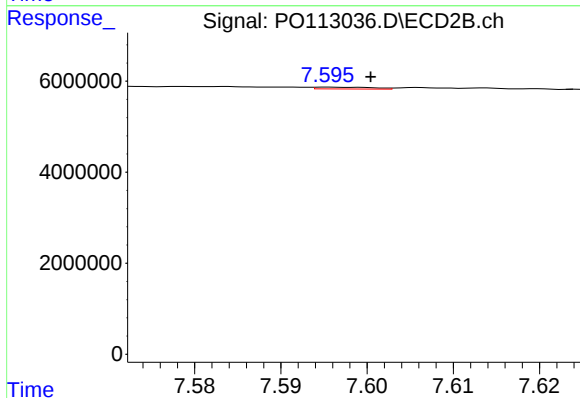


#39 AR-1262-4

R.T.: 7.595 min
Delta R.T.: -0.005 min
Response: 186362
Conc: 0.64 ng/ml

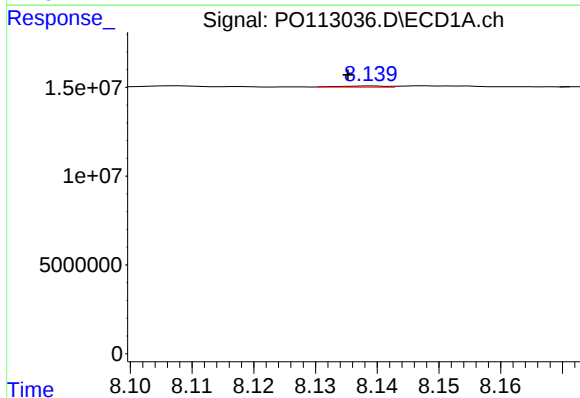


#40 AR-1262-5

R.T.: 8.139 min
Delta R.T.: 0.004 min
Response: 324743
Conc: 0.78 ng/ml

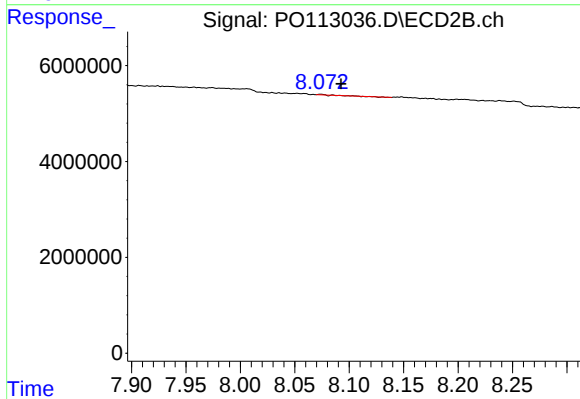

#40 AR-1262-5


R.T.: 8.074 min
Delta R.T.: -0.019 min
Response: 59366
Conc: 0.55 ng/ml

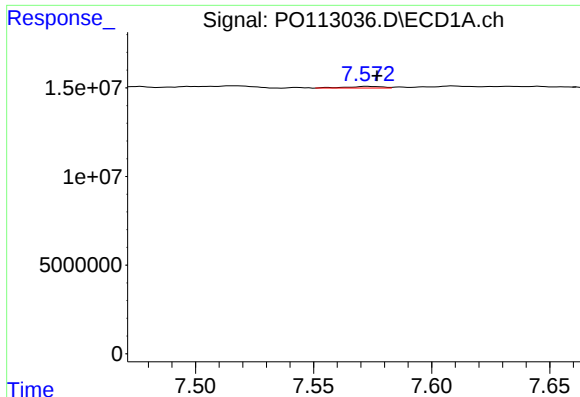

#41 AR-1268-1


R.T.: 7.573 min
Delta R.T.: -0.004 min
Response: 1018381
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

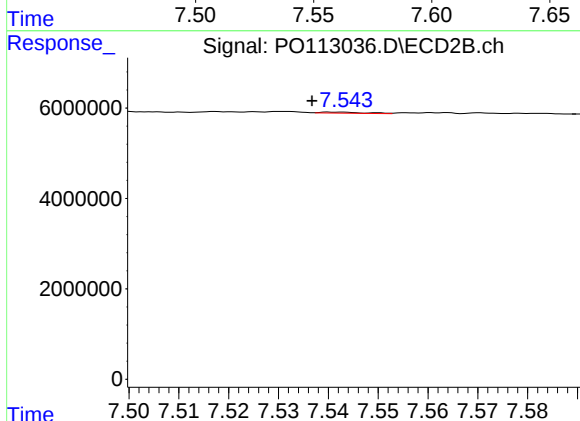


#41 AR-1268-1

R.T.: 7.540 min
Delta R.T.: 0.003 min
Response: 151680
Conc: 0.30 ng/ml

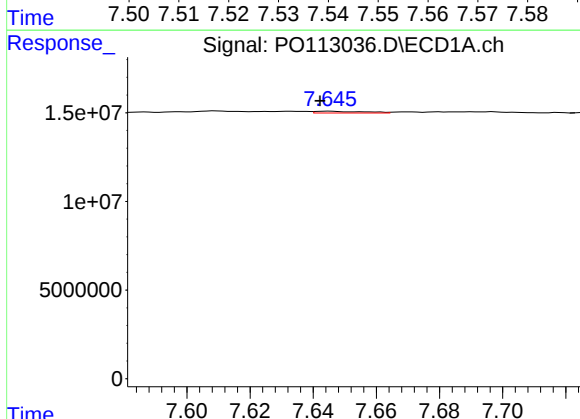


#42 AR-1268-2

R.T.: 7.645 min
Delta R.T.: 0.003 min
Response: 1041931
Conc: 0.72 ng/ml

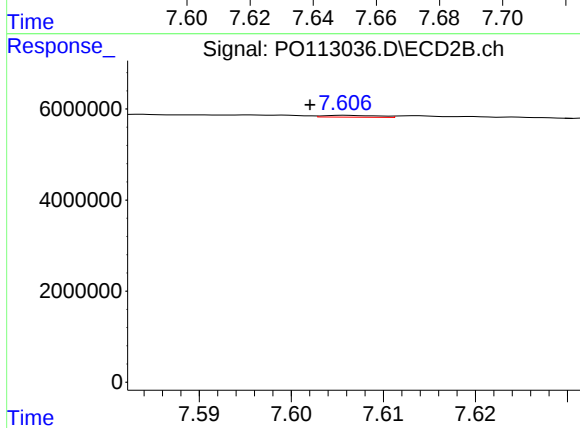

#42 AR-1268-2


R.T.: 7.606 min
Delta R.T.: 0.004 min
Response: 167706
Conc: 0.40 ng/ml

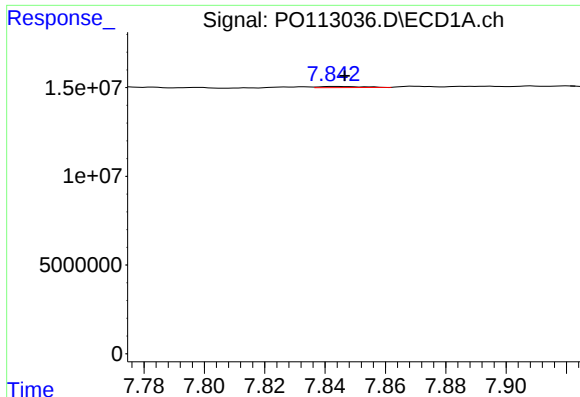

#43 AR-1268-3


R.T.: 7.844 min
Delta R.T.: -0.003 min
Response: 649042
Conc: 0.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

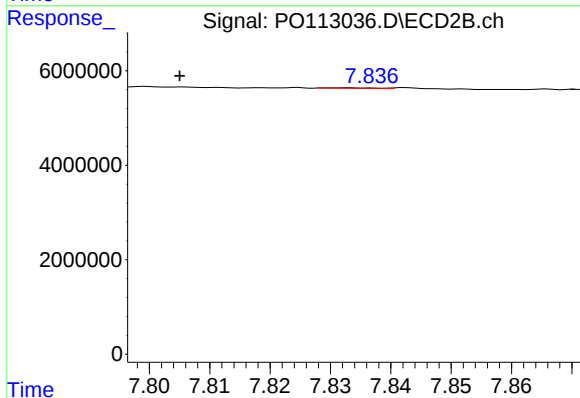


#43 AR-1268-3

R.T.: 7.832 min
Delta R.T.: 0.027 min
Response: 47713
Conc: 0.15 ng/ml

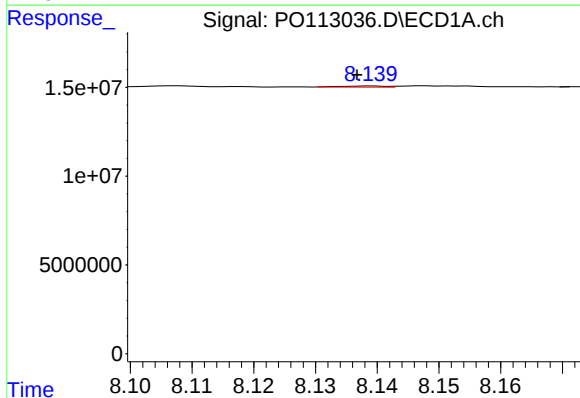


#44 AR-1268-4

R.T.: 8.139 min
Delta R.T.: 0.002 min
Response: 324743
Conc: 0.70 ng/ml

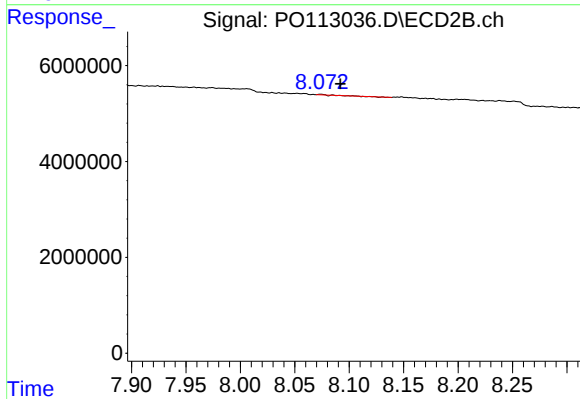

#44 AR-1268-4


R.T.: 8.074 min
Delta R.T.: -0.018 min
Response: 59366
Conc: 0.49 ng/ml

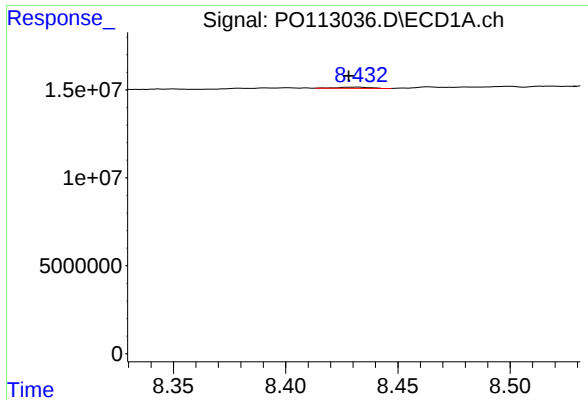

#45 AR-1268-5

R.T.: 8.433 min
Delta R.T.: 0.005 min
Response: 665471
Conc: 0.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

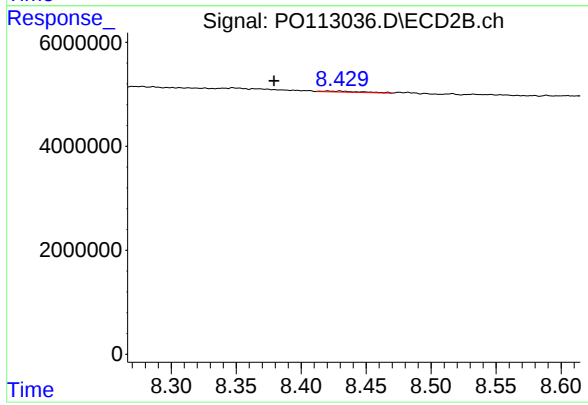

#45 AR-1268-5

R.T.: 8.421 min
Delta R.T.: 0.041 min
Response: 401091
Conc: 0.51 ng/ml