

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081920\
 Data File : P0070680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2020 15:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 16:25:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.364	3.549	1748004	1011419	26.434	22.956
2)	SA Decachlor...	9.991	8.739	1627741	1001656	19.010	18.045
Target Compounds							
9)	L2 AR-1221-2	4.707f	3.888f	27892	12691	44.335	28.682 #
20)	L4 AR-1242-5	6.643	5.654	9883	36733	4.798	22.022 #
24)	L5 AR-1248-4	6.610	0.000	11023	0	3.240	N.D. #
25)	L5 AR-1248-5	6.643	0.000	9883	0	3.107	N.D. #
26)	L6 AR-1254-1	6.573	5.654	180013	36733	50.587	10.489 #
28)	L6 AR-1254-3	7.189f	6.223	34347	6590	5.964	1.337 #
29)	L6 AR-1254-4	7.467	0.000	5075	0	0.973	N.D. #
31)	L7 AR-1260-1	0.000	6.351	0	1930	N.D.	0.598 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081920\
Data File : PO070680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2020 15:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 16:25:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

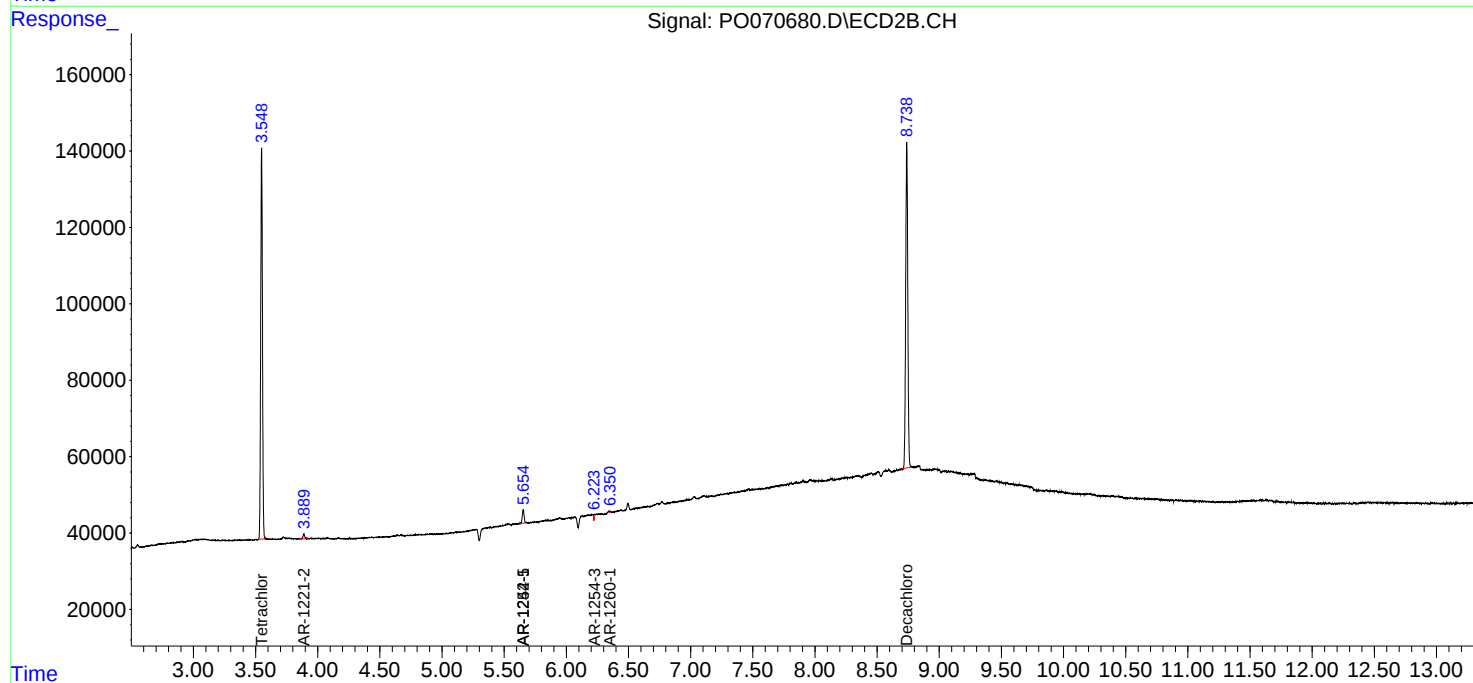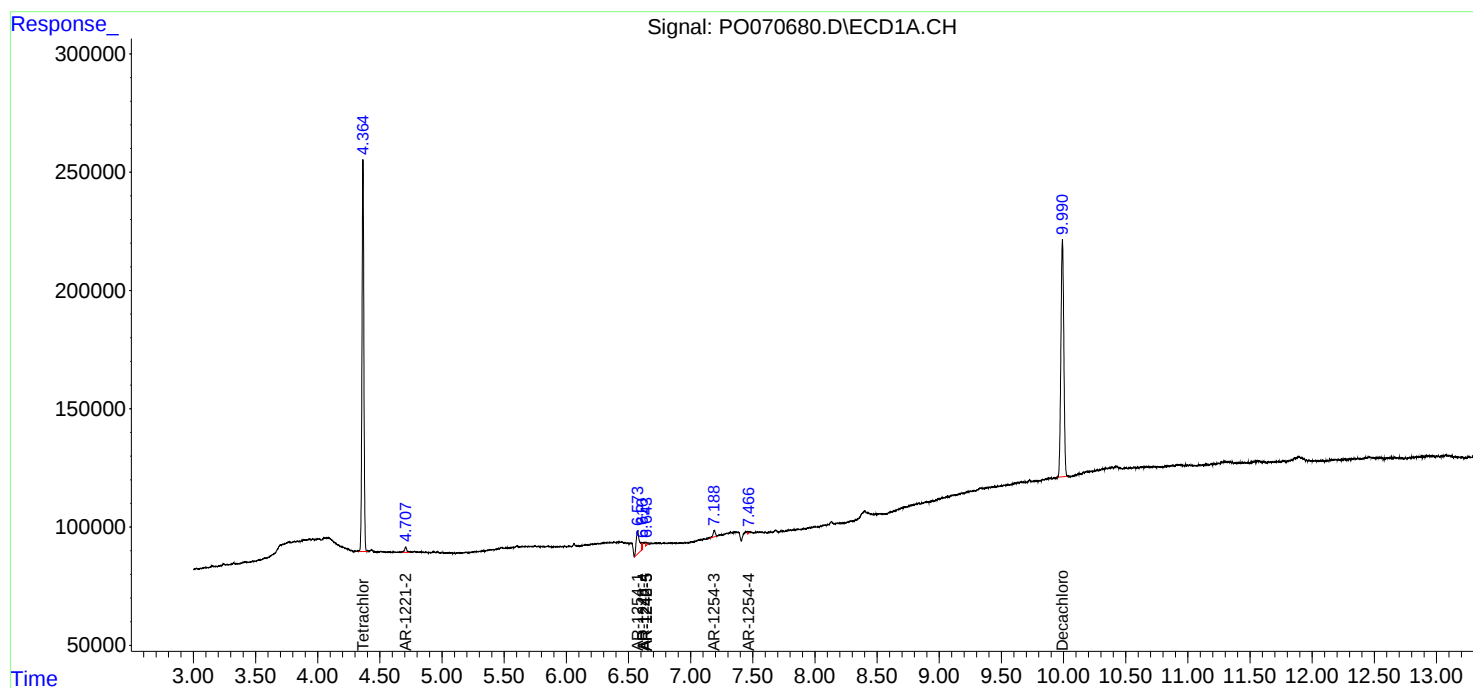


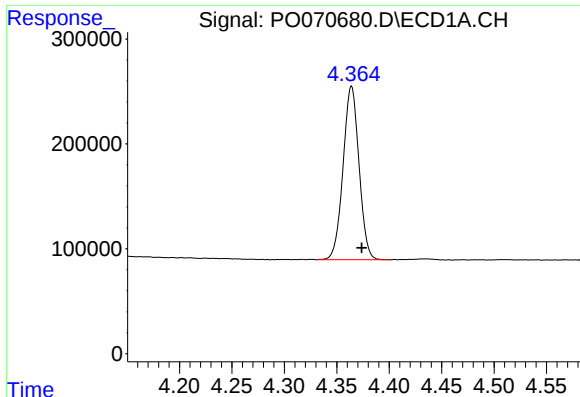

#1 Tetrachloro-m-xylene


R.T.: 4.364 min
Delta R.T.: -0.010 min
Response: 1748004
Conc: 26.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

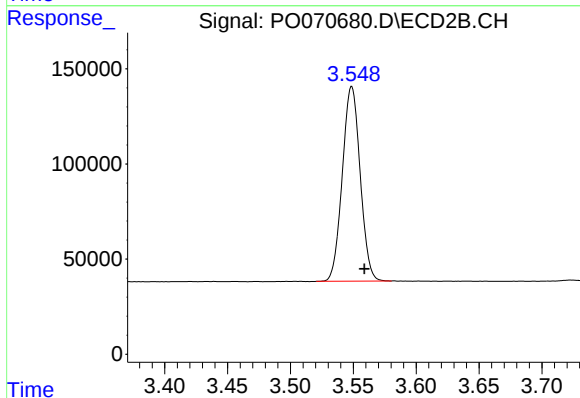


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.010 min
Response: 1011419
Conc: 22.96 ng/ml

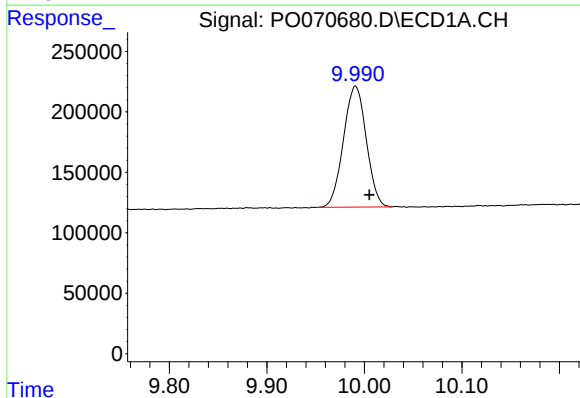


#2 Decachlorobiphenyl

R.T.: 9.991 min
Delta R.T.: -0.014 min
Response: 1627741
Conc: 19.01 ng/ml

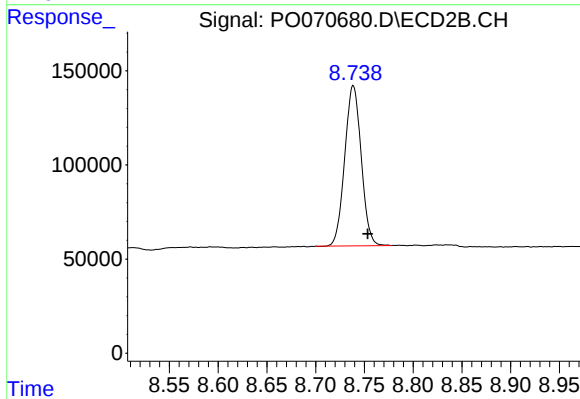

#2 Decachlorobiphenyl


R.T.: 8.739 min
Delta R.T.: -0.015 min
Response: 1001656
Conc: 18.05 ng/ml

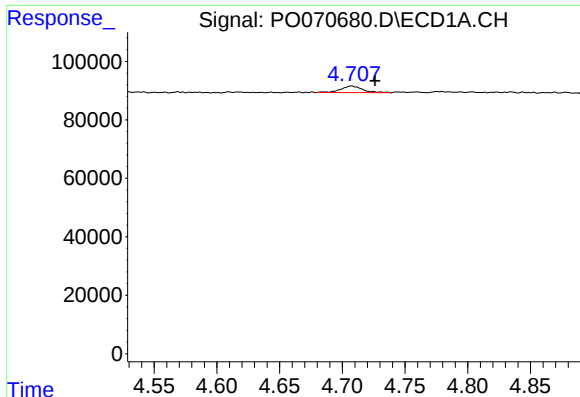

#9 AR-1221-2


R.T.: 4.707 min
Delta R.T.: -0.019 min
Response: 27892
Conc: 44.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

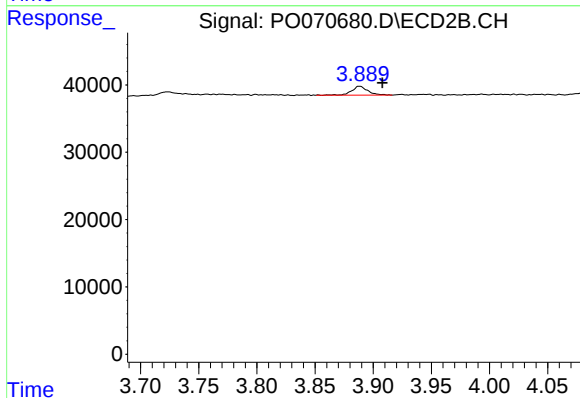


#9 AR-1221-2

R.T.: 3.888 min
Delta R.T.: -0.020 min
Response: 12691
Conc: 28.68 ng/ml

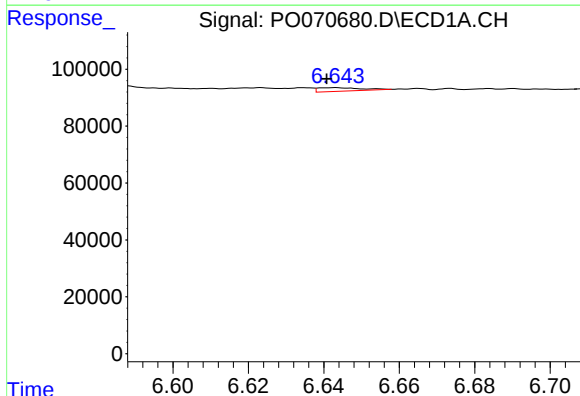


#20 AR-1242-5

R.T.: 6.643 min
Delta R.T.: 0.003 min
Response: 9883
Conc: 4.80 ng/ml

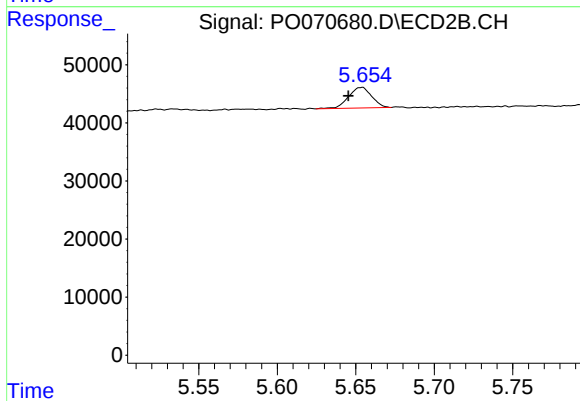

#20 AR-1242-5


R.T.: 5.654 min
Delta R.T.: 0.009 min
Response: 36733
Conc: 22.02 ng/ml

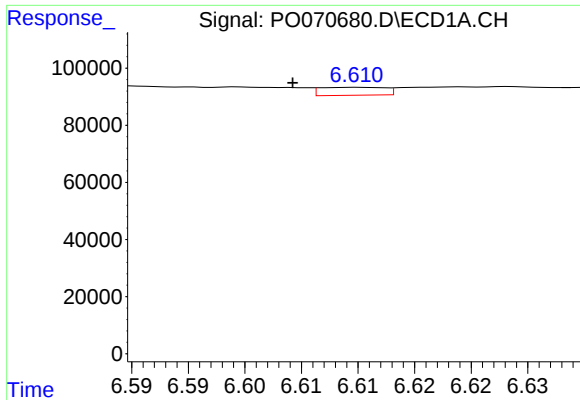

#24 AR-1248-4


R.T.: 6.610 min
Delta R.T.: 0.006 min
Response: 11023
Conc: 3.24 ng/ml

Instrument :
ECD_O
ClientSampleId :

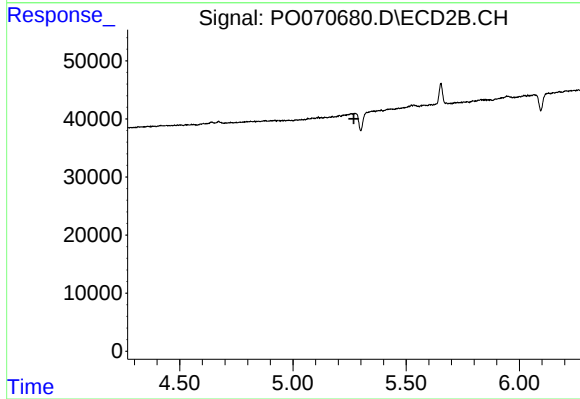


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.269 min
Response: 0
Conc: N.D.

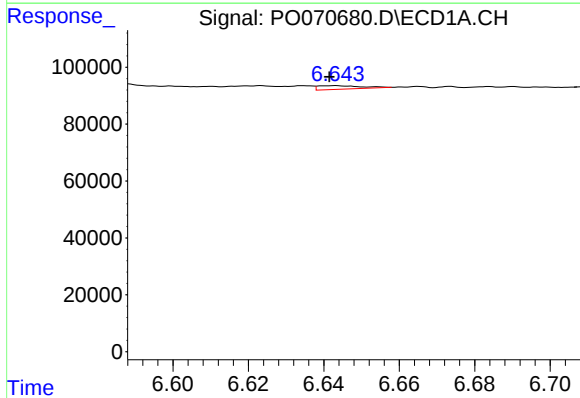


#25 AR-1248-5

R.T.: 6.643 min
Delta R.T.: 0.002 min
Response: 9883
Conc: 3.11 ng/ml

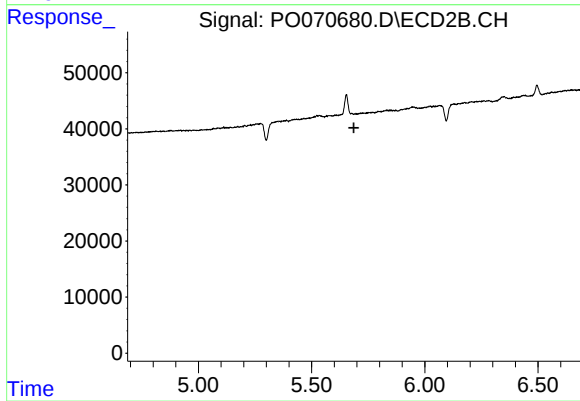

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.687 min
Response: 0
Conc: N.D.

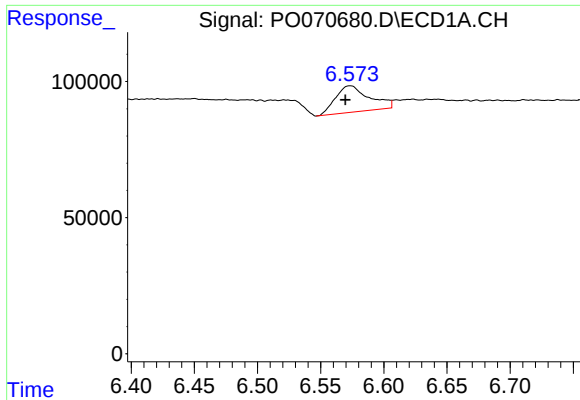

#26 AR-1254-1


R.T.: 6.573 min
Delta R.T.: 0.004 min
Response: 180013
Conc: 50.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

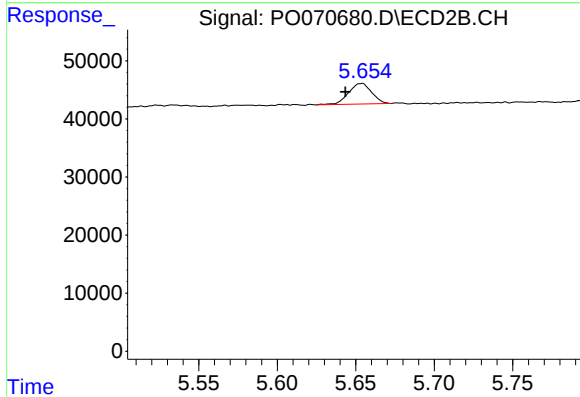


#26 AR-1254-1

R.T.: 5.654 min
Delta R.T.: 0.011 min
Response: 36733
Conc: 10.49 ng/ml

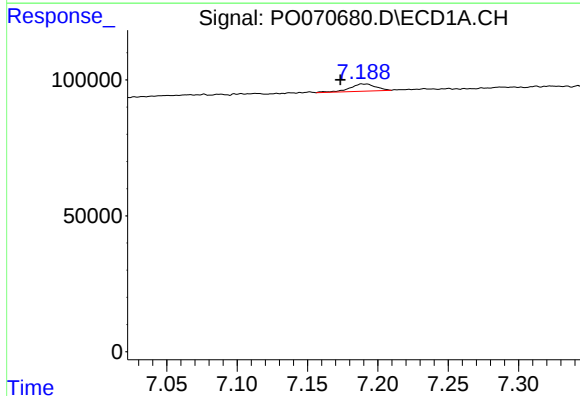


#28 AR-1254-3

R.T.: 7.189 min
Delta R.T.: 0.015 min
Response: 34347
Conc: 5.96 ng/ml

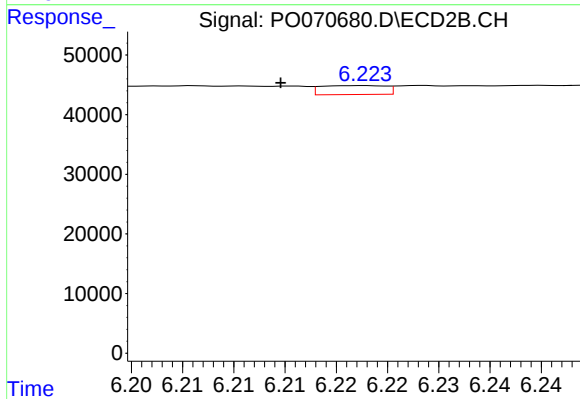

#28 AR-1254-3


R.T.: 6.223 min
Delta R.T.: 0.008 min
Response: 6590
Conc: 1.34 ng/ml

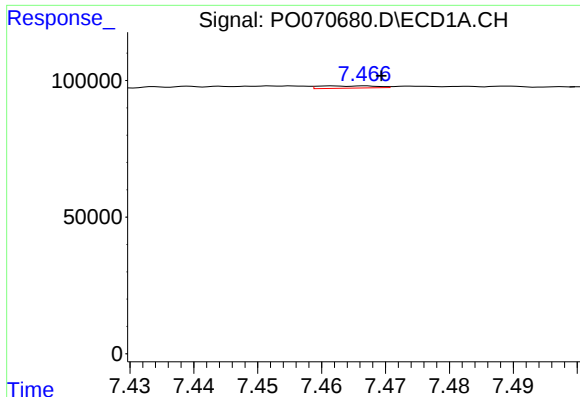

#29 AR-1254-4


R.T.: 7.467 min
Delta R.T.: -0.002 min
Response: 5075
Conc: 0.97 ng/ml

Instrument :
ECD_O
ClientSampleId :

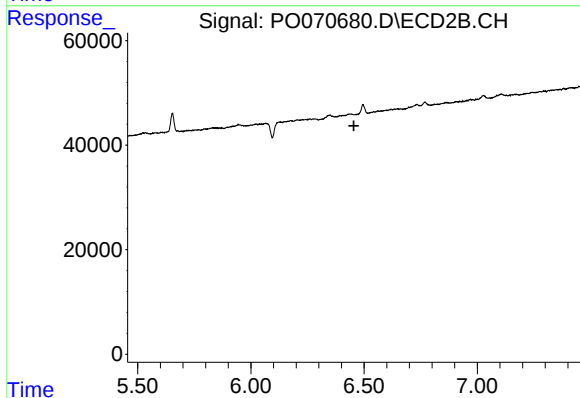


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

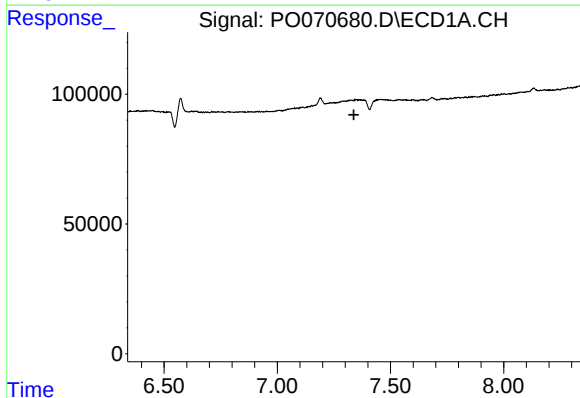

#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

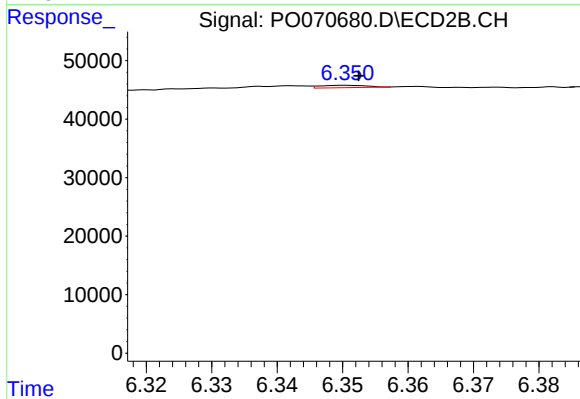

#31 AR-1260-1

R.T.: 6.351 min
Delta R.T.: -0.002 min
Response: 1930
Conc: 0.60 ng/ml