

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081920\
 Data File : P0070683.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2020 16:29
 Operator : DD\AJ
 Sample : L3716-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 08:47:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 06 13:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.364	3.548	1451714	853160	21.954	19.364
2) SA Decachlor...	9.991	8.738	1459210	893359	17.042	16.094

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081920\
Data File : P0070683.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2020 16:29
Operator : DD\AJ
Sample : L3716-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIPE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 08:47:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

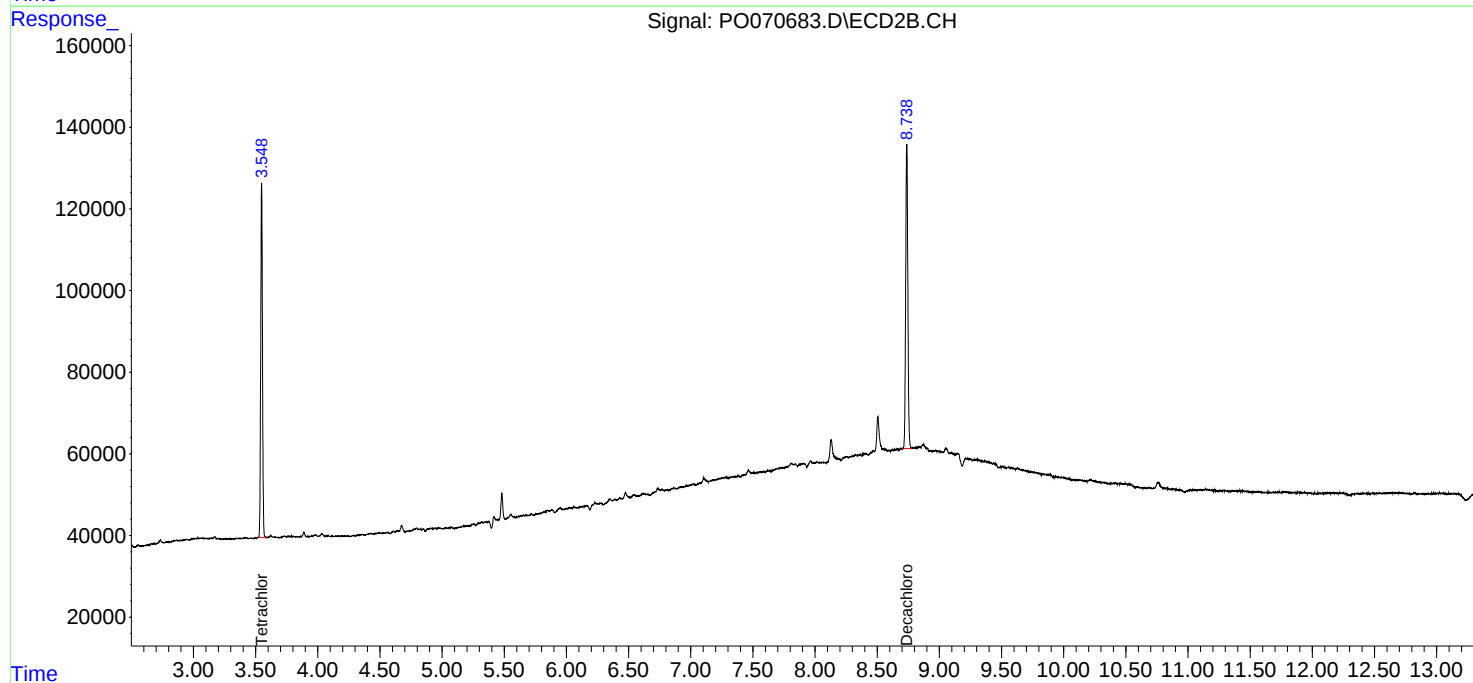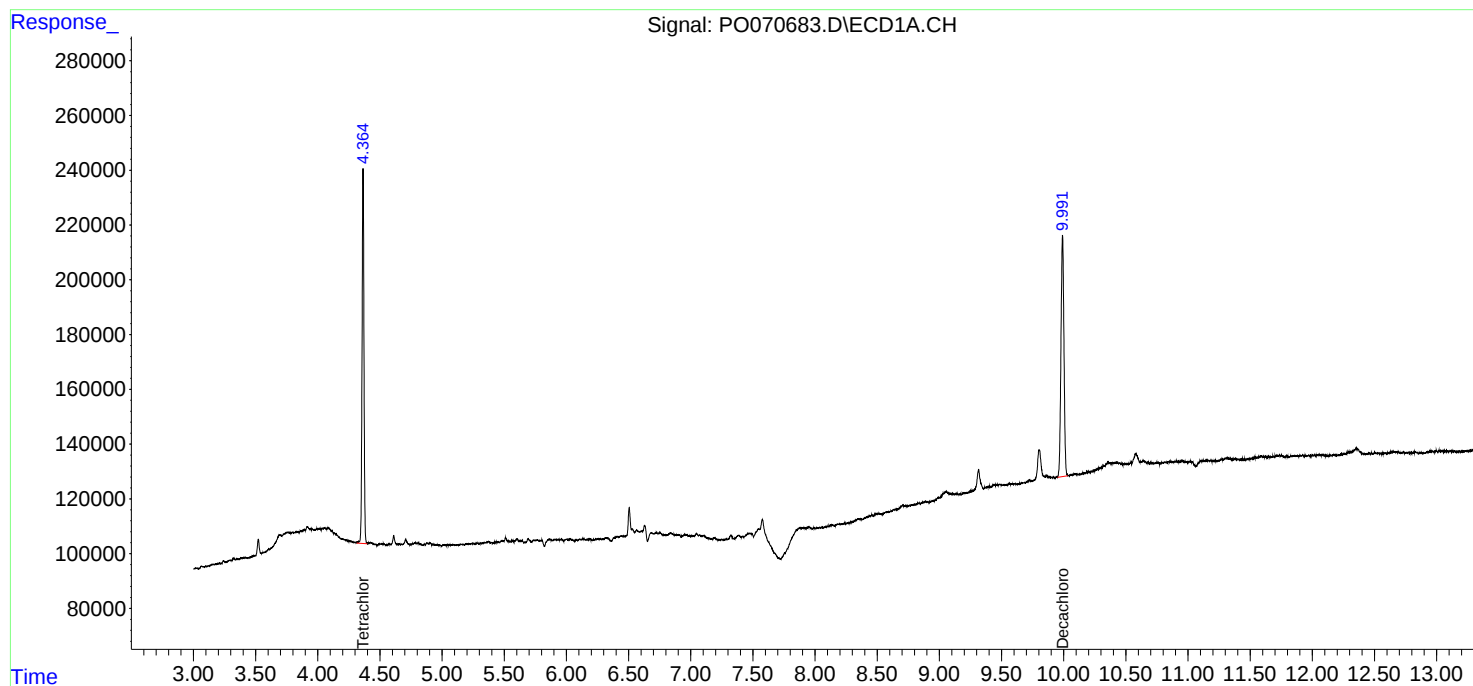


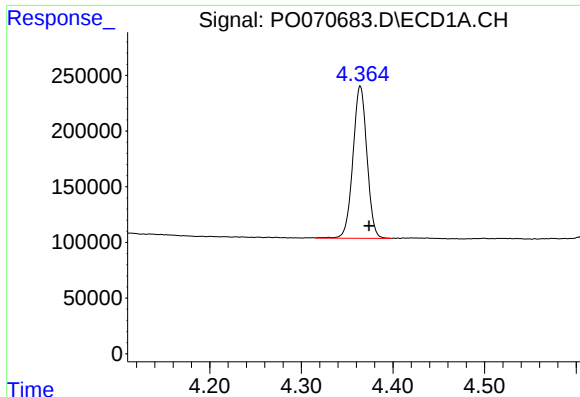

#1 Tetrachloro-m-xylene


R.T.: 4.364 min
Delta R.T.: -0.010 min
Response: 1451714
Conc: 21.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-1

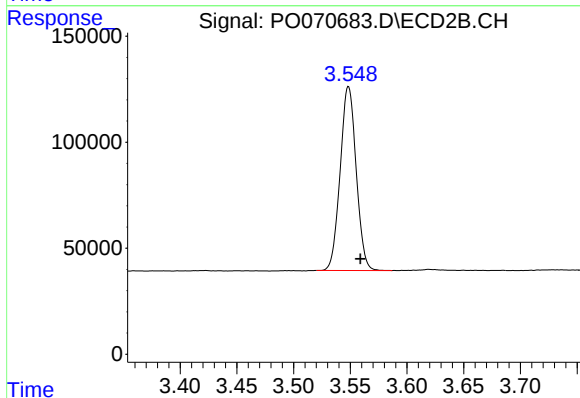


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: -0.010 min
Response: 853160
Conc: 19.36 ng/ml

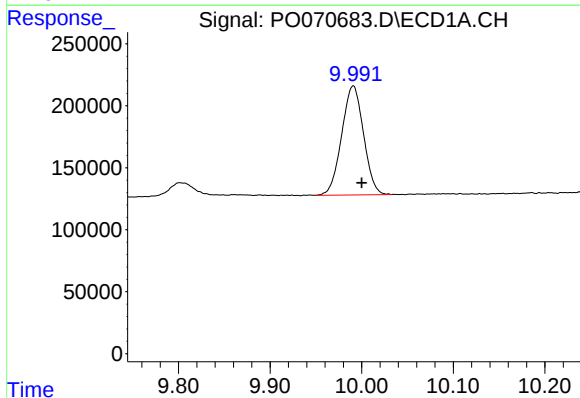

#2 Decachlorobiphenyl

R.T.: 9.991 min
Delta R.T.: -0.009 min
Response: 1459210
Conc: 17.04 ng/ml

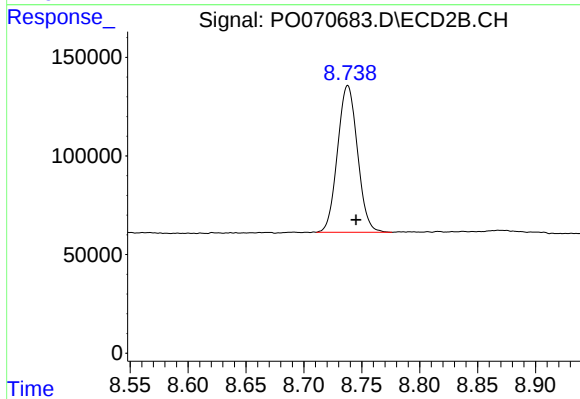

#2 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.007 min
Response: 893359
Conc: 16.09 ng/ml