

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0081920\
Data File : P0070691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2020 18:45
Operator : DD\AJ
Sample : L3690-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NWB-1518-1517-1516

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:47:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.555	1384701	793187	20.940	18.003
2) SA Decachlor...	9.993	8.739	1106237	639571	12.920	11.522

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO081920\
Data File : PO070691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2020 18:45
Operator : DD\AJ
Sample : L3690-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NWB-1518-1517-1516

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:47:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO080620.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 06 13:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

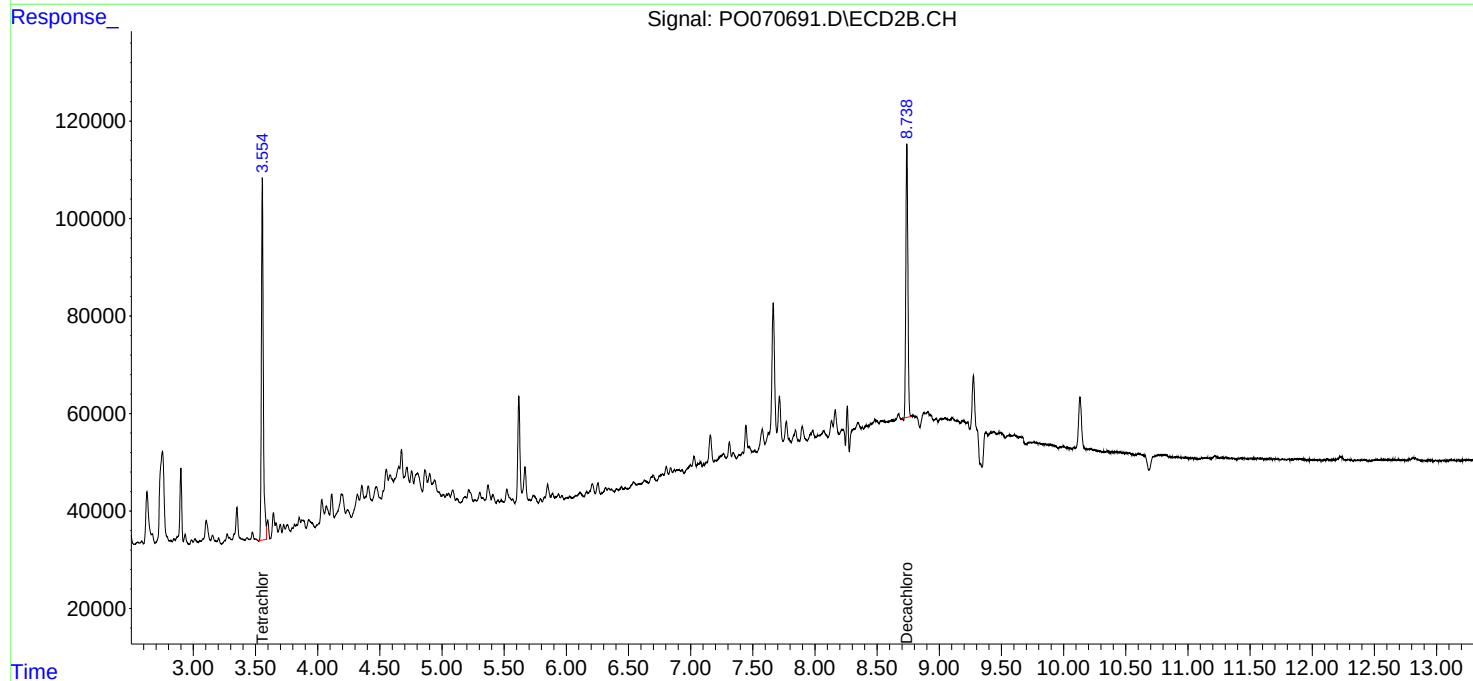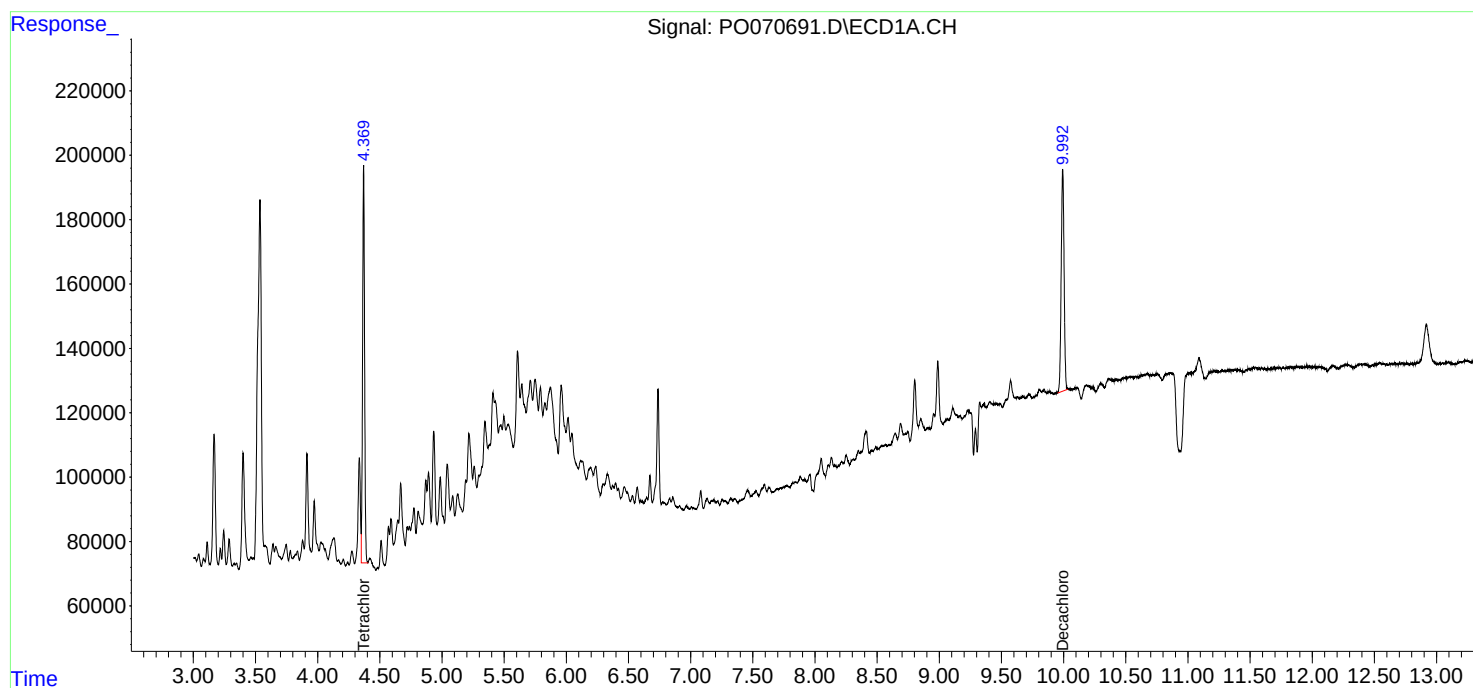


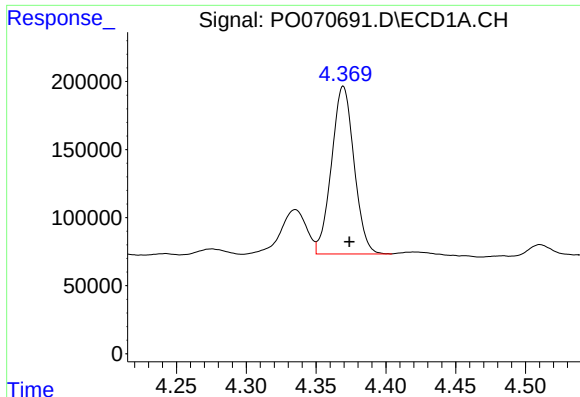

#1 Tetrachloro-m-xylene


R.T.: 4.370 min
Delta R.T.: -0.004 min
Response: 1384701
Conc: 20.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
NWB-1518-1517-1516

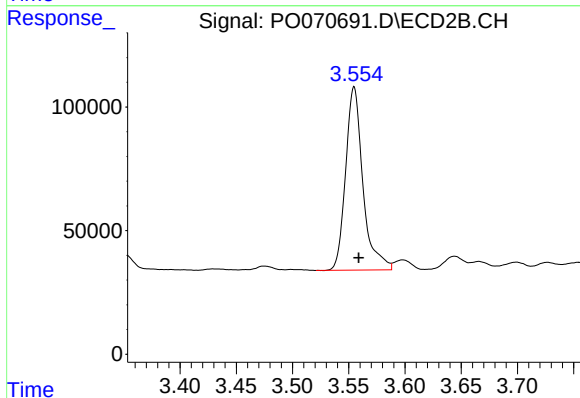


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: -0.004 min
Response: 793187
Conc: 18.00 ng/ml

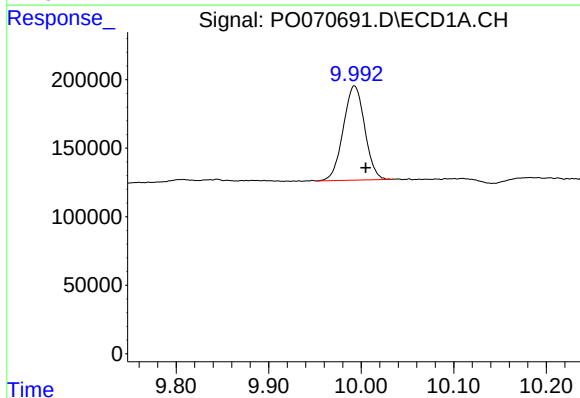

#2 Decachlorobiphenyl

R.T.: 9.993 min
Delta R.T.: -0.012 min
Response: 1106237
Conc: 12.92 ng/ml

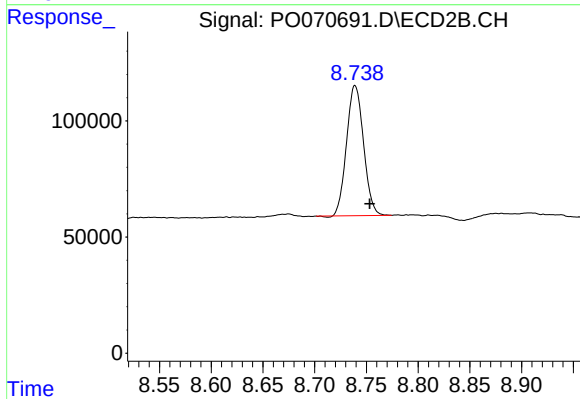

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.014 min
Response: 639571
Conc: 11.52 ng/ml