

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082018\
Data File : P0048289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2018 14:05
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:17:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.627	5116529	6677357	25.342	27.175
2) SA Decachlor...	10.073	8.609	3459718	3107475	21.212	19.769

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082018\
Data File : P0048289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2018 14:05
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:17:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

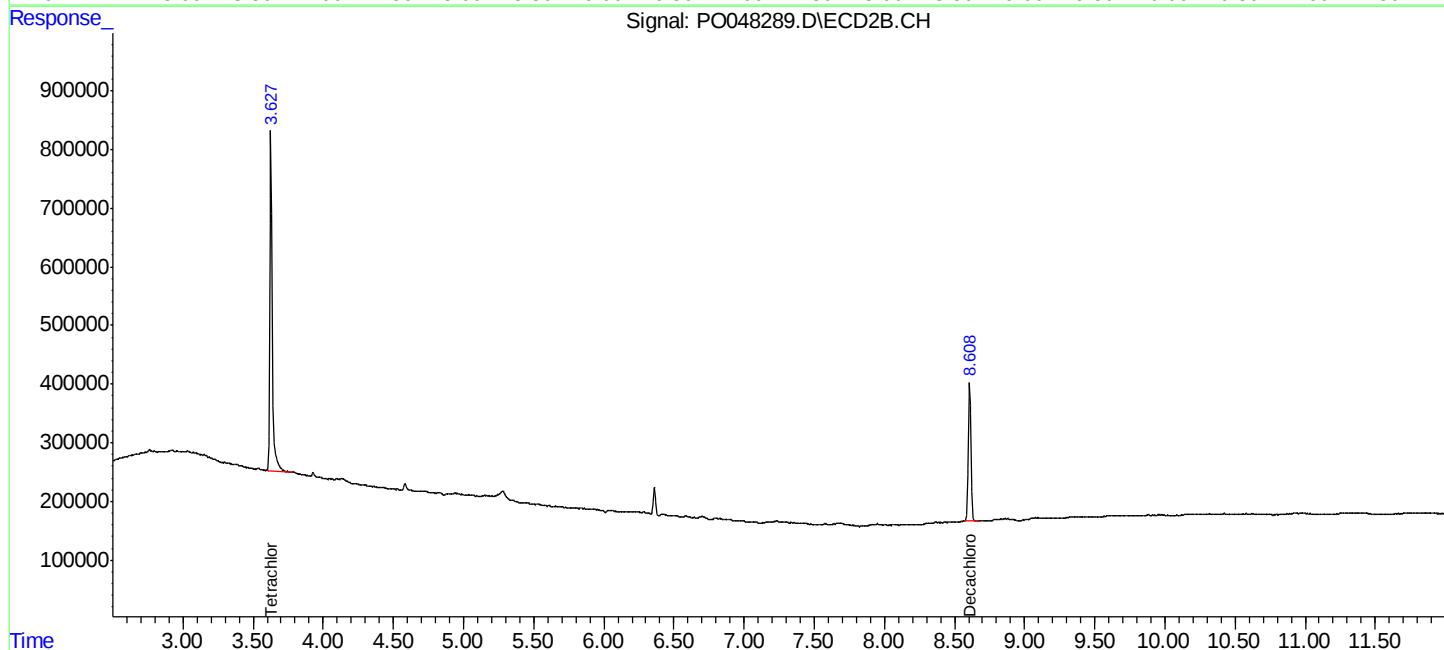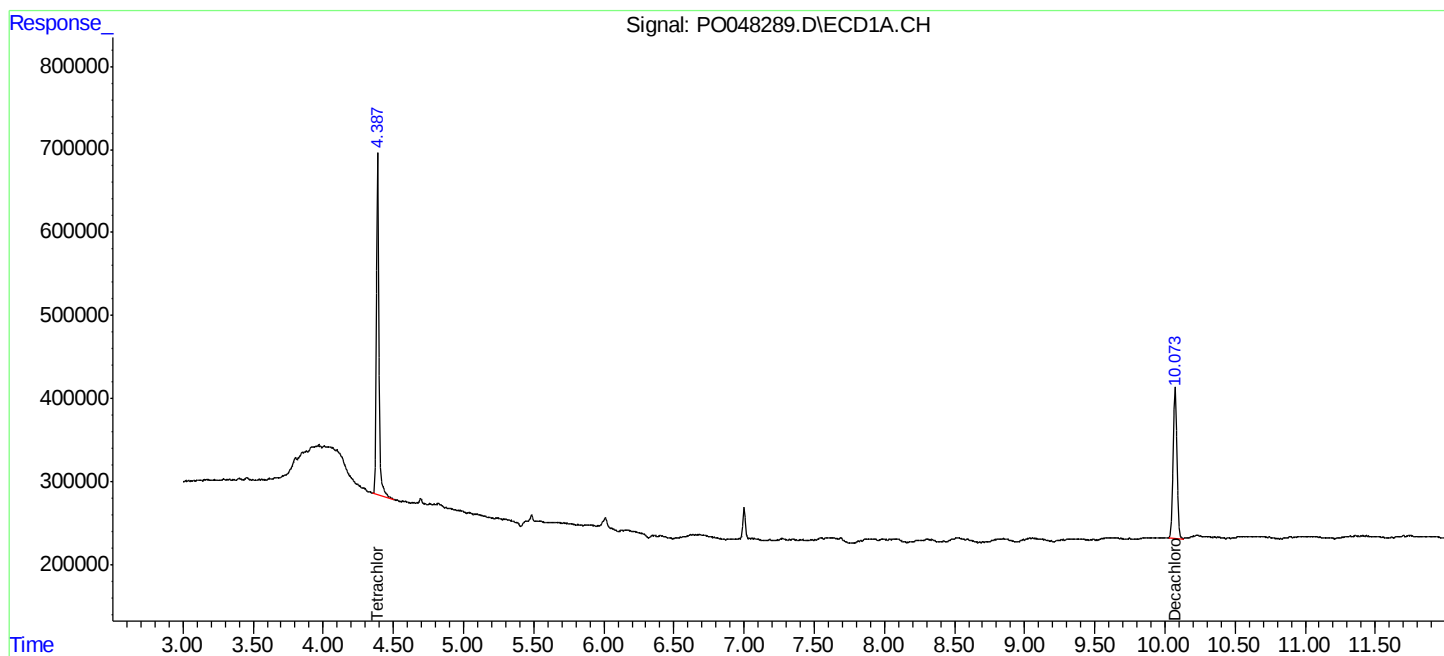


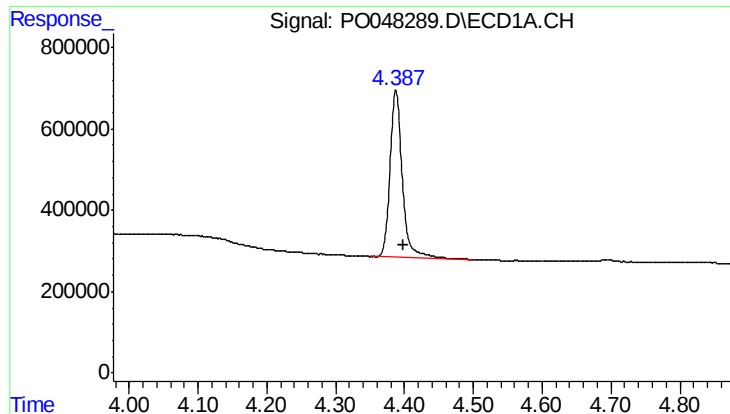

#1 Tetrachloro-m-xylene


R.T.: 4.387 min
Delta R.T.: -0.010 min
Response: 5116529
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

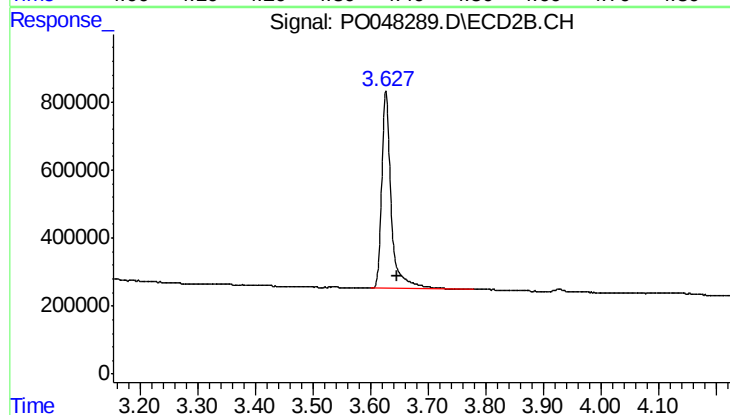


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: -0.018 min
Response: 6677357
Conc: 27.18 ng/ml

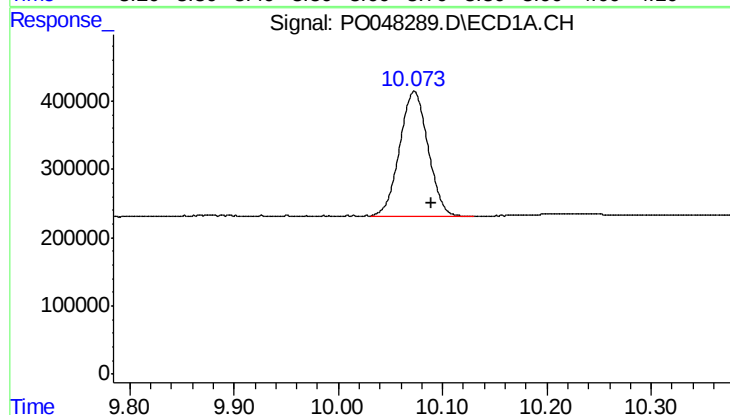

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: -0.017 min
Response: 3459718
Conc: 21.21 ng/ml

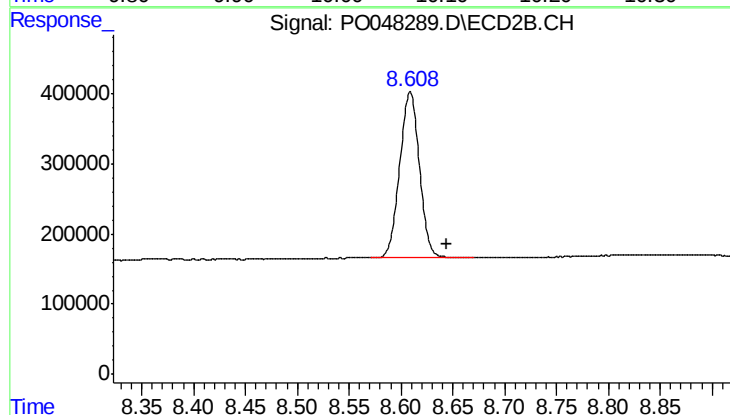

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: -0.036 min
Response: 3107475
Conc: 19.77 ng/ml