

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
 Data File : P0070719.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2020 14:43
 Operator : DD\AJ
 Sample : L3710-06RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1-5-WATER-DRUMRE

Manual Integrations
 APPROVED

Ankita
 8/21/2020 3:31:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:46:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.364	3.551	726584	486826	10.430	12.093
2) SA Decachlor...	9.986	8.733	246283	156087	2.631	2.772m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082020\
Data File : PO070719.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2020 14:43
Operator : DD\AJ
Sample : L3710-06RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1-5-WATER-DRUMRE


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:46:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

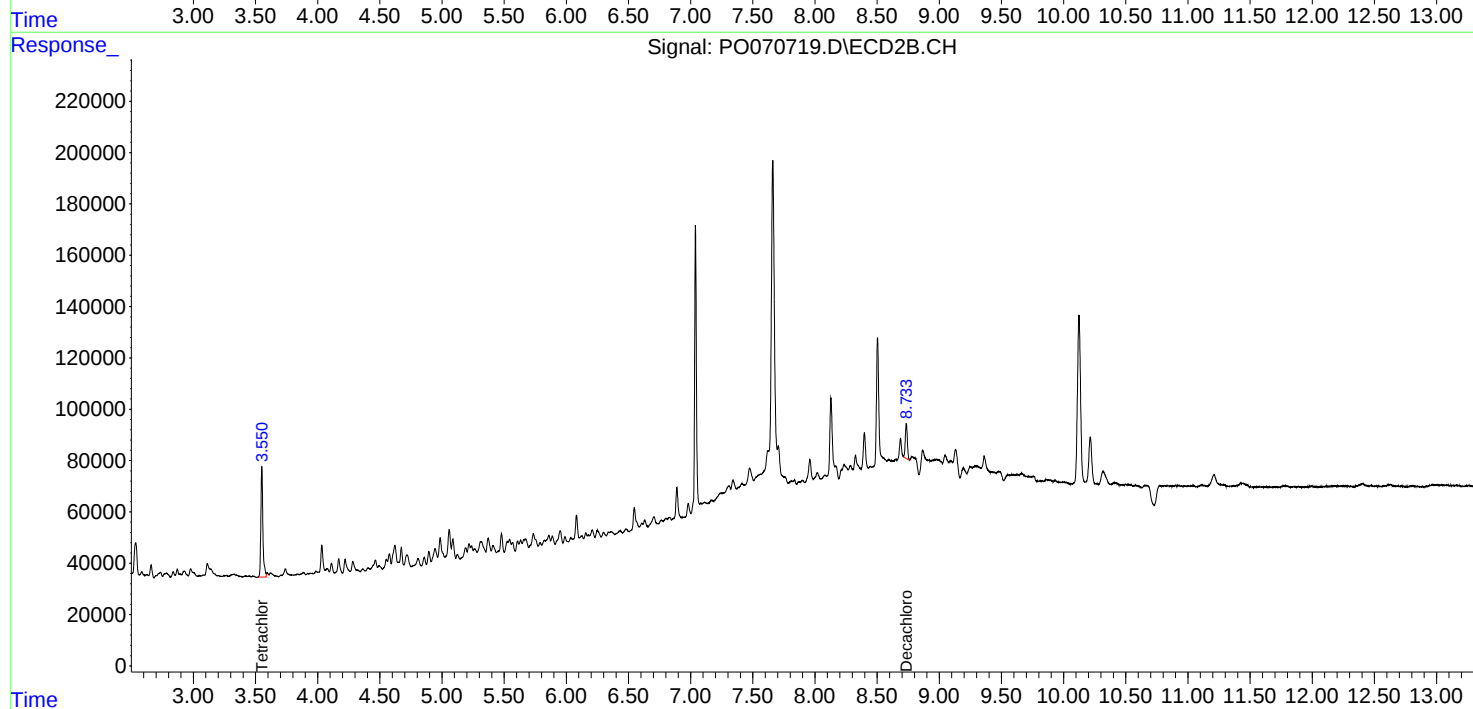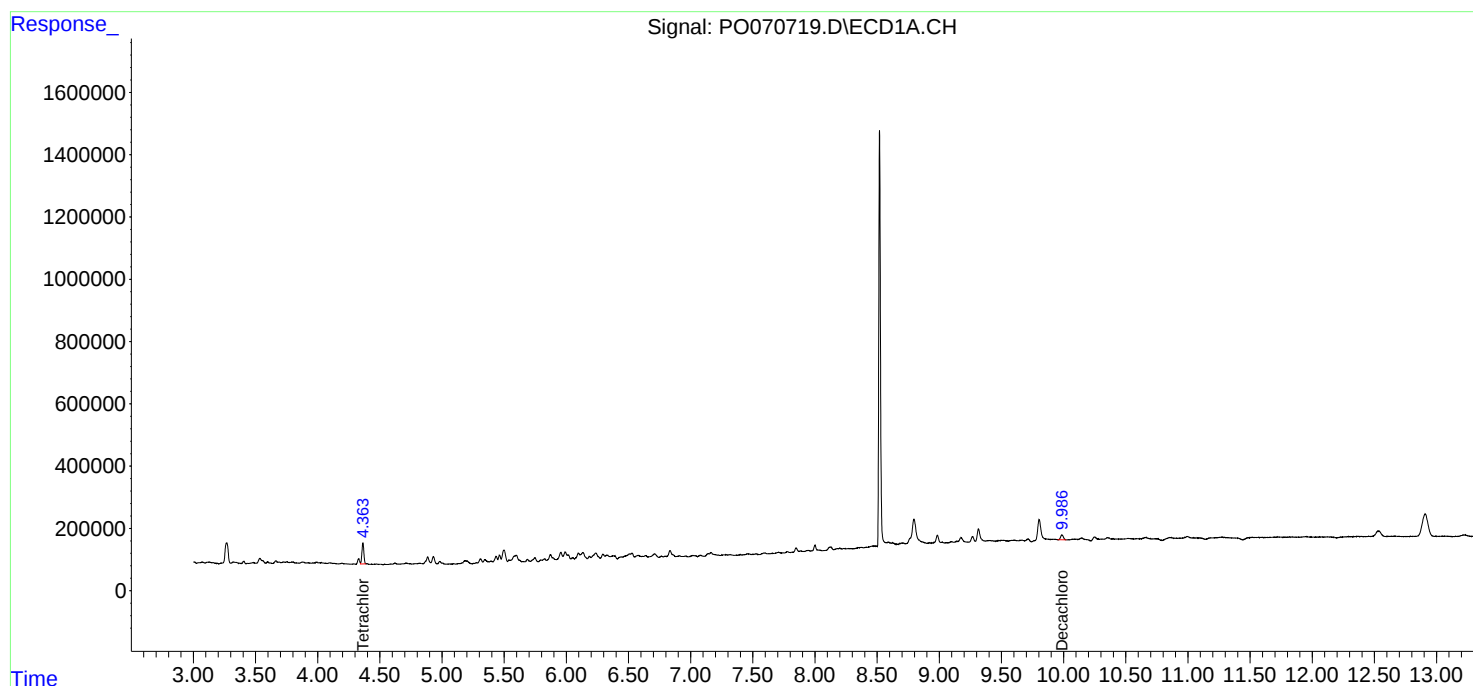

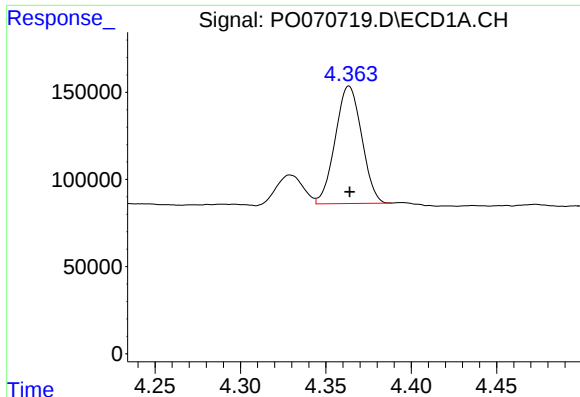


#1 Tetrachloro-m-xylene

R.T.: 4.364 min
Delta R.T.: 0.000 min
Response: 726584
Conc: 10.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
1-5-WATER-DRUMRE


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:43 PM

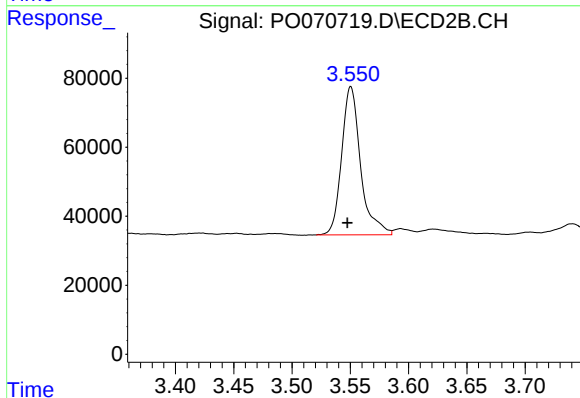


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.003 min
Response: 486826
Conc: 12.09 ng/ml

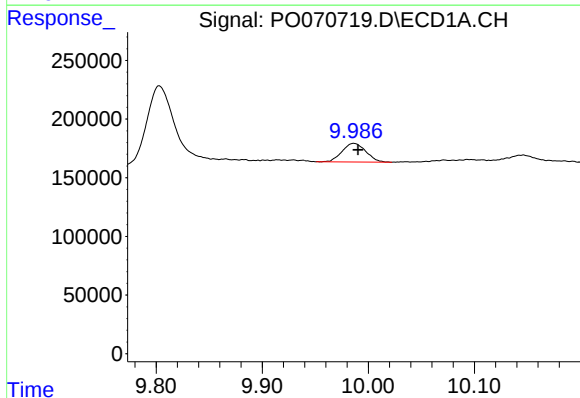

#2 Decachlorobiphenyl

R.T.: 9.986 min
Delta R.T.: -0.004 min
Response: 246283
Conc: 2.63 ng/ml

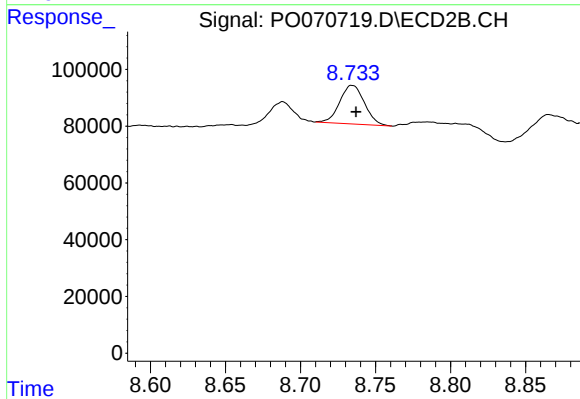

#2 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.004 min
Response: 156087
Conc: 2.77 ng/ml m