

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
 Data File : P0070725.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2020 16:26
 Operator : DD\AJ
 Sample : L3720-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MP-081920-BD-0-2-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:49:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.362	3.546	1740278	1035995	24.982	25.735
2) SA Decachlor...	9.989	8.736	1670972	1053992	17.848	18.717

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
Data File : P0070725.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2020 16:26
Operator : DD\AJ
Sample : L3720-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MP-081920-BD-0-2-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:49:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

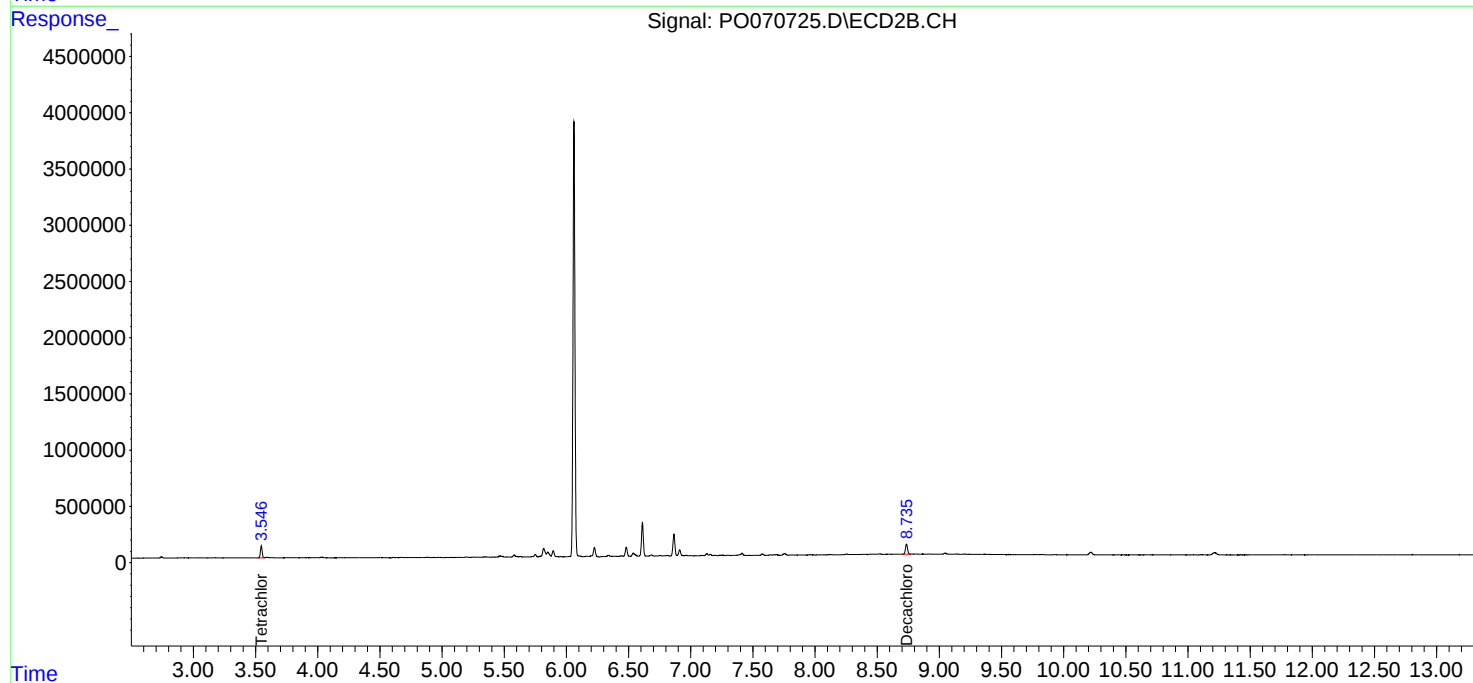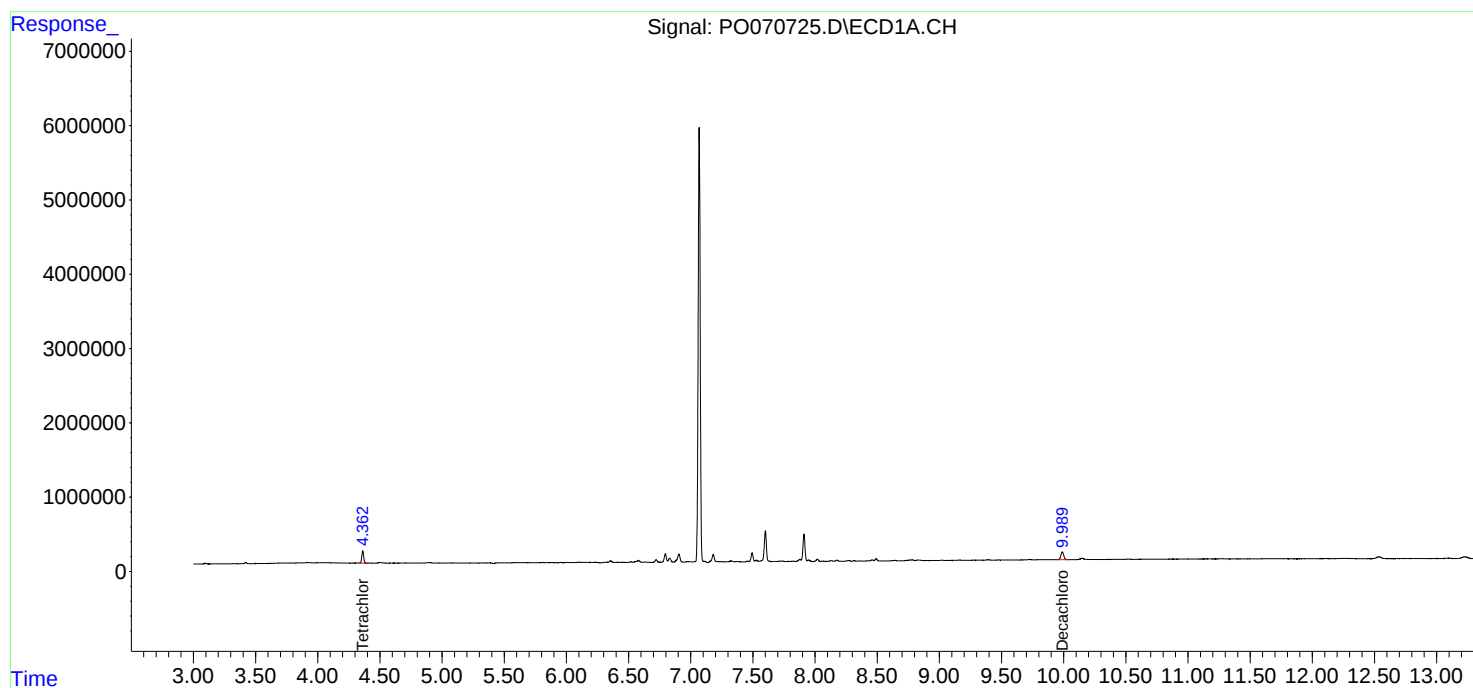


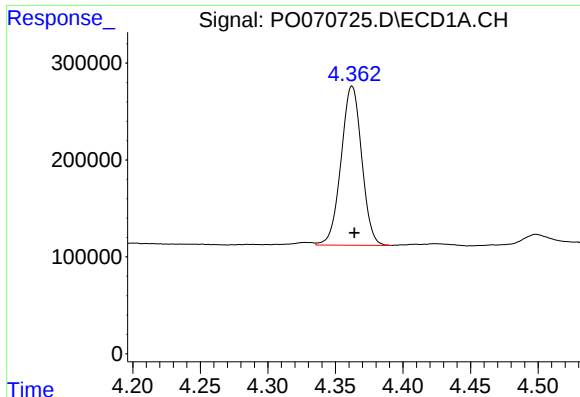

#1 Tetrachloro-m-xylene


R.T.: 4.362 min
Delta R.T.: -0.002 min
Response: 1740278
Conc: 24.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MP-081920-BD-0-2-COMP

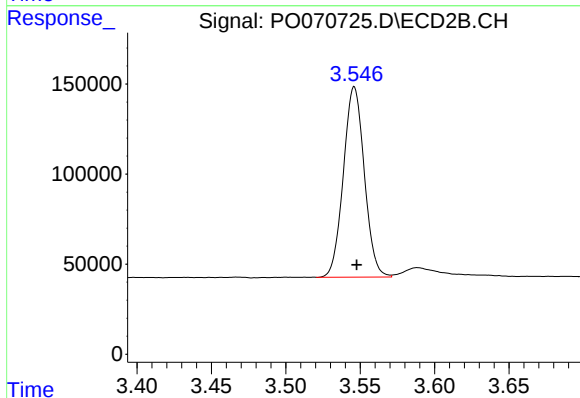


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.002 min
Response: 1035995
Conc: 25.73 ng/ml

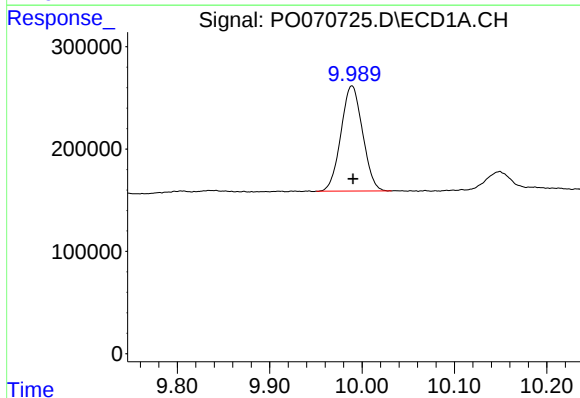

#2 Decachlorobiphenyl

R.T.: 9.989 min
Delta R.T.: -0.001 min
Response: 1670972
Conc: 17.85 ng/ml

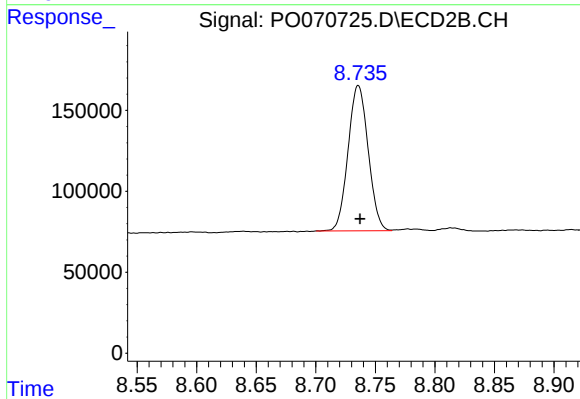

#2 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.001 min
Response: 1053992
Conc: 18.72 ng/ml