

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
 Data File : P0070726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2020 16:43
 Operator : DD\AJ
 Sample : L3729-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1-(0-1)

Manual Integrations
 APPROVED

Ankita
 8/21/2020 3:31:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:50:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.360	3.545	1756580	1054040	25.216	26.183
2)	SA Decachlor...	9.988	8.734	2114969	1368789	22.591	24.307m
Target Compounds							
26)	L6 AR-1254-1	6.555	5.627	107590	105244	32.188m	37.973
27)	L6 AR-1254-2	6.786	5.788	251500	101511	47.784m	40.954m
28)	L6 AR-1254-3	7.163	6.198	498995	127828	91.781	31.984m#
29)	L6 AR-1254-4	7.457	6.439	169967	114183	32.785	38.062
30)	L6 AR-1254-5	7.877	6.860	319485	211189	60.418	53.443

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082020\
Data File : PO070726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2020 16:43
Operator : DD\AJ
Sample : L3729-14
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:50:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

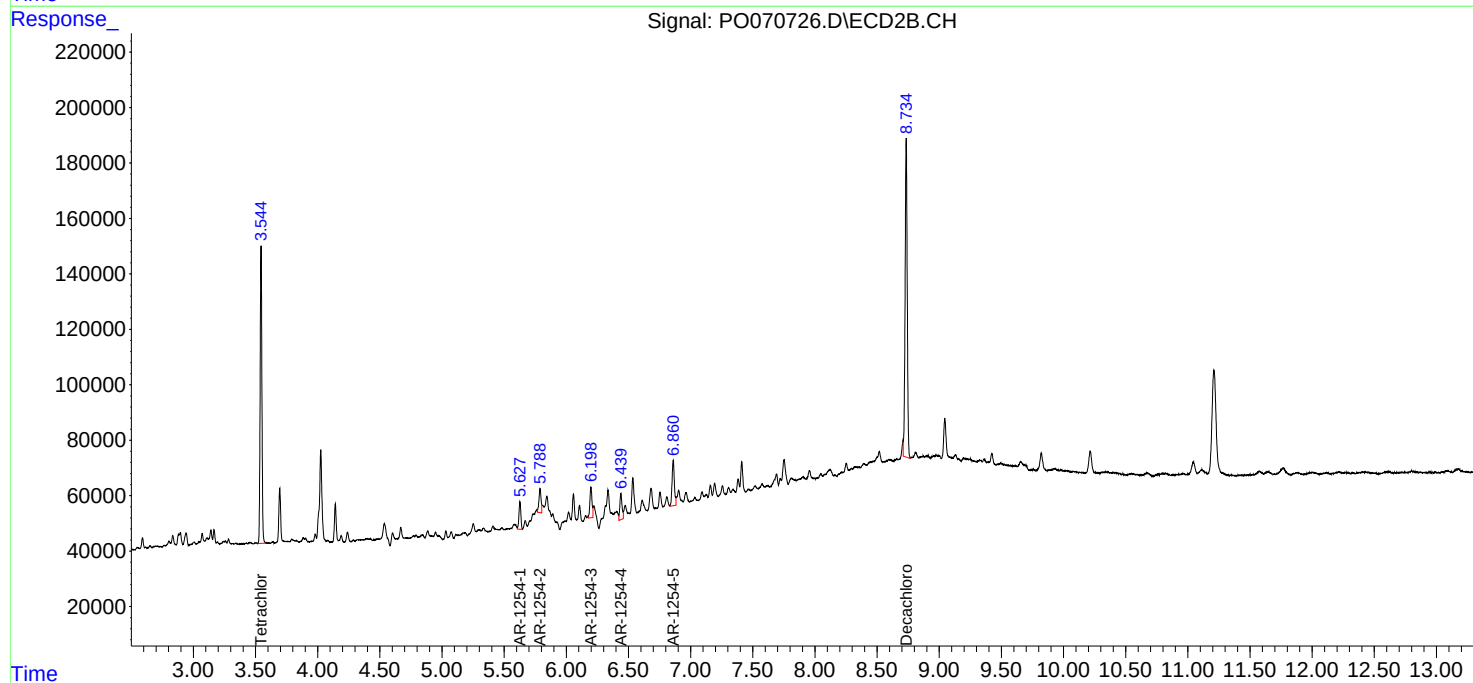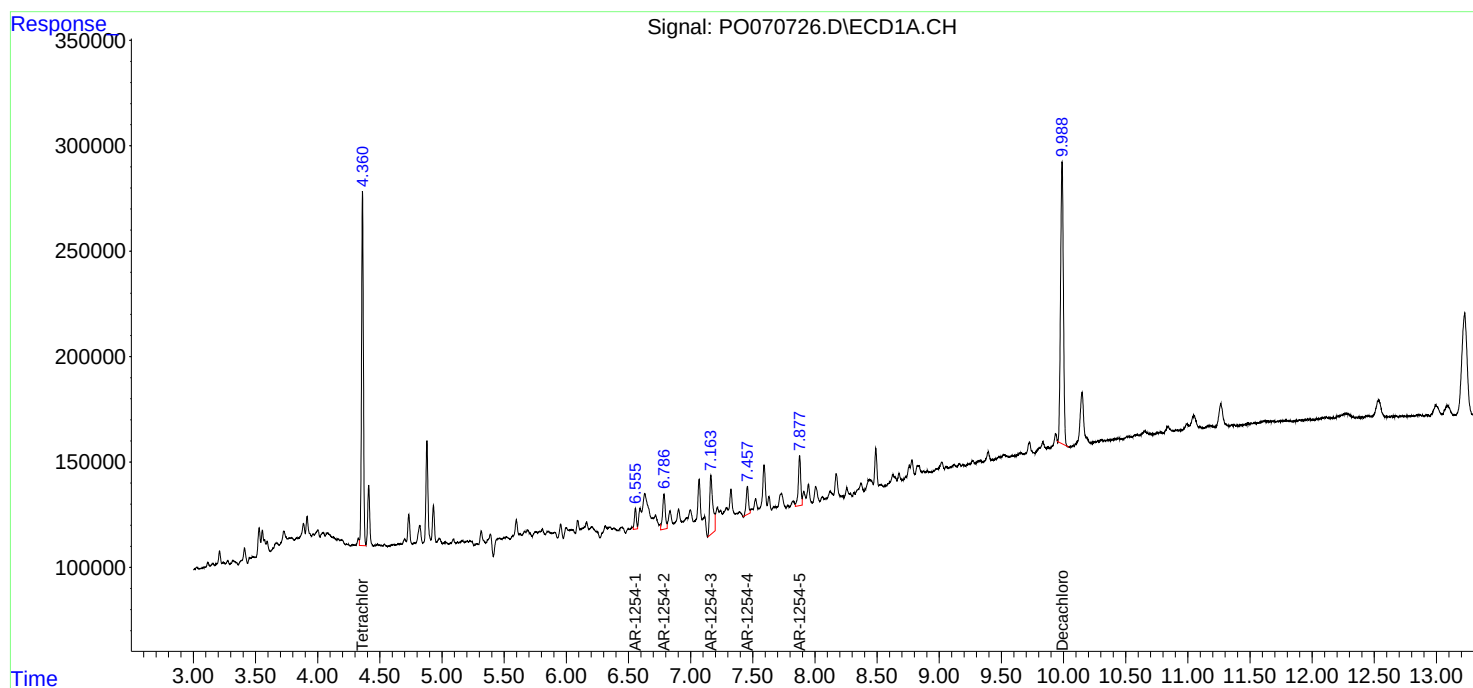

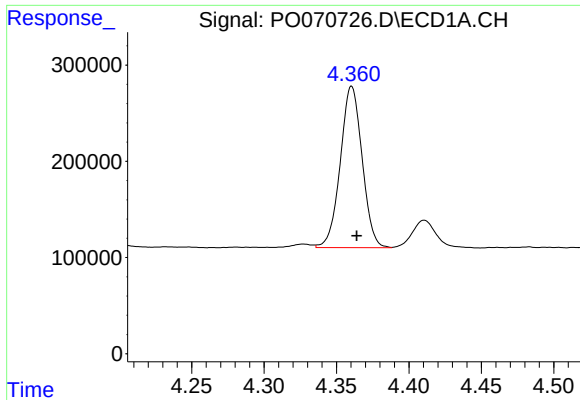


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: -0.004 min
Response: 1756580
Conc: 25.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:47 PM

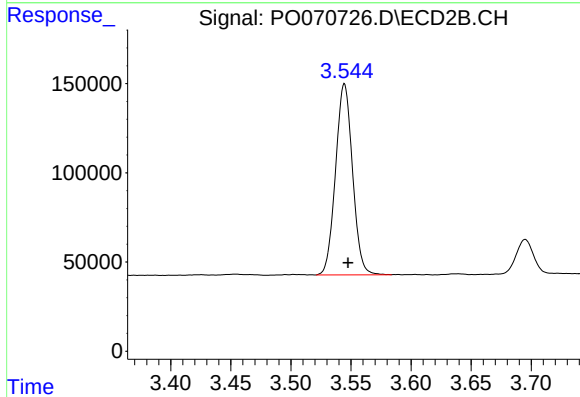


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.003 min
Response: 1054040
Conc: 26.18 ng/ml

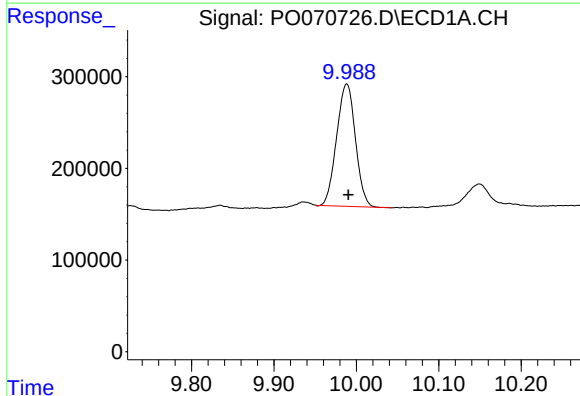


#2 Decachlorobiphenyl

R.T.: 9.988 min
Delta R.T.: -0.002 min
Response: 2114969
Conc: 22.59 ng/ml

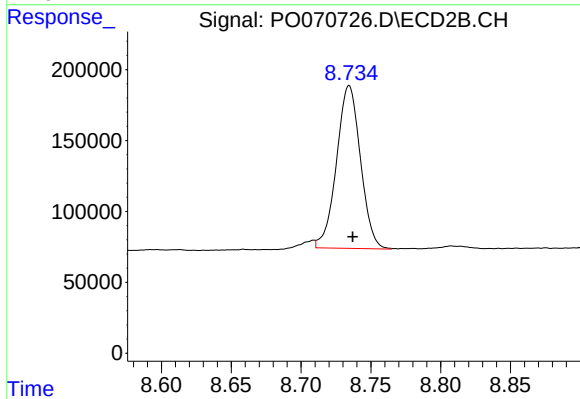

#2 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.003 min
Response: 1368789
Conc: 24.31 ng/ml m

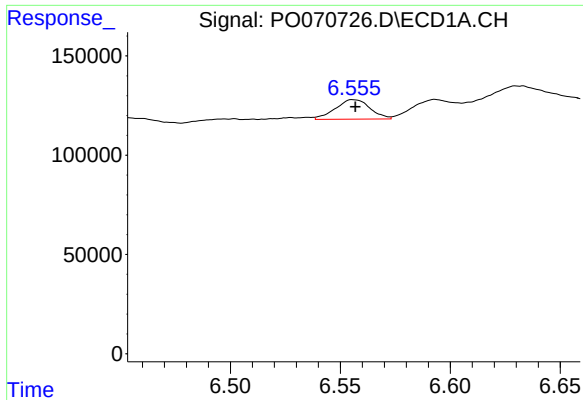


#26 AR-1254-1

R.T.: 6.555 min
Delta R.T.: -0.002 min
Response: 107590
Conc: 32.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:47 PM

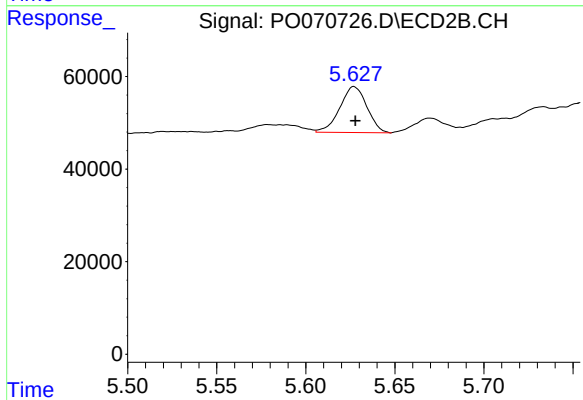


#26 AR-1254-1

R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 105244
Conc: 37.97 ng/ml

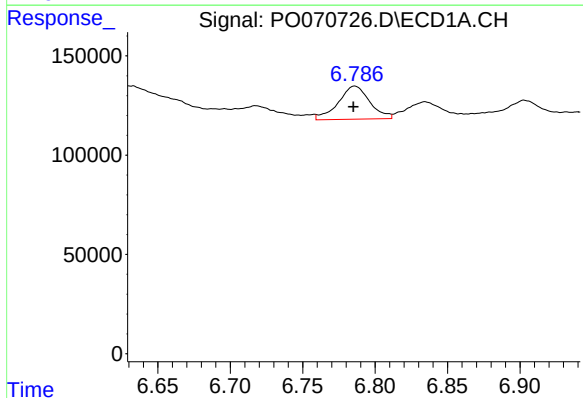


#27 AR-1254-2

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 251500
Conc: 47.78 ng/ml m

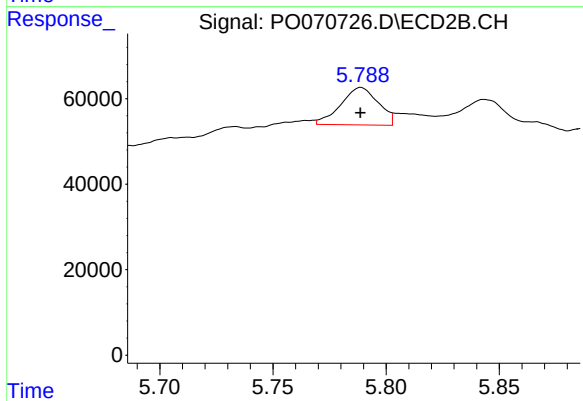

#27 AR-1254-2

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 101511
Conc: 40.95 ng/ml m

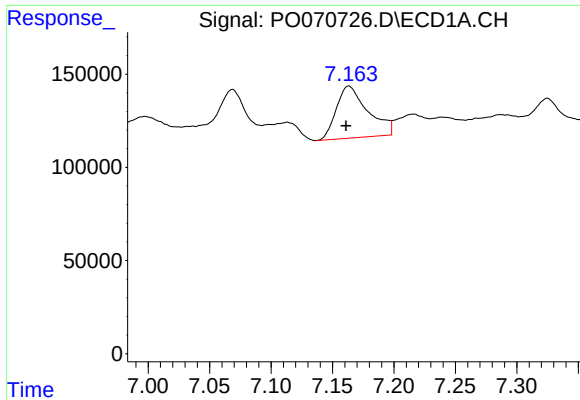


#28 AR-1254-3

R.T.: 7.163 min
Delta R.T.: 0.002 min
Response: 498995
Conc: 91.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:47 PM

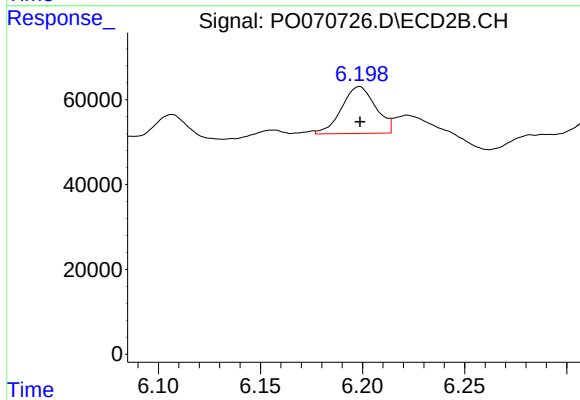


#28 AR-1254-3

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 127828
Conc: 31.98 ng/ml m

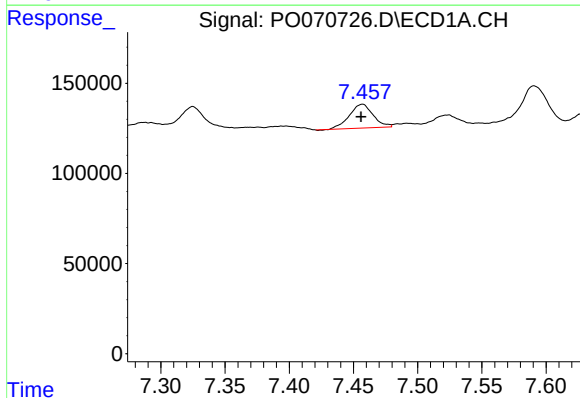


#29 AR-1254-4

R.T.: 7.457 min
Delta R.T.: 0.000 min
Response: 169967
Conc: 32.79 ng/ml

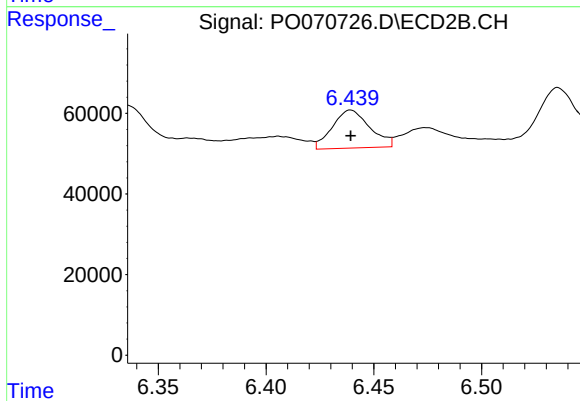

#29 AR-1254-4

R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 114183
Conc: 38.06 ng/ml

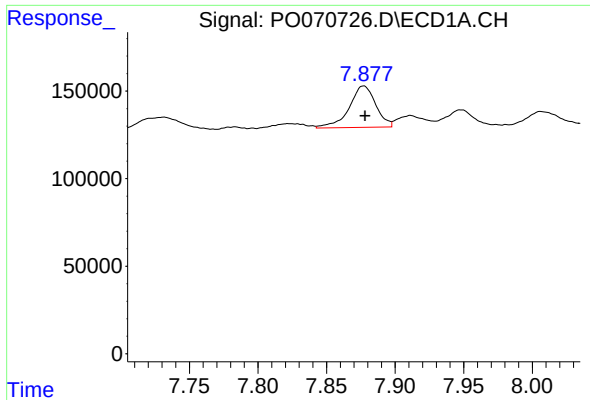


#30 AR-1254-5

R.T.: 7.877 min
Delta R.T.: -0.001 min
Response: 319485
Conc: 60.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1-(0-1)

Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:47 PM

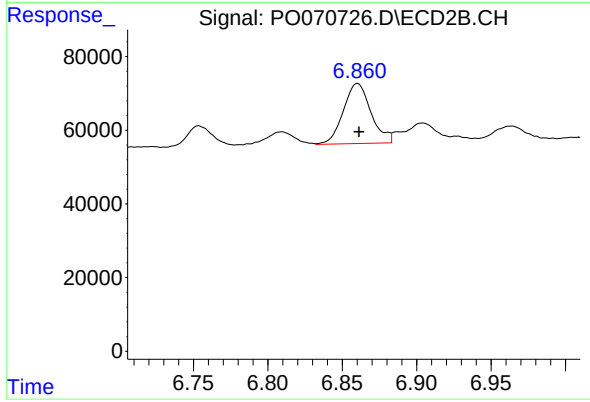

#30 AR-1254-5

R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 211189
Conc: 53.44 ng/ml