

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
 Data File : P0070727.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2020 17:00
 Operator : DD\AJ
 Sample : L3729-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2-(1-2)

Manual Integrations
 APPROVED

Ankita
 8/21/2020 3:31:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:50:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.361	3.545	1743331	1051081	25.026	26.109
2) SA Decachlor...	9.988	8.734	1932825	1254688	20.645	22.281m
Target Compounds						
26) L6 AR-1254-1	6.557	5.628	196240	164919	58.710m	59.504
27) L6 AR-1254-2	6.786	5.790	368040	222602	69.927m	89.809 #
28) L6 AR-1254-3	7.166	6.199	752547	225111	138.417	56.326m#
29) L6 AR-1254-4	7.457	6.440	241877	170964	46.656	56.989
30) L6 AR-1254-5	7.878	6.861	395260	240532	74.748	60.868

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082020\
Data File : PO070727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2020 17:00
Operator : DD\AJ
Sample : L3729-15
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:50:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

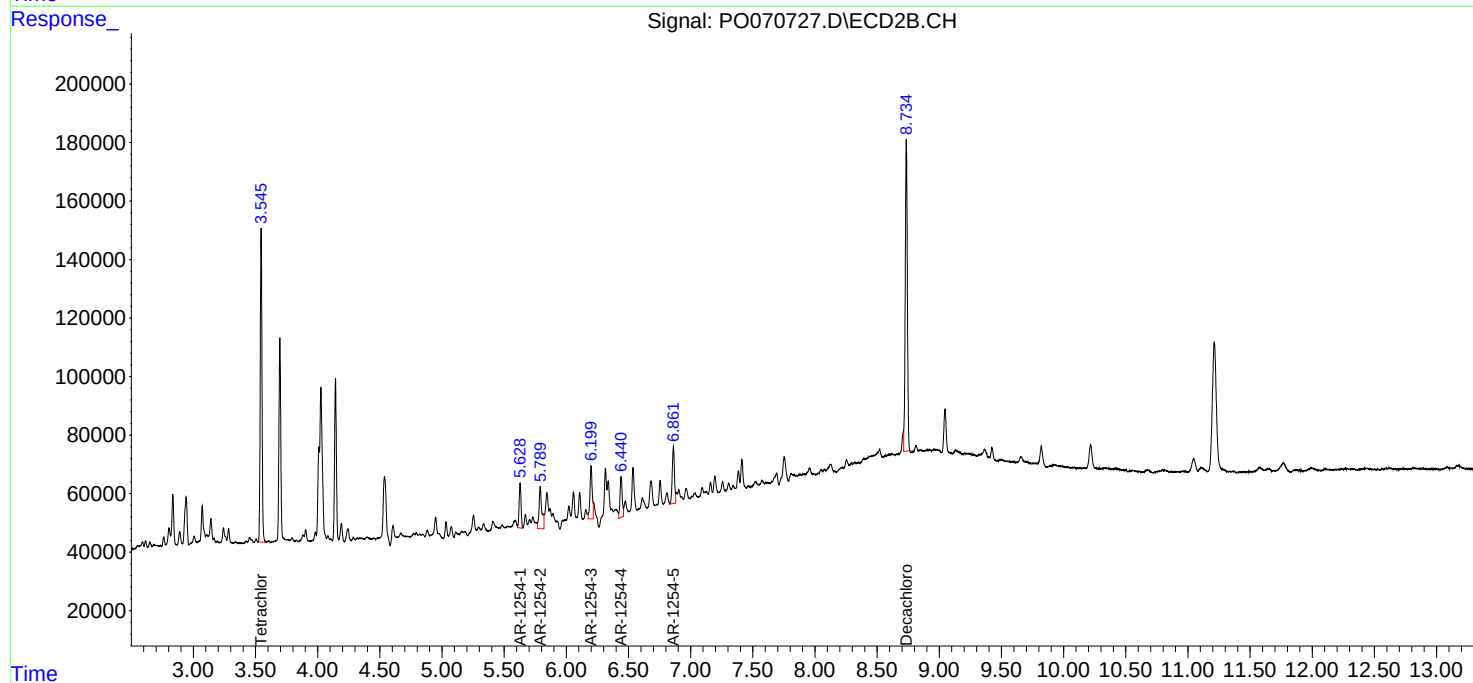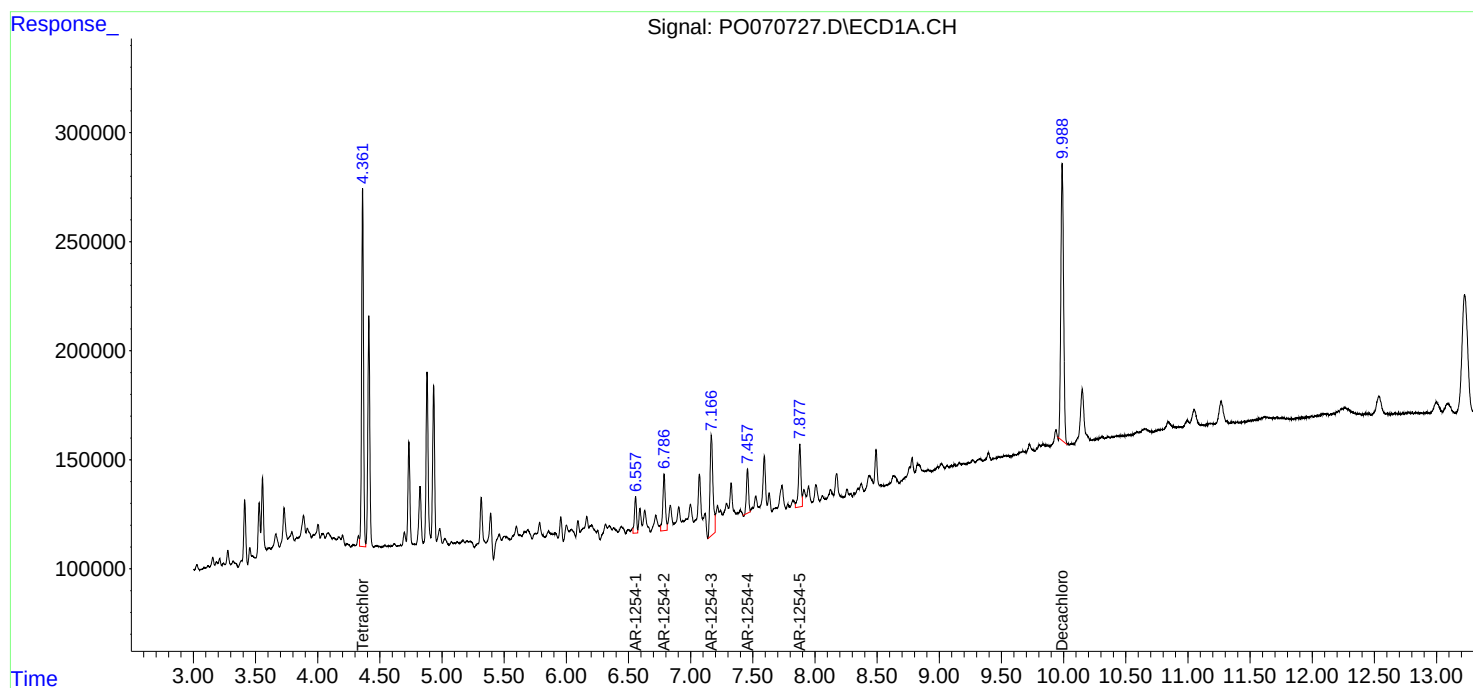

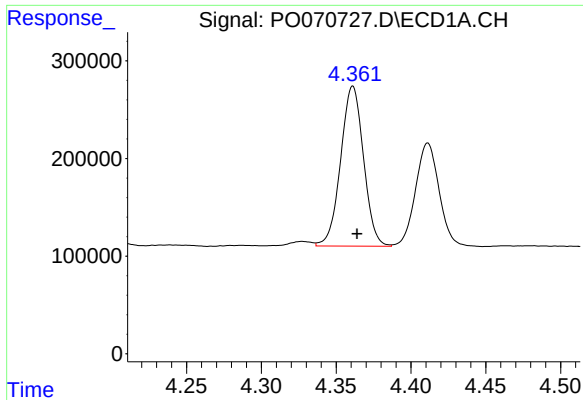


#1 Tetrachloro-m-xylene

R.T.: 4.361 min
Delta R.T.: -0.003 min
Response: 1743331
Conc: 25.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:49 PM

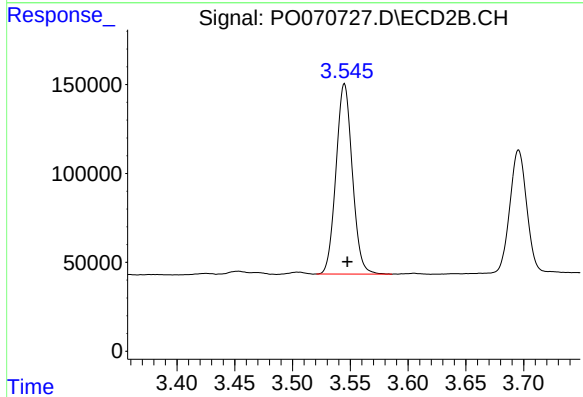


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.003 min
Response: 1051081
Conc: 26.11 ng/ml

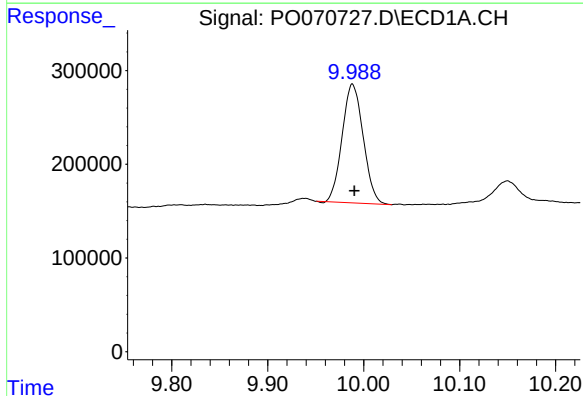


#2 Decachlorobiphenyl

R.T.: 9.988 min
Delta R.T.: -0.002 min
Response: 1932825
Conc: 20.65 ng/ml

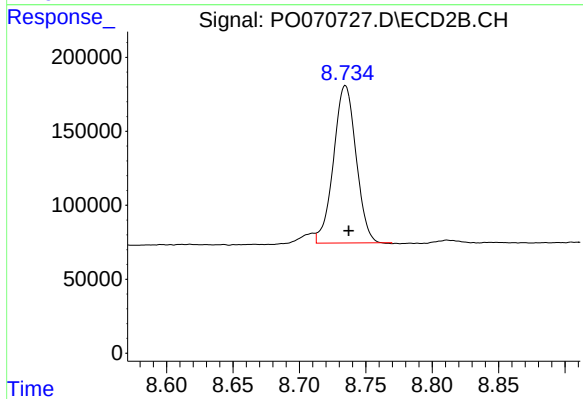

#2 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.003 min
Response: 1254688
Conc: 22.28 ng/ml m

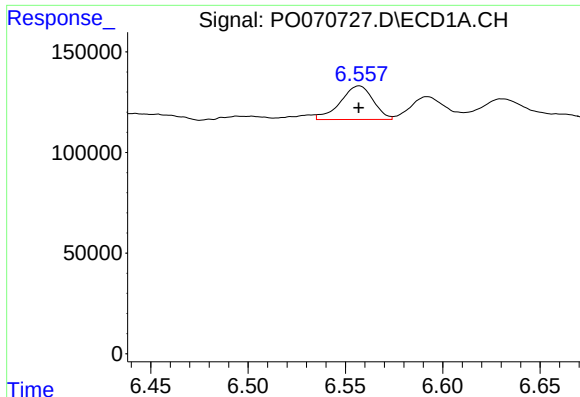


#26 AR-1254-1

R.T.: 6.557 min
Delta R.T.: 0.000 min
Response: 196240
Conc: 58.71 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:49 PM

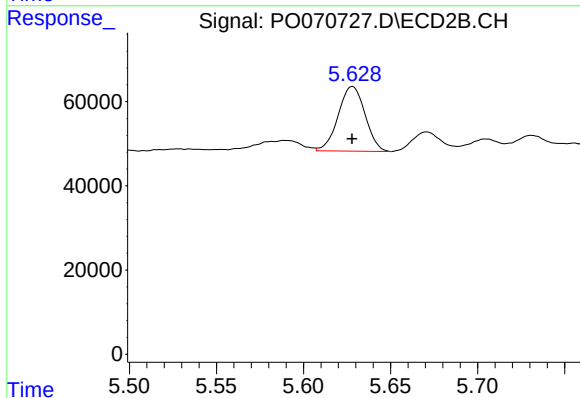


#26 AR-1254-1

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 164919
Conc: 59.50 ng/ml

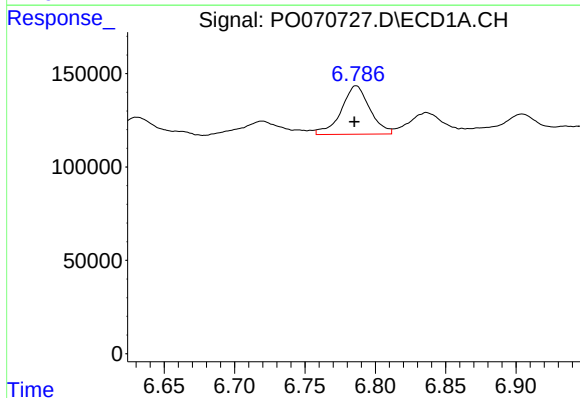


#27 AR-1254-2

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 368040
Conc: 69.93 ng/ml m

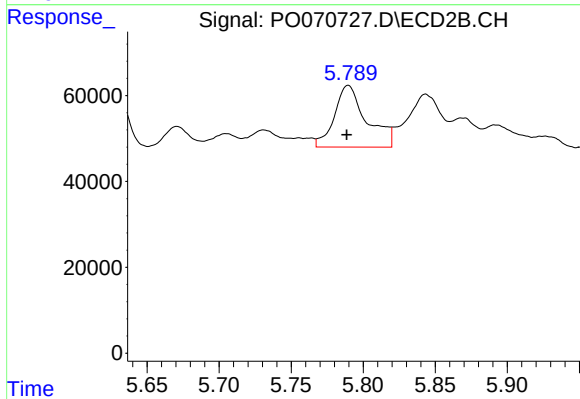

#27 AR-1254-2

R.T.: 5.790 min
Delta R.T.: 0.001 min
Response: 222602
Conc: 89.81 ng/ml

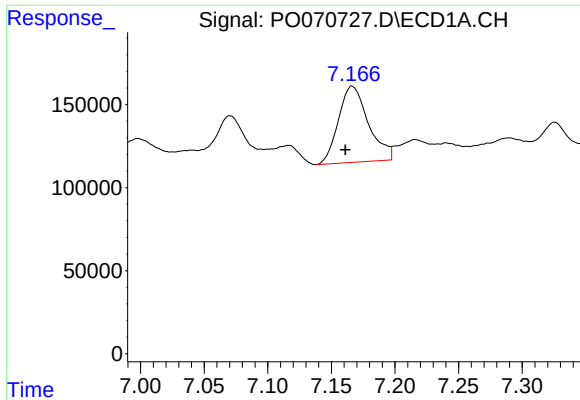


#28 AR-1254-3

R.T.: 7.166 min
Delta R.T.: 0.005 min
Response: 752547
Conc: 138.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:49 PM

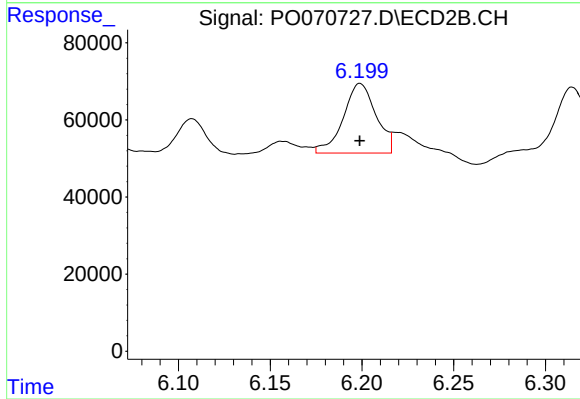


#28 AR-1254-3

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 225111
Conc: 56.33 ng/ml m

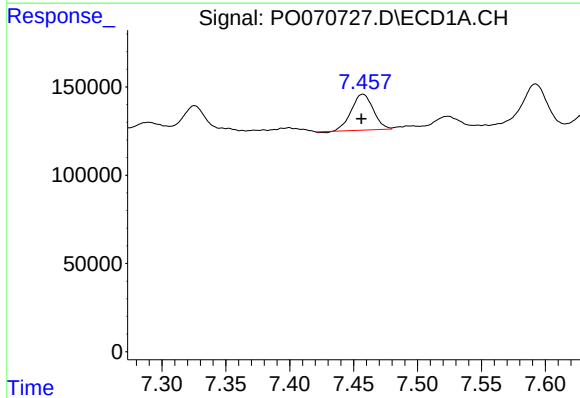


#29 AR-1254-4

R.T.: 7.457 min
Delta R.T.: 0.001 min
Response: 241877
Conc: 46.66 ng/ml

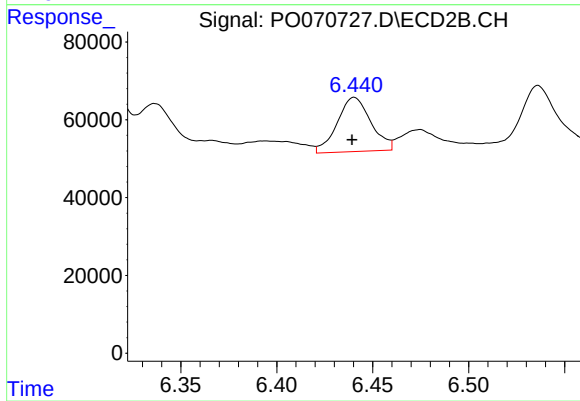

#29 AR-1254-4

R.T.: 6.440 min
Delta R.T.: 0.001 min
Response: 170964
Conc: 56.99 ng/ml

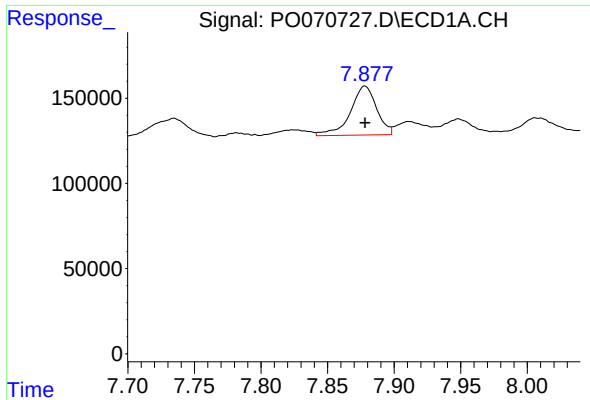


#30 AR-1254-5

R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 395260
Conc: 74.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2-(1-2)

Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:49 PM

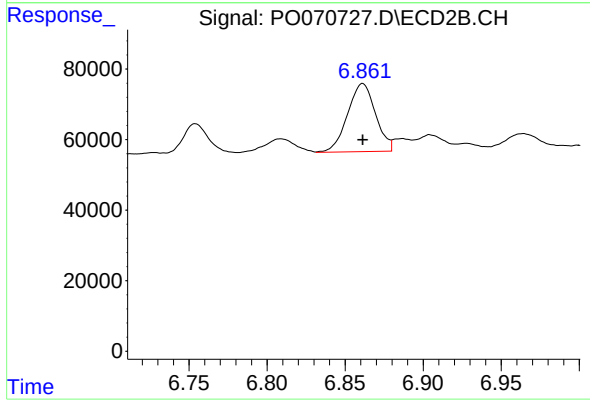

#30 AR-1254-5

R.T.: 6.861 min
Delta R.T.: 0.000 min
Response: 240532
Conc: 60.87 ng/ml