

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082020\
 Data File : P0070738.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2020 20:08
 Operator : DD\AJ
 Sample : L3740-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-3C

Manual Integrations
 APPROVED

Ankita
 8/21/2020 3:31:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:47:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.363	3.547	1675399	1028742	24.051	25.555
2) SA Decachlor...	9.990	8.737	1826510	1009993	19.510	17.936

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082020\
Data File : PO070738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2020 20:08
Operator : DD\AJ
Sample : L3740-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-3C


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:47:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

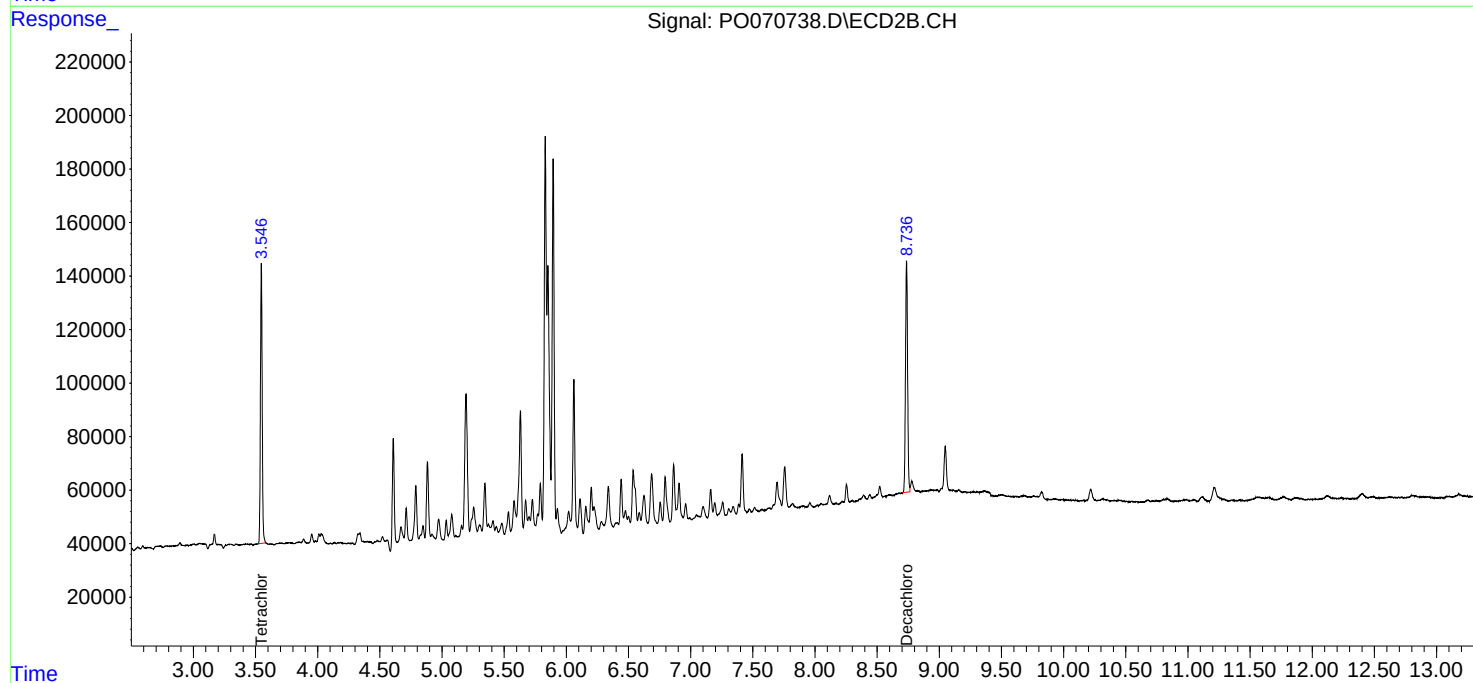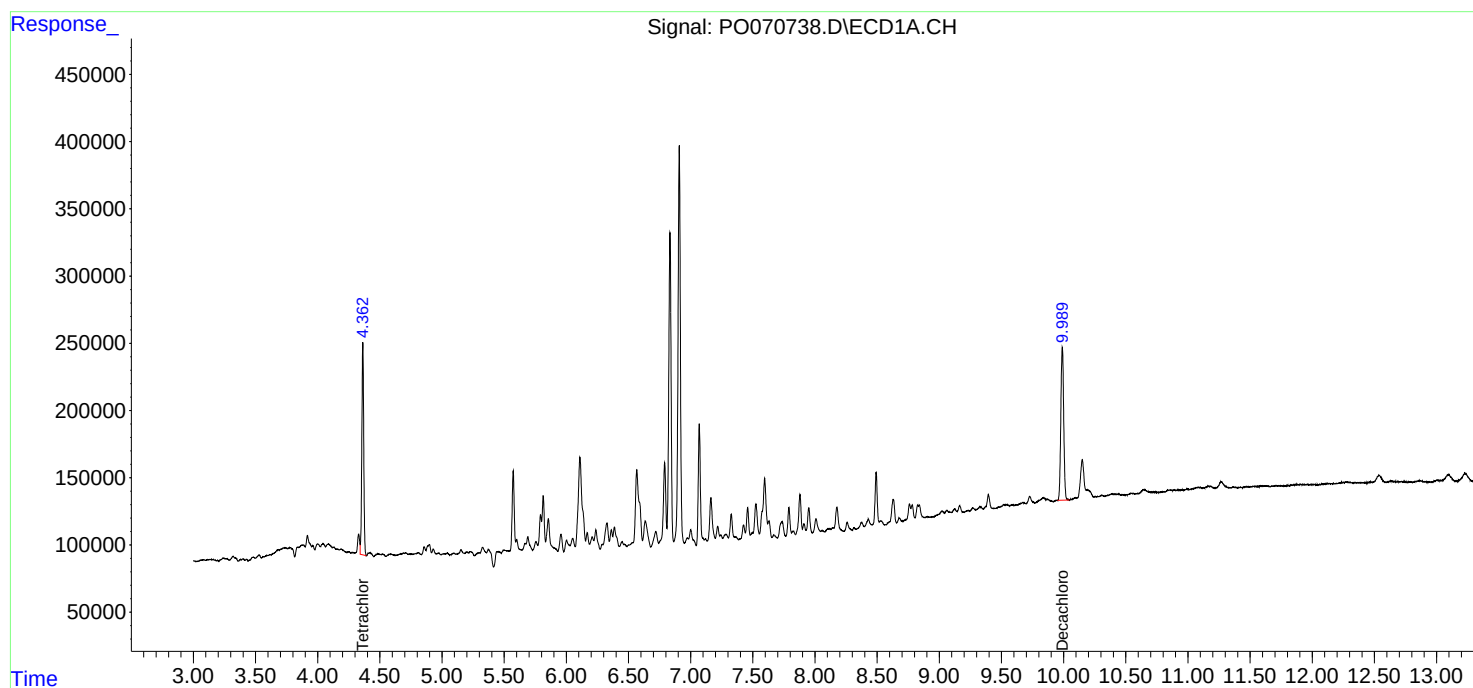

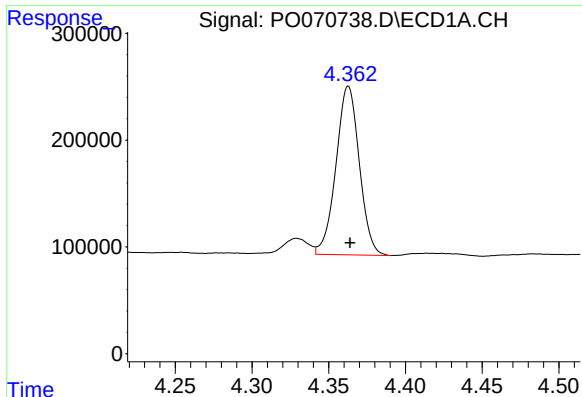


#1 Tetrachloro-m-xylene

R.T.: 4.363 min
Delta R.T.: -0.001 min
Response: 1675399
Conc: 24.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-3C


Manual Integrations
APPROVED

Ankita
8/21/2020 3:31:55 PM

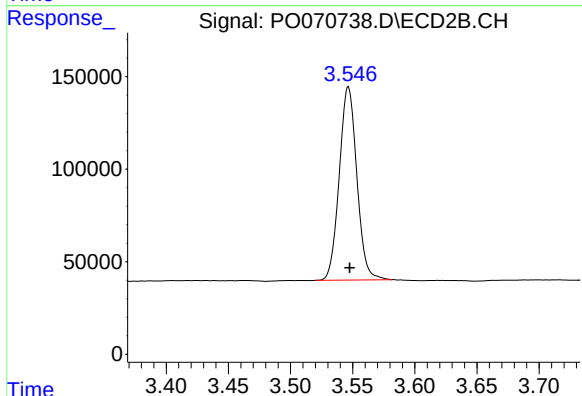


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.001 min
Response: 1028742
Conc: 25.55 ng/ml

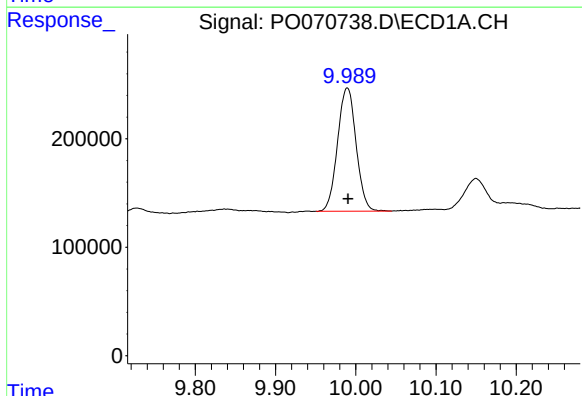

#2 Decachlorobiphenyl

R.T.: 9.990 min
Delta R.T.: 0.000 min
Response: 1826510
Conc: 19.51 ng/ml

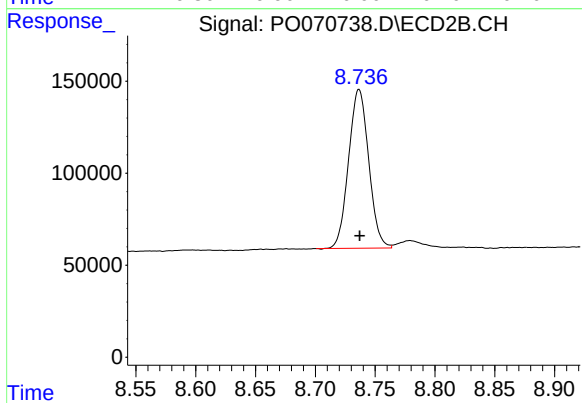

#2 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: 0.000 min
Response: 1009993
Conc: 17.94 ng/ml