

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : P0113087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 14:09
 Operator : YP/AJ
 Sample : Q2901-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HVAC DUCT SEALANT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 14:48:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.664	3.655	161.7E6	96941280	19.747	19.156
2)	SA Decachlor...	8.682	8.627	128.1E6	37043078	18.485	19.549
Target Compounds							
3)	L1 AR-1016-1	4.748	4.729	59050653	37625352	221.176	220.581
4)	L1 AR-1016-2	4.766	4.747	84187843	53522987	209.719	207.730
5)	L1 AR-1016-3	4.823	4.922	62598571	31393677	245.463	224.860
6)	L1 AR-1016-4	4.942	4.964	48137864	196.9E6	220.747	1687.141 #
7)	L1 AR-1016-5	5.199	5.176	259.7E6	153.6E6	1171.886	1077.757
8)	L2 AR-1221-1	0.000	3.861	0	672336	N.D.	10.652 #
9)	L2 AR-1221-2	3.965	3.951	2839727	3873018	42.038	82.982 #
10)	L2 AR-1221-3	4.036	4.023	7368922	8280273	33.291	55.769 #
11)	L3 AR-1232-1	4.036	4.023	7368922	8280273	42.349	70.529 #
12)	L3 AR-1232-2	4.527	4.747	25676297	53522987	257.142	436.762 #
13)	L3 AR-1232-3	4.766	4.922	84187843	31393677	444.321	495.593
14)	L3 AR-1232-4	4.942	5.005	48137864	87108470	511.183	1549.389 #
15)	L3 AR-1232-5	4.985	5.176	323.3E6	153.6E6	5219.984	2566.047 #
16)	L4 AR-1242-1	4.748	4.729	59050653	37625352	256.818	260.375
17)	L4 AR-1242-2	4.766	4.747	84187843	53522987	244.999	246.751
18)	L4 AR-1242-3	4.823	4.922	62598571	31393677	282.123	268.404
19)	L4 AR-1242-4	4.942	5.005	48137864	87108470	277.511	740.483 #
20)	L4 AR-1242-5	5.593	5.526	207.3E6	590.2E6	1035.522	3957.296 #
21)	L5 AR-1248-1	4.748	4.729	59050653	37625352	338.464	337.411
22)	L5 AR-1248-2	4.985	4.964	323.3E6	196.9E6	1336.863	1225.194
23)	L5 AR-1248-3	5.199	5.005	259.7E6	87108470	814.525	513.428 #
24)	L5 AR-1248-4	5.552	5.176	1063.4E6	153.6E6	2128.557	771.070 #
25)	L5 AR-1248-5	5.593	5.565	207.3E6	119.1E6	606.962	561.058
26)	L6 AR-1254-1	5.552	5.526	1063.4E6	590.2E6	1969.406	1871.432
27)	L6 AR-1254-2	5.702	5.674	888.1E6	472.2E6	1799.851	1684.561
28)	L6 AR-1254-3	6.105	6.074	1144.6E6	620.2E6	1549.053	1487.573
29)	L6 AR-1254-4	6.334	6.301	511.1E6	251.6E6	917.623	915.347
30)	L6 AR-1254-5	6.752	6.716	522.3E6	242.8E6	745.112	679.291
31)	L7 AR-1260-1	6.236	6.204	581.7E6	310.6E6	1304.408	1217.645
32)	L7 AR-1260-2	6.426	6.392	507.2E6	239.3E6	738.635	692.297
33)	L7 AR-1260-3	6.791	6.542	240.1E6	206.2E6	388.856	693.323 #
34)	L7 AR-1260-4	7.050	7.012	133.4E6	58110377	297.856	280.388
35)	L7 AR-1260-5	7.294	7.254	226.5E6	85277853	187.093	182.051
36)	L8 AR-1262-1	6.791	6.754	240.1E6	108.4E6	262.195	261.552
37)	L8 AR-1262-2	7.294	7.254	226.5E6	85277853	149.793	164.734
38)	L8 AR-1262-3	7.576	7.535	34477105	12823012	62.221	71.401
39)	L8 AR-1262-4	7.639	7.598	106.7E6	37415439	109.057	129.063
40)	L8 AR-1262-5	8.137	8.091	29195179	4146477	70.033	38.276 #
41)	L9 AR-1268-1	7.576	7.535	34477105	12823012	20.034	25.170 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
Data File : P0113087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 14:09
Operator : YP/AJ
Sample : Q2901-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 14:48:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.639	7.598	106.7E6	37415439	73.649	90.070
43)	L9 AR-1268-3	7.845	7.804	3726937	1300165	3.090	3.982 #
44)	L9 AR-1268-4	8.137	8.091	29195179	4146477	63.376	34.430 #
45)	L9 AR-1268-5	8.429	8.378	5183173	1333447	1.626	1.707



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 14:09
Operator : YP/AJ
Sample : Q2901-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 14:48:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

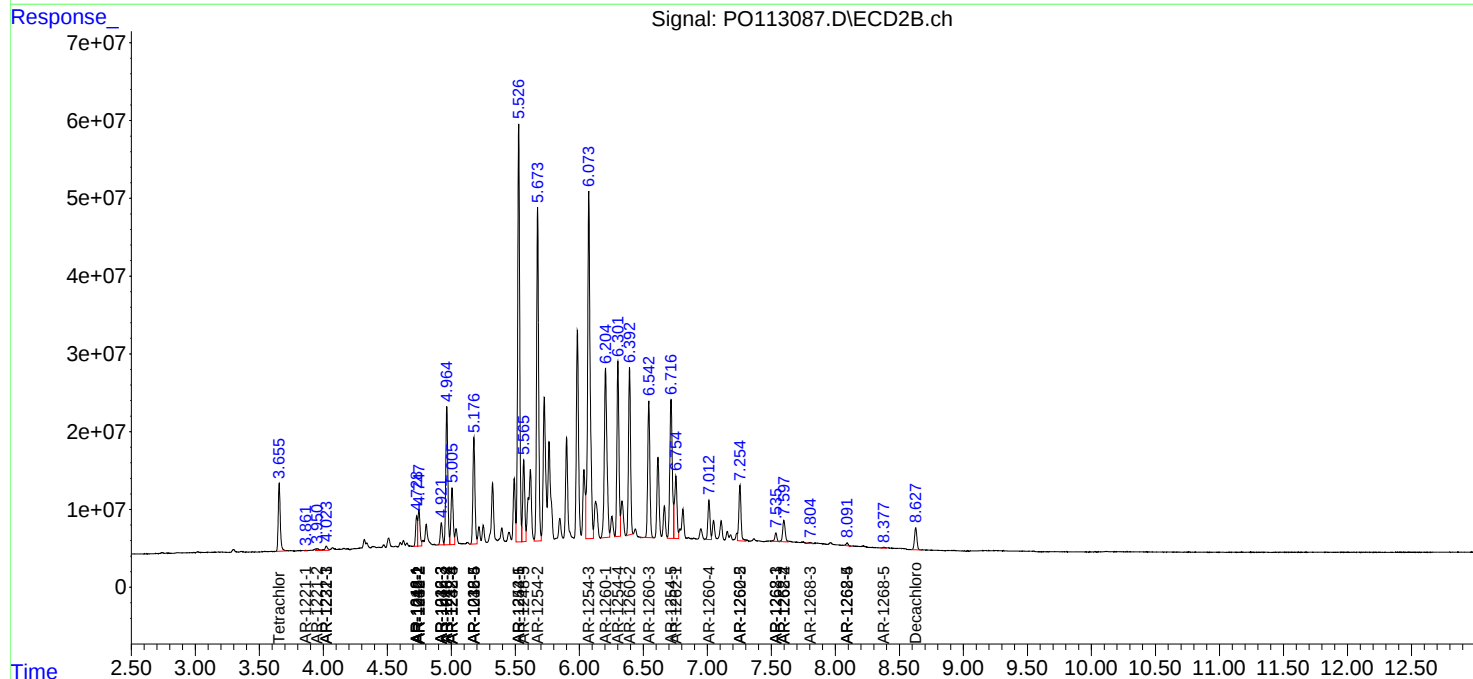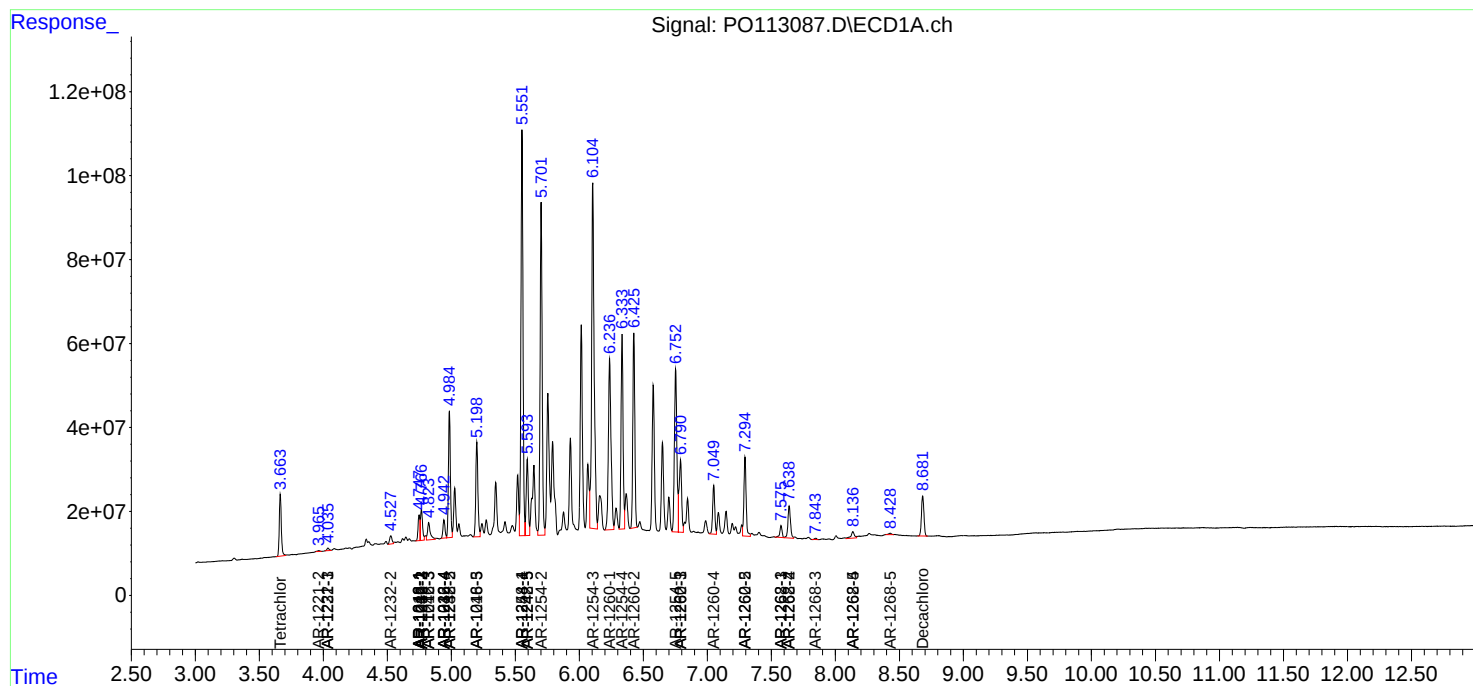


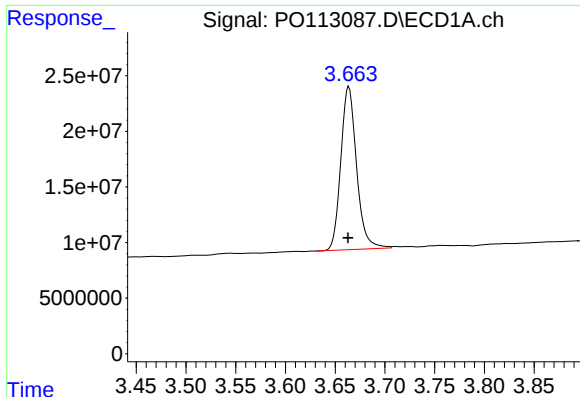

#1 Tetrachloro-m-xylene


R.T.: 3.664 min
Delta R.T.: 0.000 min
Response: 161662657
Conc: 19.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

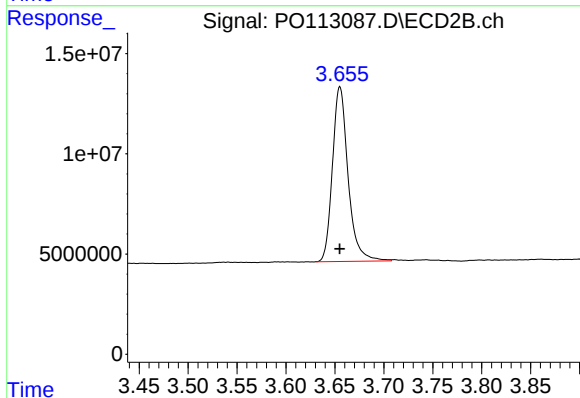


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 96941280
Conc: 19.16 ng/ml

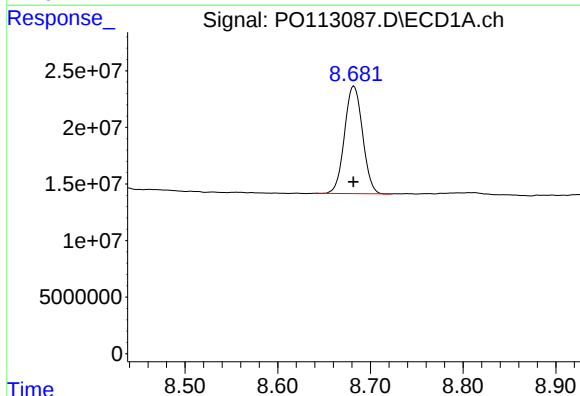


#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: 0.000 min
Response: 128127063
Conc: 18.48 ng/ml

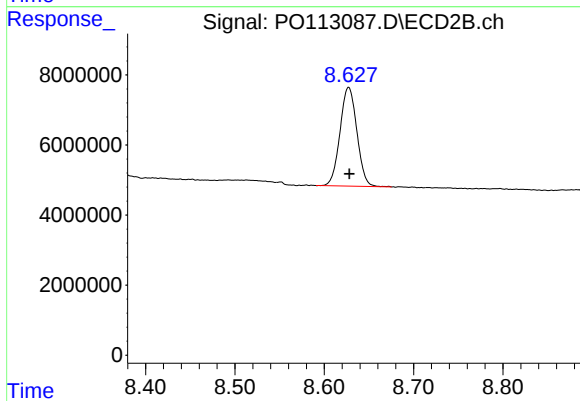

#2 Decachlorobiphenyl


R.T.: 8.627 min
Delta R.T.: -0.001 min
Response: 37043078
Conc: 19.55 ng/ml

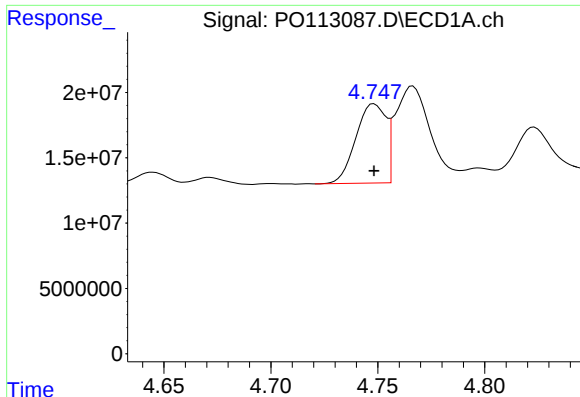

#3 AR-1016-1


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 59050653
Conc: 221.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

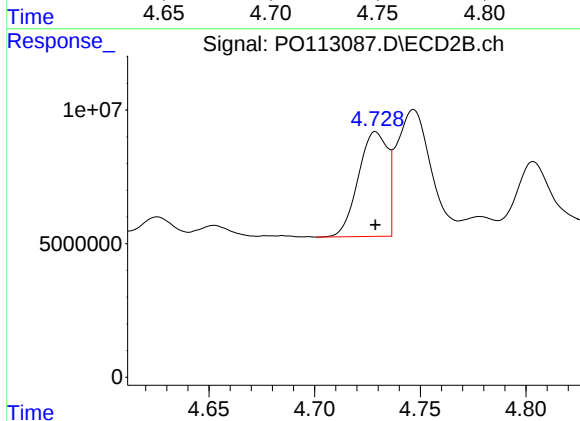


#3 AR-1016-1

R.T.: 4.729 min
Delta R.T.: 0.000 min
Response: 37625352
Conc: 220.58 ng/ml

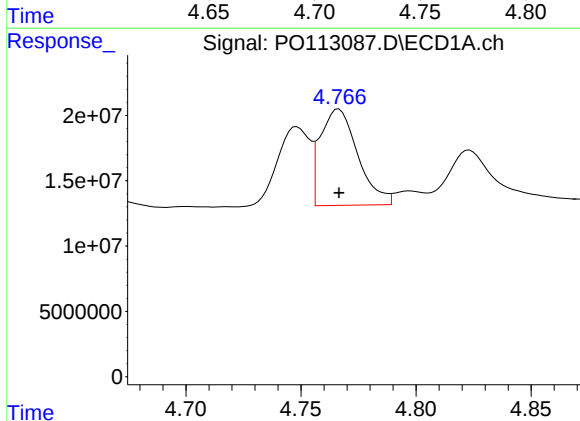


#4 AR-1016-2

R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 84187843
Conc: 209.72 ng/ml

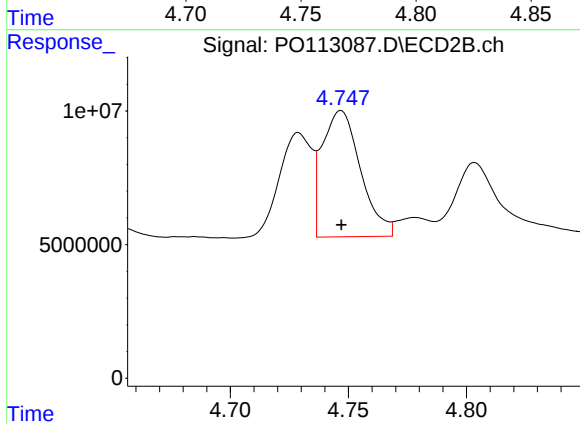

#4 AR-1016-2


R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 53522987
Conc: 207.73 ng/ml

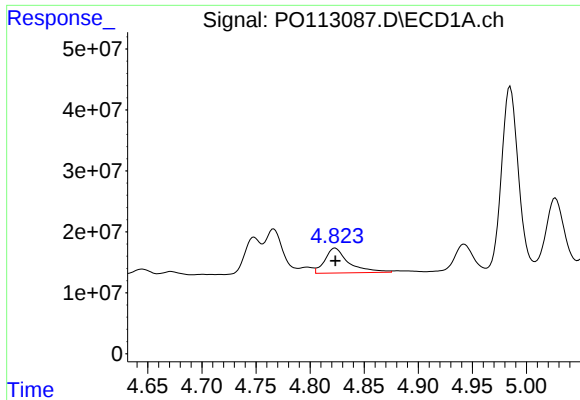

#5 AR-1016-3


R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 62598571
Conc: 245.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

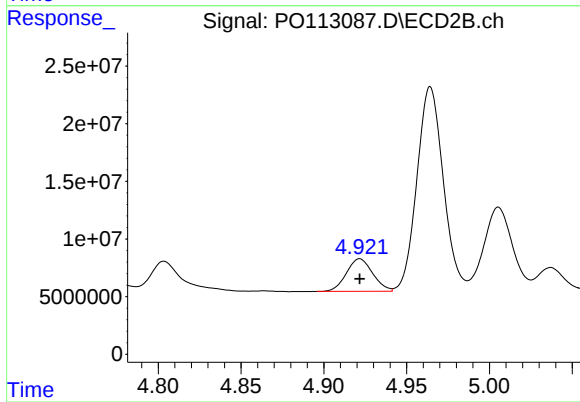


#5 AR-1016-3

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 31393677
Conc: 224.86 ng/ml

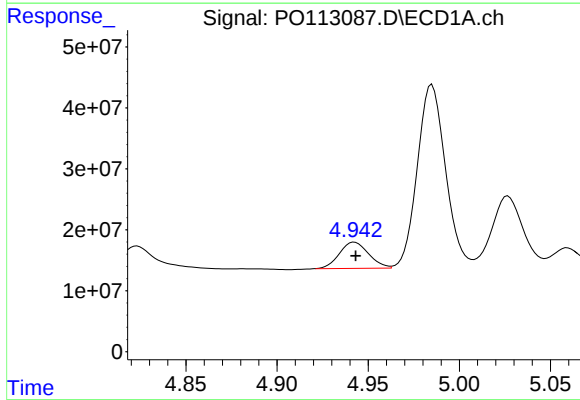


#6 AR-1016-4

R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 48137864
Conc: 220.75 ng/ml

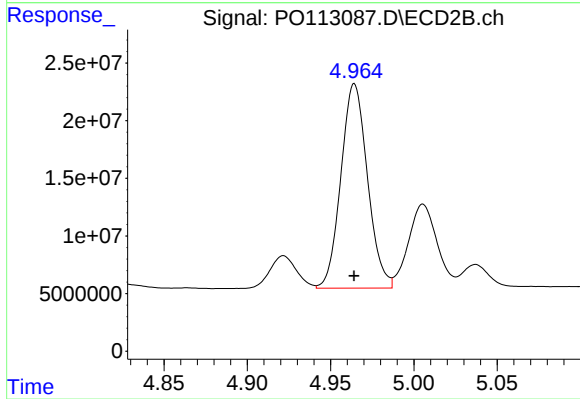

#6 AR-1016-4


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 196887524
Conc: 1687.14 ng/ml

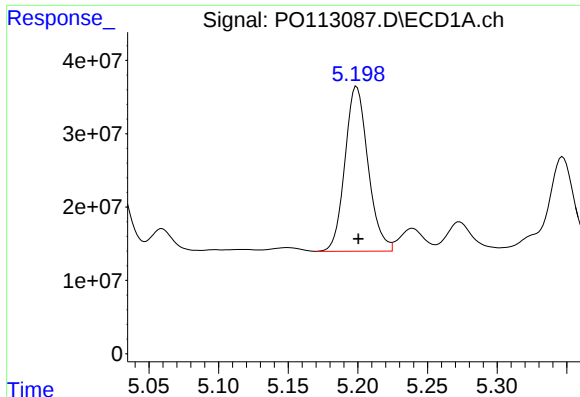

#7 AR-1016-5


R.T.: 5.199 min
Delta R.T.: -0.001 min
Response: 259722575
Conc: 1171.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

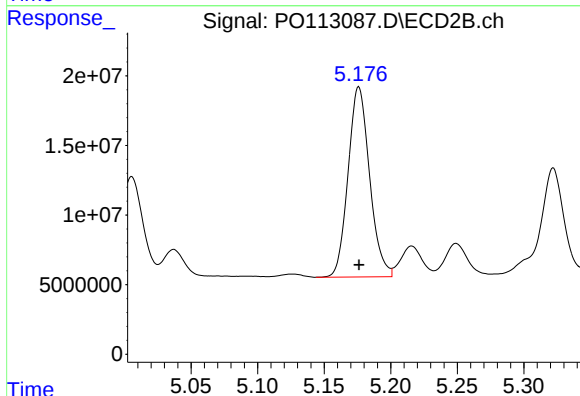


#7 AR-1016-5

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 153612678
Conc: 1077.76 ng/ml

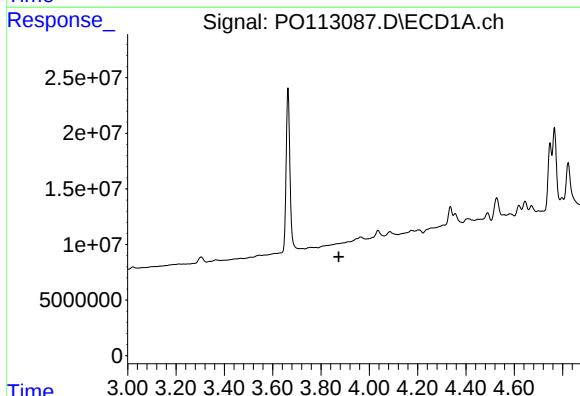


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.

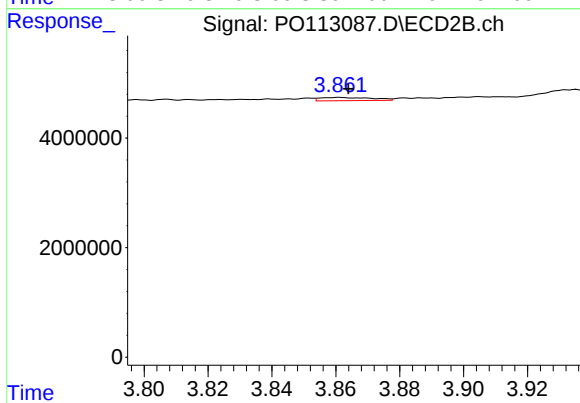

#8 AR-1221-1


R.T.: 3.861 min
Delta R.T.: -0.003 min
Response: 672336
Conc: 10.65 ng/ml

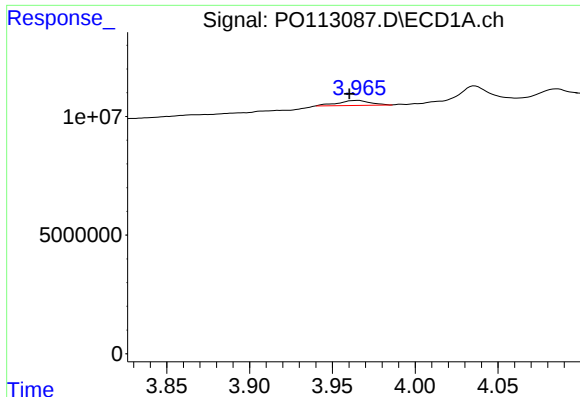

#9 AR-1221-2


R.T.: 3.965 min
Delta R.T.: 0.005 min
Response: 2839727
Conc: 42.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

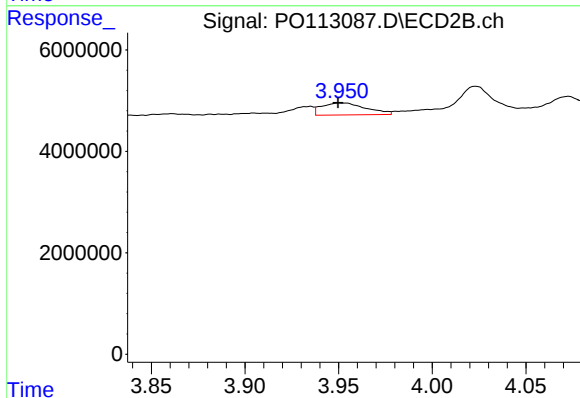


#9 AR-1221-2

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 3873018
Conc: 82.98 ng/ml

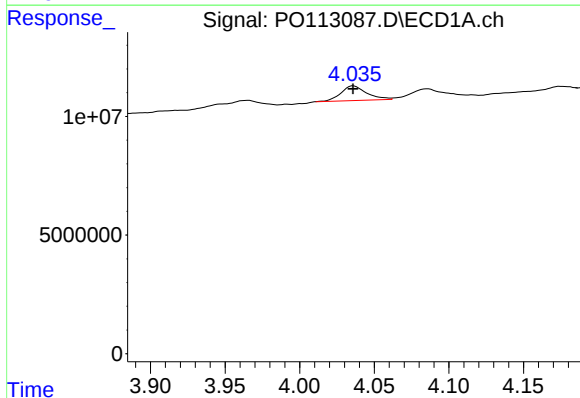


#10 AR-1221-3

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 7368922
Conc: 33.29 ng/ml

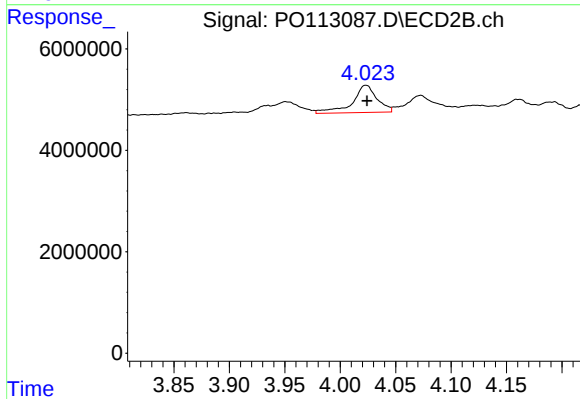

#10 AR-1221-3


R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 8280273
Conc: 55.77 ng/ml

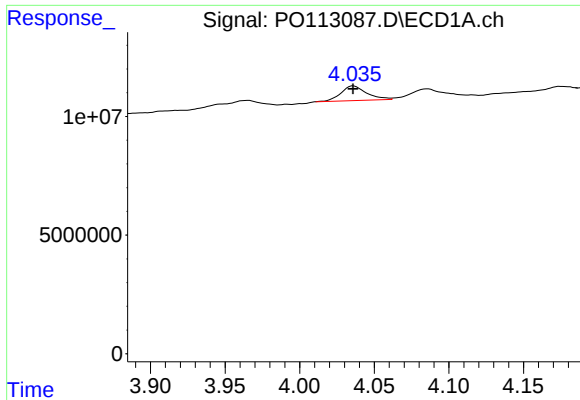

#11 AR-1232-1


R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 7368922
Conc: 42.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

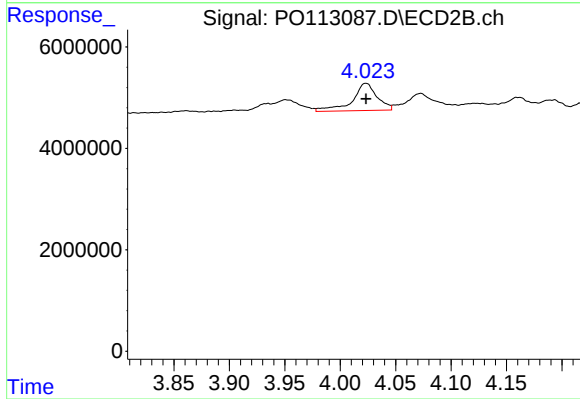


#11 AR-1232-1

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 8280273
Conc: 70.53 ng/ml

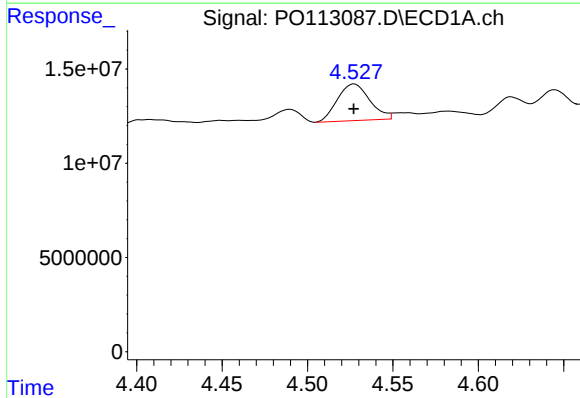


#12 AR-1232-2

R.T.: 4.527 min
Delta R.T.: 0.000 min
Response: 25676297
Conc: 257.14 ng/ml

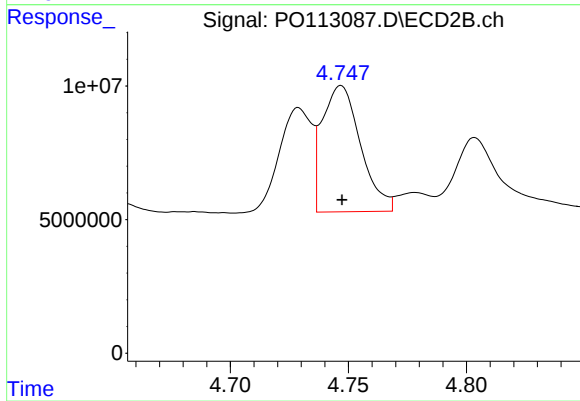

#12 AR-1232-2


R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 53522987
Conc: 436.76 ng/ml

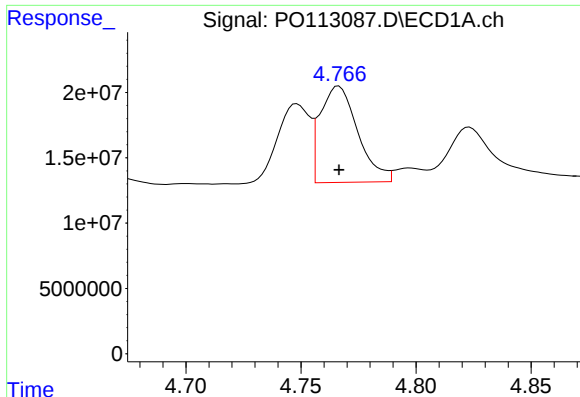

#13 AR-1232-3


R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 84187843
Conc: 444.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

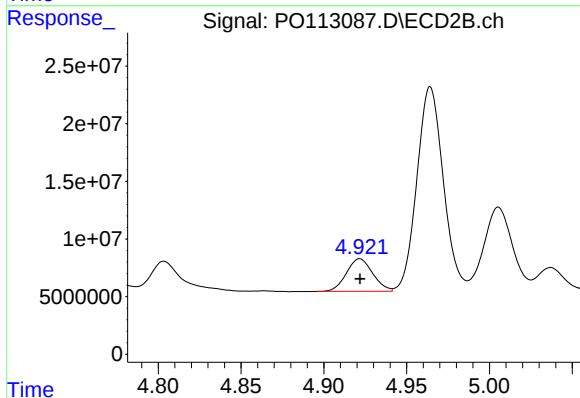


#13 AR-1232-3

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 31393677
Conc: 495.59 ng/ml

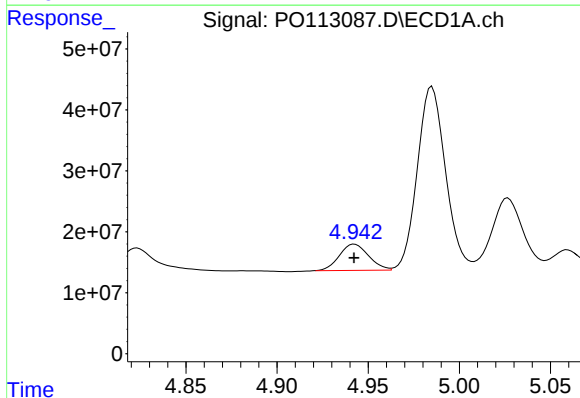


#14 AR-1232-4

R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 48137864
Conc: 511.18 ng/ml

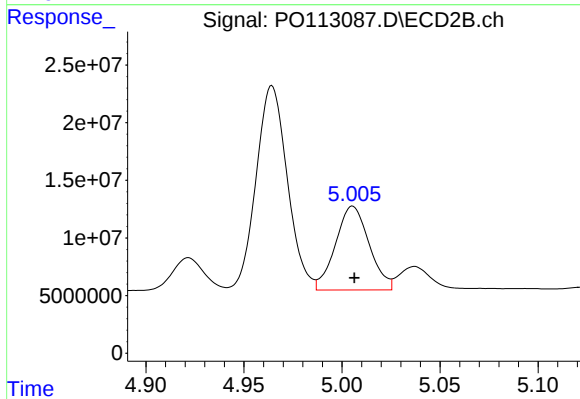

#14 AR-1232-4


R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 87108470
Conc: 1549.39 ng/ml

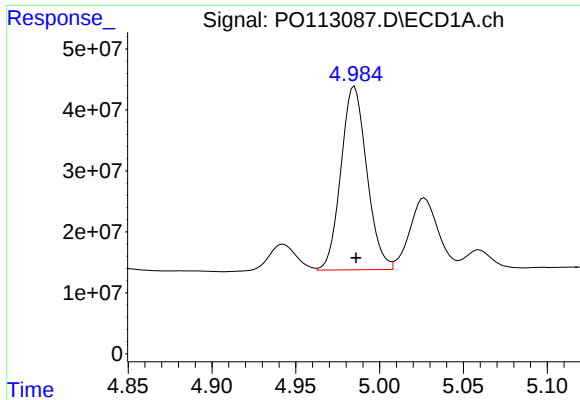

#15 AR-1232-5


R.T.: 4.985 min
Delta R.T.: -0.001 min
Response: 323341285
Conc: 5219.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

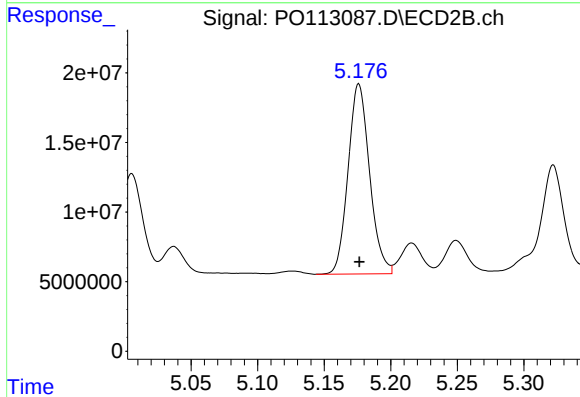


#15 AR-1232-5

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 153612678
Conc: 2566.05 ng/ml

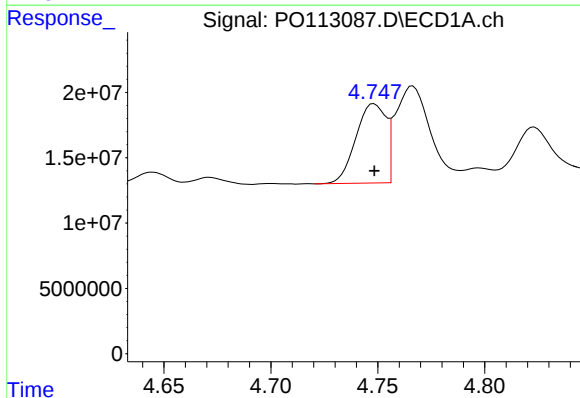


#16 AR-1242-1

R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 59050653
Conc: 256.82 ng/ml

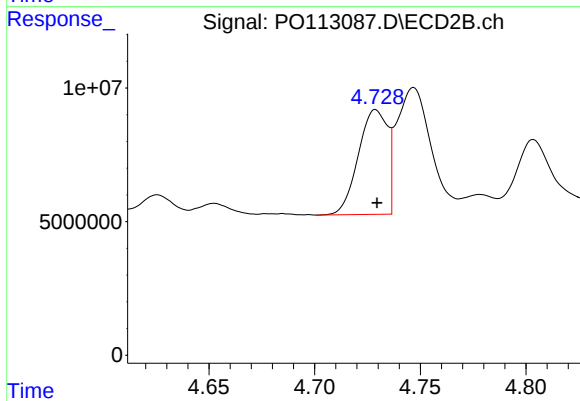

#16 AR-1242-1


R.T.: 4.729 min
Delta R.T.: 0.000 min
Response: 37625352
Conc: 260.38 ng/ml

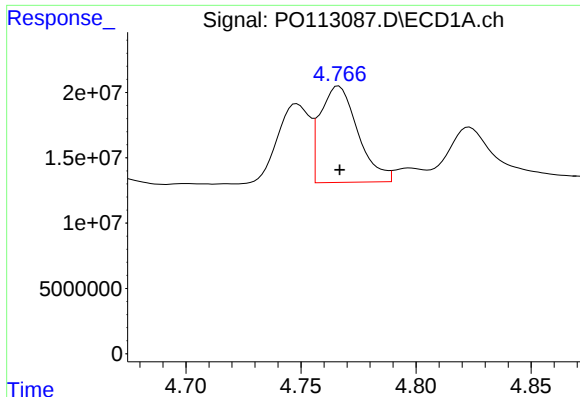

#17 AR-1242-2


R.T.: 4.766 min
Delta R.T.: 0.000 min
Response: 84187843
Conc: 245.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

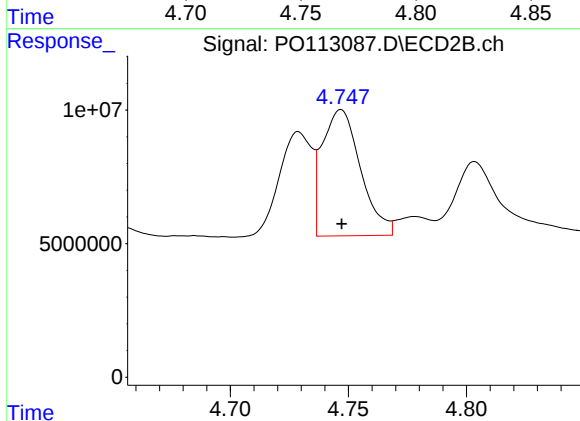


#17 AR-1242-2

R.T.: 4.747 min
Delta R.T.: 0.000 min
Response: 53522987
Conc: 246.75 ng/ml

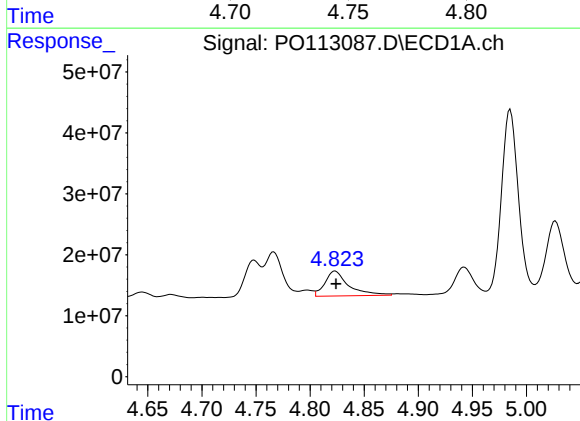


#18 AR-1242-3

R.T.: 4.823 min
Delta R.T.: 0.000 min
Response: 62598571
Conc: 282.12 ng/ml

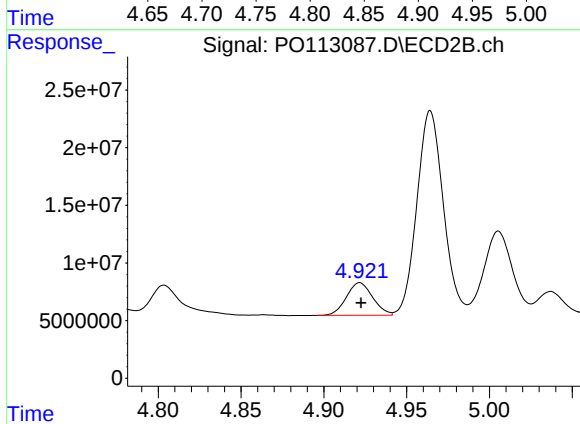

#18 AR-1242-3


R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 31393677
Conc: 268.40 ng/ml

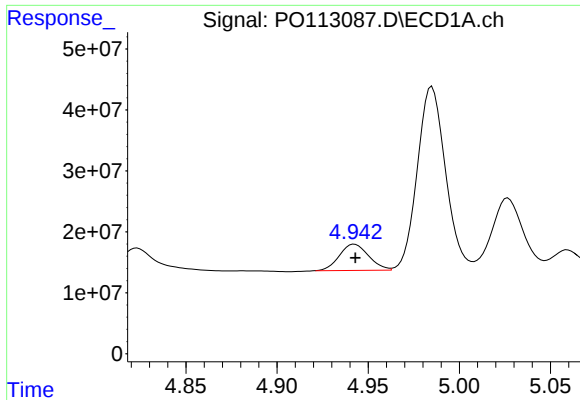

#19 AR-1242-4


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 48137864
Conc: 277.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

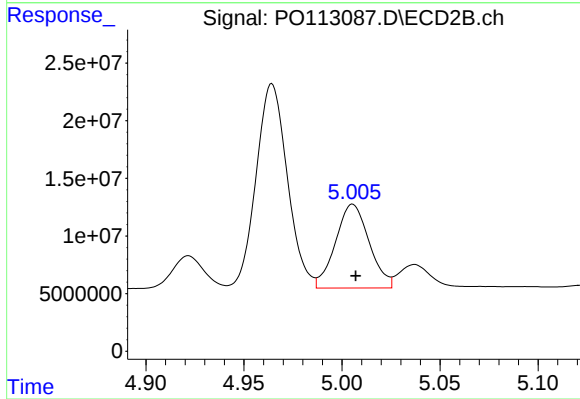


#19 AR-1242-4

R.T.: 5.005 min
Delta R.T.: -0.002 min
Response: 87108470
Conc: 740.48 ng/ml

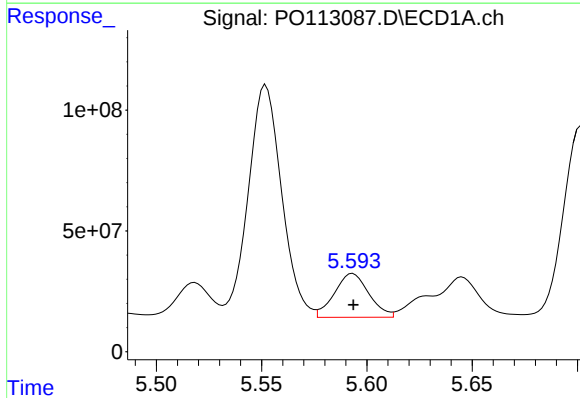


#20 AR-1242-5

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 207272525
Conc: 1035.52 ng/ml

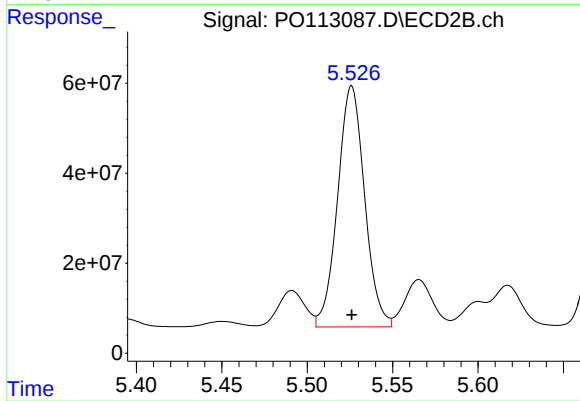

#20 AR-1242-5


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 590163140
Conc: 3957.30 ng/ml

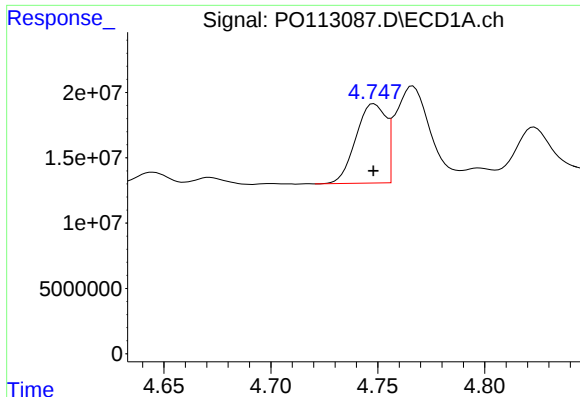

#21 AR-1248-1


R.T.: 4.748 min
Delta R.T.: 0.000 min
Response: 59050653
Conc: 338.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

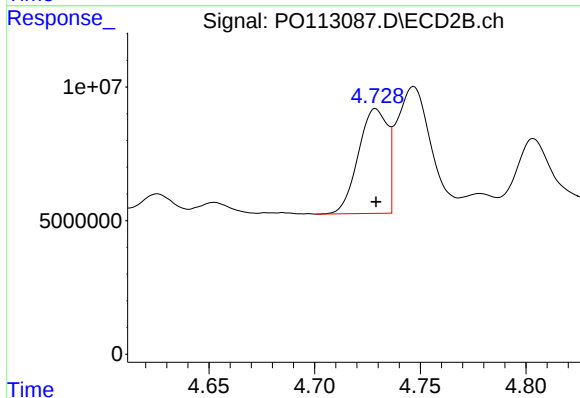


#21 AR-1248-1

R.T.: 4.729 min
Delta R.T.: 0.000 min
Response: 37625352
Conc: 337.41 ng/ml

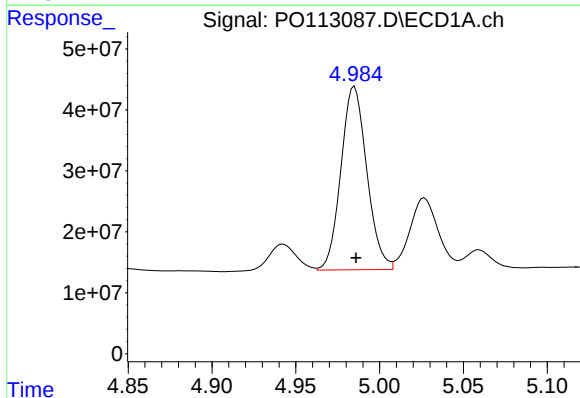


#22 AR-1248-2

R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 323341285
Conc: 1336.86 ng/ml

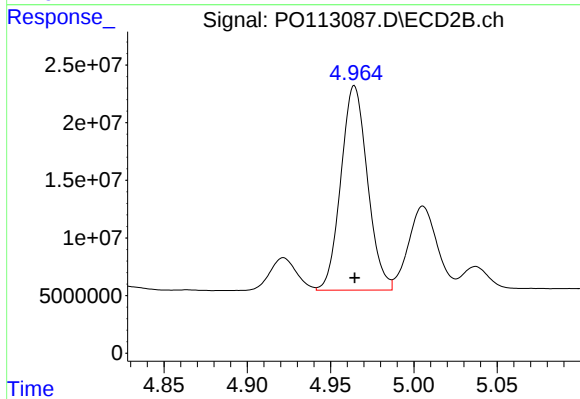

#22 AR-1248-2


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 196887524
Conc: 1225.19 ng/ml

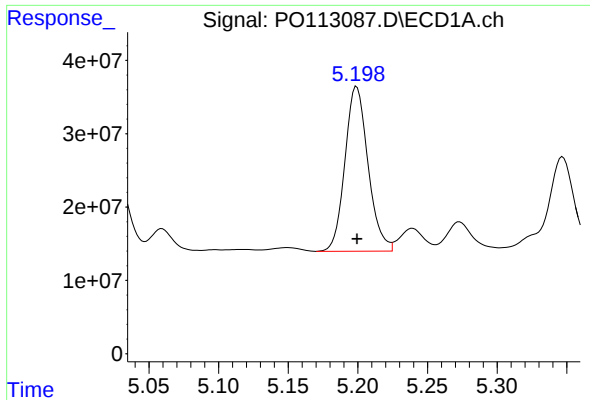

#23 AR-1248-3


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 259722575
Conc: 814.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

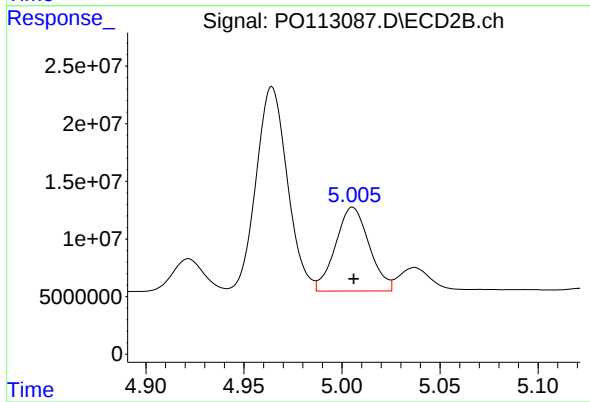


#23 AR-1248-3

R.T.: 5.005 min
Delta R.T.: 0.000 min
Response: 87108470
Conc: 513.43 ng/ml

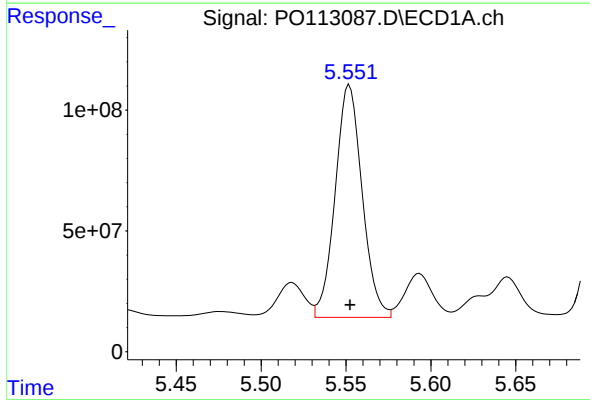


#24 AR-1248-4

R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 1063436514
Conc: 2128.56 ng/ml

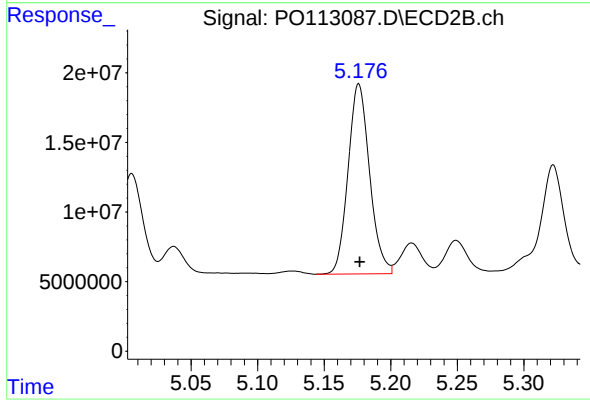

#24 AR-1248-4


R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 153612678
Conc: 771.07 ng/ml

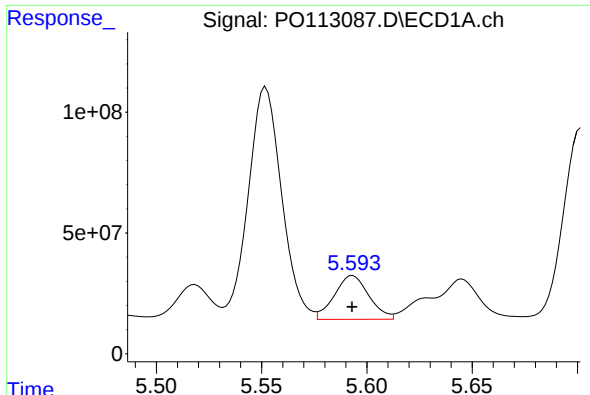

#25 AR-1248-5


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 207272525
Conc: 606.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

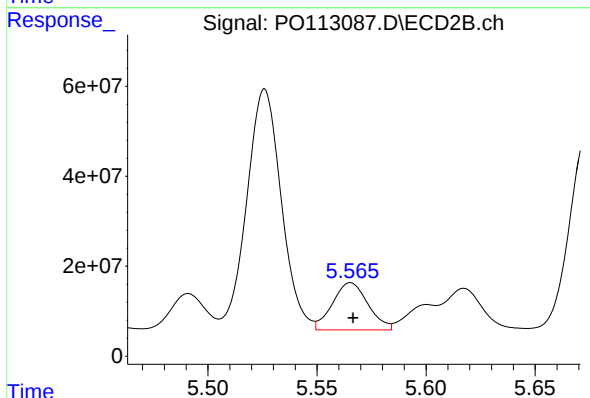


#25 AR-1248-5

R.T.: 5.565 min
Delta R.T.: -0.001 min
Response: 119110620
Conc: 561.06 ng/ml

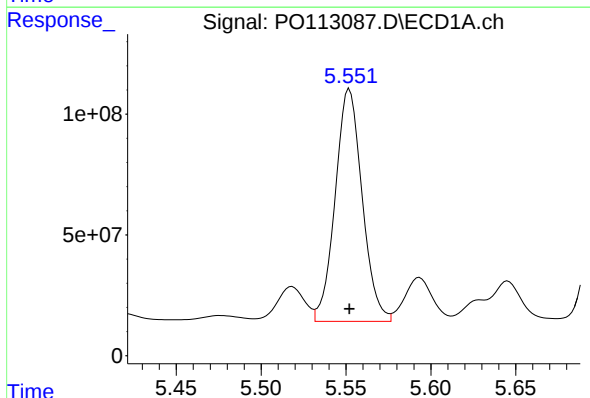


#26 AR-1254-1

R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 1063436514
Conc: 1969.41 ng/ml

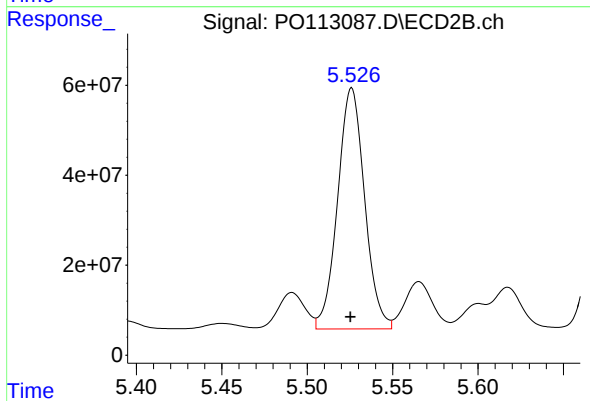

#26 AR-1254-1


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 590163140
Conc: 1871.43 ng/ml

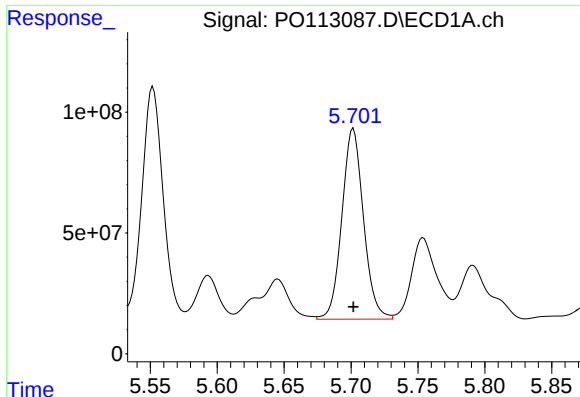

#27 AR-1254-2


R.T.: 5.702 min
Delta R.T.: 0.000 min
Response: 888143715
Conc: 1799.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

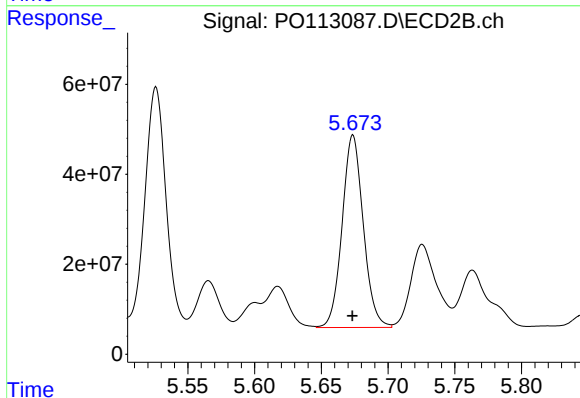


#27 AR-1254-2

R.T.: 5.674 min
Delta R.T.: 0.000 min
Response: 472248520
Conc: 1684.56 ng/ml

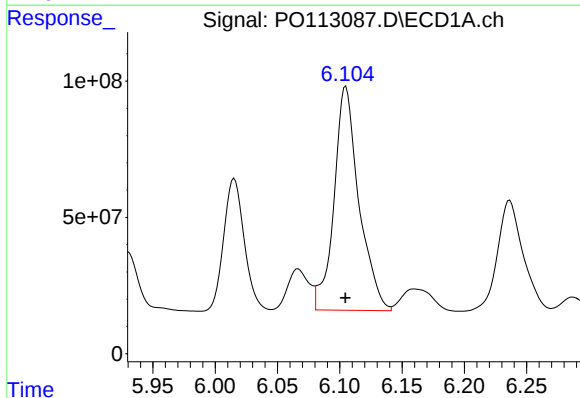


#28 AR-1254-3

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 1144559922
Conc: 1549.05 ng/ml

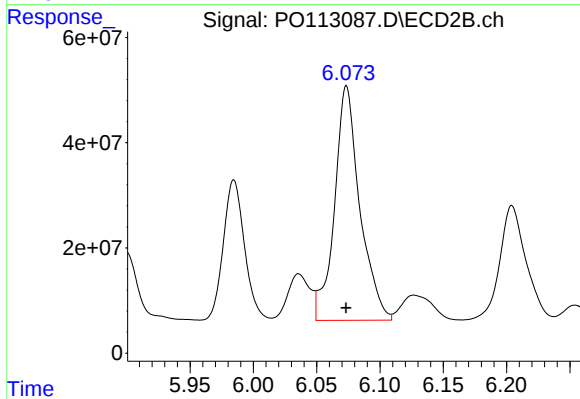

#28 AR-1254-3


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 620202452
Conc: 1487.57 ng/ml

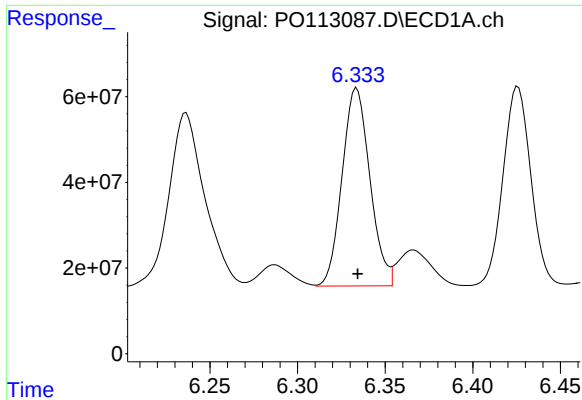

#29 AR-1254-4


R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 511115359
Conc: 917.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

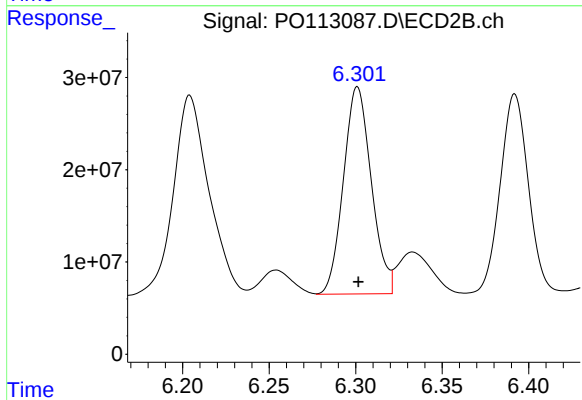


#29 AR-1254-4

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 251570055
Conc: 915.35 ng/ml

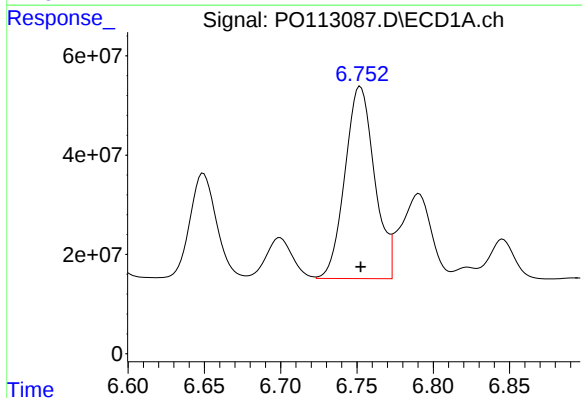


#30 AR-1254-5

R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 522304067
Conc: 745.11 ng/ml

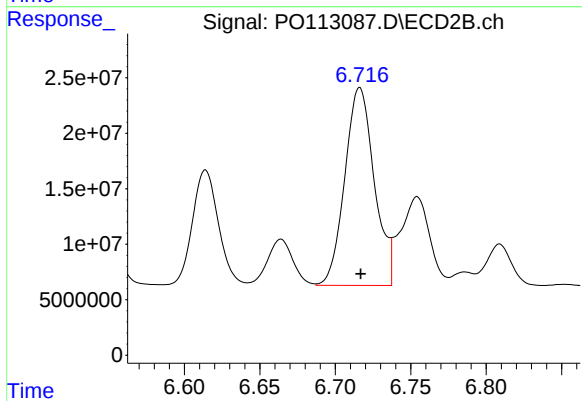

#30 AR-1254-5


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 242840084
Conc: 679.29 ng/ml

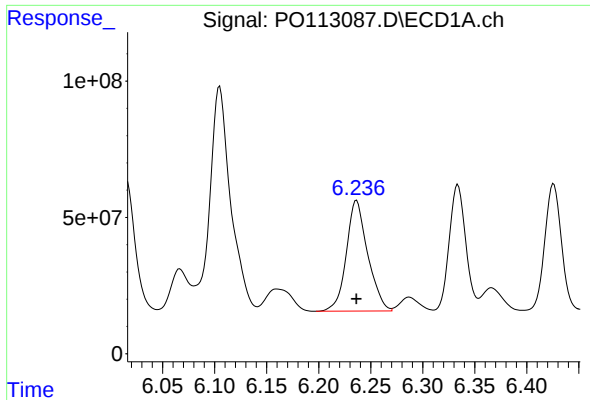

#31 AR-1260-1


R.T.: 6.236 min
Delta R.T.: 0.000 min
Response: 581740526
Conc: 1304.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

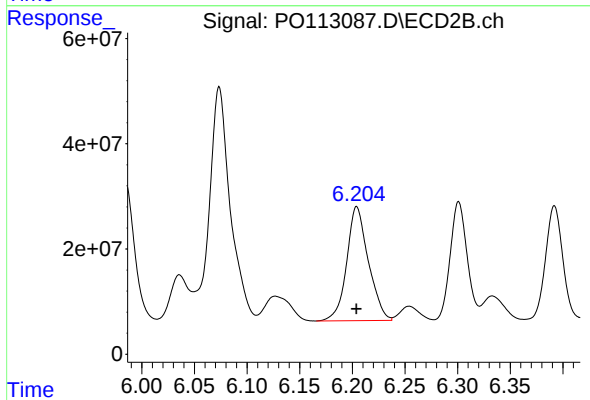


#31 AR-1260-1

R.T.: 6.204 min
Delta R.T.: 0.000 min
Response: 310583232
Conc: 1217.64 ng/ml

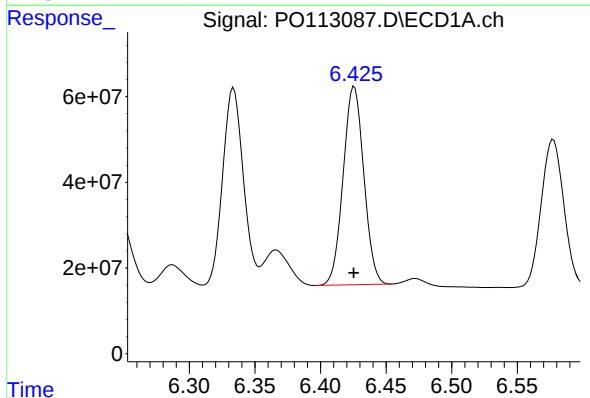


#32 AR-1260-2

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 507236421
Conc: 738.64 ng/ml

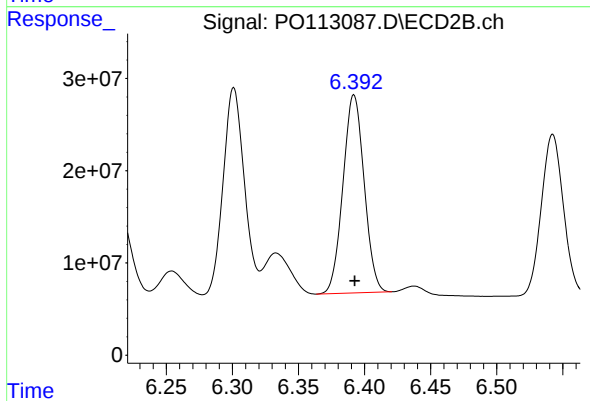

#32 AR-1260-2


R.T.: 6.392 min
Delta R.T.: 0.000 min
Response: 239335242
Conc: 692.30 ng/ml

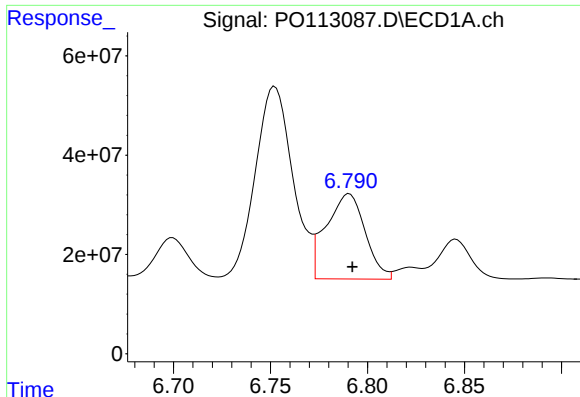

#33 AR-1260-3


R.T.: 6.791 min
Delta R.T.: -0.002 min
Response: 240108246
Conc: 388.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

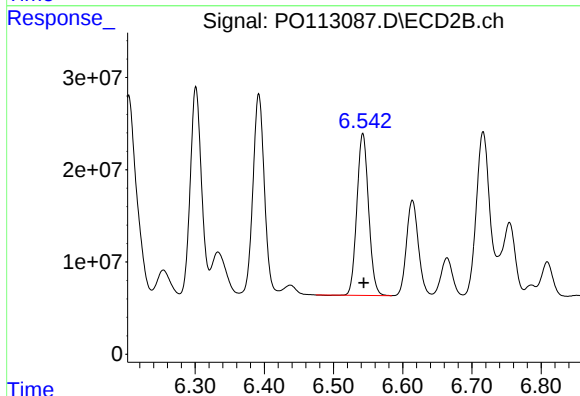


#33 AR-1260-3

R.T.: 6.542 min
Delta R.T.: -0.001 min
Response: 206217611
Conc: 693.32 ng/ml

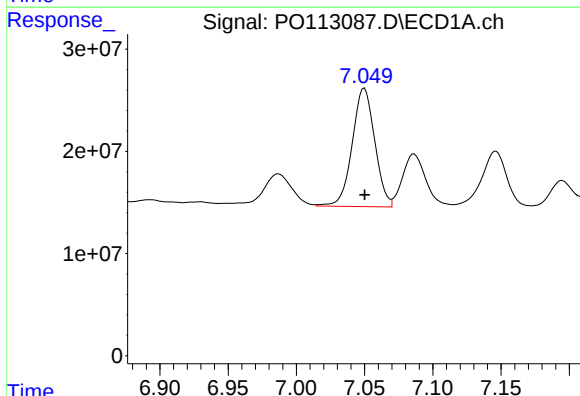


#34 AR-1260-4

R.T.: 7.050 min
Delta R.T.: 0.000 min
Response: 133401965
Conc: 297.86 ng/ml

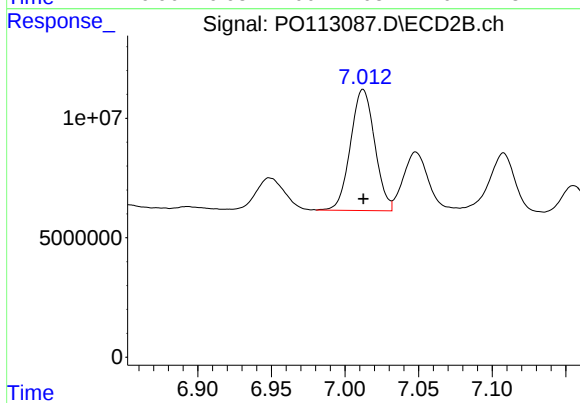

#34 AR-1260-4


R.T.: 7.012 min
Delta R.T.: 0.000 min
Response: 58110377
Conc: 280.39 ng/ml

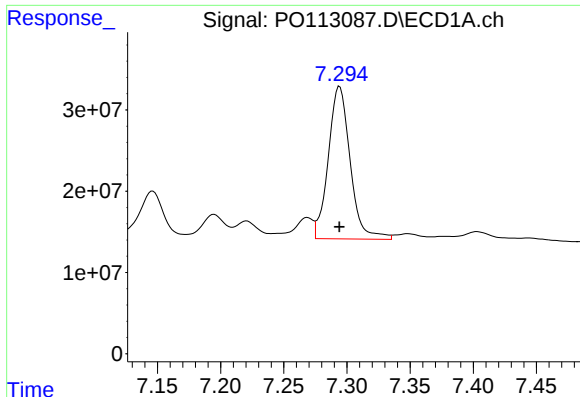

#35 AR-1260-5


R.T.: 7.294 min
Delta R.T.: 0.000 min
Response: 226510318
Conc: 187.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

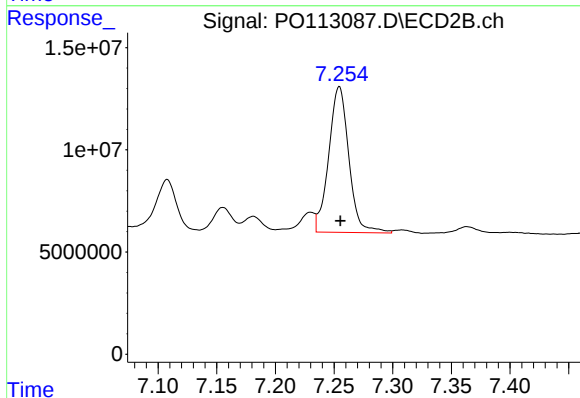


#35 AR-1260-5

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 85277853
Conc: 182.05 ng/ml

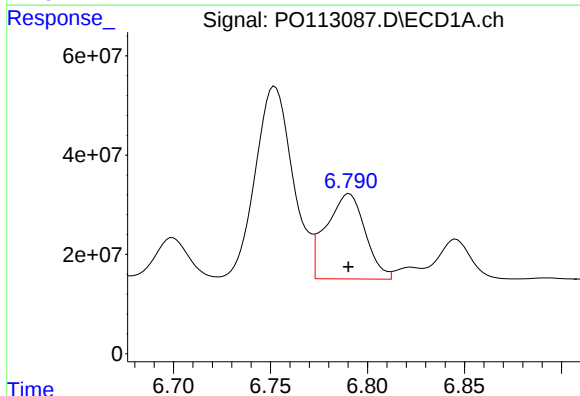


#36 AR-1262-1

R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 240108246
Conc: 262.19 ng/ml

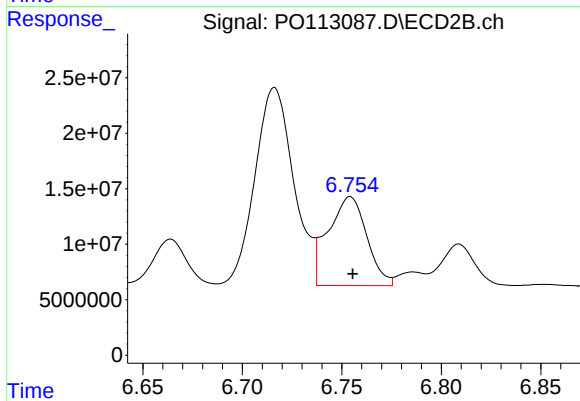

#36 AR-1262-1


R.T.: 6.754 min
Delta R.T.: -0.001 min
Response: 108443345
Conc: 261.55 ng/ml

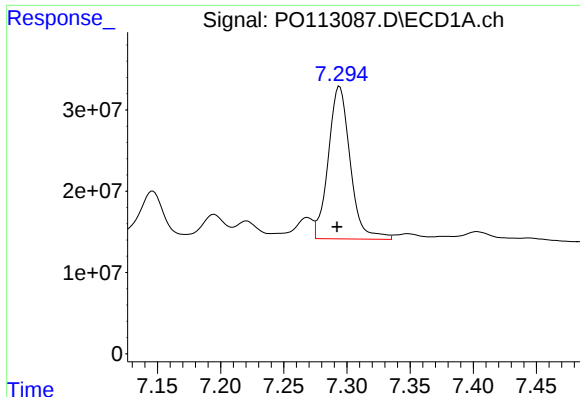

#37 AR-1262-2


R.T.: 7.294 min
Delta R.T.: 0.002 min
Response: 226510318
Conc: 149.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

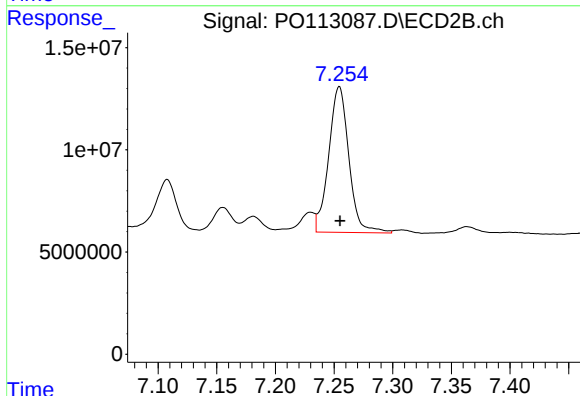


#37 AR-1262-2

R.T.: 7.254 min
Delta R.T.: 0.000 min
Response: 85277853
Conc: 164.73 ng/ml

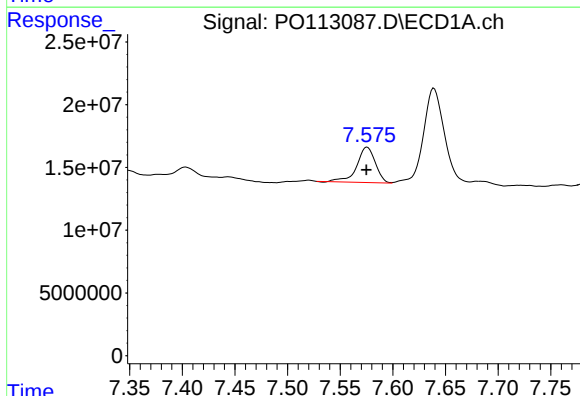


#38 AR-1262-3

R.T.: 7.576 min
Delta R.T.: 0.000 min
Response: 34477105
Conc: 62.22 ng/ml

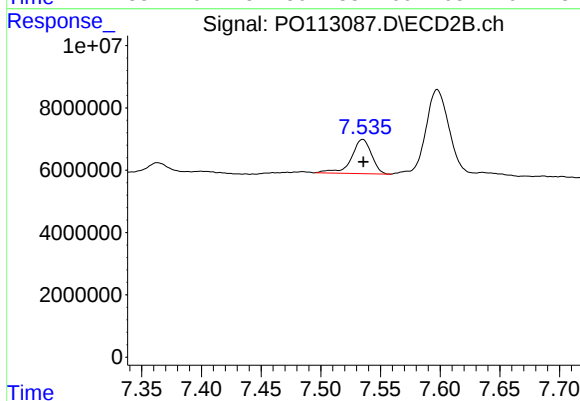

#38 AR-1262-3


R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 12823012
Conc: 71.40 ng/ml

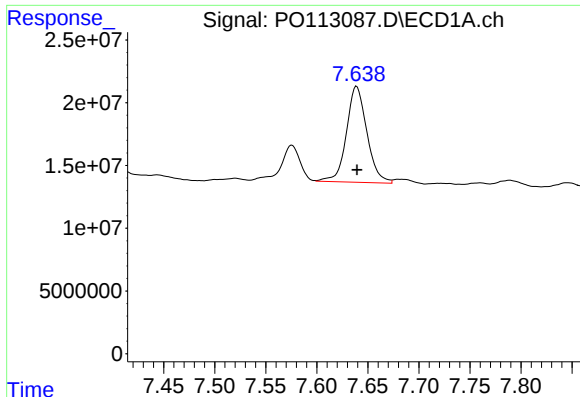

#39 AR-1262-4


R.T.: 7.639 min
Delta R.T.: 0.000 min
Response: 106654295
Conc: 109.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

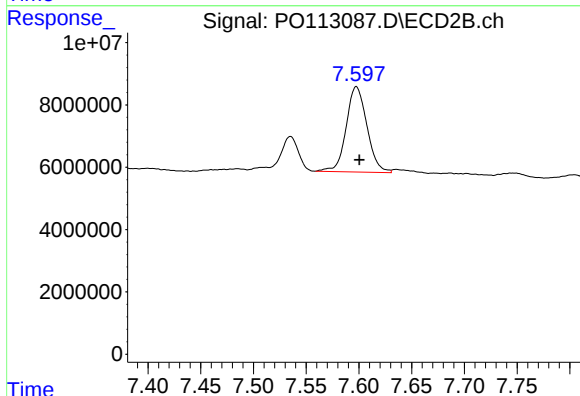


#39 AR-1262-4

R.T.: 7.598 min
Delta R.T.: -0.003 min
Response: 37415439
Conc: 129.06 ng/ml

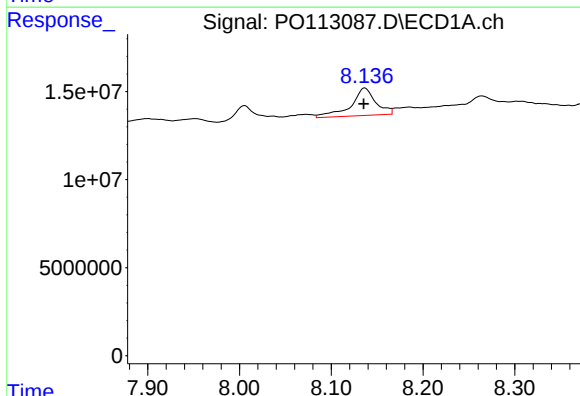


#40 AR-1262-5

R.T.: 8.137 min
Delta R.T.: 0.001 min
Response: 29195179
Conc: 70.03 ng/ml

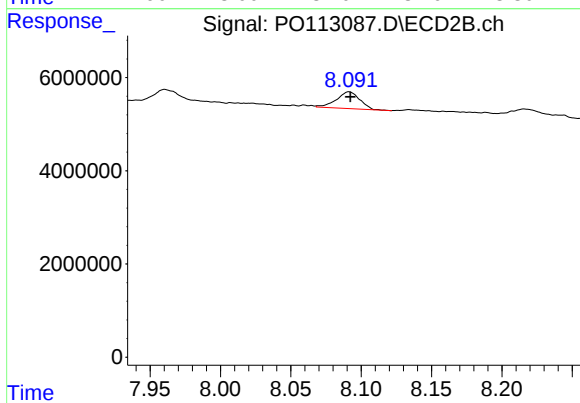

#40 AR-1262-5


R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 4146477
Conc: 38.28 ng/ml

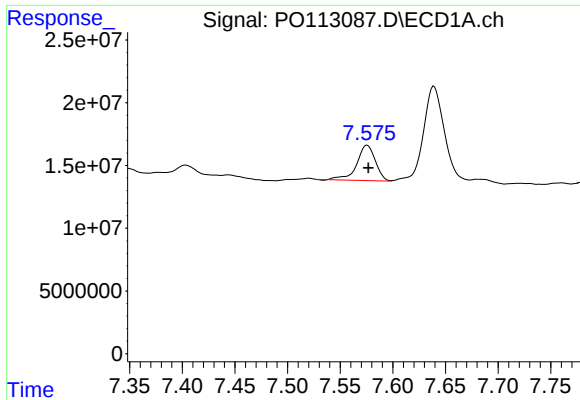

#41 AR-1268-1


R.T.: 7.576 min
Delta R.T.: -0.001 min
Response: 34477105
Conc: 20.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

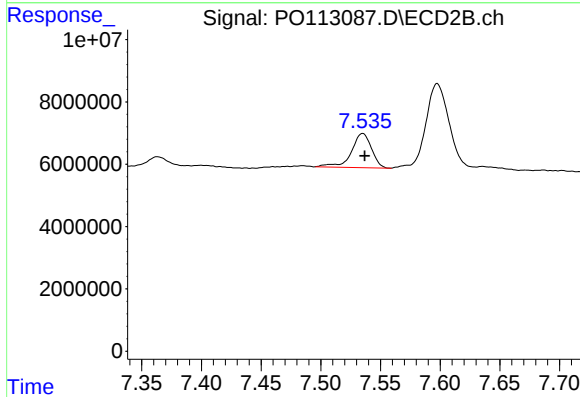


#41 AR-1268-1

R.T.: 7.535 min
Delta R.T.: -0.002 min
Response: 12823012
Conc: 25.17 ng/ml

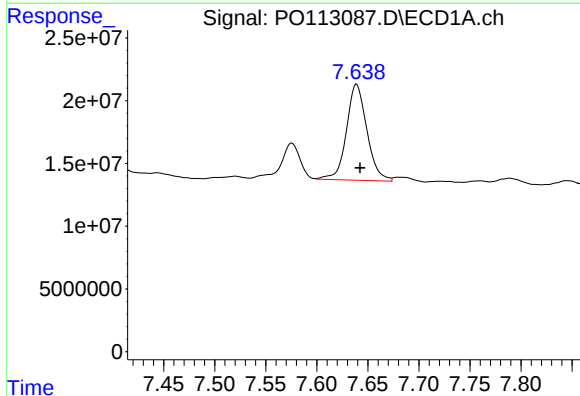


#42 AR-1268-2

R.T.: 7.639 min
Delta R.T.: -0.003 min
Response: 106654295
Conc: 73.65 ng/ml

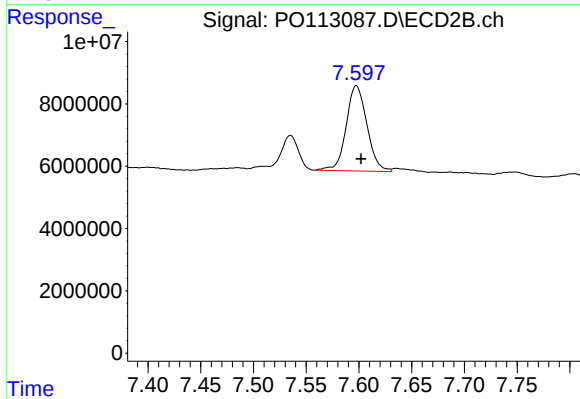

#42 AR-1268-2


R.T.: 7.598 min
Delta R.T.: -0.004 min
Response: 37415439
Conc: 90.07 ng/ml

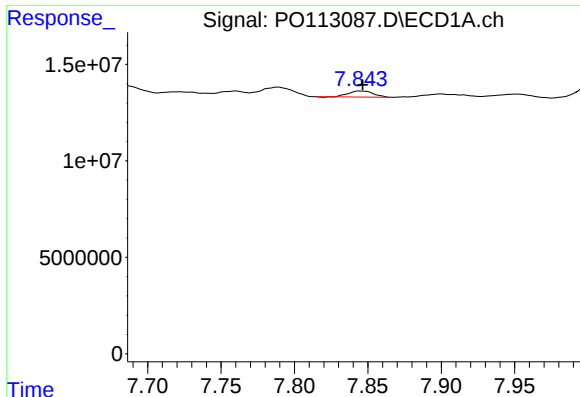

#43 AR-1268-3


R.T.: 7.845 min
Delta R.T.: -0.002 min
Response: 3726937
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

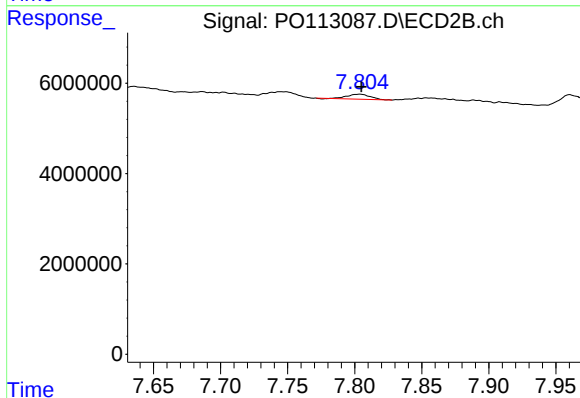


#43 AR-1268-3

R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 1300165
Conc: 3.98 ng/ml

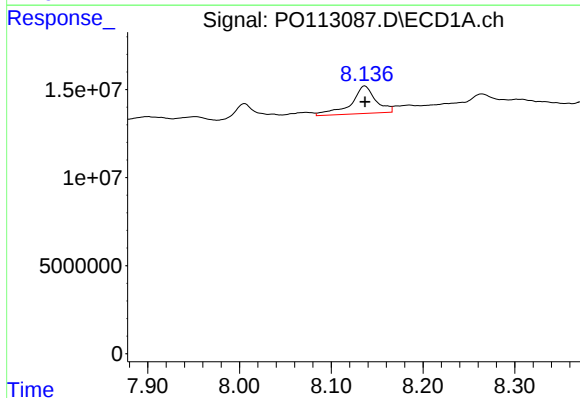


#44 AR-1268-4

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 29195179
Conc: 63.38 ng/ml

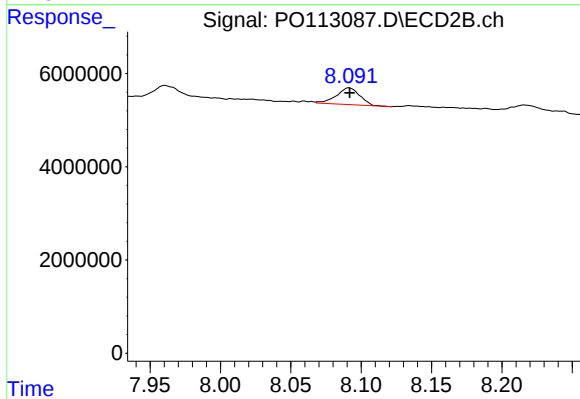

#44 AR-1268-4


R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 4146477
Conc: 34.43 ng/ml

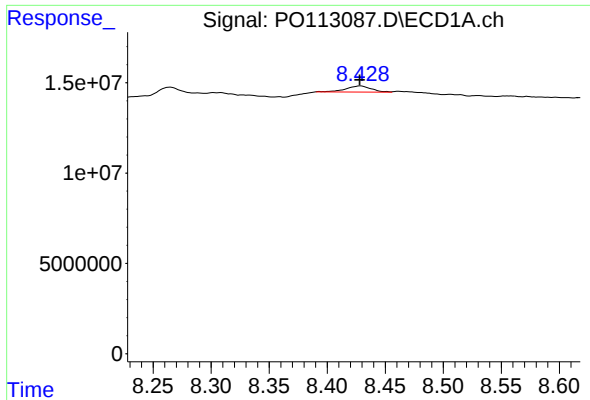

#45 AR-1268-5

R.T.: 8.429 min
Delta R.T.: 0.000 min
Response: 5183173
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANT

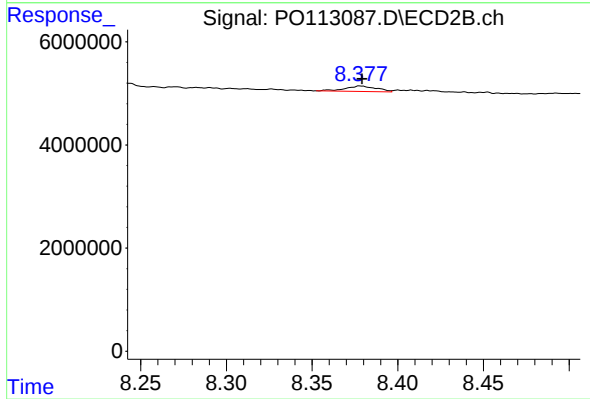

#45 AR-1268-5

R.T.: 8.378 min
Delta R.T.: 0.000 min
Response: 1333447
Conc: 1.71 ng/ml