

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : P0113083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 12:55
 Operator : YP/AJ
 Sample : Q2894-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2A2B2C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2025
 Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 13:41:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.655	166.5E6	100.9E6	20.333m	19.945m
2) SA Decachlor...	8.681	8.627	136.7E6	39511998	19.723	20.852

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 12:55
Operator : YP/AJ
Sample : Q2894-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2A2B2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 13:41:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

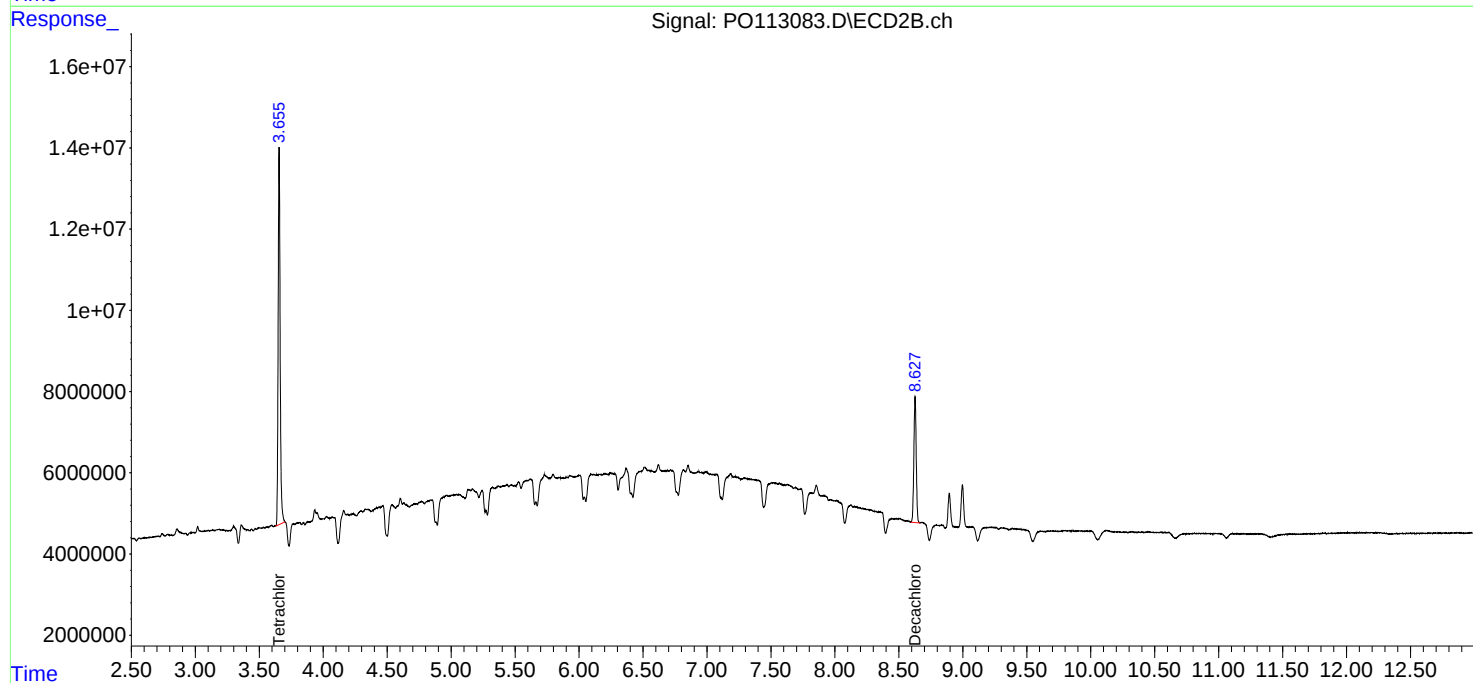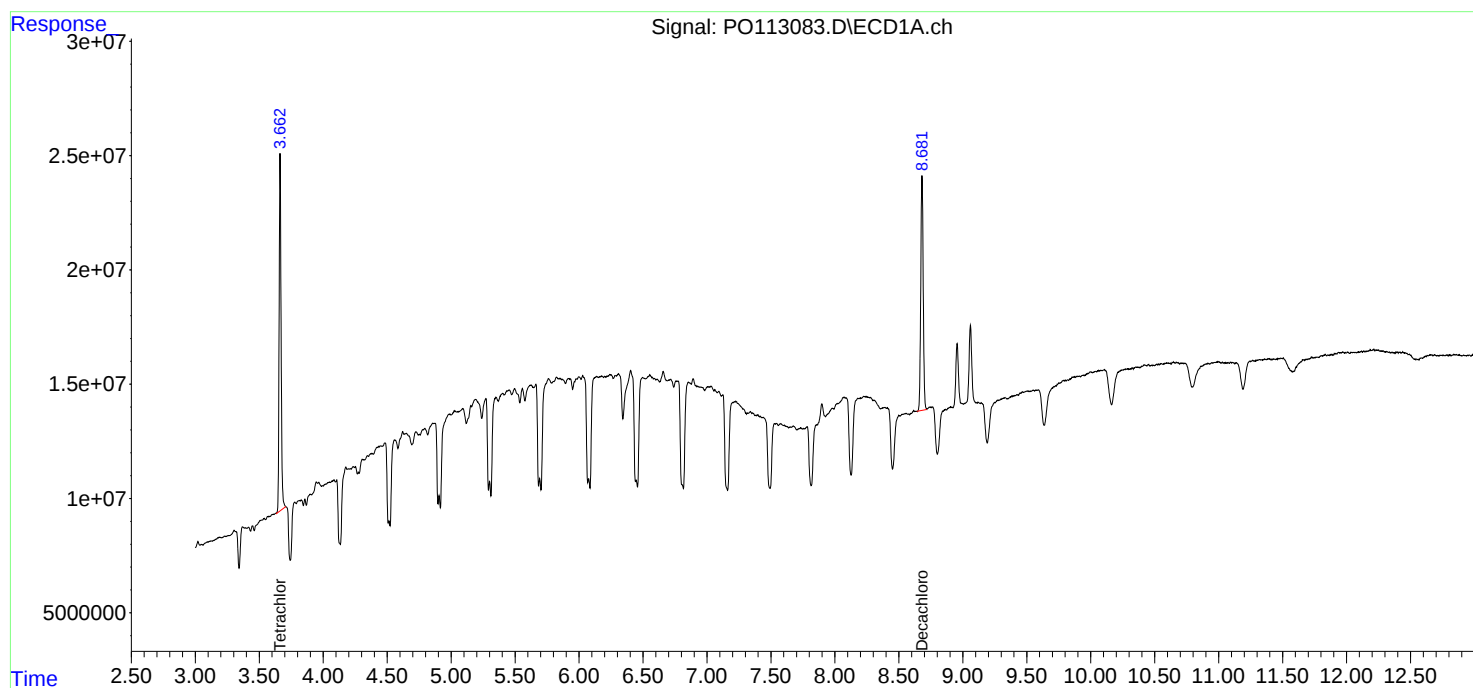

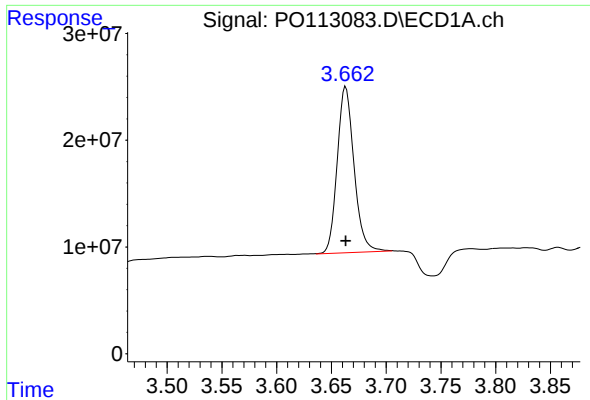


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 166459673
Conc: 20.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
2A2B2C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2025
Supervised By :mohammad ahmed 08/22/2025

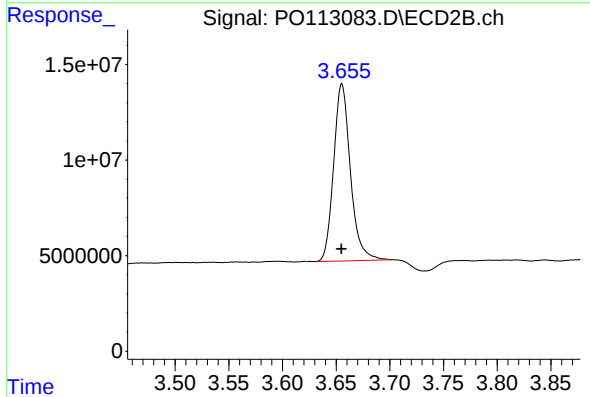


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: 0.000 min
Response: 100936502
Conc: 19.95 ng/ml m

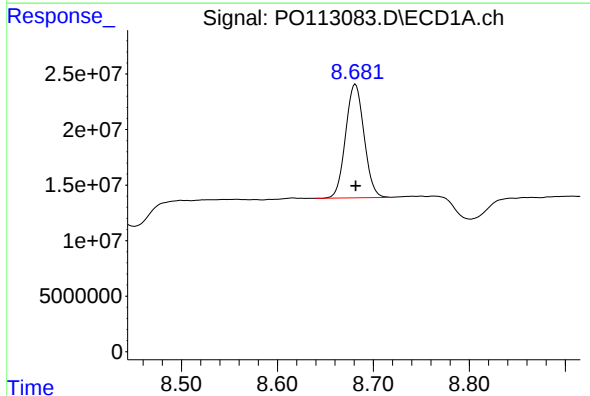

#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 136711602
Conc: 19.72 ng/ml

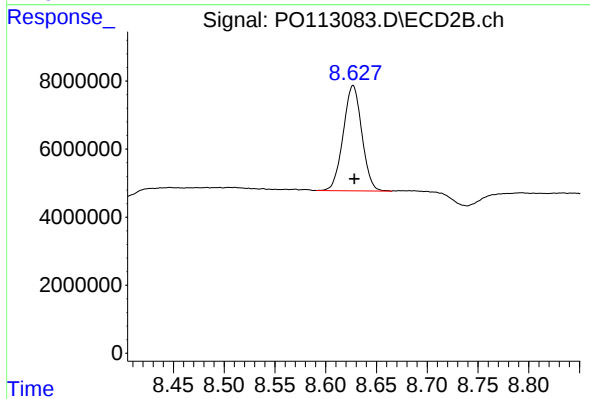

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.001 min
Response: 39511998
Conc: 20.85 ng/ml