

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082025\
 Data File : P0113109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 22:55
 Operator : YP/AJ
 Sample : Q2901-01DL 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HVAC DUCT SEALANTDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:44:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.662	3.653	25968704	16094505	3.172	3.180
2)	SA Decachlor...	8.681	8.626	21081195	6213264	3.041	3.279
Target Compounds							
26)	L6 AR-1254-1	5.551	5.525	190.4E6	111.3E6	352.535	352.856
27)	L6 AR-1254-2	5.701	5.672	158.2E6	91476947	320.551	326.308
28)	L6 AR-1254-3	6.104	6.072	192.9E6	113.0E6	261.091	270.999
29)	L6 AR-1254-4	6.332	6.300	76933925	42240494	138.122	153.694
30)	L6 AR-1254-5	6.751	6.716	85938804	43646545	122.599	122.091


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082025\
Data File : PO113109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 22:55
Operator : YP/AJ
Sample : Q2901-01DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANTDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:44:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

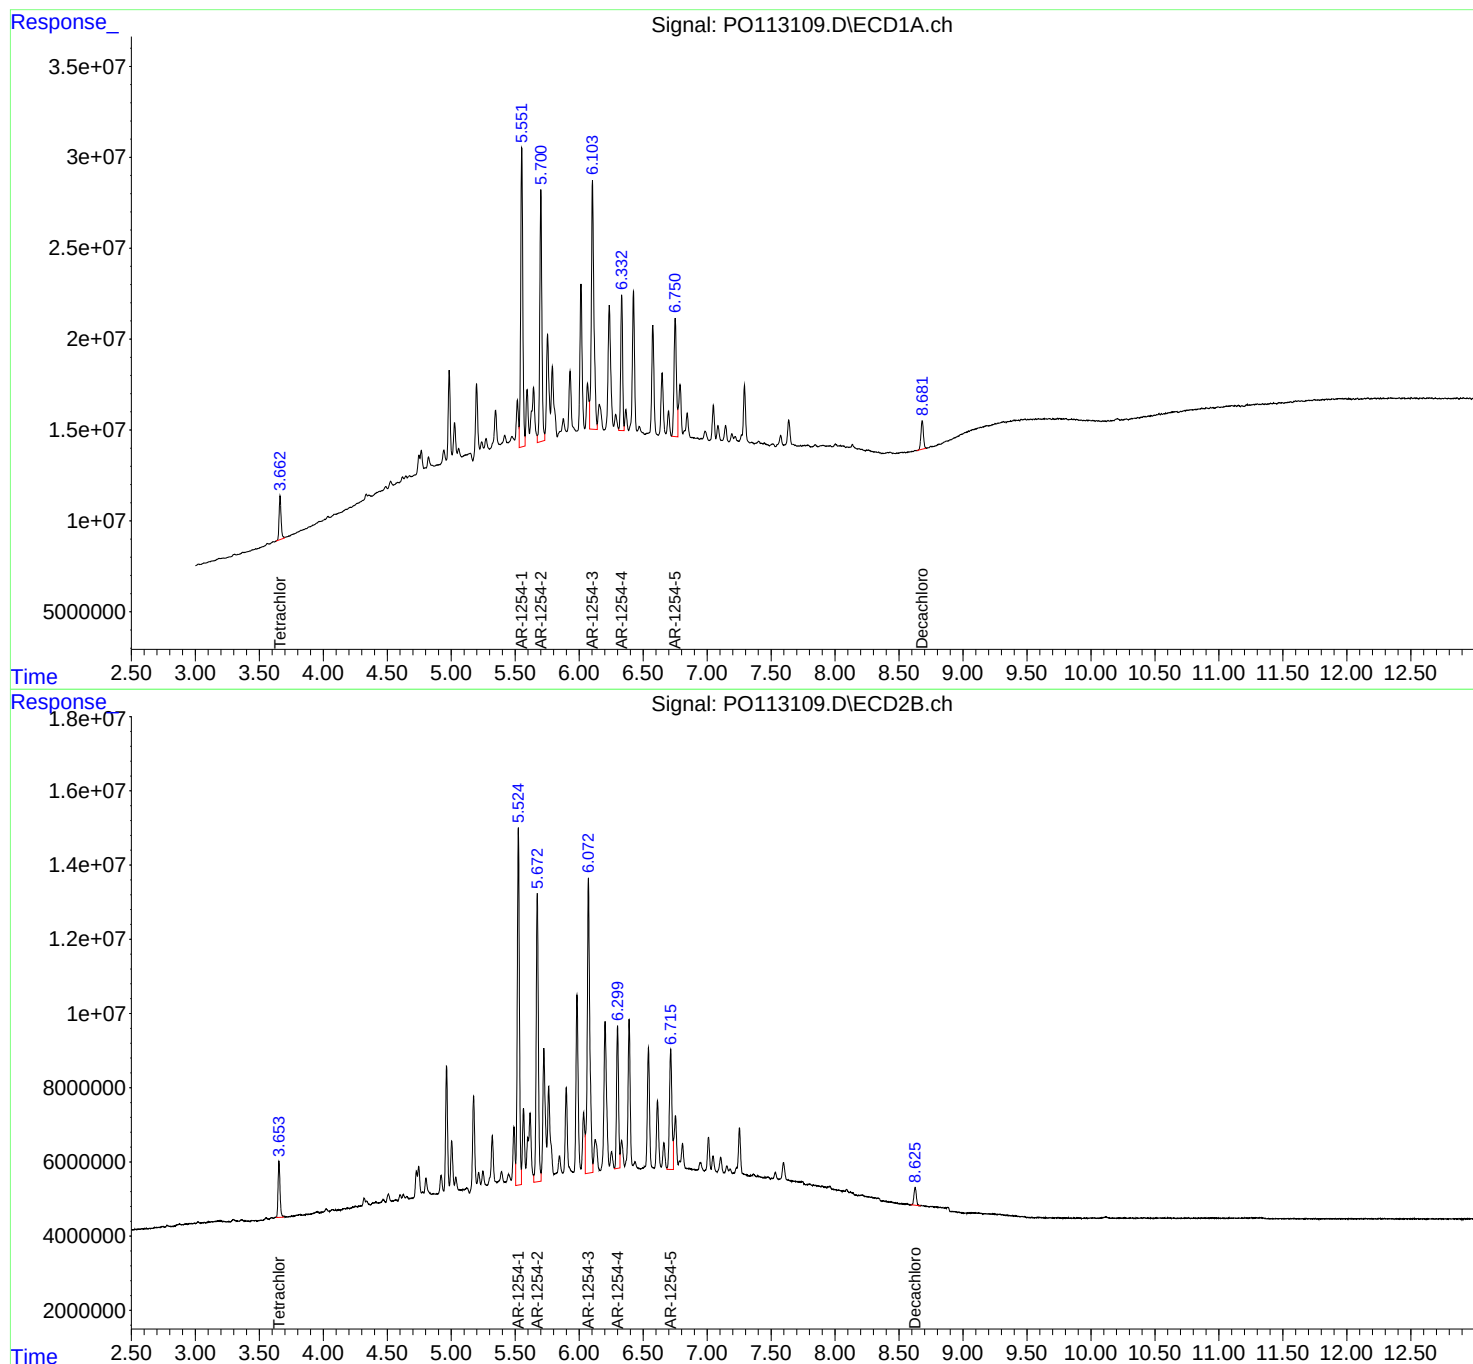


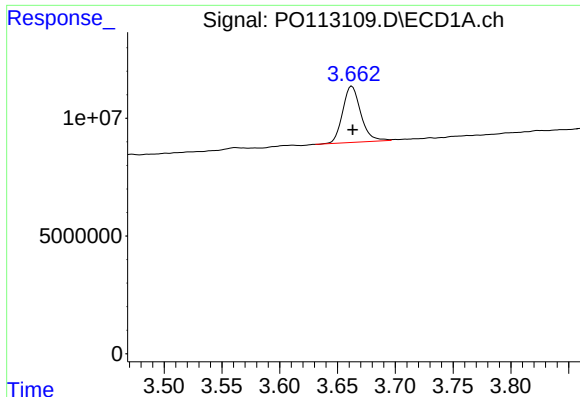

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 25968704
Conc: 3.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANTDL

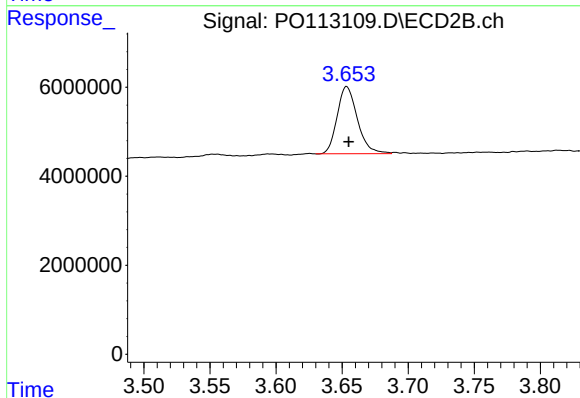


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.001 min
Response: 16094505
Conc: 3.18 ng/ml

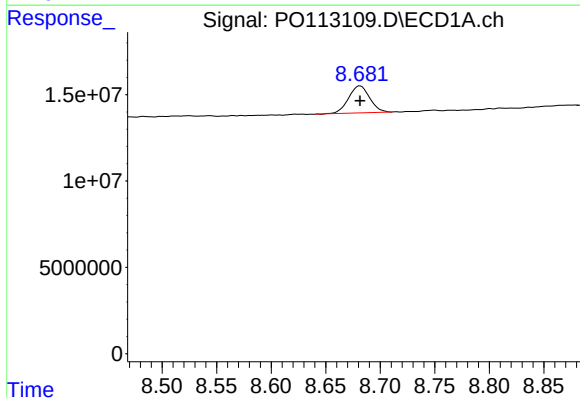


#2 Decachlorobiphenyl

R.T.: 8.681 min
Delta R.T.: 0.000 min
Response: 21081195
Conc: 3.04 ng/ml

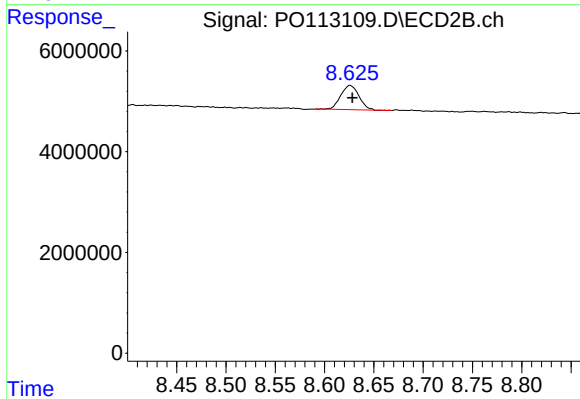

#2 Decachlorobiphenyl


R.T.: 8.626 min
Delta R.T.: -0.002 min
Response: 6213264
Conc: 3.28 ng/ml

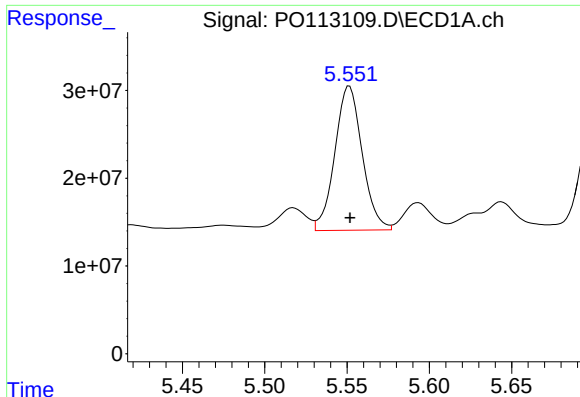

#26 AR-1254-1


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 190361051
Conc: 352.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANTDL

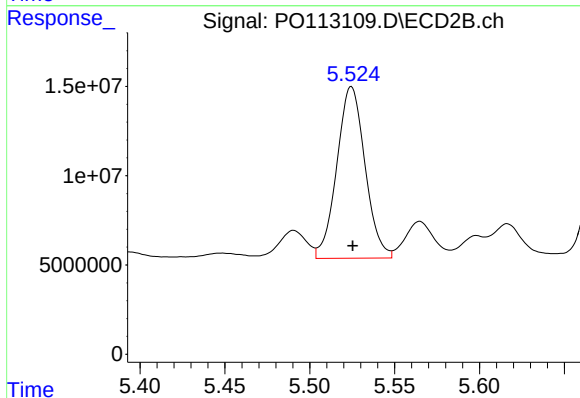


#26 AR-1254-1

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 111274594
Conc: 352.86 ng/ml

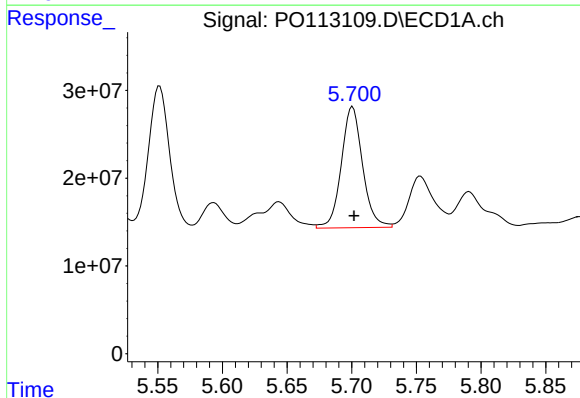


#27 AR-1254-2

R.T.: 5.701 min
Delta R.T.: -0.001 min
Response: 158177399
Conc: 320.55 ng/ml

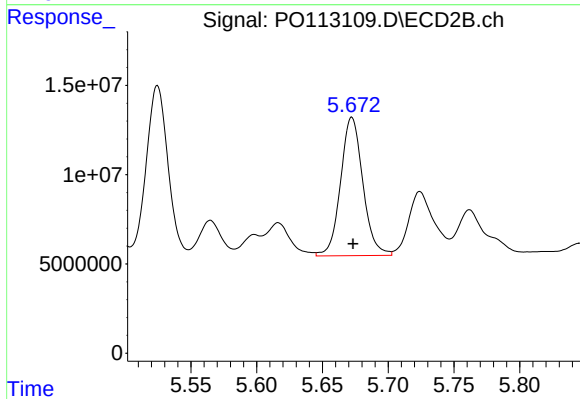

#27 AR-1254-2


R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 91476947
Conc: 326.31 ng/ml

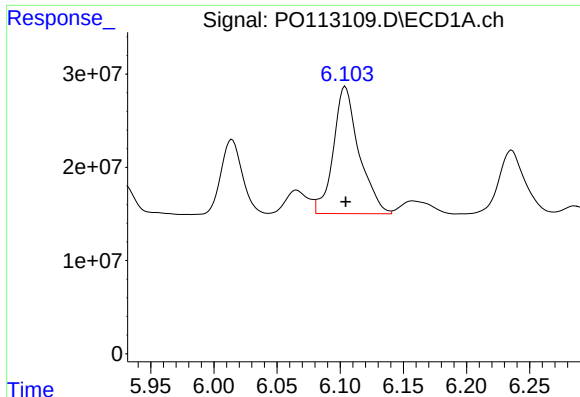

#28 AR-1254-3


R.T.: 6.104 min
Delta R.T.: 0.000 min
Response: 192914354
Conc: 261.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANTDL

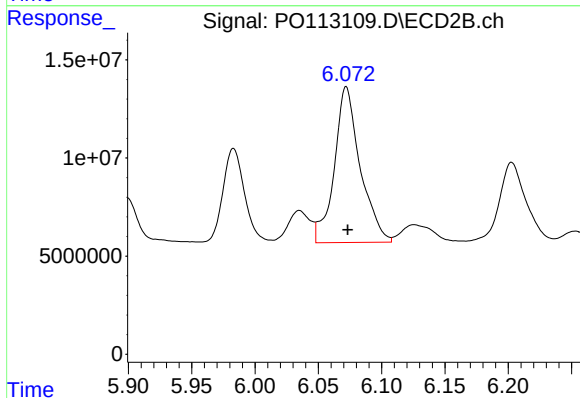


#28 AR-1254-3

R.T.: 6.072 min
Delta R.T.: -0.001 min
Response: 112985679
Conc: 271.00 ng/ml

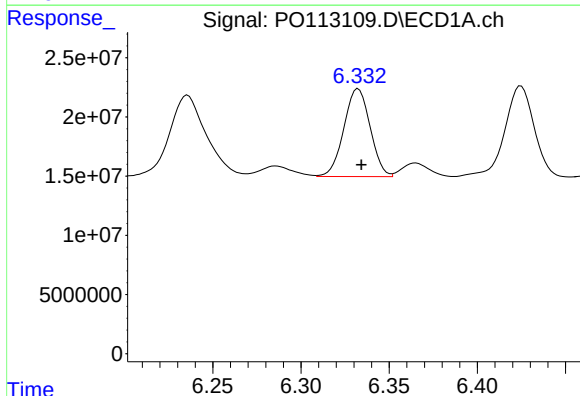


#29 AR-1254-4

R.T.: 6.332 min
Delta R.T.: -0.002 min
Response: 76933925
Conc: 138.12 ng/ml

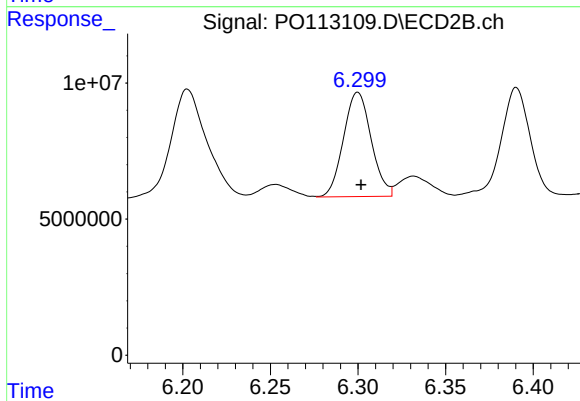

#29 AR-1254-4


R.T.: 6.300 min
Delta R.T.: -0.002 min
Response: 42240494
Conc: 153.69 ng/ml

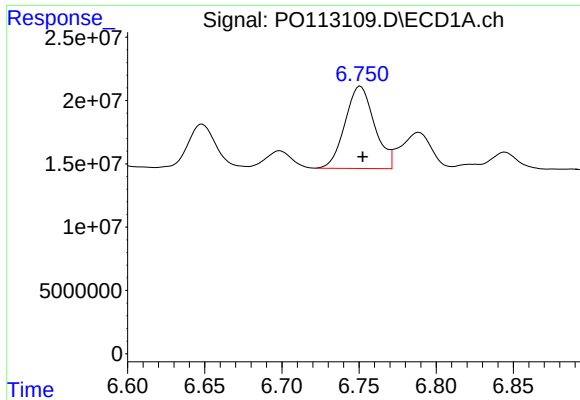

#30 AR-1254-5

R.T.: 6.751 min
Delta R.T.: -0.002 min
Response: 85938804
Conc: 122.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
HVAC DUCT SEALANTDL

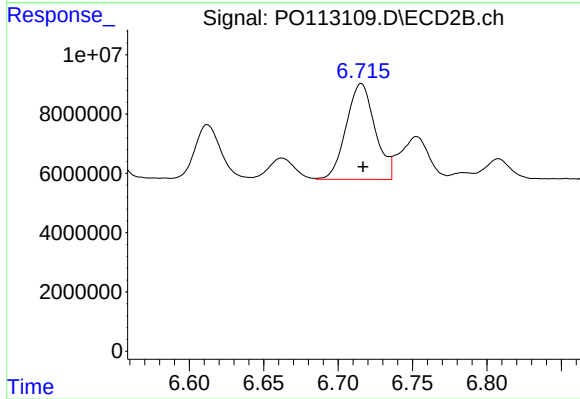

#30 AR-1254-5

R.T.: 6.716 min
Delta R.T.: -0.001 min
Response: 43646545
Conc: 122.09 ng/ml