

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082118\
 Data File : P0048379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2018 19:31
 Operator : SM/SJ
 Sample : J4539-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-BASELINE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:49:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.631	3390327	5023623	16.792	20.445
2) SA Decachlor...	10.072	8.609	2558699	2554617	15.688	16.252
Target Compounds						
3) L1 AR-1016-1	5.323	0.000	80168	0	16.784	N.D. #
4) L1 AR-1016-2	5.629	0.000	16095	0	2.734	N.D. #
5) L1 AR-1016-3	5.762	0.000	4656	0	0.939	N.D. #
6) L1 AR-1016-4	6.041	0.000	81349	0	17.489	N.D. #
7) L1 AR-1016-5	6.187	0.000	56737	0	10.884	N.D. #
8) L2 AR-1221-1	4.602	3.795	16863	122790	7.625	52.035 #
9) L2 AR-1221-2	4.694	0.000	43909	0	26.852	N.D. #
10) L2 AR-1221-3	4.772	4.063	8650	184757	1.675	31.962 #
11) L3 AR-1232-1	5.092	0.000	22200	0	10.323	N.D. #
12) L3 AR-1232-2	5.576	0.000	12009	0	4.081	N.D. #
13) L3 AR-1232-3	5.576	0.000	12009	0	2.795	N.D. #
14) L3 AR-1232-4	5.629	0.000	16095	0	5.815	N.D. #
15) L3 AR-1232-5	5.762	0.000	4656	0	2.085	N.D. #
16) L4 AR-1242-1	5.576	0.000	12009	0	1.634	N.D. #
17) L4 AR-1242-2	5.629	0.000	16095	0	3.477	N.D. #
18) L4 AR-1242-3	5.762	0.000	4656	0	1.212	N.D. #
19) L4 AR-1242-4	6.041	0.000	81349	0	21.161	N.D. #
20) L4 AR-1242-5	6.187	0.000	56737	0	13.254	N.D. #
21) L5 AR-1248-1	6.041	0.000	81349	0	13.009	N.D. #
22) L5 AR-1248-2	6.187	0.000	56737	0	10.415	N.D. #
23) L5 AR-1248-3	6.444	0.000	36573	0	5.197	N.D. #
24) L5 AR-1248-4	6.444	0.000	36573	0	5.448	N.D. #
25) L5 AR-1248-5	6.633	0.000	104046	0	14.701	N.D. #
26) L6 AR-1254-1	6.633	0.000	104046	0	8.508	N.D. #
27) L6 AR-1254-2	6.913	0.000	29728	0	3.986	N.D. #
28) L6 AR-1254-3	7.000	0.000	229591	0	17.605	N.D. #
29) L6 AR-1254-4	7.272	6.363	30084	259754	3.087	23.973 #
30) L6 AR-1254-5	7.543	0.000	39648	0	5.367	N.D. #
31) L7 AR-1260-1	7.171	0.000	453	0	0.048	N.D. #
32) L7 AR-1260-2	7.375	6.363	145458	259754	13.044	19.373 #
33) L7 AR-1260-3	7.691	0.000	42857	0	3.331	N.D. #
34) L7 AR-1260-4	8.304	0.000	84231	0	4.735	N.D. #
35) L7 AR-1260-5	8.620	0.000	68598	0	6.007	N.D. #
36) L8 AR-1262-1	7.171	6.363	453	259754	0.055	22.910 #
37) L8 AR-1262-2	7.375	6.544	145458	210401	15.009	18.645
38) L8 AR-1262-3	7.763	0.000	97409	0	7.937	N.D. #

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD_0\Data\P0082118\
 Data File : P0048379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2018 19:31
 Operator : SM/SJ
 Sample : J4539-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MS-BASELINE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:49:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39) L8	AR-1262-4	7.990	0.000	47948	0	4.072	N.D. #
40) L8	AR-1262-5	8.304	0.000	84231	0	3.920	N.D. #
41) L9	AR-1268-1	8.620	0.000	68598	0	2.956	N.D. #
42) L9	AR-1268-2	8.722	0.000	10559	0	0.493	N.D. #
43) L9	AR-1268-3	8.940	0.000	5839	0	0.323	N.D. #
44) L9	AR-1268-4	9.357	0.000	4867	0	0.610	N.D. #
45) L9	AR-1268-5	9.790	0.000	8815	0	0.162	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\PO082118\
Data File : PO048379.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2018 19:31
Operator : SM/SJ
Sample : J4539-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:49:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

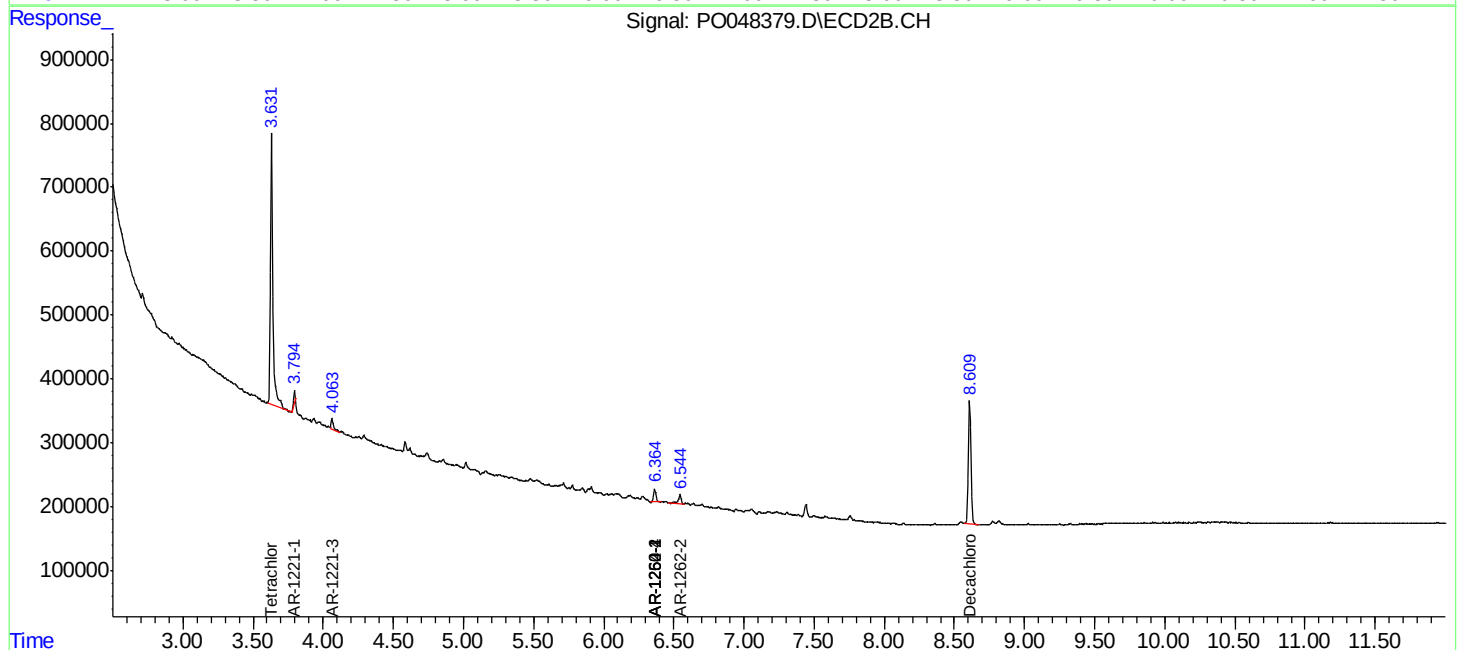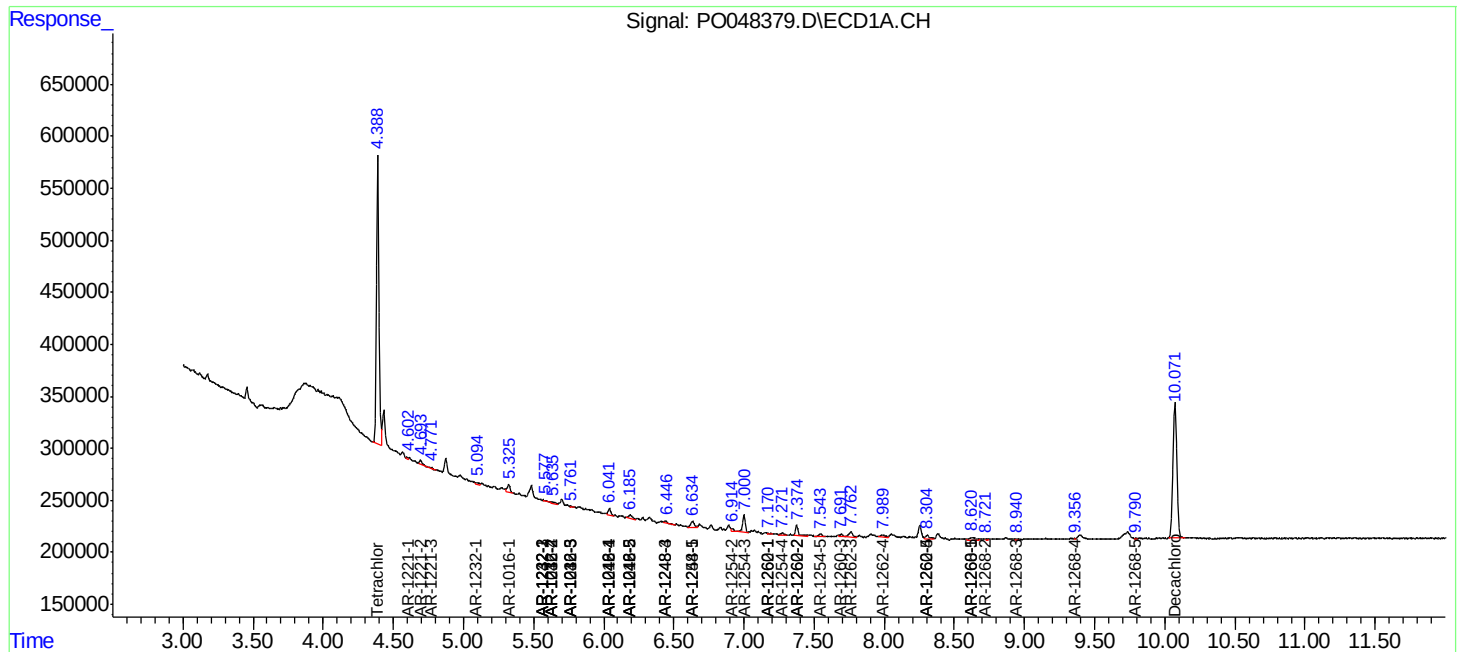


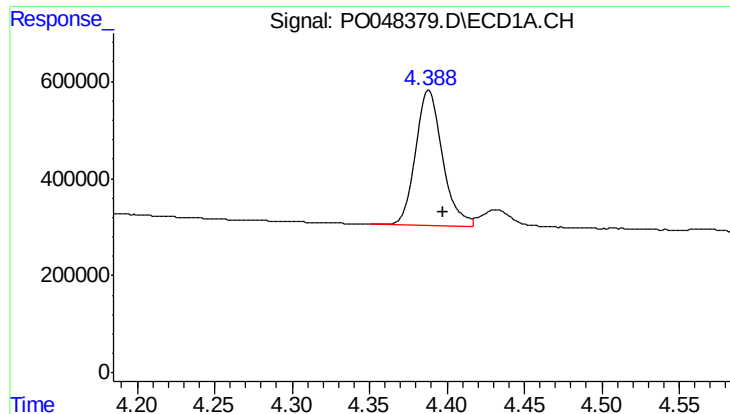

#1 Tetrachloro-m-xylene


R.T.: 4.388 min
Delta R.T.: -0.009 min
Response: 3390327
Conc: 16.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

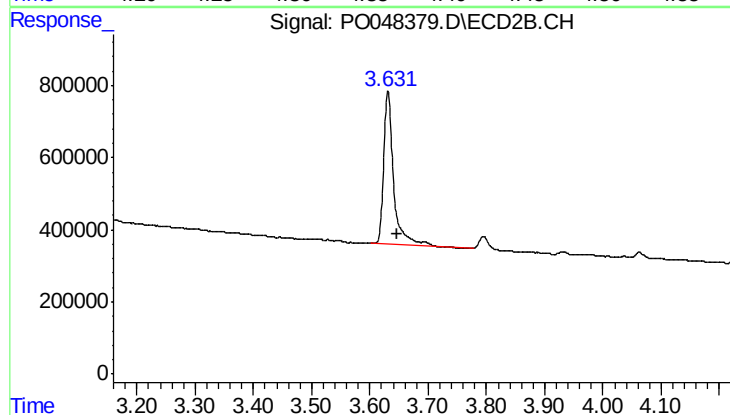


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.014 min
Response: 5023623
Conc: 20.44 ng/ml

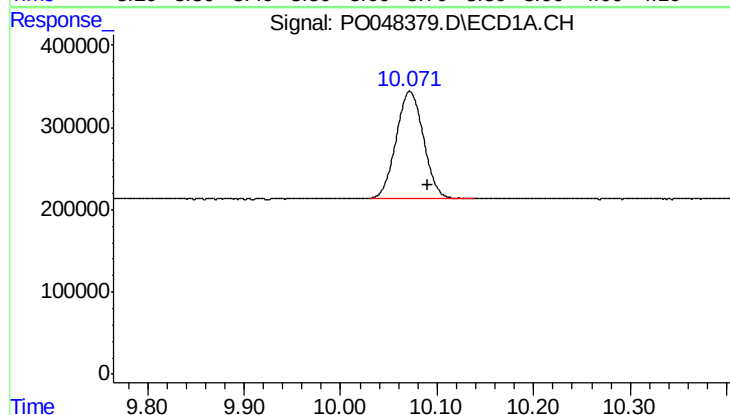


#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: -0.018 min
Response: 2558699
Conc: 15.69 ng/ml

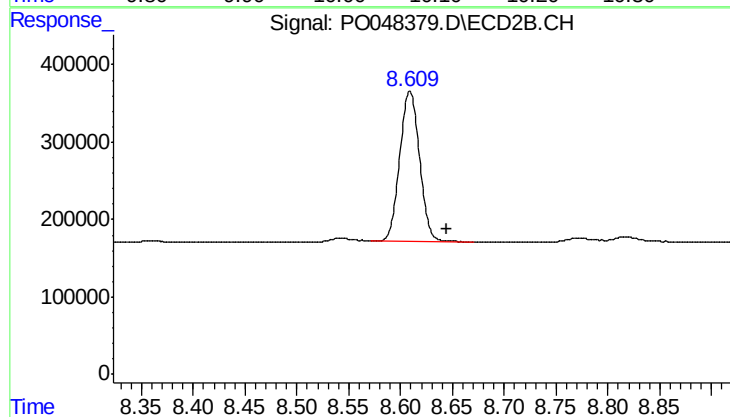

#2 Decachlorobiphenyl


R.T.: 8.609 min
Delta R.T.: -0.036 min
Response: 2554617
Conc: 16.25 ng/ml

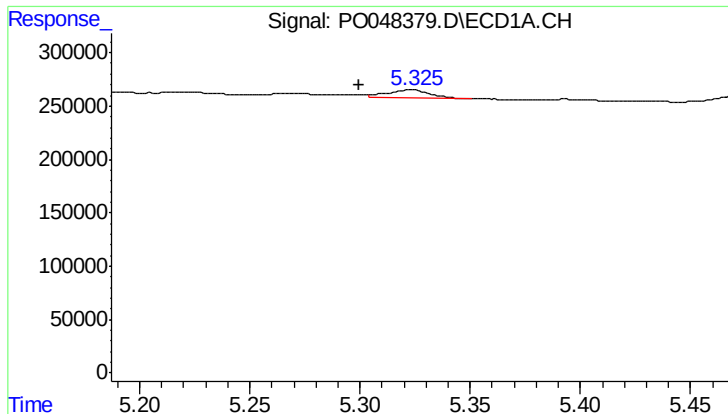

#3 AR-1016-1


R.T.: 5.323 min
Delta R.T.: 0.024 min
Response: 80168
Conc: 16.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

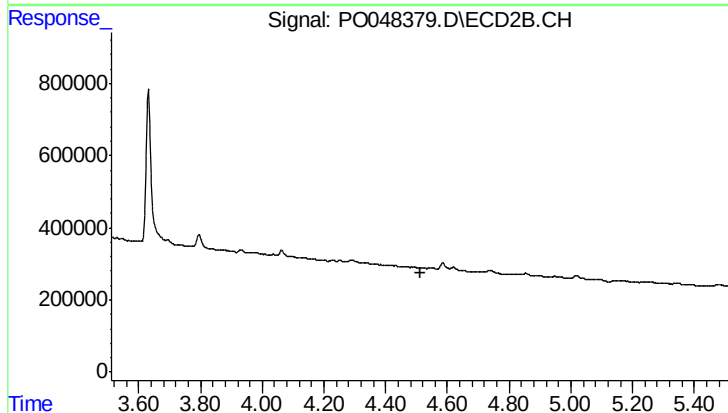


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T.: 4.511 min
Response: 0
Conc: N.D.

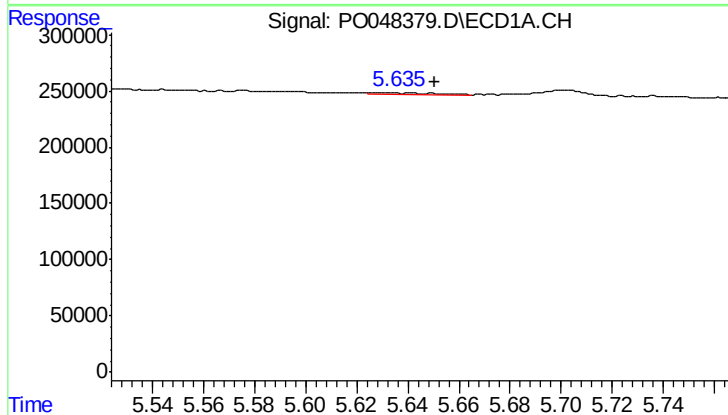


#4 AR-1016-2

R.T.: 5.629 min
Delta R.T.: -0.022 min
Response: 16095
Conc: 2.73 ng/ml

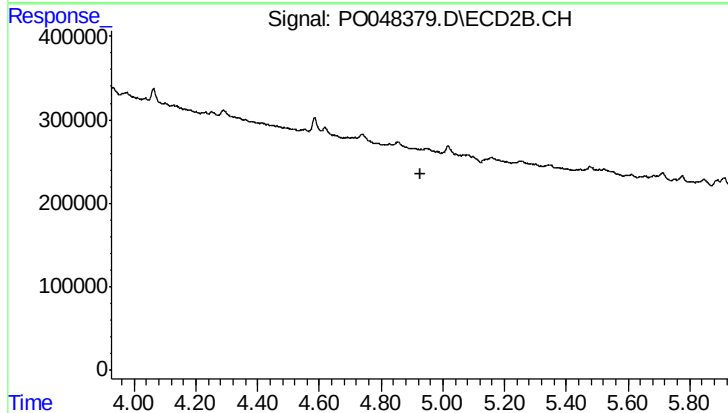

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 4.926 min
Response: 0
Conc: N.D.

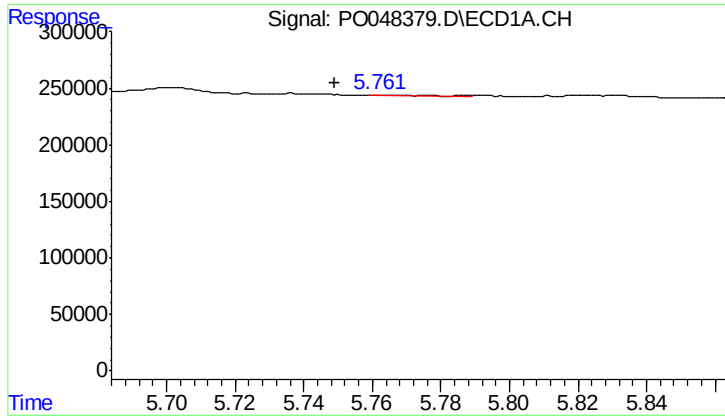

#5 AR-1016-3


R.T.: 5.762 min
Delta R.T.: 0.013 min
Response: 4656
Conc: 0.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

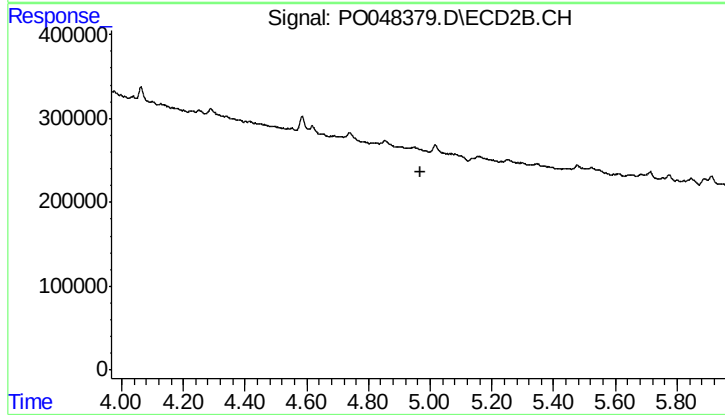


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T.: 4.967 min
Response: 0
Conc: N.D.

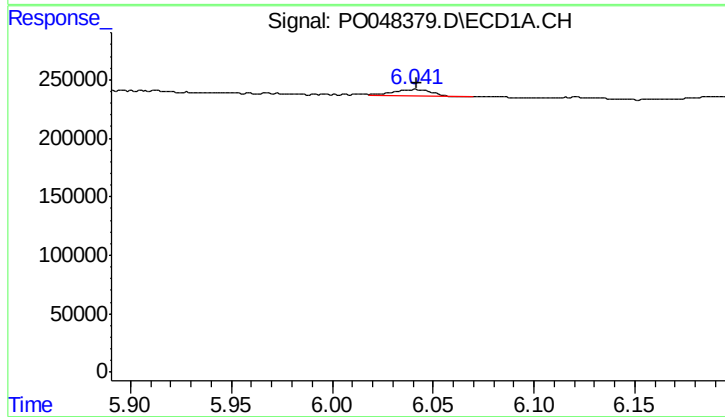


#6 AR-1016-4

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 81349
Conc: 17.49 ng/ml

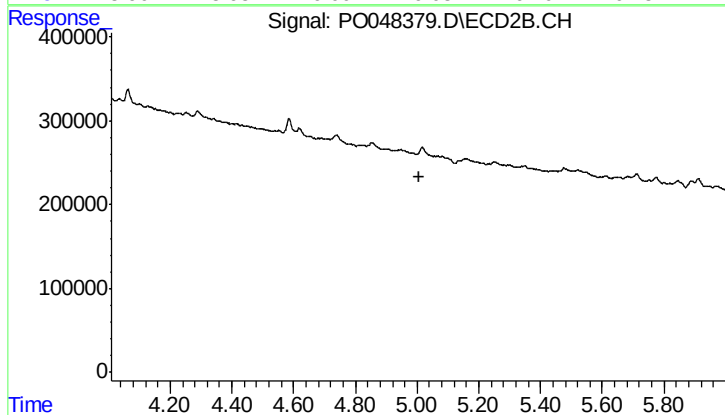

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.009 min
Response: 0
Conc: N.D.

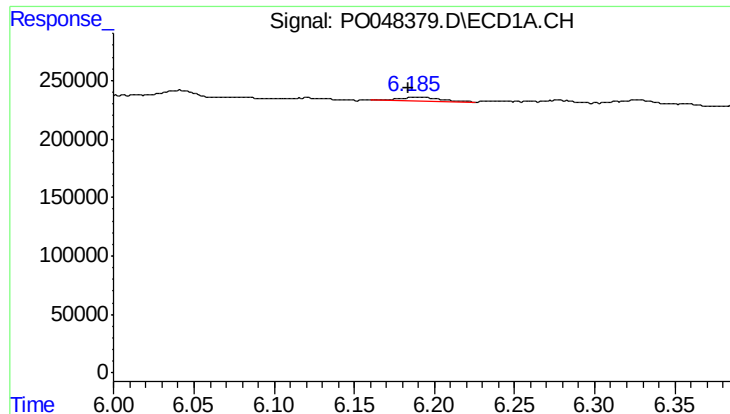

#7 AR-1016-5


R.T.: 6.187 min
Delta R.T.: 0.003 min
Response: 56737
Conc: 10.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

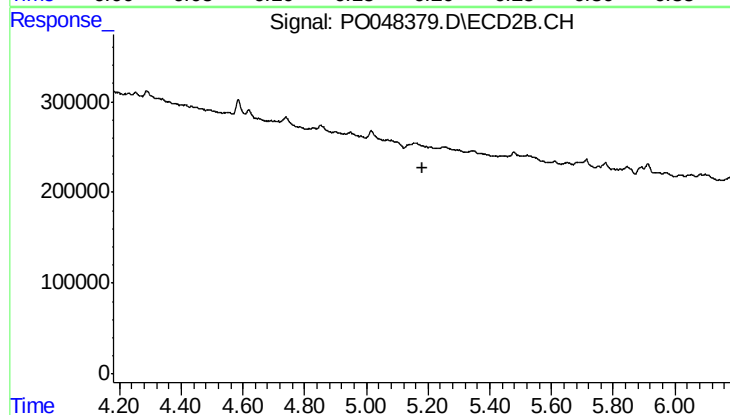


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 5.180 min
Response: 0
Conc: N.D.

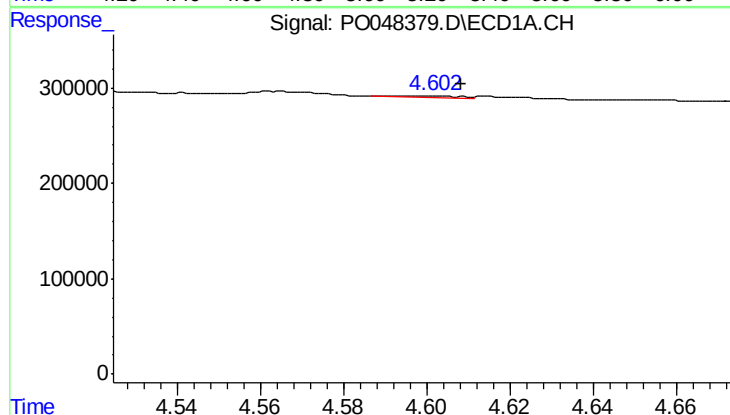


#8 AR-1221-1

R.T.: 4.602 min
Delta R.T.: -0.006 min
Response: 16863
Conc: 7.63 ng/ml

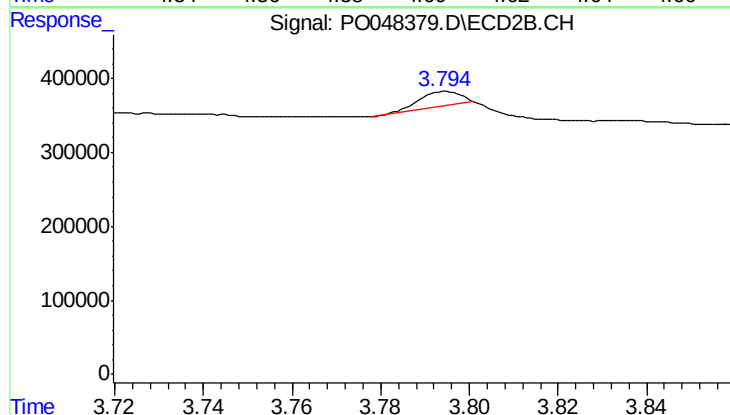

#8 AR-1221-1


R.T.: 3.795 min
Delta R.T.: -0.066 min
Response: 122790
Conc: 52.04 ng/ml

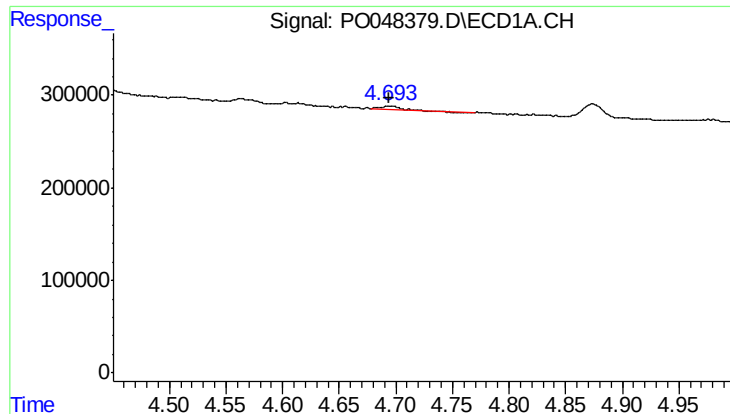

#9 AR-1221-2


R.T.: 4.694 min
Delta R.T.: 0.000 min
Response: 43909
Conc: 26.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

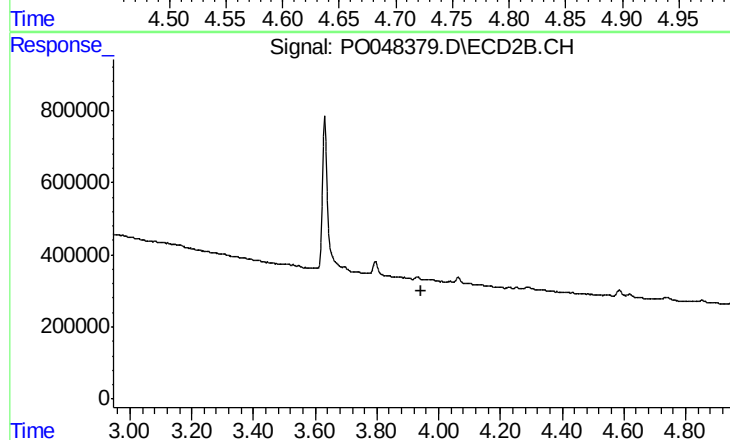


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 3.946 min
Response: 0
Conc: N.D.

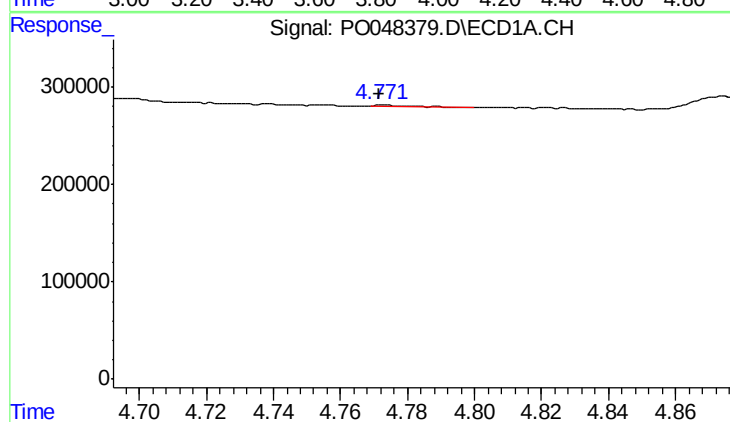


#10 AR-1221-3

R.T.: 4.772 min
Delta R.T.: 0.001 min
Response: 8650
Conc: 1.68 ng/ml

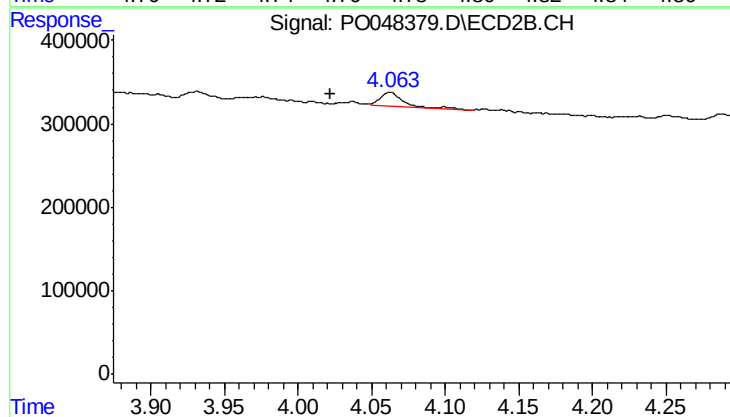

#10 AR-1221-3


R.T.: 4.063 min
Delta R.T.: 0.040 min
Response: 184757
Conc: 31.96 ng/ml

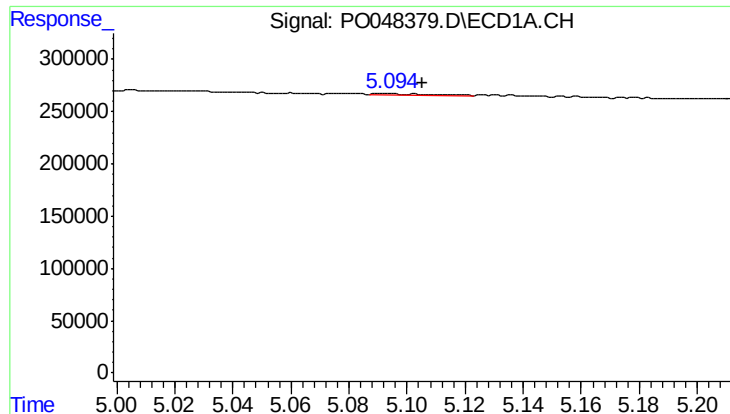

#11 AR-1232-1


R.T.: 5.092 min
Delta R.T.: -0.014 min
Response: 22200
Conc: 10.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

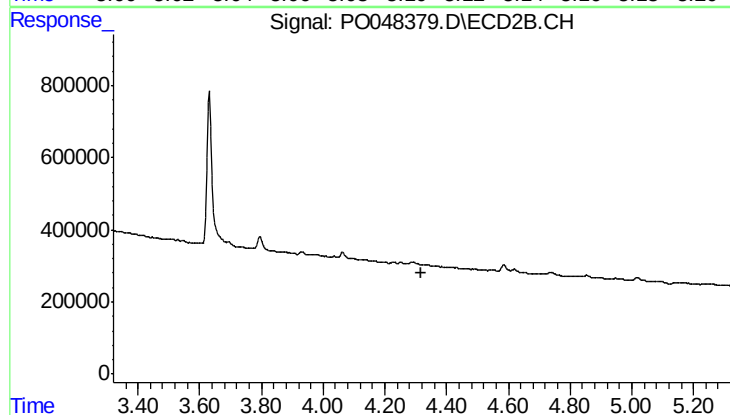


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.320 min
Response: 0
Conc: N.D.

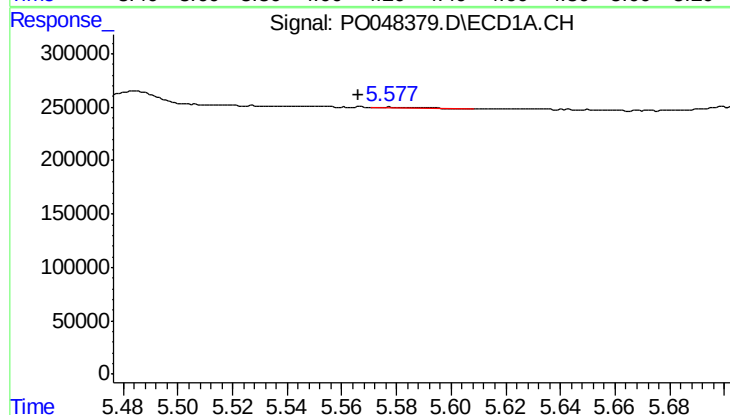


#12 AR-1232-2

R.T.: 5.576 min
Delta R.T.: 0.010 min
Response: 12009
Conc: 4.08 ng/ml

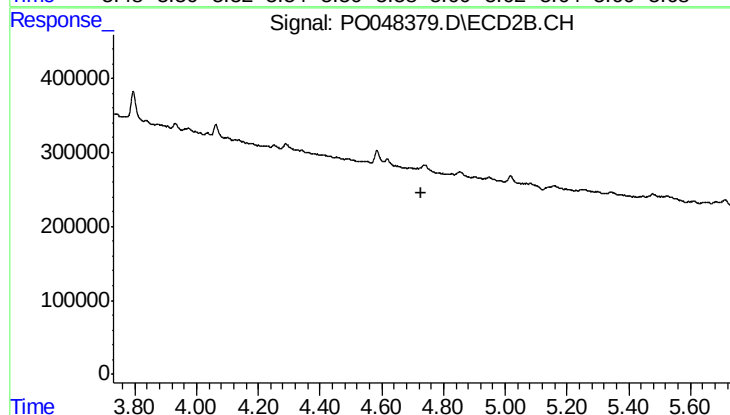

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.730 min
Response: 0
Conc: N.D.

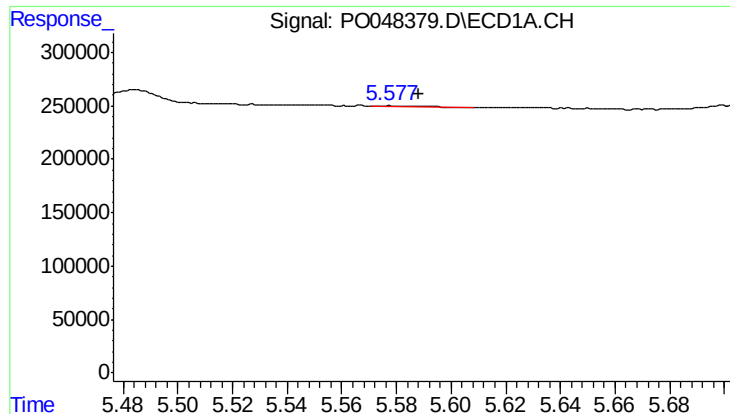

#13 AR-1232-3


R.T.: 5.576 min
Delta R.T.: -0.013 min
Response: 12009
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

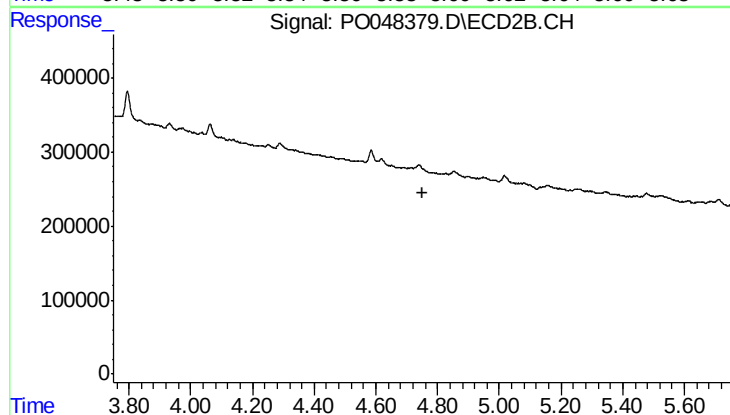


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T.: 4.749 min
Response: 0
Conc: N.D.

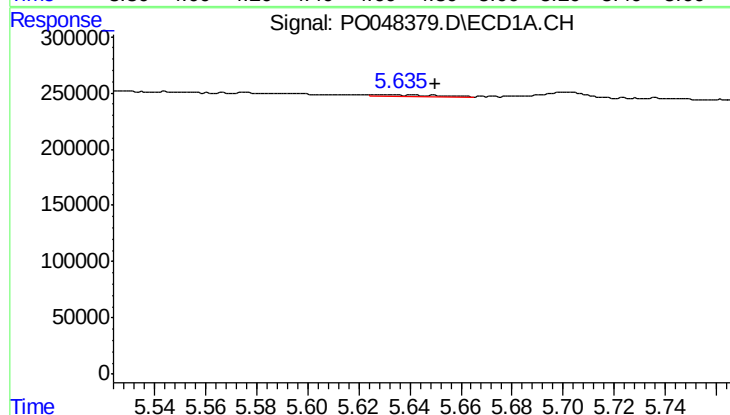


#14 AR-1232-4

R.T.: 5.629 min
Delta R.T.: -0.021 min
Response: 16095
Conc: 5.81 ng/ml

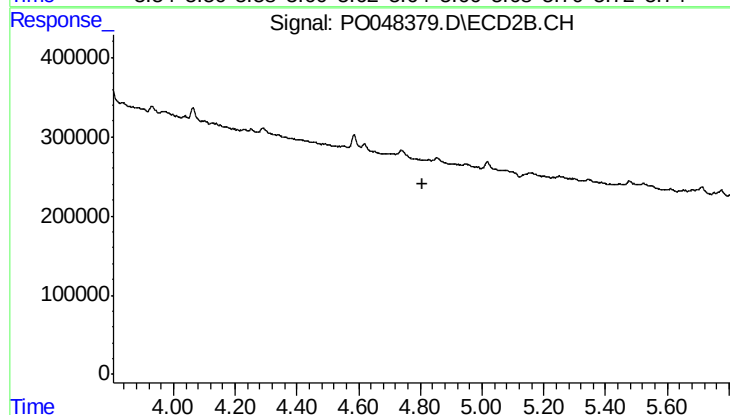

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

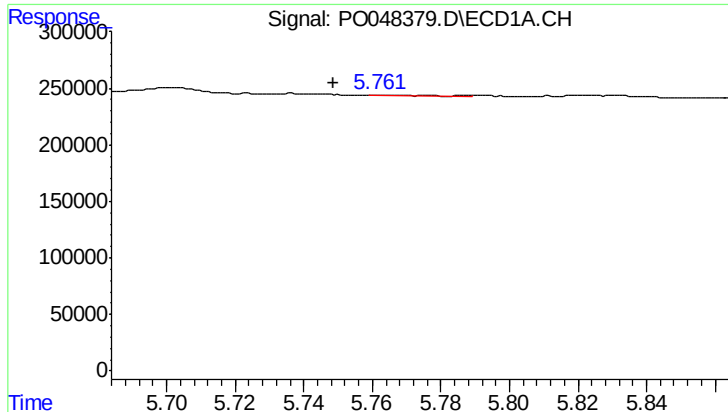

#15 AR-1232-5


R.T.: 5.762 min
Delta R.T.: 0.013 min
Response: 4656
Conc: 2.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

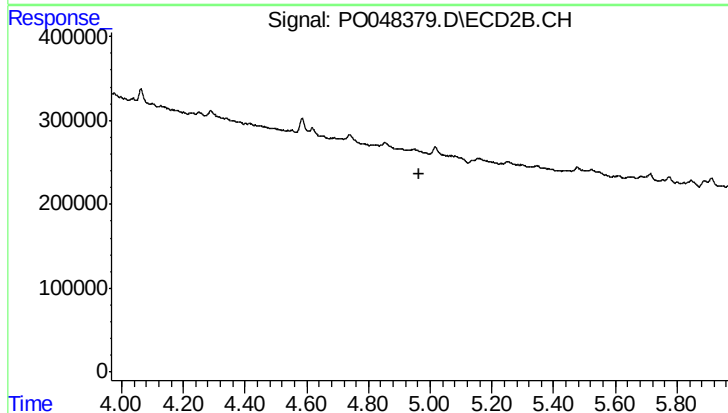


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

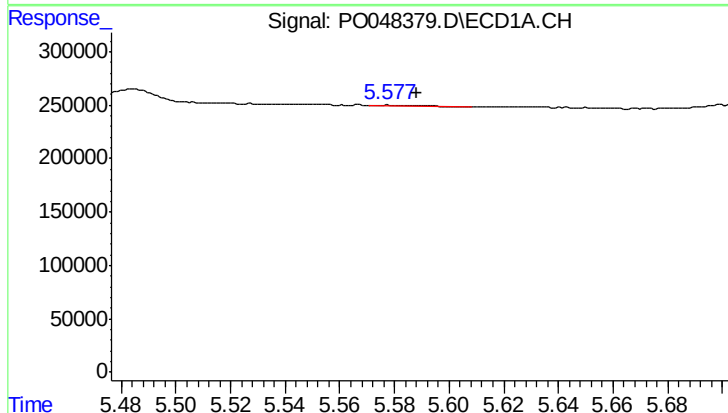


#16 AR-1242-1

R.T.: 5.576 min
Delta R.T.: -0.012 min
Response: 12009
Conc: 1.63 ng/ml

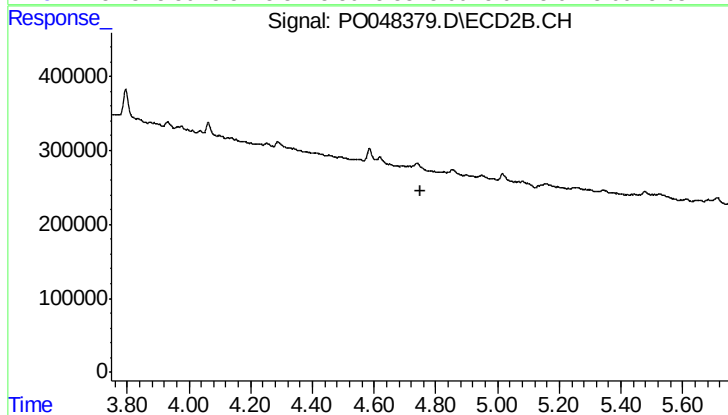

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T.: 4.749 min
Response: 0
Conc: N.D.

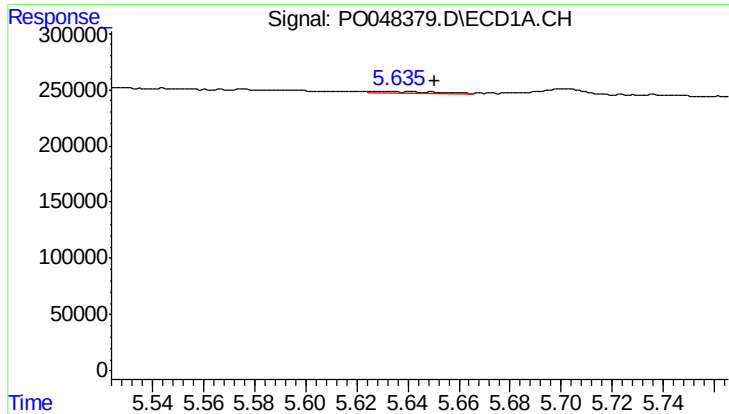

#17 AR-1242-2


R.T.: 5.629 min
Delta R.T.: -0.022 min
Response: 16095
Conc: 3.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

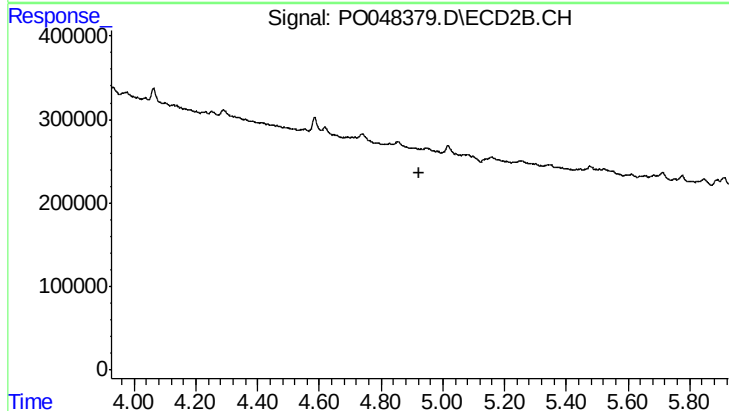


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T.: 4.926 min
Response: 0
Conc: N.D.

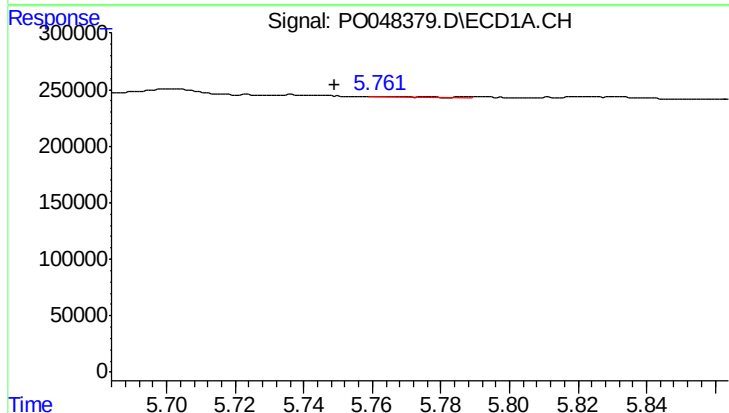


#18 AR-1242-3

R.T.: 5.762 min
Delta R.T.: 0.013 min
Response: 4656
Conc: 1.21 ng/ml

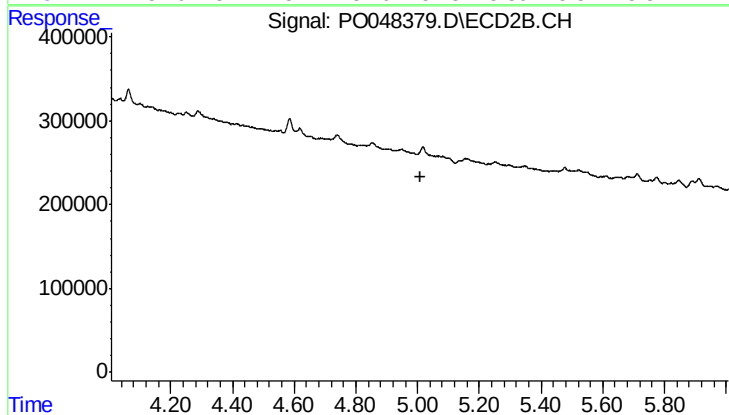

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

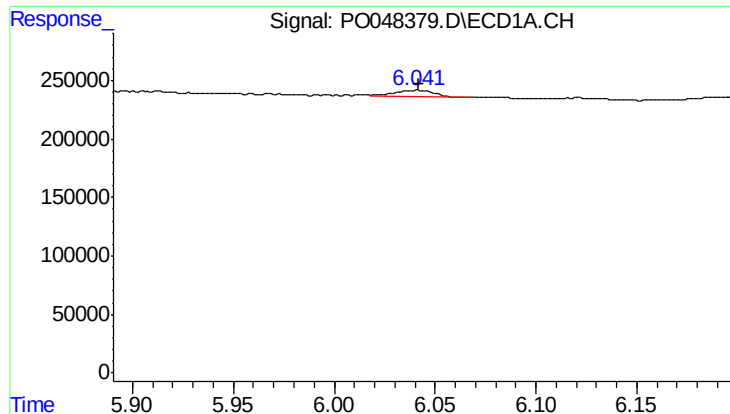

#19 AR-1242-4


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 81349
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

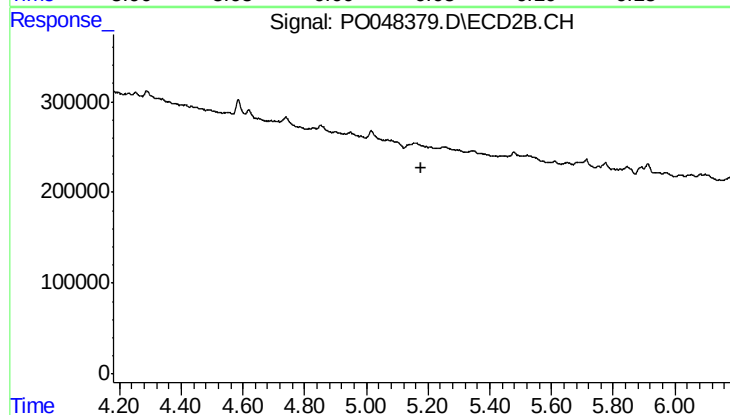


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.180 min
Response: 0
Conc: N.D.

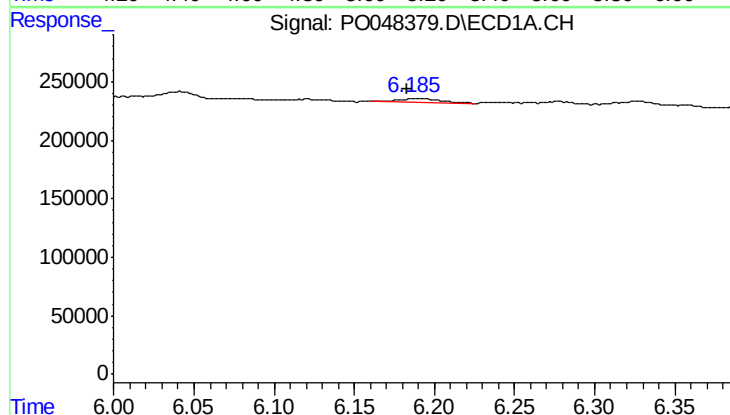


#20 AR-1242-5

R.T.: 6.187 min
Delta R.T.: 0.004 min
Response: 56737
Conc: 13.25 ng/ml

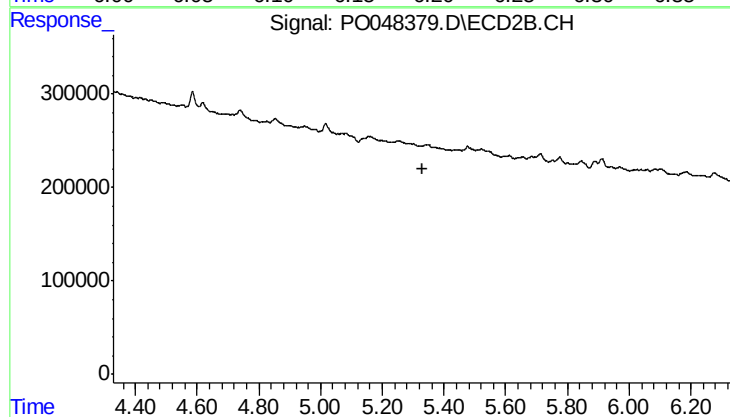

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 5.329 min
Response: 0
Conc: N.D.

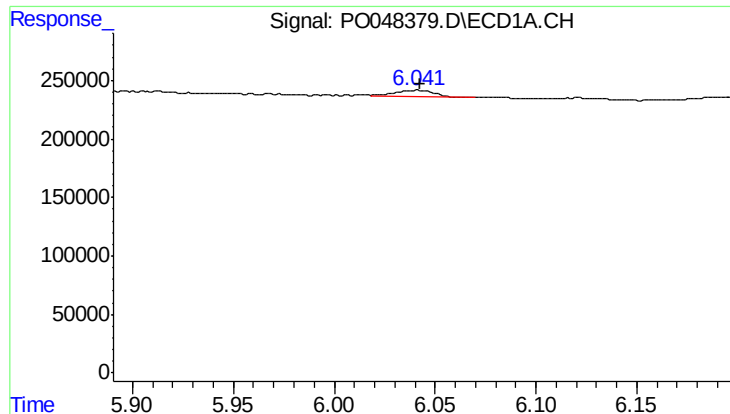

#21 AR-1248-1


R.T.: 6.041 min
Delta R.T.: -0.002 min
Response: 81349
Conc: 13.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

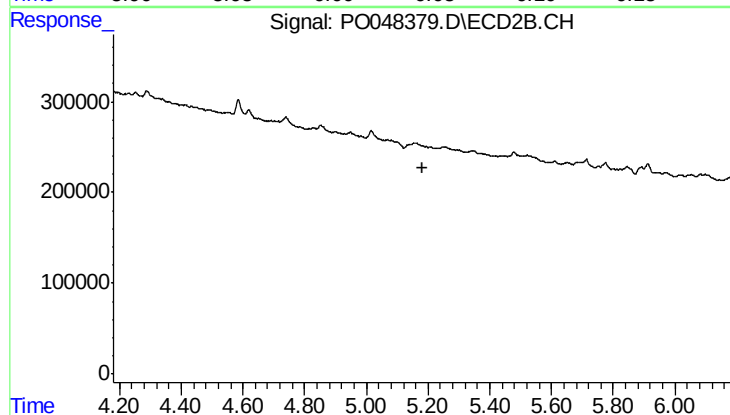


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T.: 5.180 min
Response: 0
Conc: N.D.

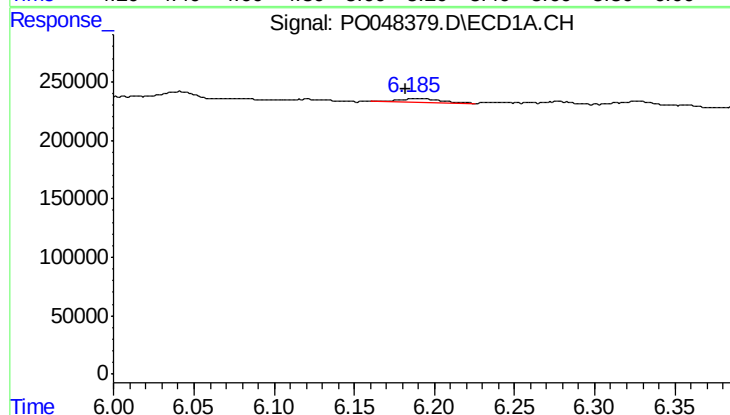


#22 AR-1248-2

R.T.: 6.187 min
Delta R.T.: 0.004 min
Response: 56737
Conc: 10.42 ng/ml

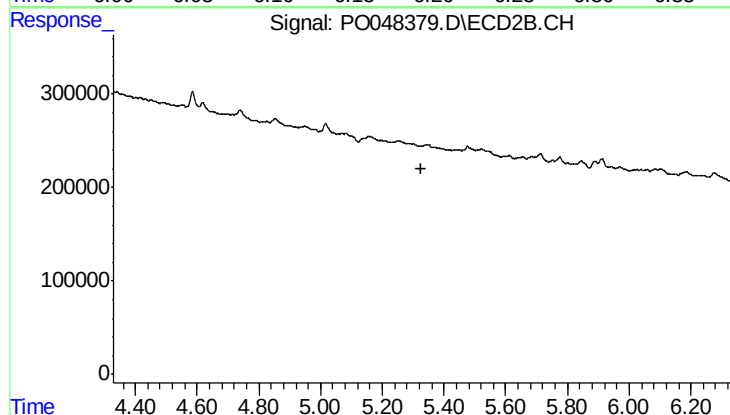

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

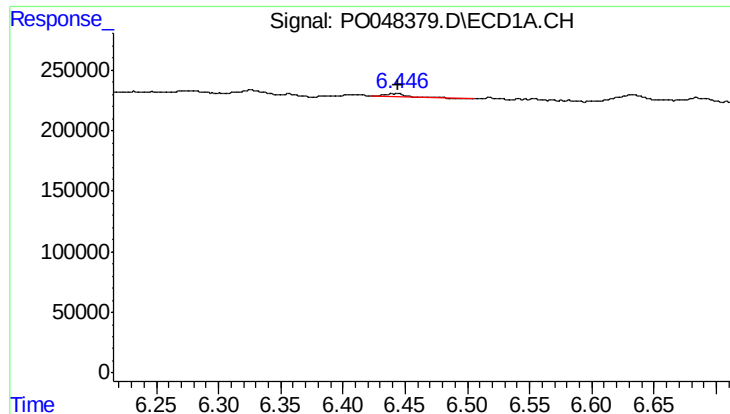

#23 AR-1248-3


R.T.: 6.444 min
Delta R.T.: -0.001 min
Response: 36573
Conc: 5.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

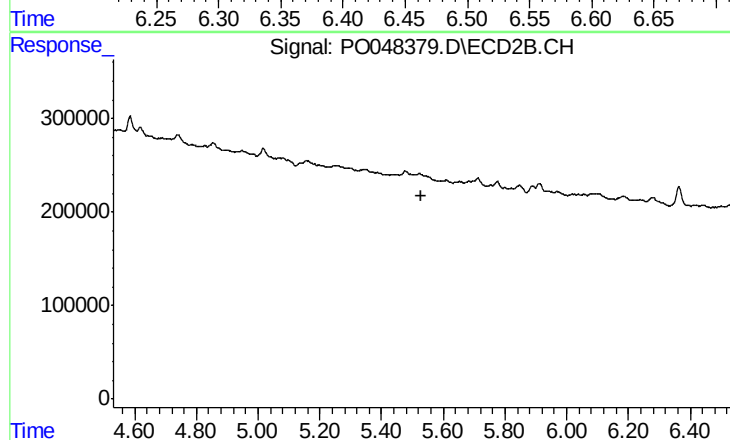


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.531 min
Response: 0
Conc: N.D.

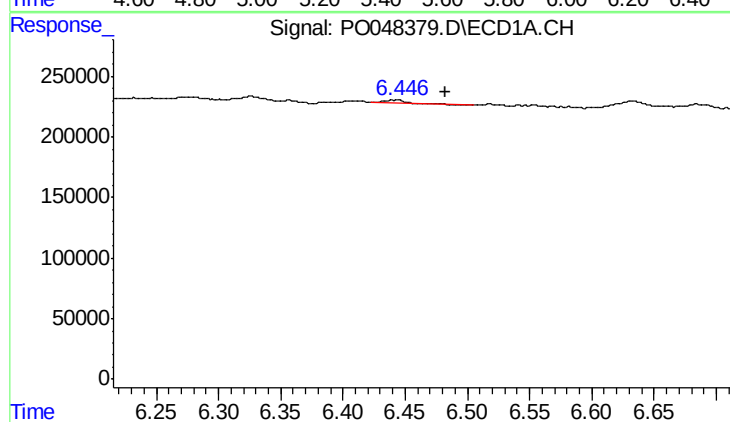


#24 AR-1248-4

R.T.: 6.444 min
Delta R.T.: -0.039 min
Response: 36573
Conc: 5.45 ng/ml

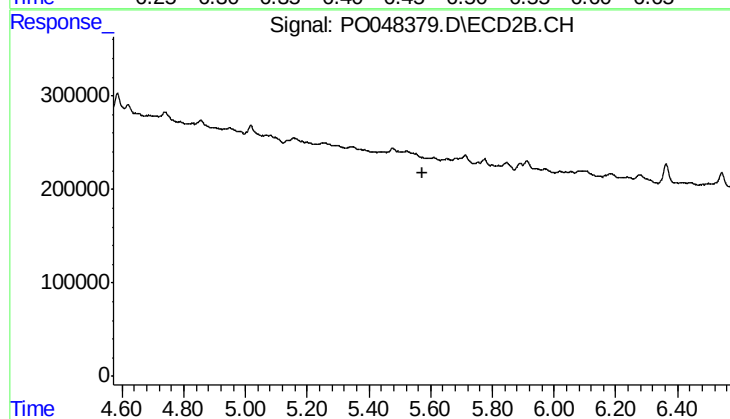

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.572 min
Response: 0
Conc: N.D.

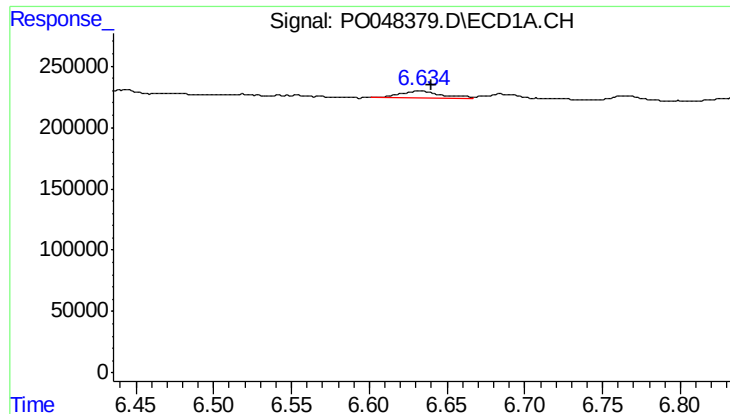

#25 AR-1248-5


R.T.: 6.633 min
Delta R.T.: -0.007 min
Response: 104046
Conc: 14.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

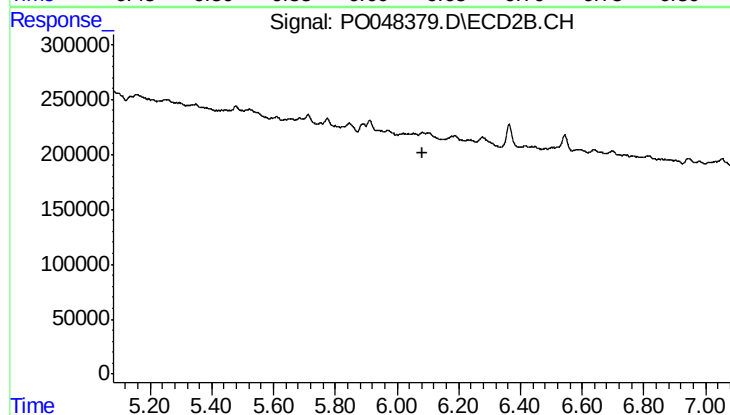


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.081 min
Response: 0
Conc: N.D.

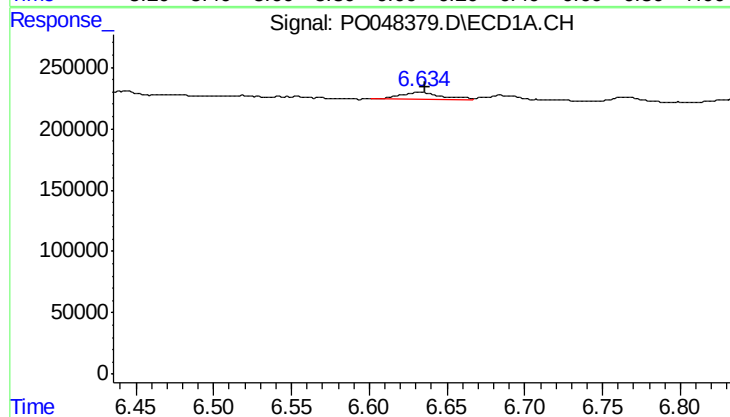


#26 AR-1254-1

R.T.: 6.633 min
Delta R.T.: -0.003 min
Response: 104046
Conc: 8.51 ng/ml

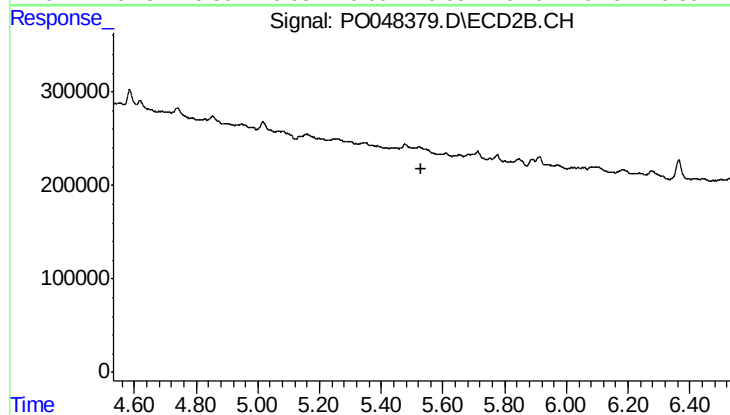

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 5.531 min
Response: 0
Conc: N.D.

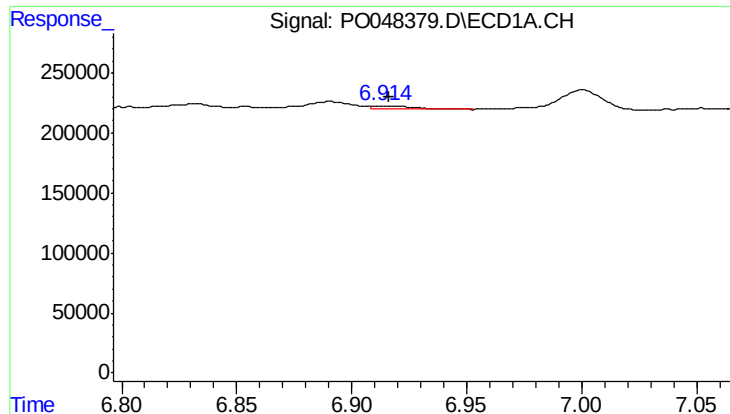

#27 AR-1254-2


R.T.: 6.913 min
Delta R.T.: -0.003 min
Response: 29728
Conc: 3.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

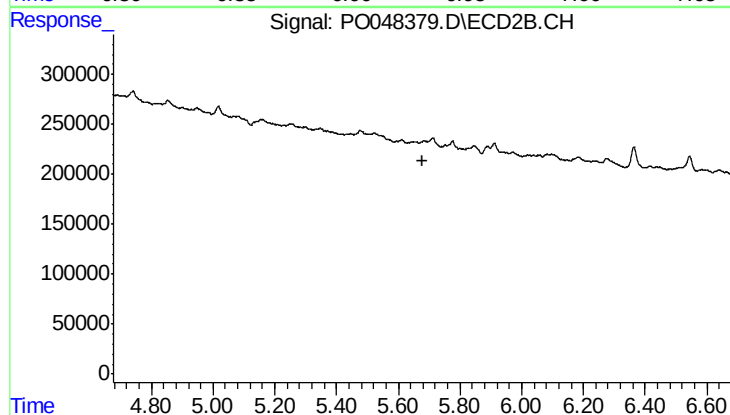


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.677 min
Response: 0
Conc: N.D.

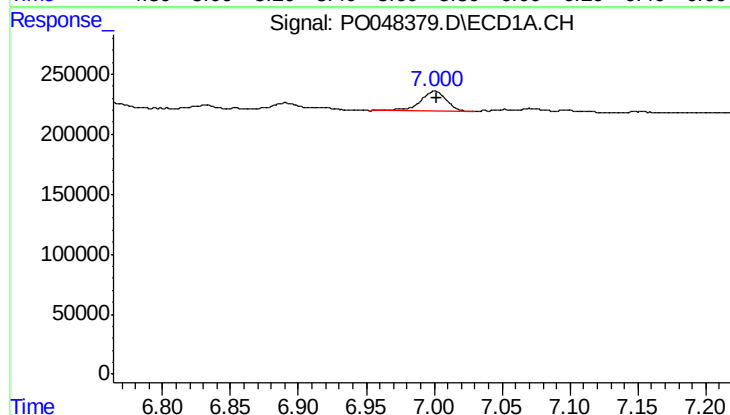


#28 AR-1254-3

R.T.: 7.000 min
Delta R.T.: -0.002 min
Response: 229591
Conc: 17.60 ng/ml

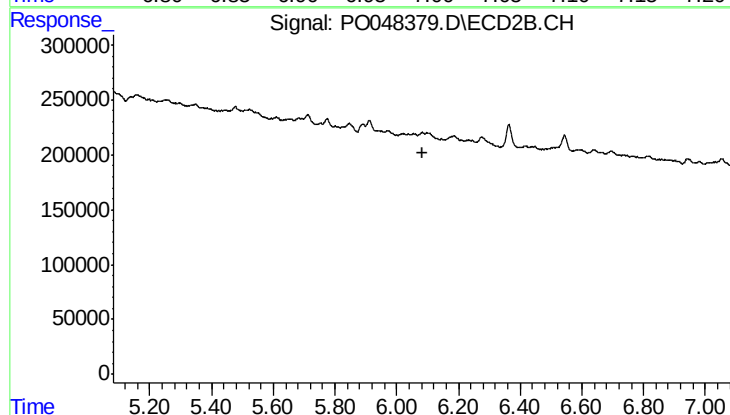

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.082 min
Response: 0
Conc: N.D.

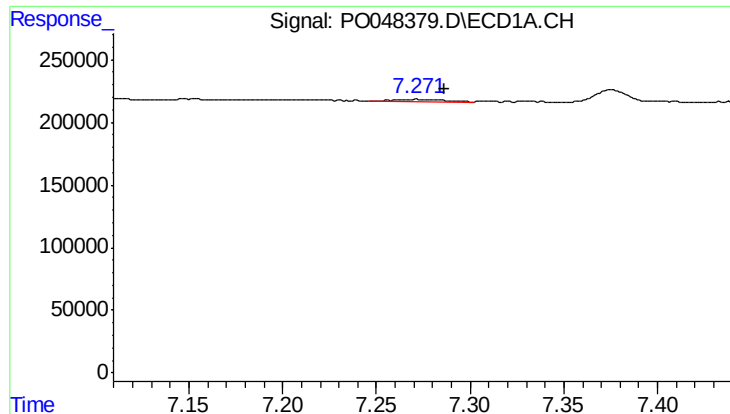

#29 AR-1254-4


R.T.: 7.272 min
Delta R.T.: -0.014 min
Response: 30084
Conc: 3.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

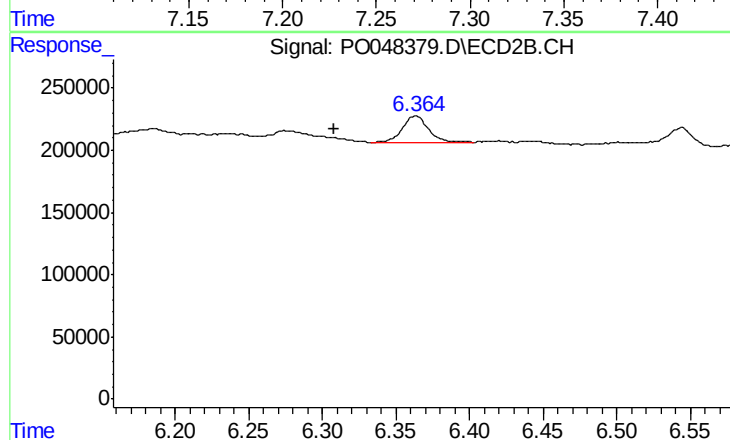


#29 AR-1254-4

R.T.: 6.363 min
Delta R.T.: 0.055 min
Response: 259754
Conc: 23.97 ng/ml

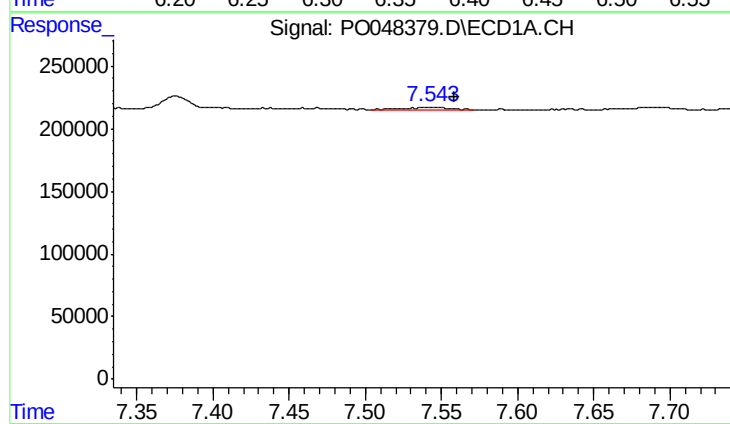


#30 AR-1254-5

R.T.: 7.543 min
Delta R.T.: -0.016 min
Response: 39648
Conc: 5.37 ng/ml

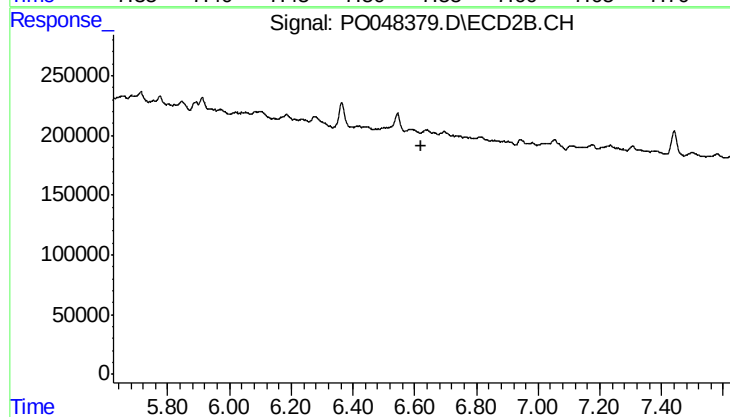

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

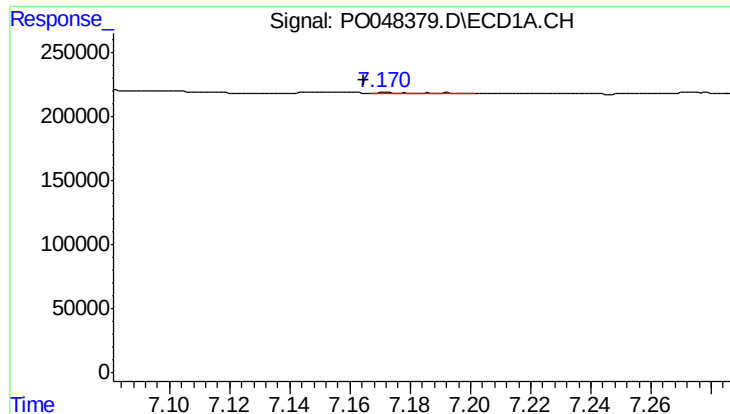

#31 AR-1260-1


R.T.: 7.171 min
Delta R.T.: 0.007 min
Response: 453
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

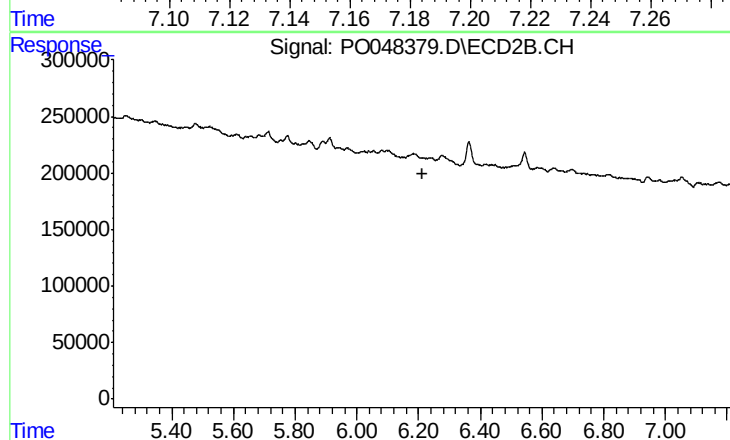


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 6.211 min
Response: 0
Conc: N.D.

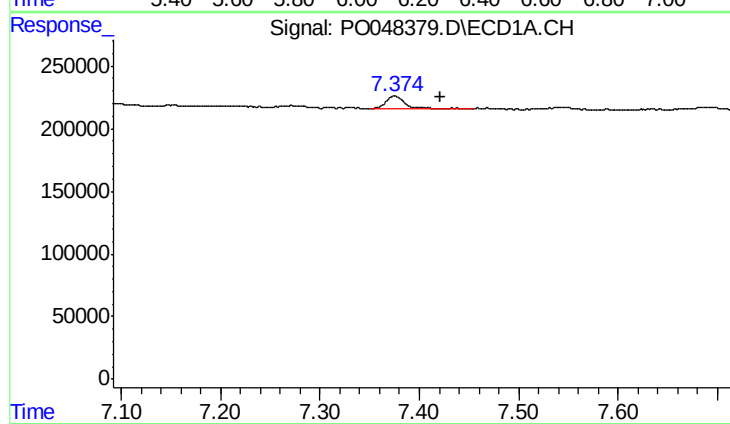


#32 AR-1260-2

R.T.: 7.375 min
Delta R.T.: -0.046 min
Response: 145458
Conc: 13.04 ng/ml

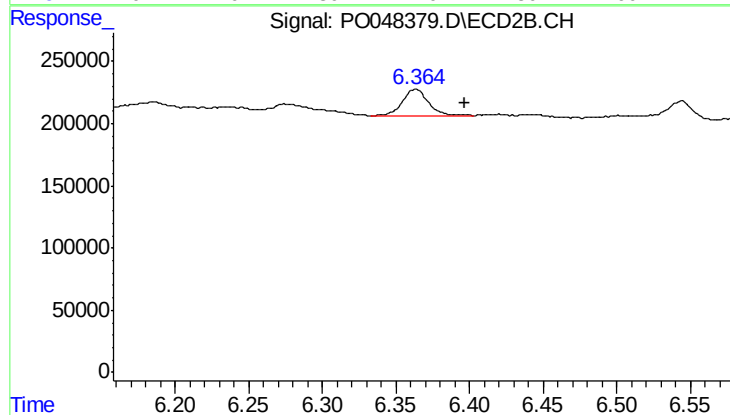

#32 AR-1260-2


R.T.: 6.363 min
Delta R.T.: -0.034 min
Response: 259754
Conc: 19.37 ng/ml

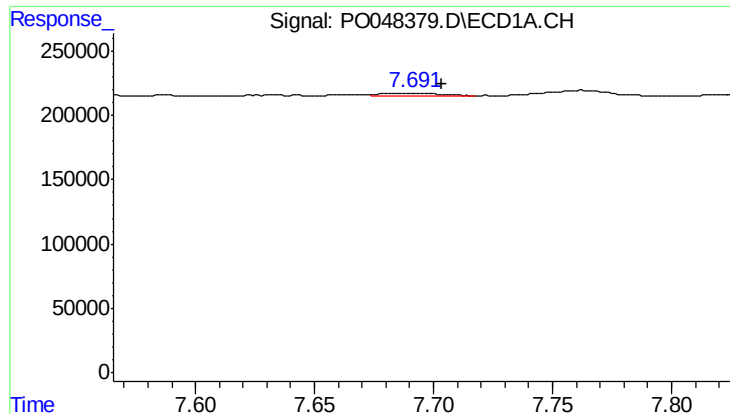

#33 AR-1260-3


R.T.: 7.691 min
Delta R.T.: -0.013 min
Response: 42857
Conc: 3.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

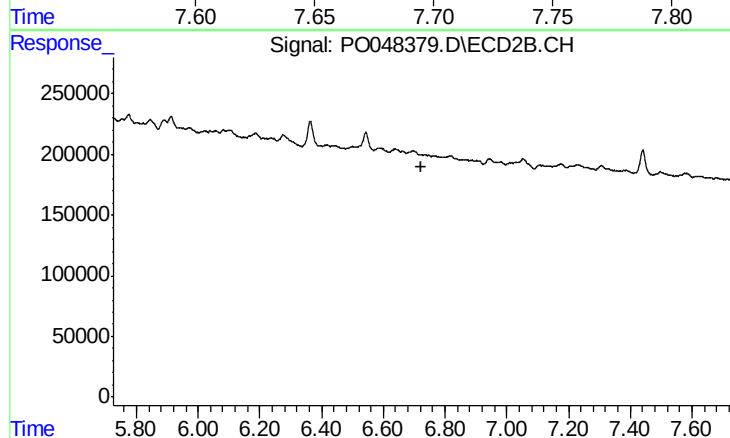


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 6.725 min
Response: 0
Conc: N.D.

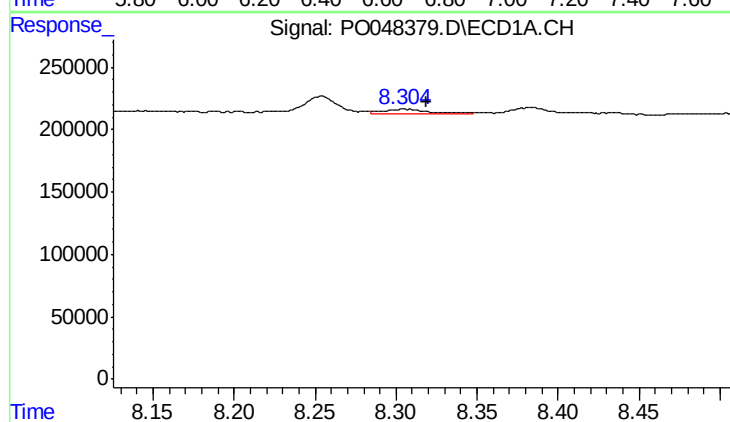


#34 AR-1260-4

R.T.: 8.304 min
Delta R.T.: -0.014 min
Response: 84231
Conc: 4.74 ng/ml

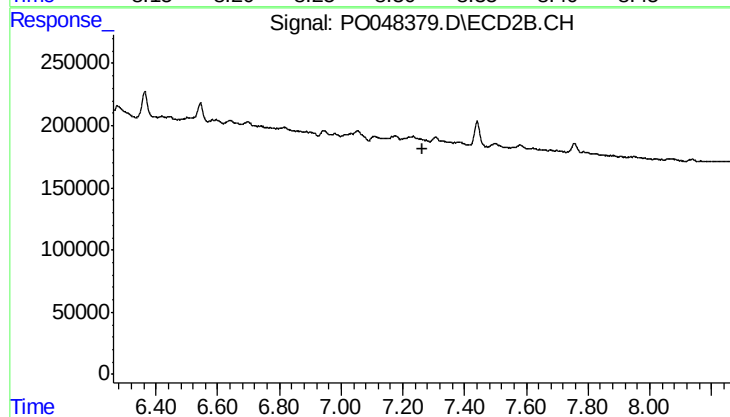

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.262 min
Response: 0
Conc: N.D.

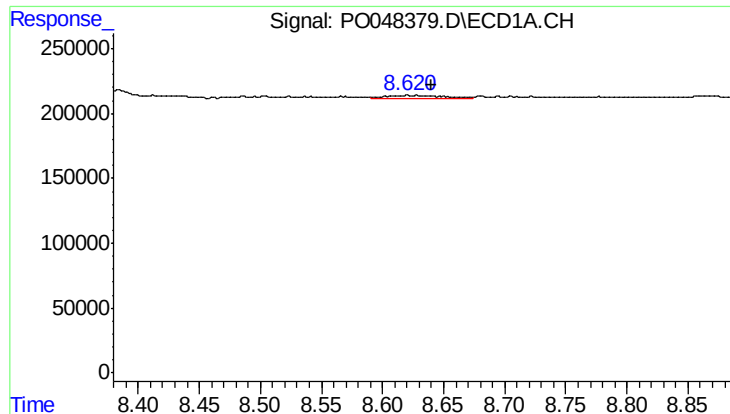

#35 AR-1260-5


R.T.: 8.620 min
Delta R.T.: -0.020 min
Response: 68598
Conc: 6.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

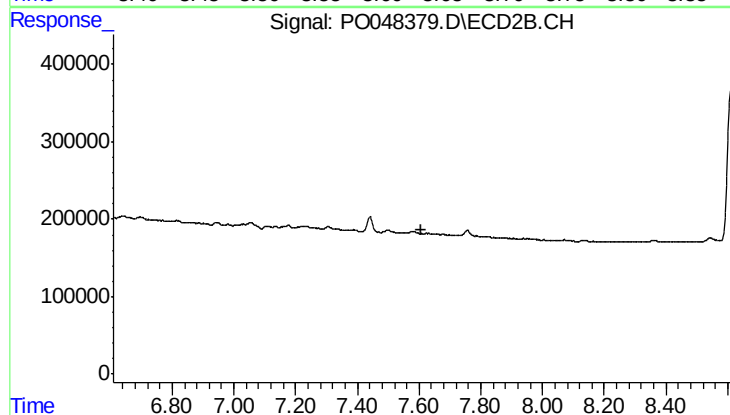


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 7.609 min
Response: 0
Conc: N.D.

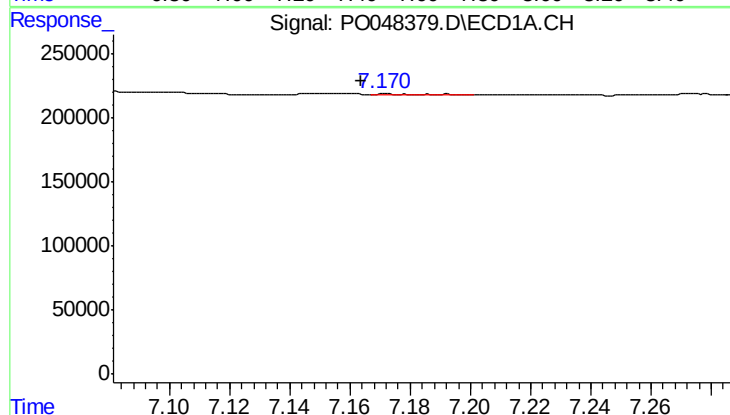


#36 AR-1262-1

R.T.: 7.171 min
Delta R.T.: 0.008 min
Response: 453
Conc: 0.05 ng/ml

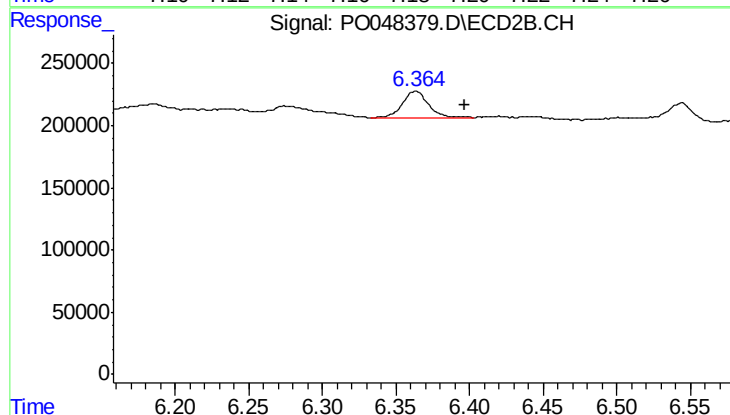

#36 AR-1262-1


R.T.: 6.363 min
Delta R.T.: -0.033 min
Response: 259754
Conc: 22.91 ng/ml

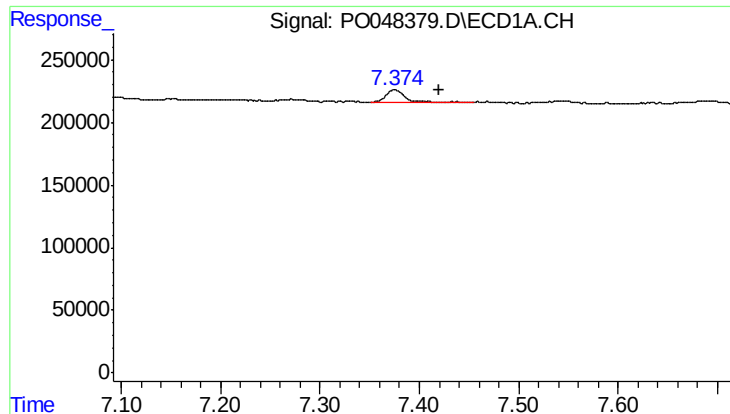

#37 AR-1262-2


R.T.: 7.375 min
Delta R.T.: -0.045 min
Response: 145458
Conc: 15.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

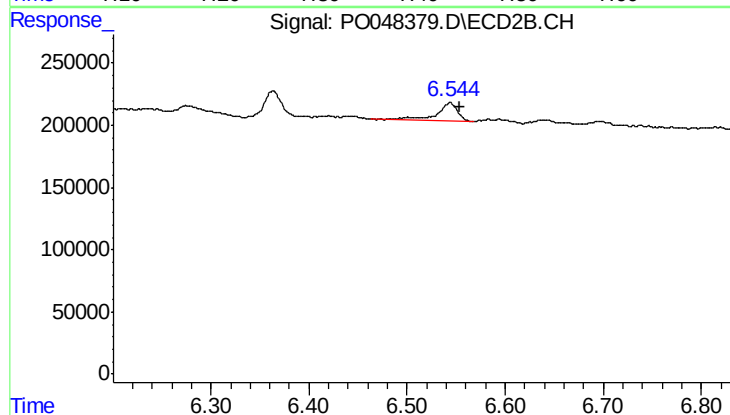


#37 AR-1262-2

R.T.: 6.544 min
Delta R.T.: -0.010 min
Response: 210401
Conc: 18.65 ng/ml

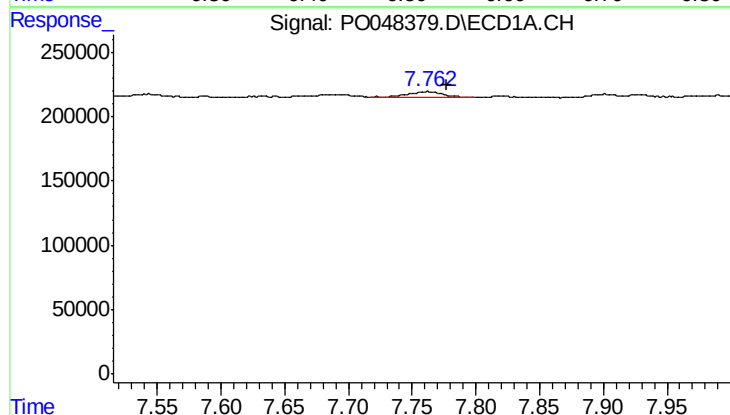


#38 AR-1262-3

R.T.: 7.763 min
Delta R.T.: -0.015 min
Response: 97409
Conc: 7.94 ng/ml

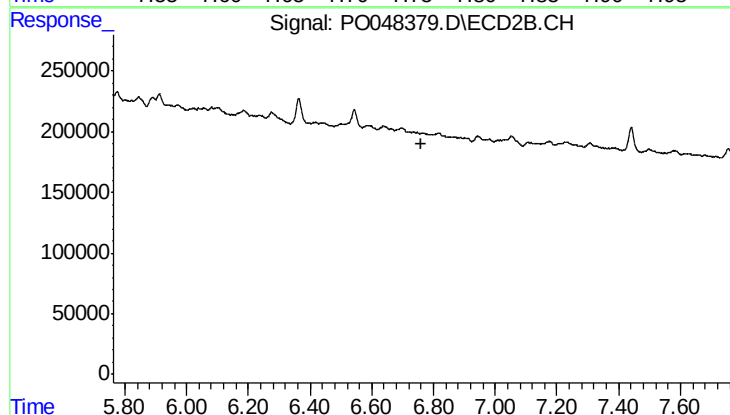

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 6.762 min
Response: 0
Conc: N.D.

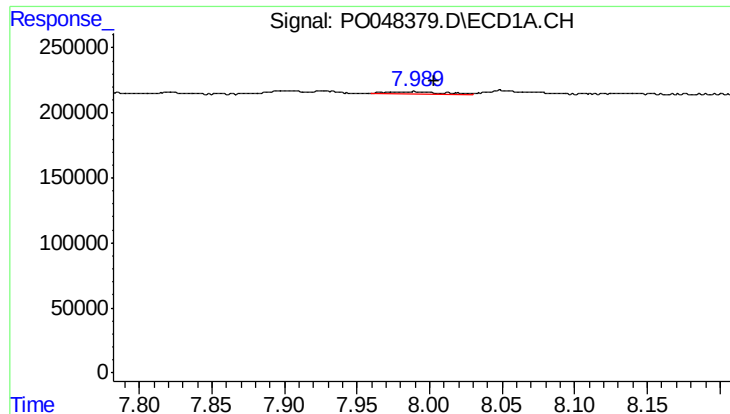

#39 AR-1262-4


R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 47948
Conc: 4.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

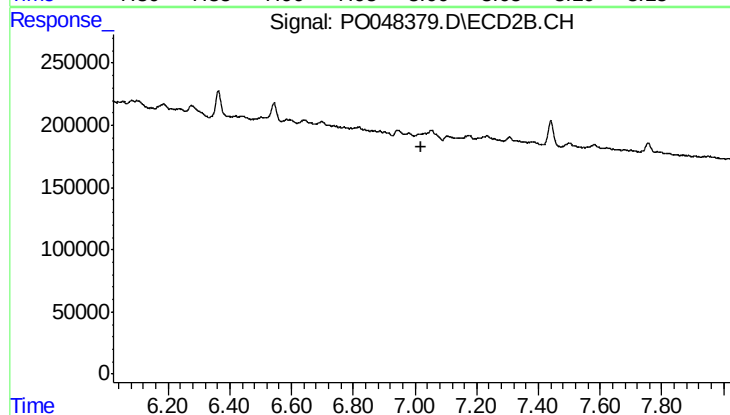


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 7.022 min
Response: 0
Conc: N.D.

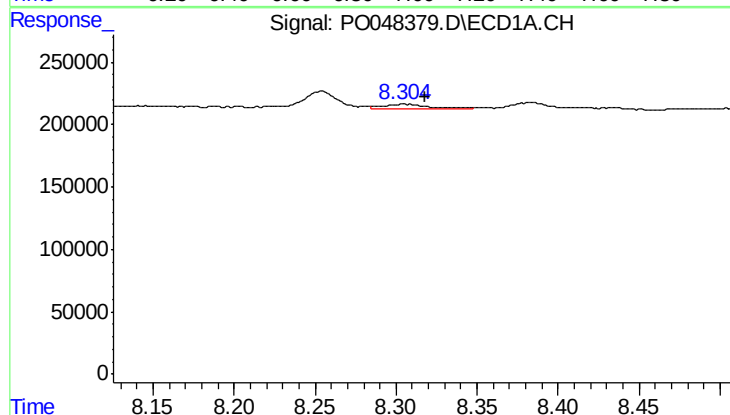


#40 AR-1262-5

R.T.: 8.304 min
Delta R.T.: -0.014 min
Response: 84231
Conc: 3.92 ng/ml

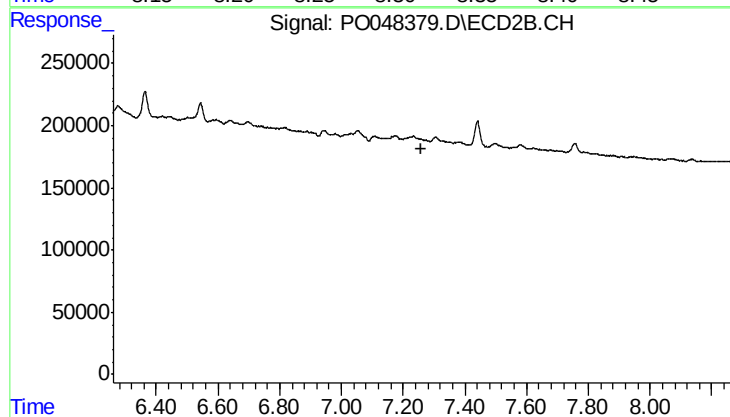

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.261 min
Response: 0
Conc: N.D.

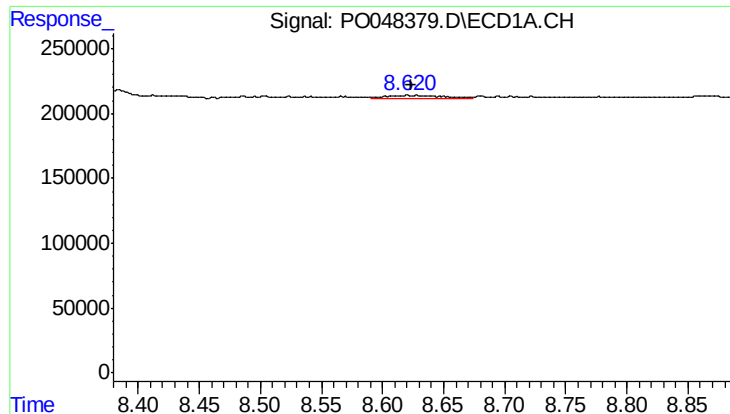

#41 AR-1268-1


R.T.: 8.620 min
Delta R.T.: -0.003 min
Response: 68598
Conc: 2.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

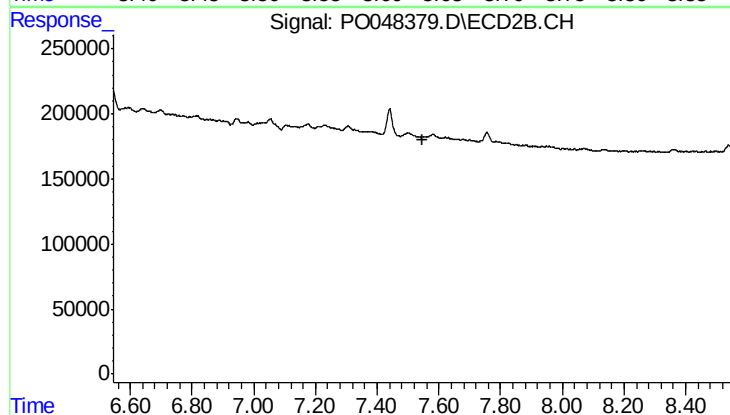


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 7.546 min
Response: 0
Conc: N.D.

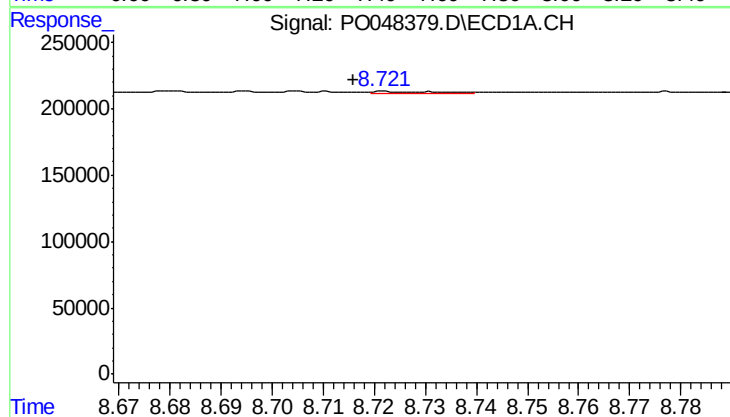


#42 AR-1268-2

R.T.: 8.722 min
Delta R.T.: 0.006 min
Response: 10559
Conc: 0.49 ng/ml

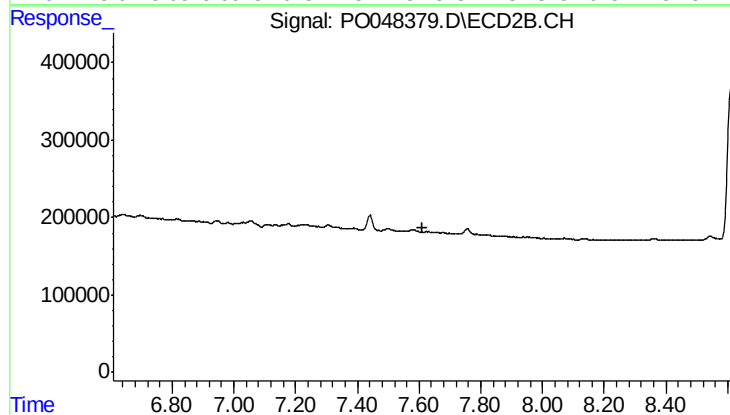

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 7.609 min
Response: 0
Conc: N.D.

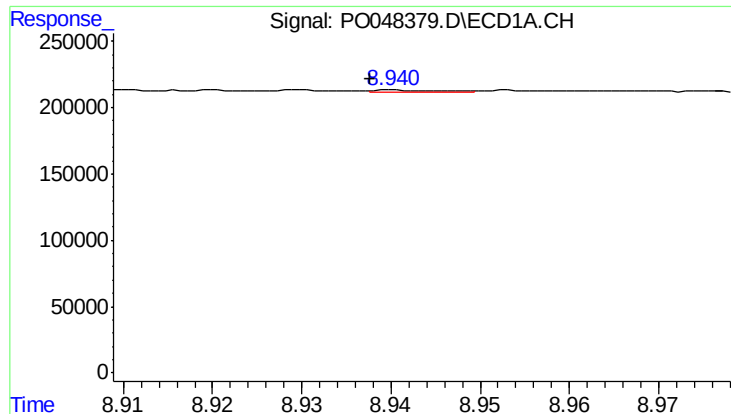

#43 AR-1268-3


R.T.: 8.940 min
Delta R.T.: 0.003 min
Response: 5839
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

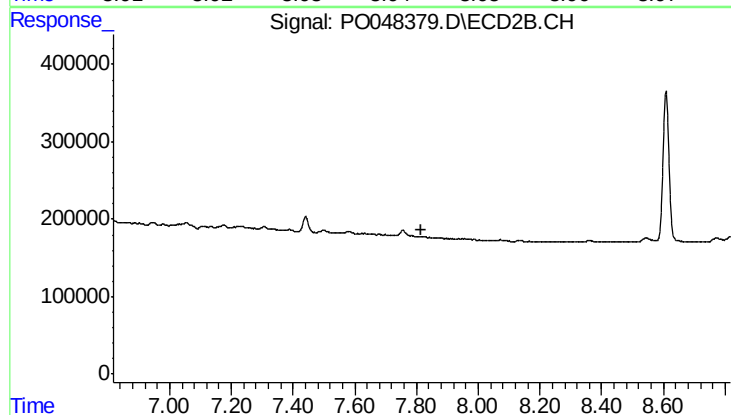


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 7.817 min
Response: 0
Conc: N.D.

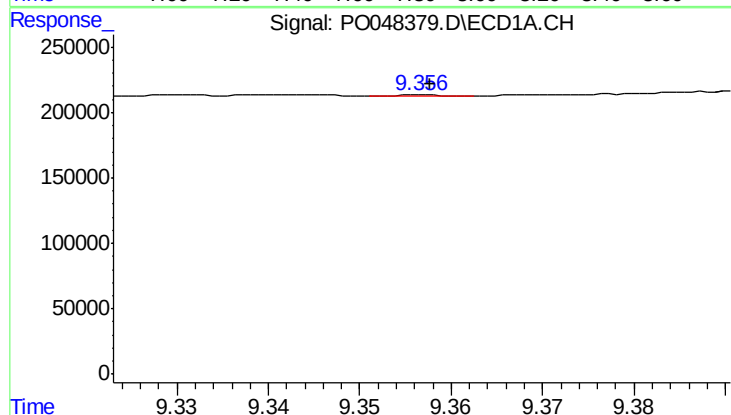


#44 AR-1268-4

R.T.: 9.357 min
Delta R.T.: -0.001 min
Response: 4867
Conc: 0.61 ng/ml

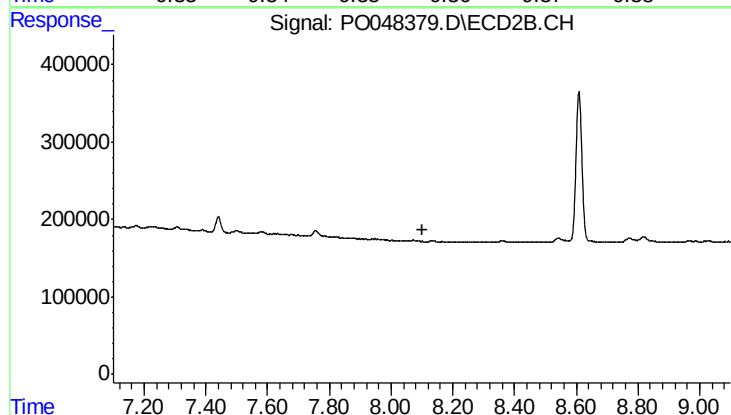

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.101 min
Response: 0
Conc: N.D.

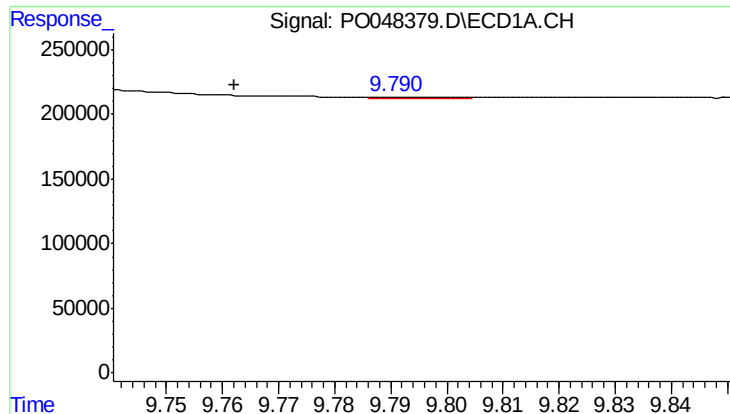

#45 AR-1268-5

R.T.: 9.790 min
Delta R.T.: 0.028 min
Response: 8815
Conc: 0.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER

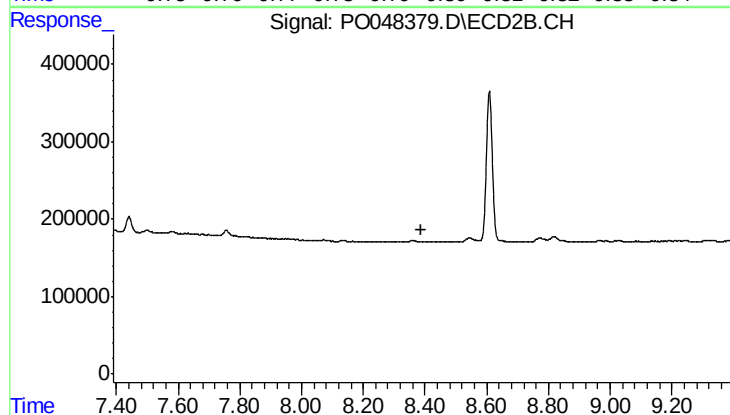

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.390 min
Response: 0
Conc: N.D.