

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0082118\
 Data File : P0048379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2018 19:31
 Operator : SM/SJ
 Sample : J4539-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MS-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 8/22/2018 5:08:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:01:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 27 02:33:29 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.631	3390327	4693563	16.792	19.102m
2) SA Decachlor...	10.072	8.609	2558699	2571095	15.688	16.356m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082118\
Data File : P0048379.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2018 19:31
Operator : SM/SJ
Sample : J4539-06
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 5:08:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:01:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

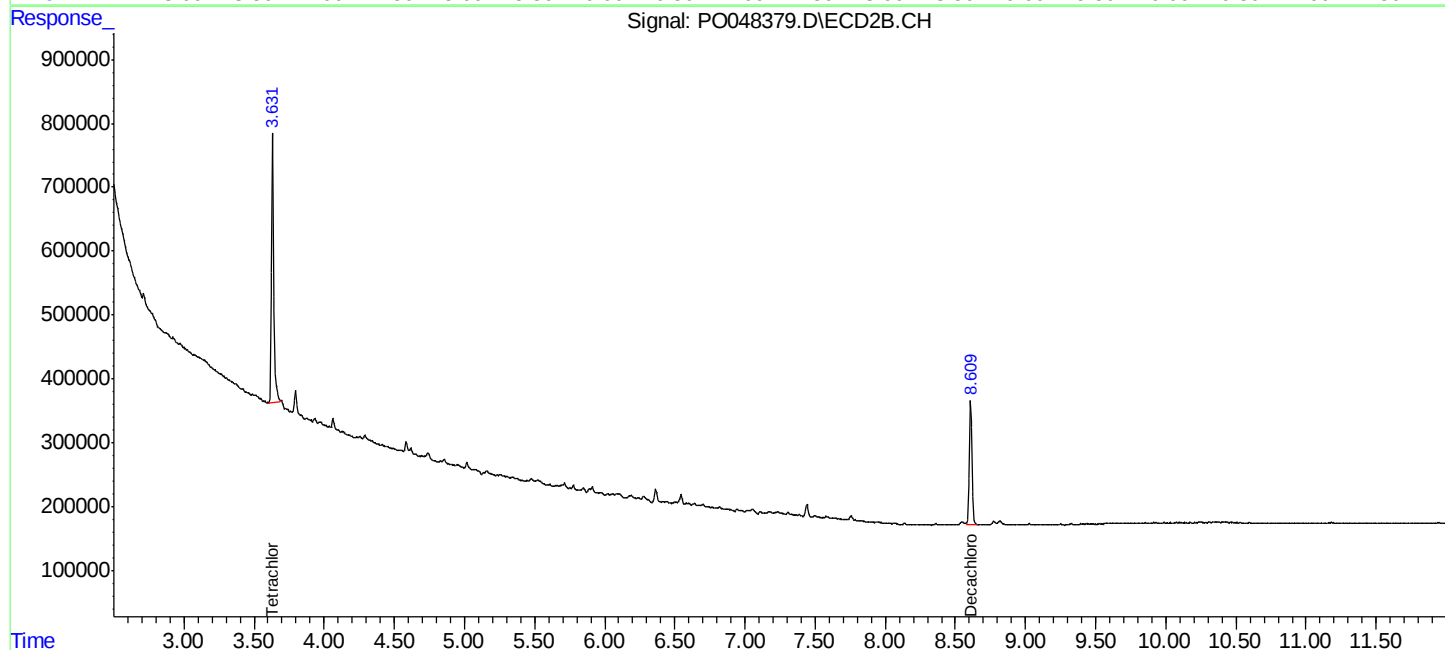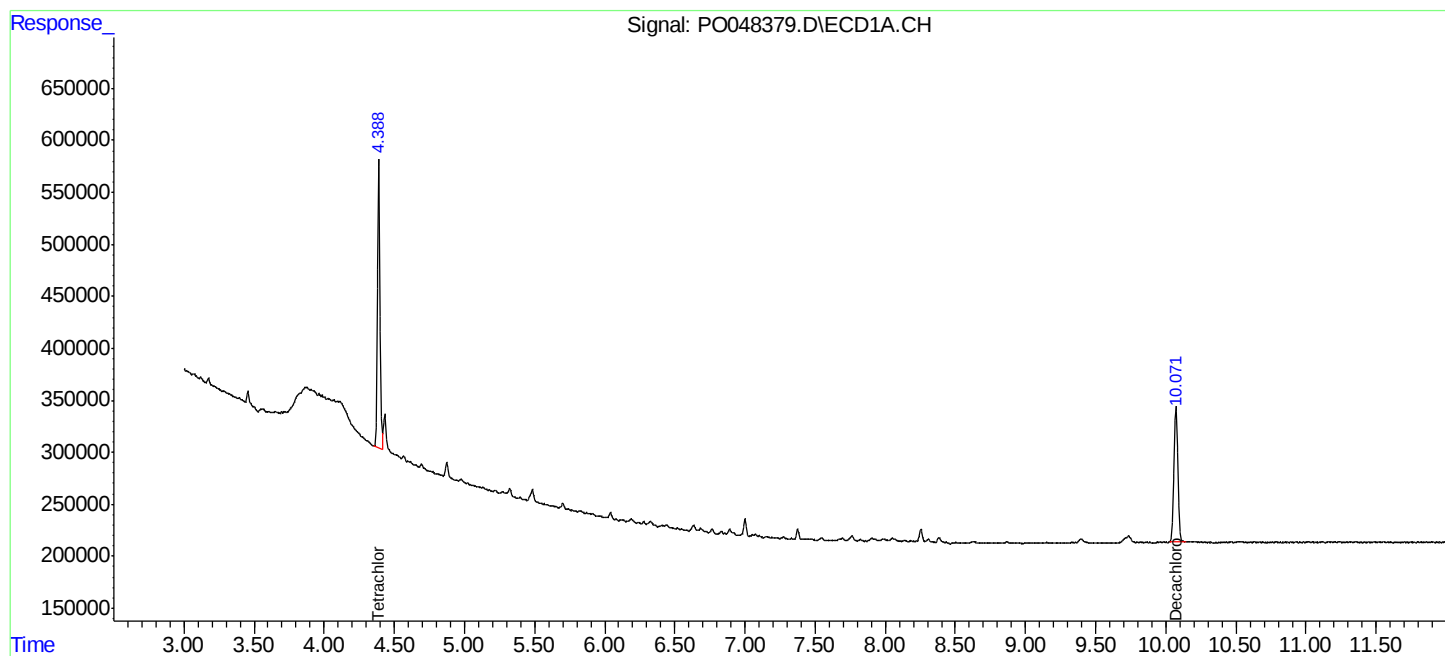

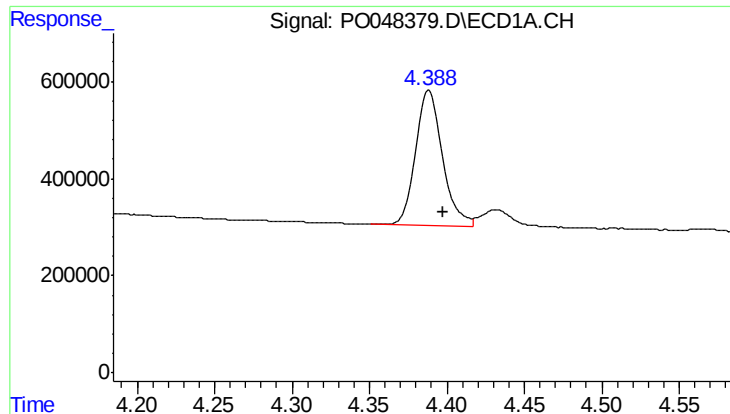


#1 Tetrachloro-m-xylene

R.T.: 4.388 min
Delta R.T.: -0.009 min
Response: 3390327
Conc: 16.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 5:08:08 PM

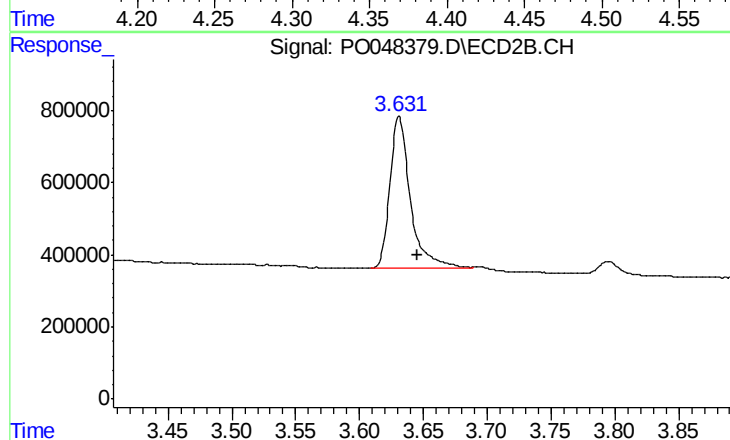


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.015 min
Response: 4693563
Conc: 19.10 ng/ml m

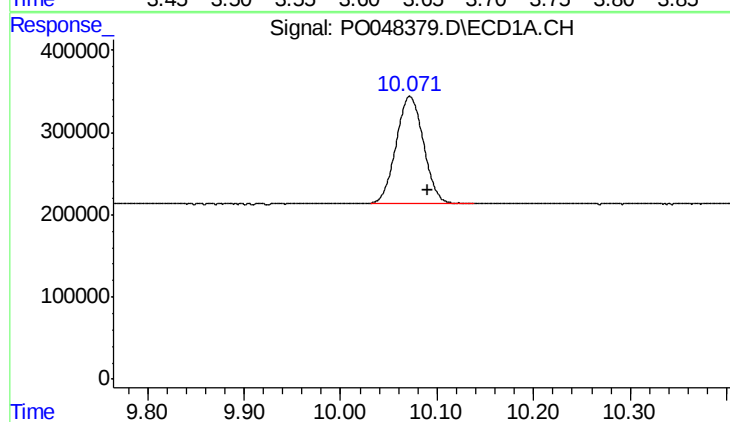

#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: -0.018 min
Response: 2558699
Conc: 15.69 ng/ml

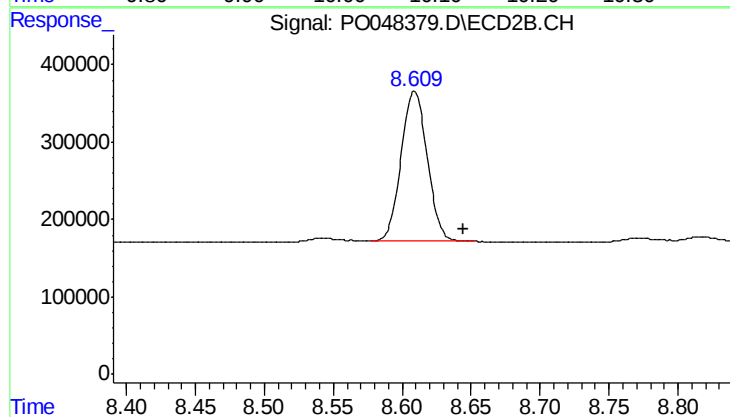

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: -0.036 min
Response: 2571095
Conc: 16.36 ng/ml m