

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082120\
 Data File : P0070755.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2020 12:08
 Operator : DD\AJ
 Sample : L3740-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-3A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 14:36:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.542	1841570	1074537	26.436	26.692
2) SA Decachlor...	9.983	8.732	2038311	1155054	21.772	20.512

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082120\
Data File : PO070755.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2020 12:08
Operator : DD\AJ
Sample : L3740-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-3A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 14:36:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

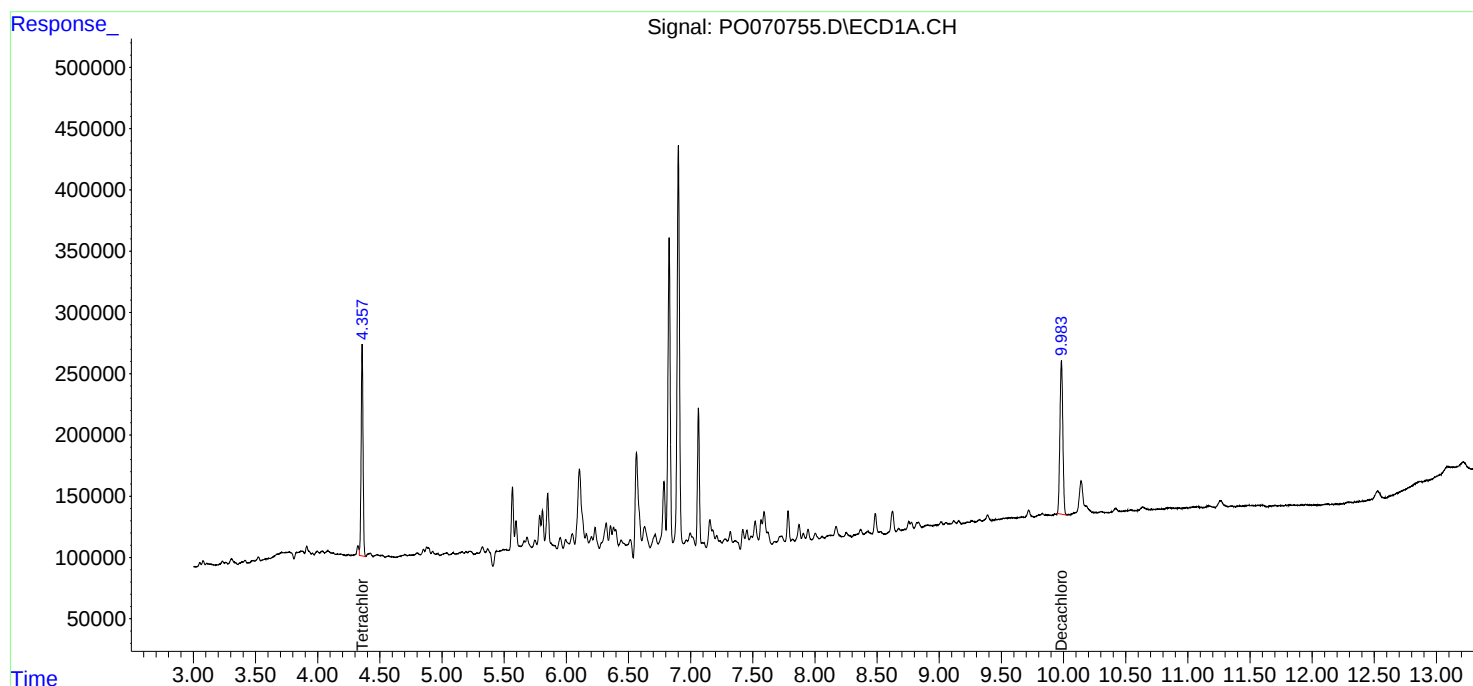


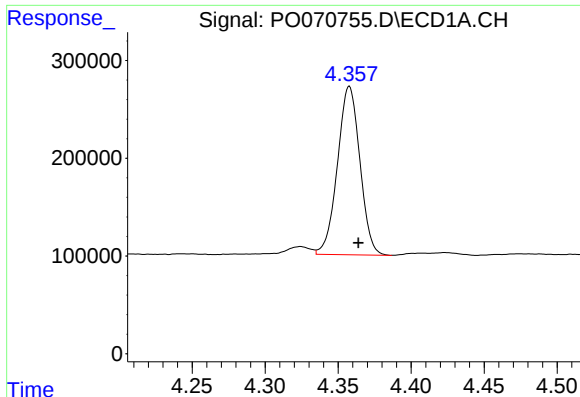

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: -0.006 min
Response: 1841570
Conc: 26.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-3A

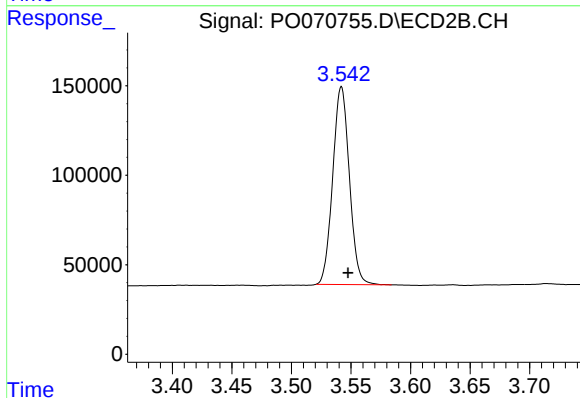


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.006 min
Response: 1074537
Conc: 26.69 ng/ml

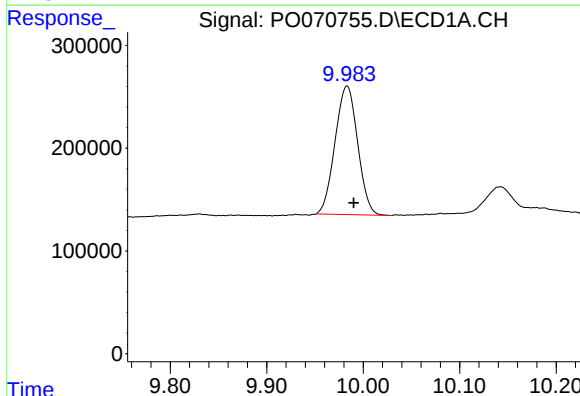

#2 Decachlorobiphenyl

R.T.: 9.983 min
Delta R.T.: -0.007 min
Response: 2038311
Conc: 21.77 ng/ml

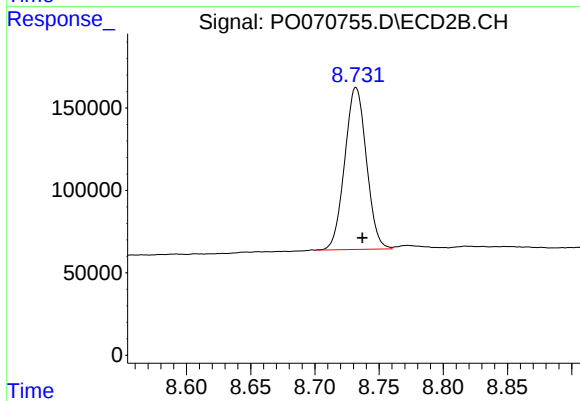

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.005 min
Response: 1155054
Conc: 20.51 ng/ml