

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082120\
 Data File : P0070760.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2020 13:33
 Operator : DD\AJ
 Sample : L3504-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-081920

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 14:38:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.358	3.543	1687708	1076870	24.227	26.750
2) SA Decachlor...	9.984	8.732	1682757	975931	17.974	17.331

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082120\
Data File : PO070760.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2020 13:33
Operator : DD\AJ
Sample : L3504-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-01-081920

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 14:38:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

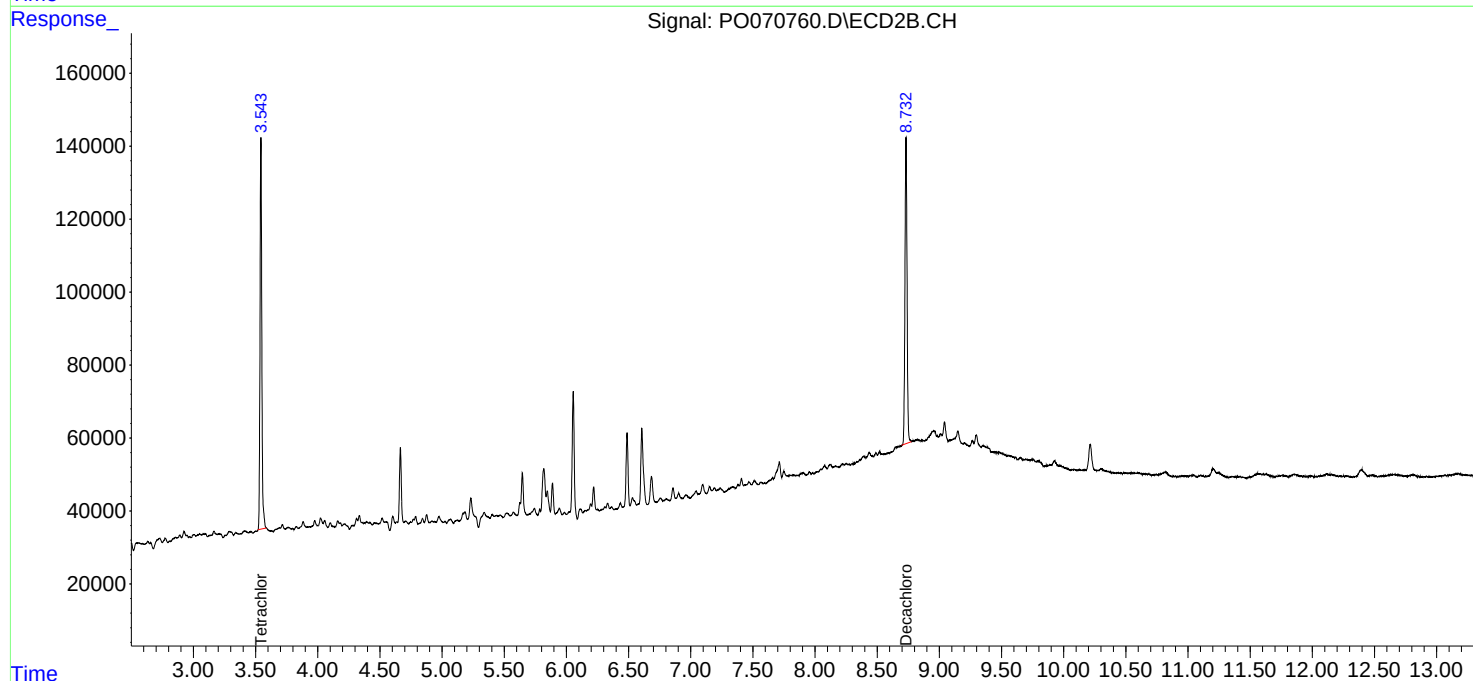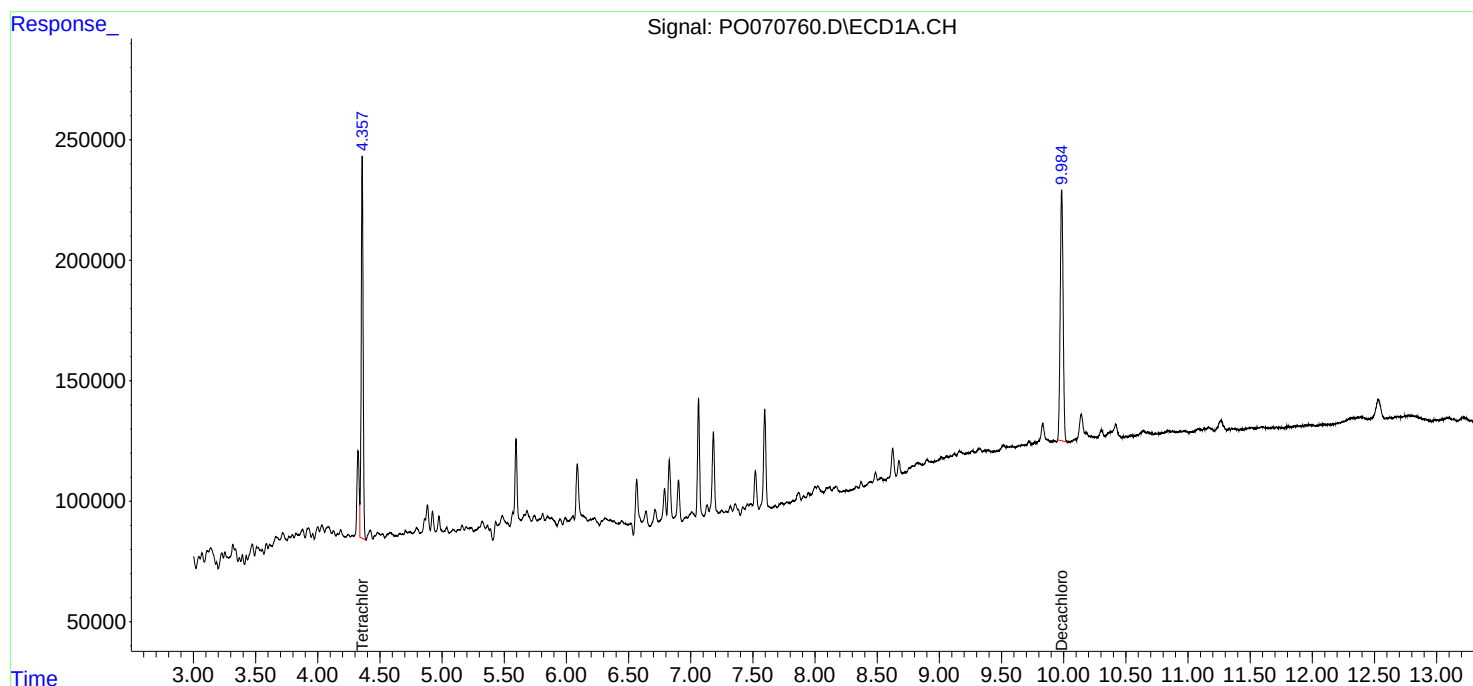


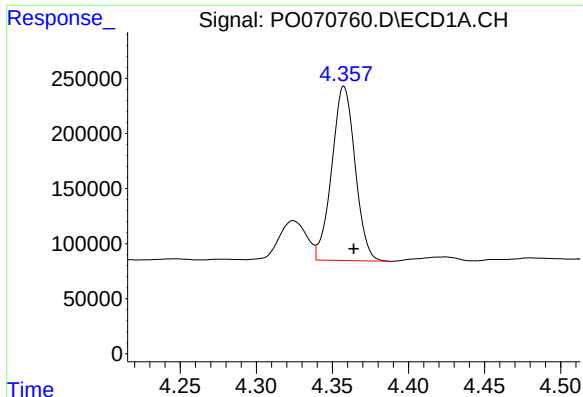

#1 Tetrachloro-m-xylene


R.T.: 4.358 min
Delta R.T.: -0.006 min
Response: 1687708
Conc: 24.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-01-081920

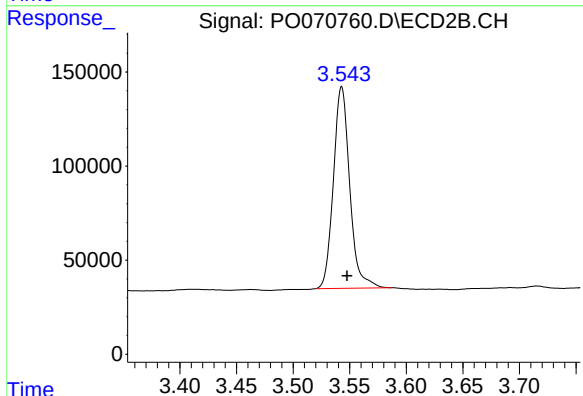


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.005 min
Response: 1076870
Conc: 26.75 ng/ml

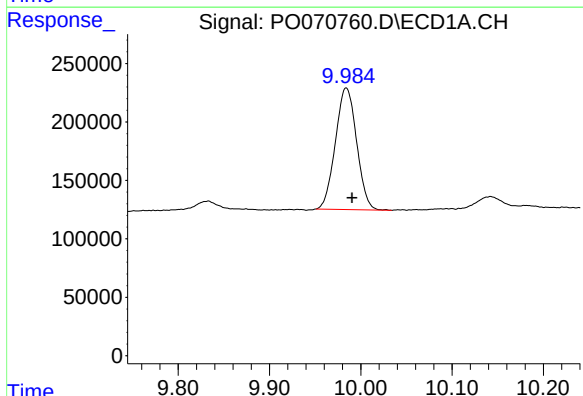

#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: -0.006 min
Response: 1682757
Conc: 17.97 ng/ml

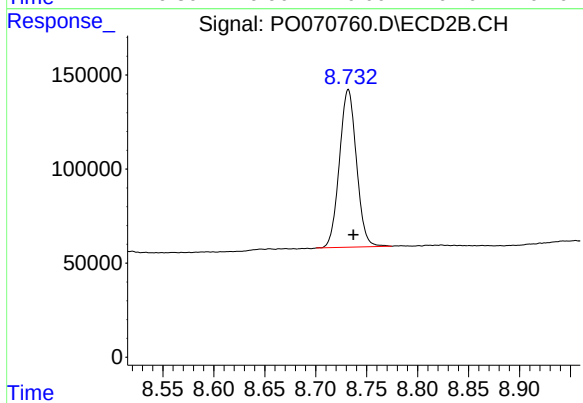

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.005 min
Response: 975931
Conc: 17.33 ng/ml