

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082120\
 Data File : P0070761.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2020 13:50
 Operator : DD\AJ
 Sample : L3720-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MP-081920-B9-0-2-COMP

Manual Integrations
 APPROVED

Ankita
 8/24/2020 11:28:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 14:39:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359	3.544	1641595	1094658	23.565	27.192
2) SA Decachlor...	9.984	8.732	1434706	812975	15.325	14.437

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082120\
Data File : PO070761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2020 13:50
Operator : DD\AJ
Sample : L3720-09
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MP-081920-B9-0-2-COMP


Manual Integrations
APPROVED

Ankita
8/24/2020 11:28:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 14:39:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

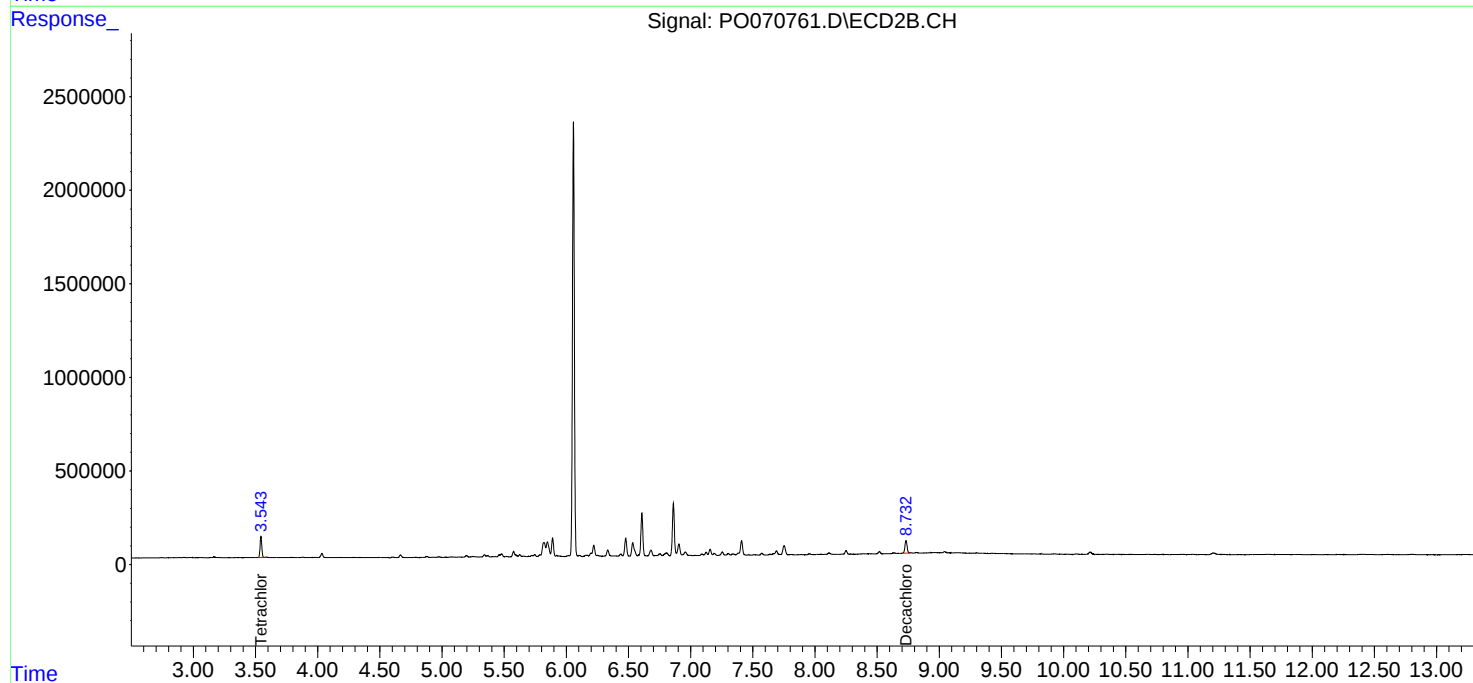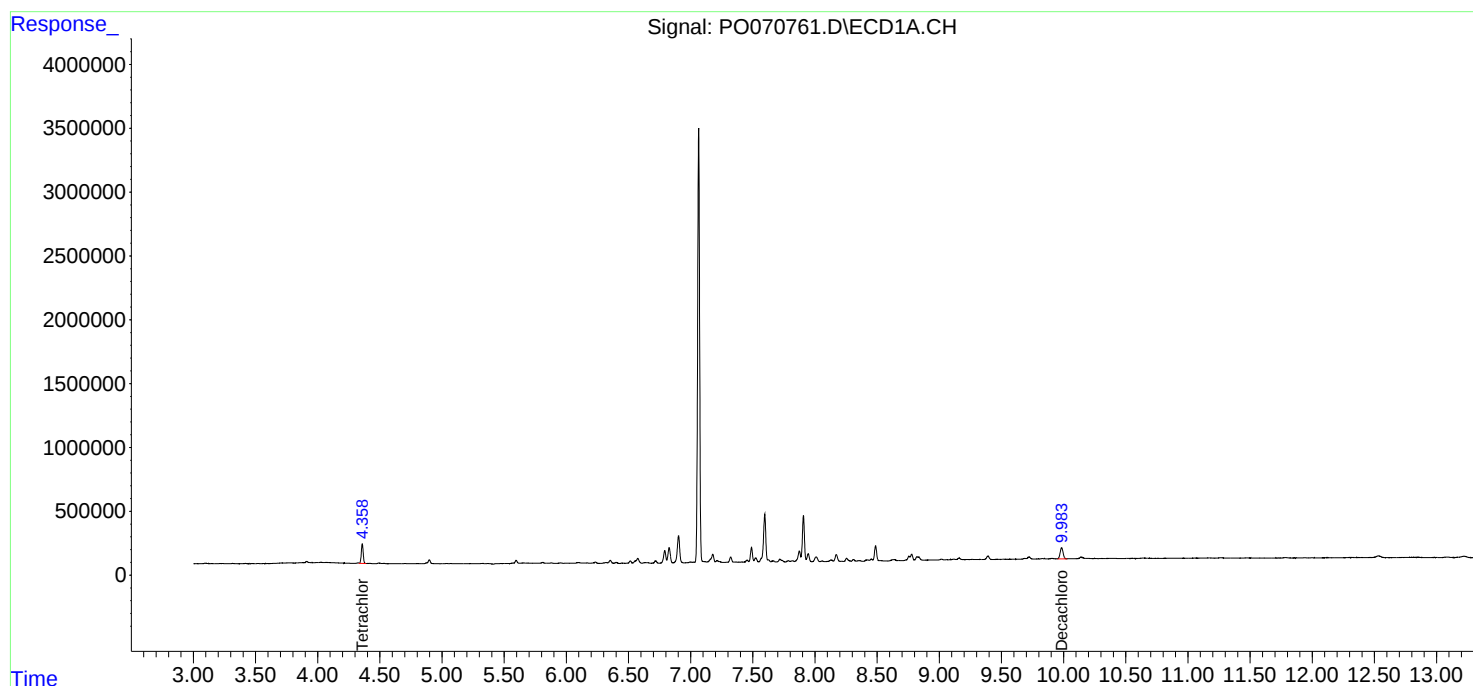

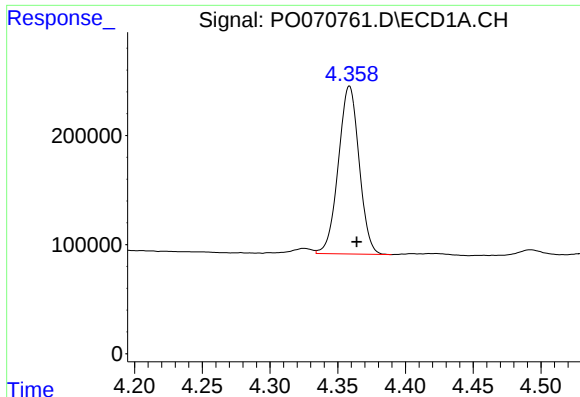


#1 Tetrachloro-m-xylene

R.T.: 4.359 min
Delta R.T.: -0.005 min
Response: 1641595
Conc: 23.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MP-081920-B9-0-2-COMP


Manual Integrations
APPROVED

Ankita
8/24/2020 11:28:23 AM

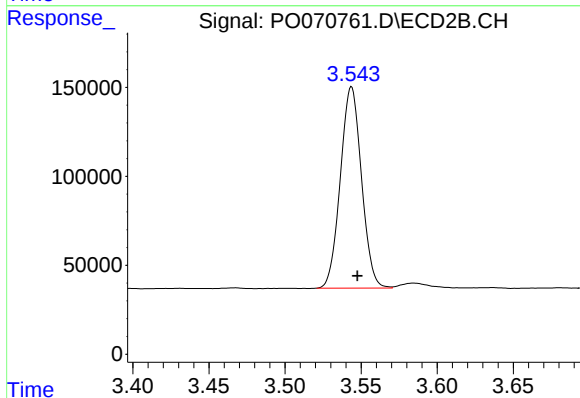


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.004 min
Response: 1094658
Conc: 27.19 ng/ml

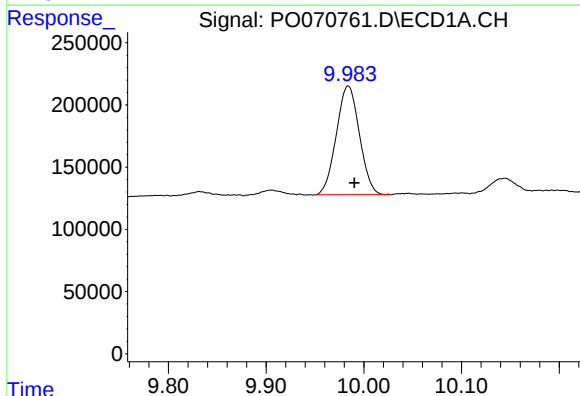

#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: -0.006 min
Response: 1434706
Conc: 15.32 ng/ml

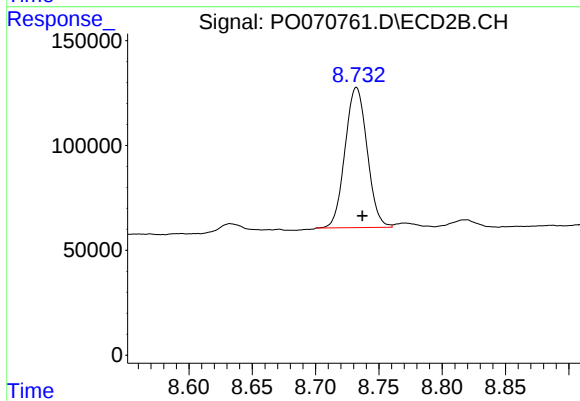

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.005 min
Response: 812975
Conc: 14.44 ng/ml