

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082124\
 Data File : P0105680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 14:21
 Operator : YP/AJ
 Sample : P3683-07 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HED930S-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/22/2024
 Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 02:50:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.724	9246937	3588851	0.989m	1.407m#
2) SA Decachlor...	10.198	8.767	7282066	2776616	1.255	1.407

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082124\
Data File : PO105680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 14:21
Operator : YP/AJ
Sample : P3683-07 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HED930S-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2024
Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 02:50:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

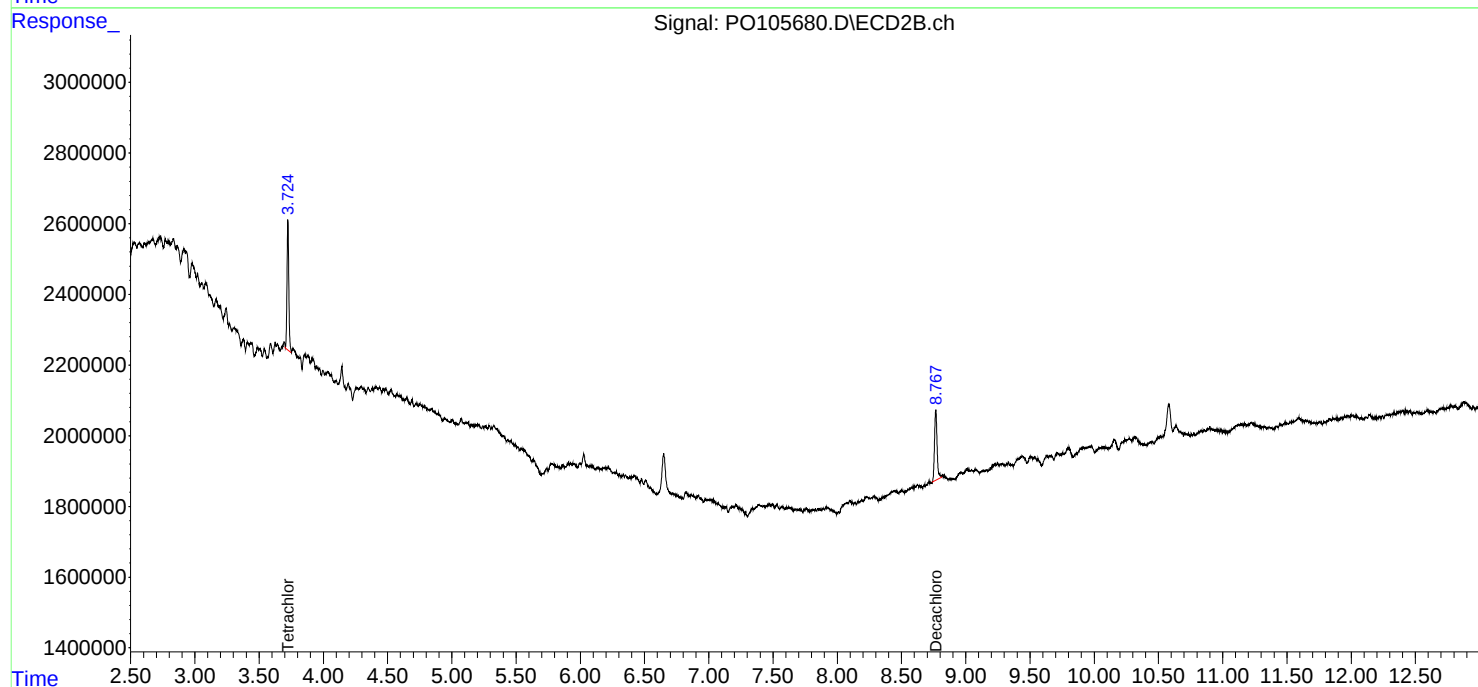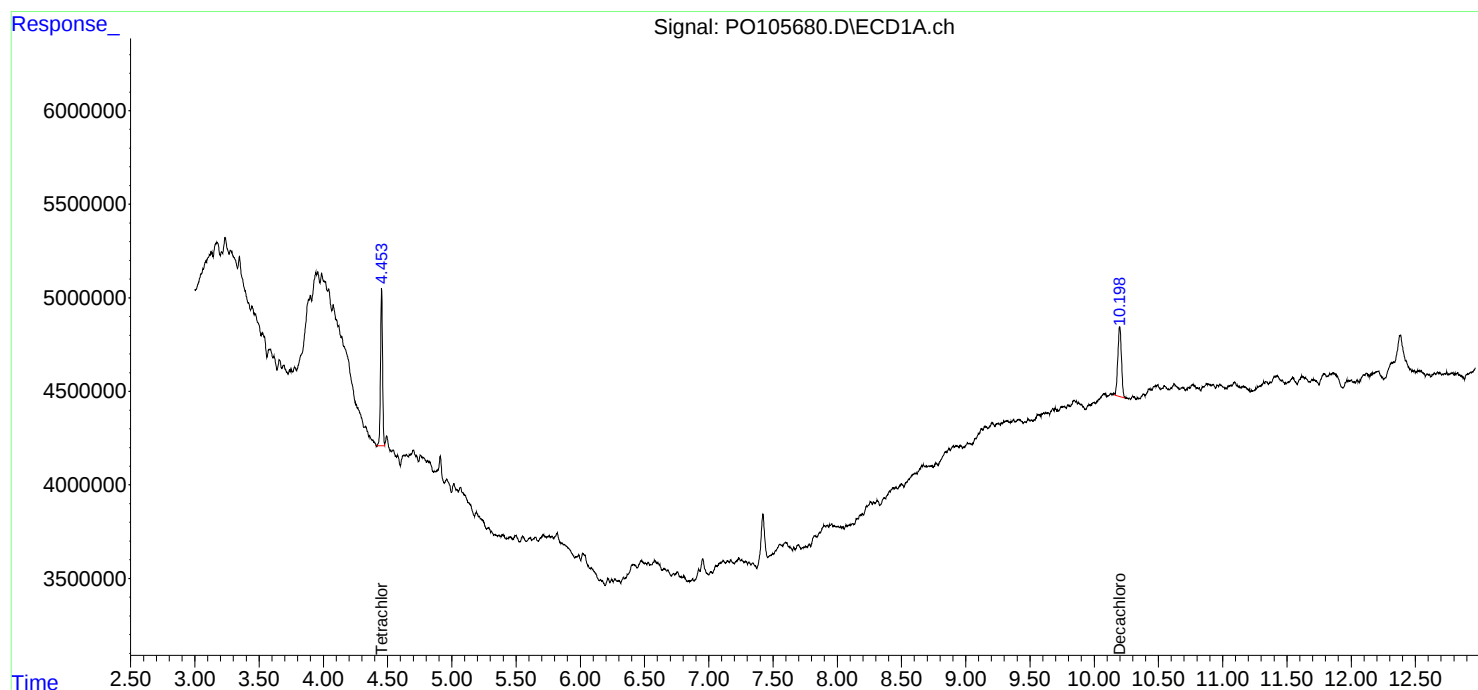

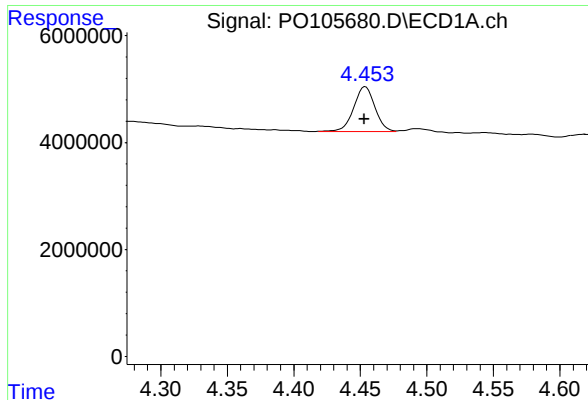


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 9246937
Conc: 0.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
HED930S-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2024
Supervised By :Ankita Jodhani 08/22/2024

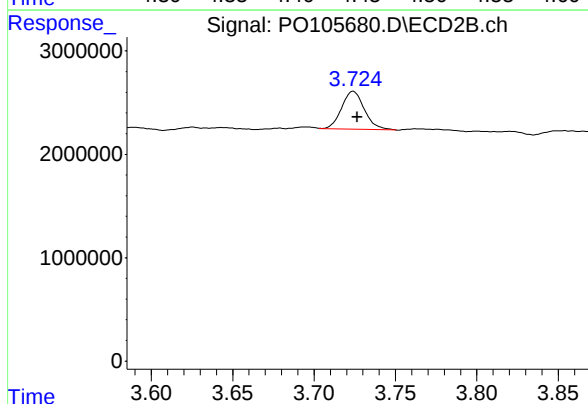


#1 Tetrachloro-m-xylene

R.T.: 3.724 min
Delta R.T.: -0.003 min
Response: 3588851
Conc: 1.41 ng/ml m

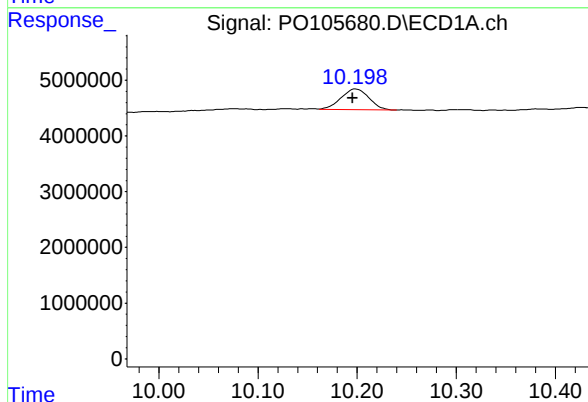

#2 Decachlorobiphenyl

R.T.: 10.198 min
Delta R.T.: 0.003 min
Response: 7282066
Conc: 1.25 ng/ml

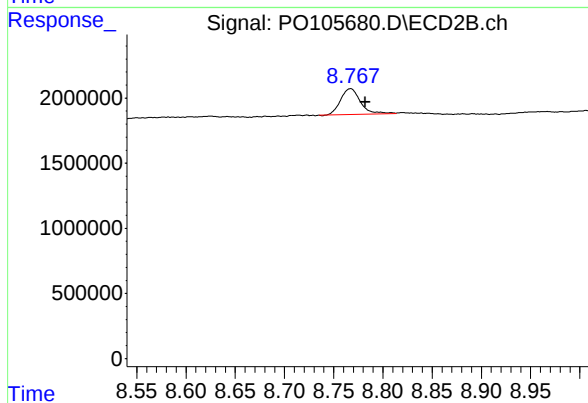

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.015 min
Response: 2776616
Conc: 1.41 ng/ml