

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082225\
 Data File : P0113175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2025 12:36
 Operator : YP/AJ
 Sample : Q2914-19 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K262-15A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/25/2025
 Supervised By :mohammad ahmed 08/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 01:59:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.662	3.653	15844919	9087155	1.935	1.796
2) SA Decachlor...	8.685	8.631	19725695	5691406	2.846m	3.004m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082225\
Data File : PO113175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2025 12:36
Operator : YP/AJ
Sample : Q2914-19 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K262-15A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/25/2025
Supervised By :mohammad ahmed 08/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 01:59:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

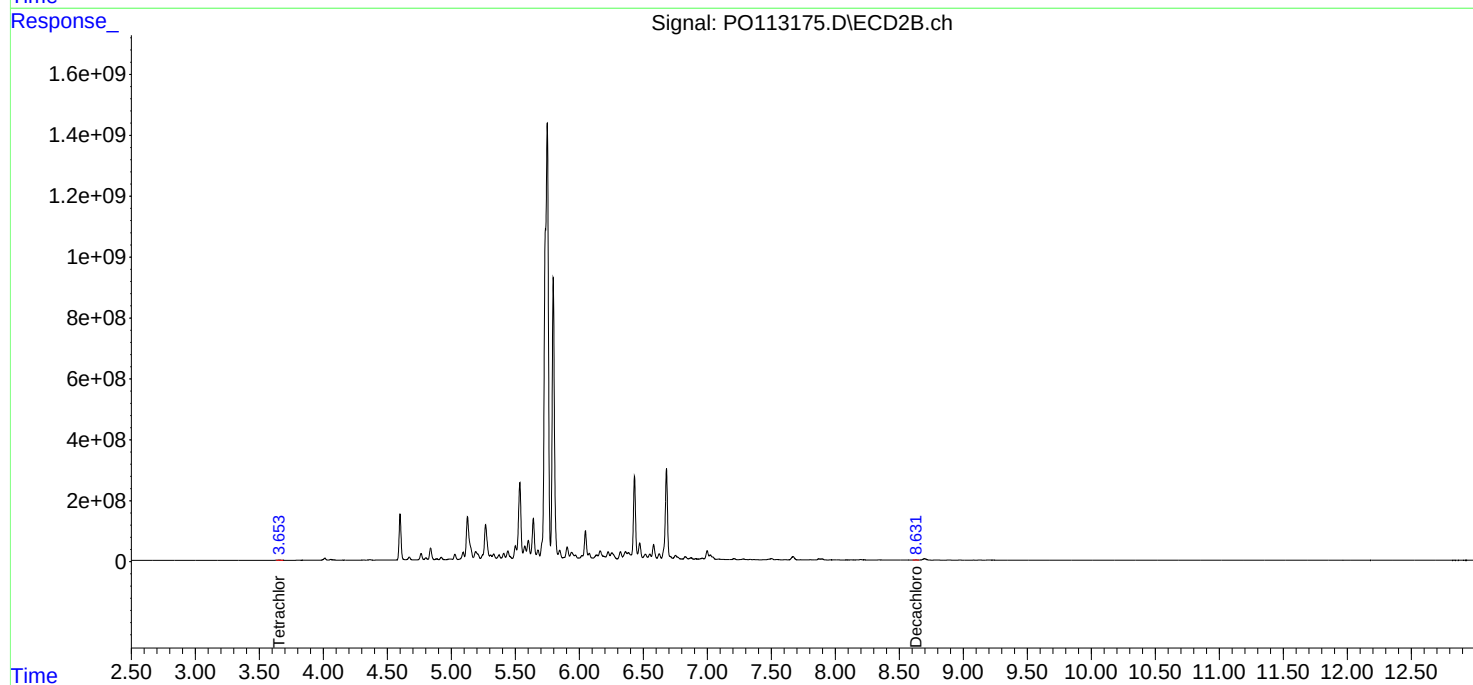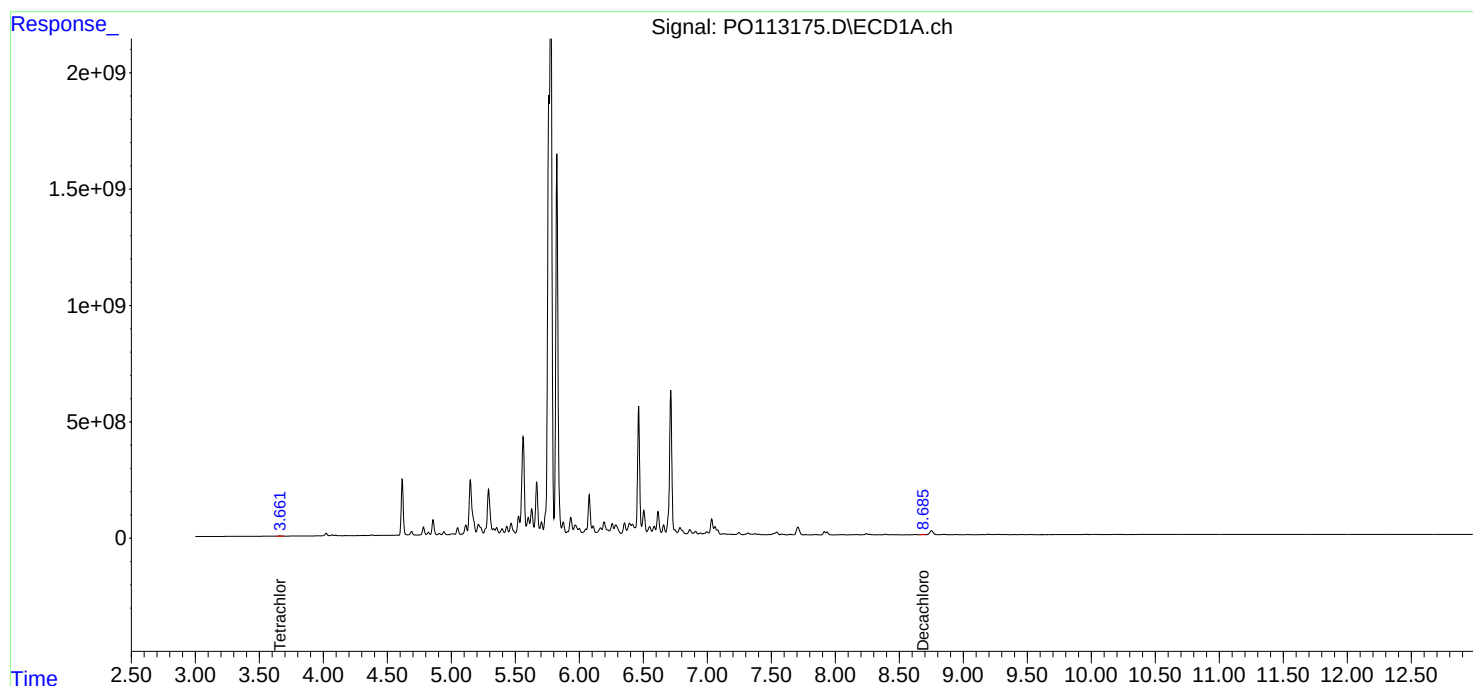

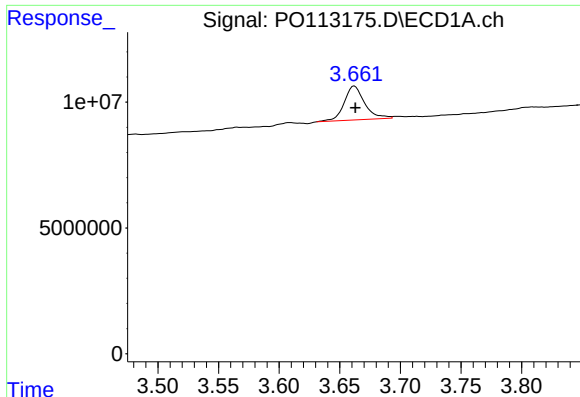

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 15844919
Conc: 1.94 ng/ml

Instrument :

ECD_O

ClientSampleId :


K262-15A

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 08/25/2025

Supervised By :mohammad ahmed 08/28/2025

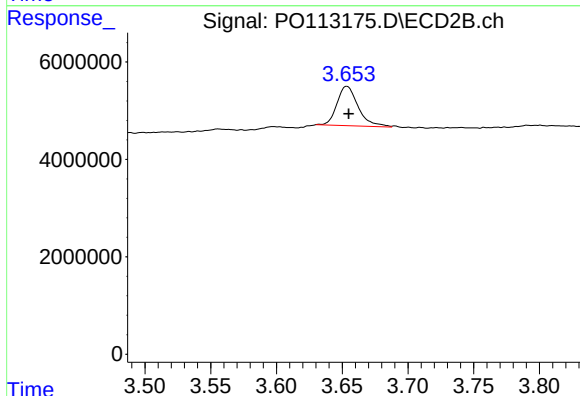


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.001 min
Response: 9087155
Conc: 1.80 ng/ml

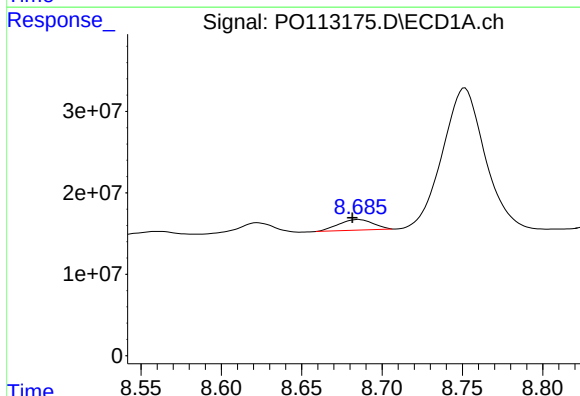

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: 0.003 min
Response: 19725695
Conc: 2.85 ng/ml m

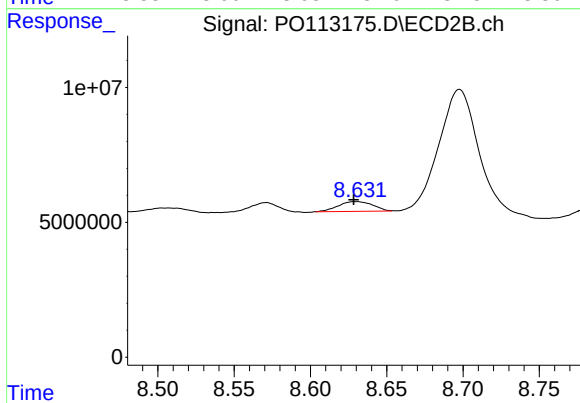

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: 0.003 min
Response: 5691406
Conc: 3.00 ng/ml m