

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0082319\
 Data File : P0059724.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Aug 2019 9:39
 Operator : SM/AJ
 Sample : K4471-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 S703-N-0.0-0.5-082119-FDRE

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 12:25:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.126	3.498	871523	793743	24.892	22.051
2) SA Decachlor...	9.602	8.361	496049	440936	9.324	10.936
Target Compounds						
31) L7 AR-1260-1	6.853	5.996	238107	174687	88.325m	76.654m
32) L7 AR-1260-2	7.109	6.183	477471	279752	128.682m	95.483m#
33) L7 AR-1260-3	7.464	6.331	328664	221883	100.315m	83.757m
34) L7 AR-1260-4	7.691	6.795	295009	181520	96.053m	80.227
35) L7 AR-1260-5	7.999	7.037	549562	506907	77.612m	92.109

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082319\
Data File : PO059724.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2019 9:39
Operator : SM/AJ
Sample : K4471-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S703-N-0.0-0.5-082119-FDRE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:25:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

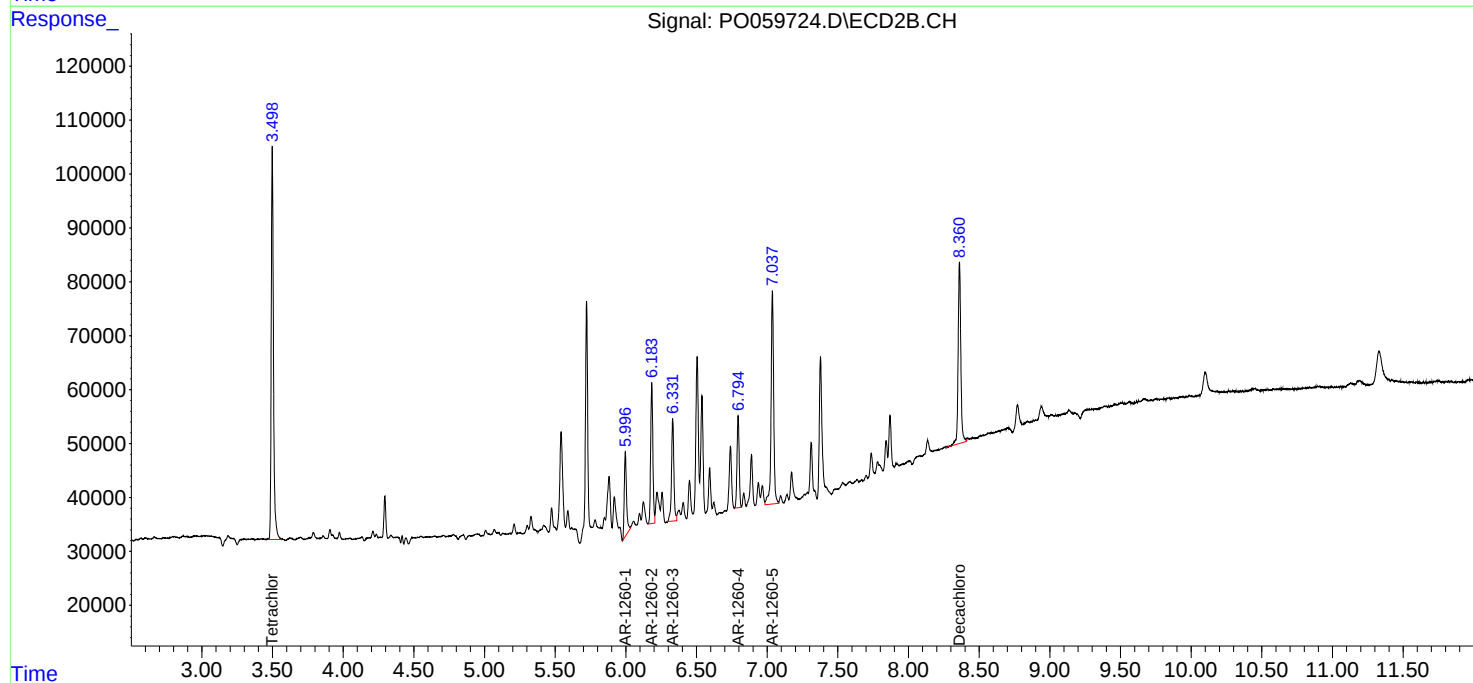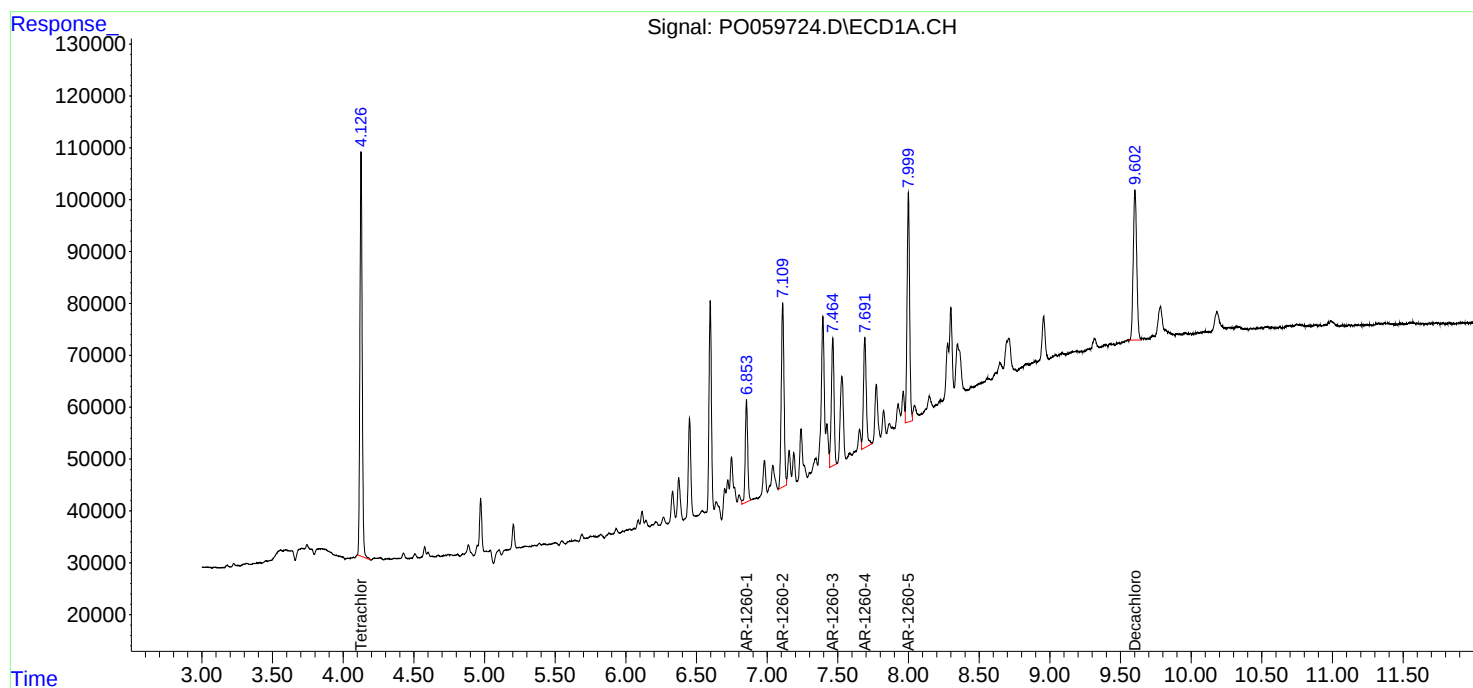

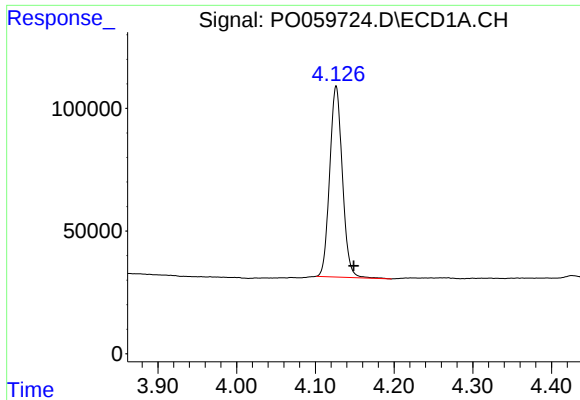


#1 Tetrachloro-m-xylene

R.T.: 4.126 min
Delta R.T.: -0.023 min
Response: 871523
Conc: 24.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
S703-N-0.0-0.5-082119-FDRE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:27 PM

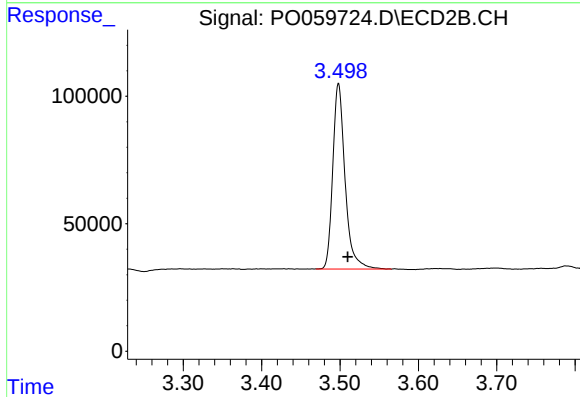


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.012 min
Response: 793743
Conc: 22.05 ng/ml

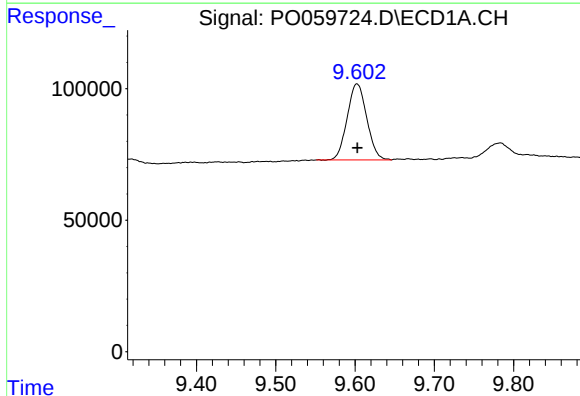


#2 Decachlorobiphenyl

R.T.: 9.602 min
Delta R.T.: 0.000 min
Response: 496049
Conc: 9.32 ng/ml

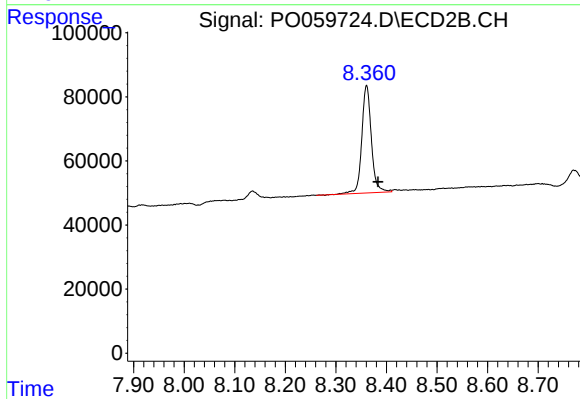

#2 Decachlorobiphenyl

R.T.: 8.361 min
Delta R.T.: -0.023 min
Response: 440936
Conc: 10.94 ng/ml

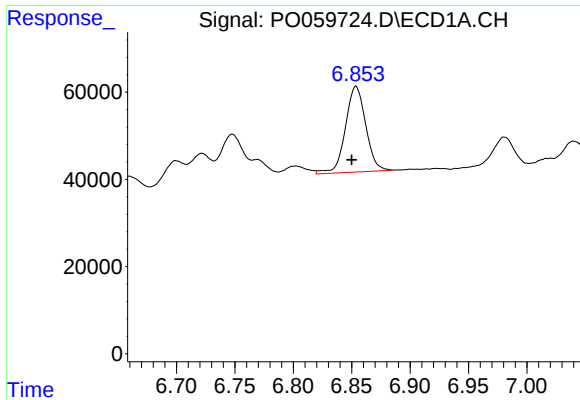


#31 AR-1260-1

R.T.: 6.853 min
Delta R.T.: 0.003 min
Response: 238107
Conc: 88.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S703-N-0.0-0.5-082119-FDRE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:27 PM

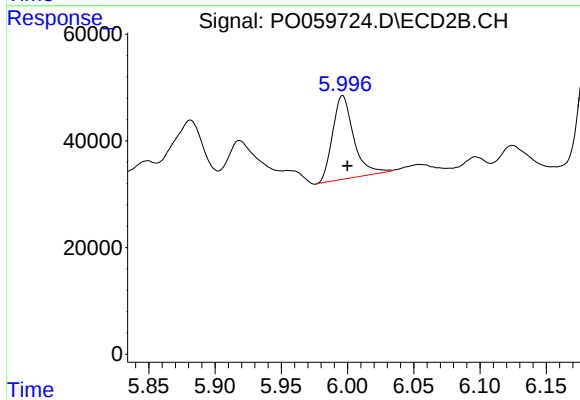


#31 AR-1260-1

R.T.: 5.996 min
Delta R.T.: -0.004 min
Response: 174687
Conc: 76.65 ng/ml m

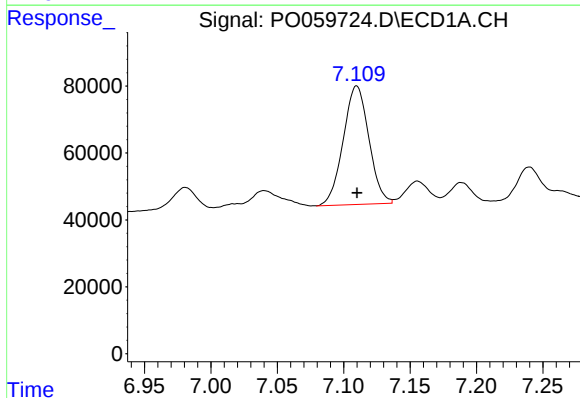


#32 AR-1260-2

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 477471
Conc: 128.68 ng/ml m

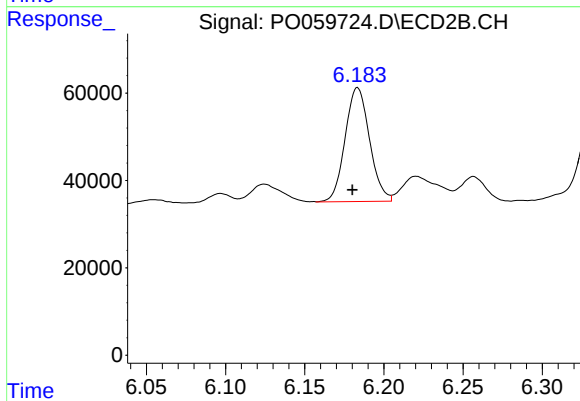

#32 AR-1260-2

R.T.: 6.183 min
Delta R.T.: 0.003 min
Response: 279752
Conc: 95.48 ng/ml m

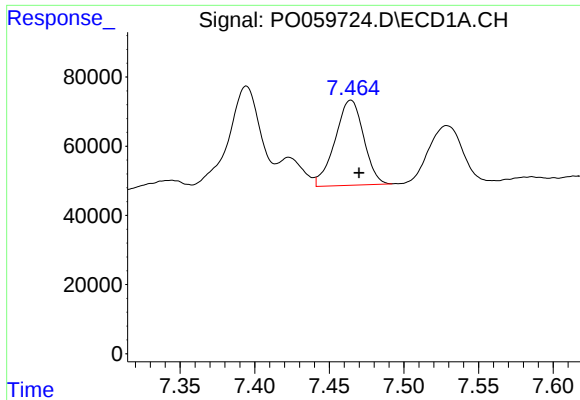


#33 AR-1260-3

R.T.: 7.464 min
Delta R.T.: -0.006 min
Response: 328664
Conc: 100.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S703-N-0.0-0.5-082119-FDRE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:27 PM

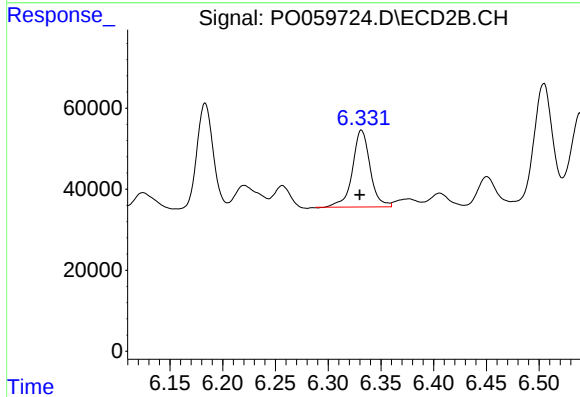


#33 AR-1260-3

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 221883
Conc: 83.76 ng/ml m

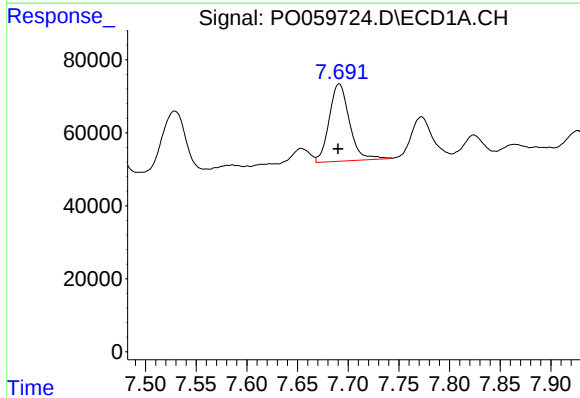


#34 AR-1260-4

R.T.: 7.691 min
Delta R.T.: 0.000 min
Response: 295009
Conc: 96.05 ng/ml m

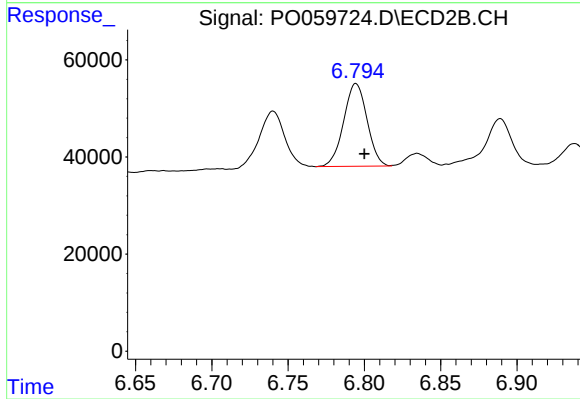

#34 AR-1260-4

R.T.: 6.795 min
Delta R.T.: -0.005 min
Response: 181520
Conc: 80.23 ng/ml

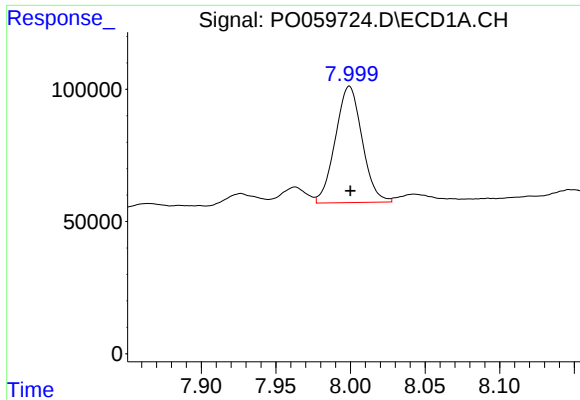


#35 AR-1260-5

R.T.: 7.999 min
Delta R.T.: -0.001 min
Response: 549562
Conc: 77.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S703-N-0.0-0.5-082119-FDRE

Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:27 PM

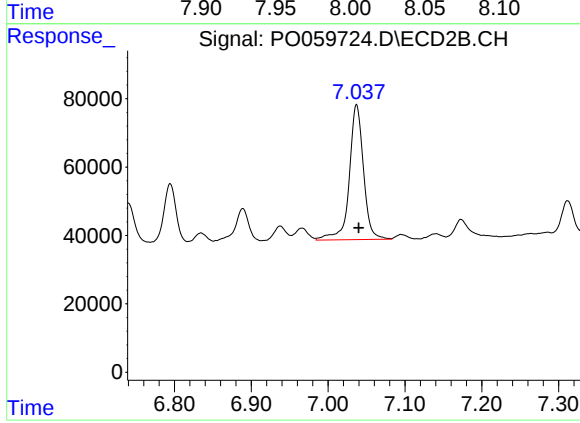

#35 AR-1260-5

R.T.: 7.037 min
Delta R.T.: -0.003 min
Response: 506907
Conc: 92.11 ng/ml