

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
 Data File : P0059730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Aug 2019 11:16
 Operator : SM/AJ
 Sample : K4497-03 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WEIR-TANK-082219-1

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:10:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 12:30:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.498	159993	155067	4.570	4.308
2) SA Decachlor...	9.598	8.358	202781	165682	3.812	4.109m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
Data File : P0059730.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2019 11:16
Operator : SM/AJ
Sample : K4497-03 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WEIR-TANK-082219-1


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:30:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

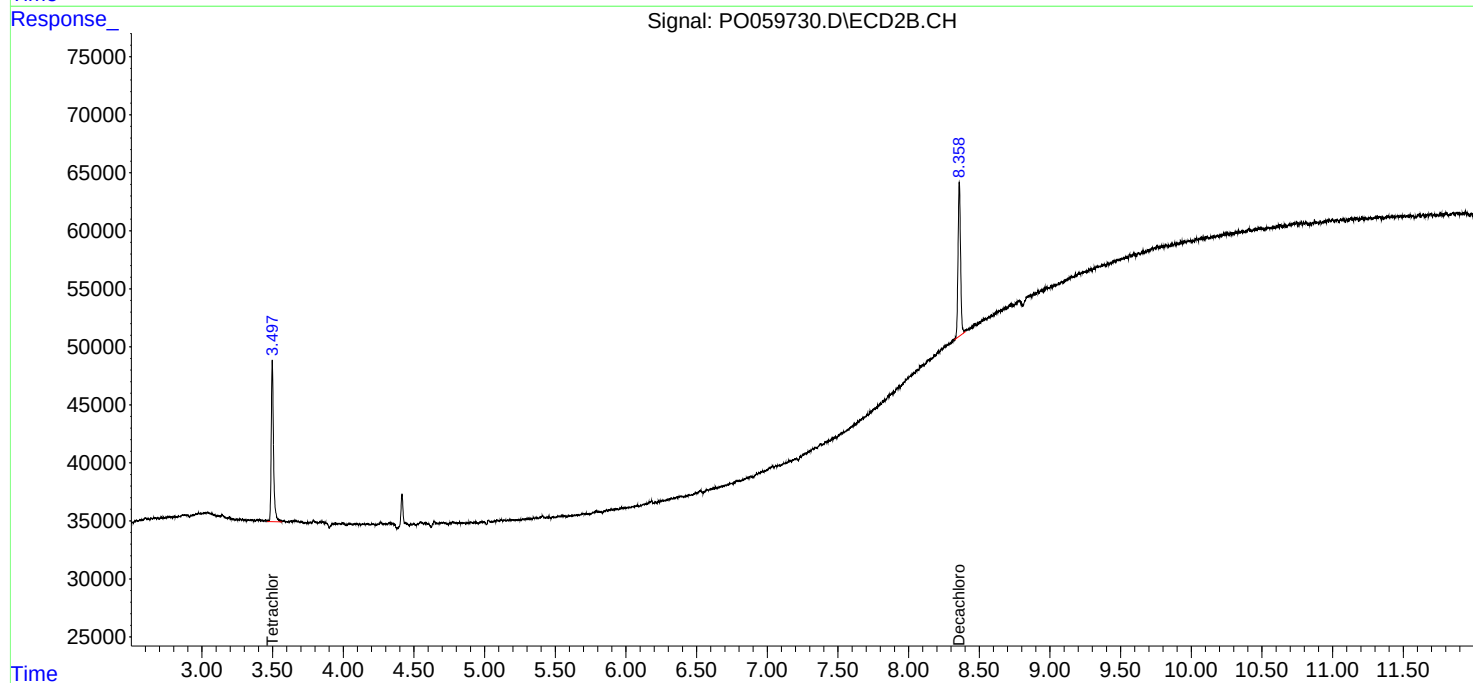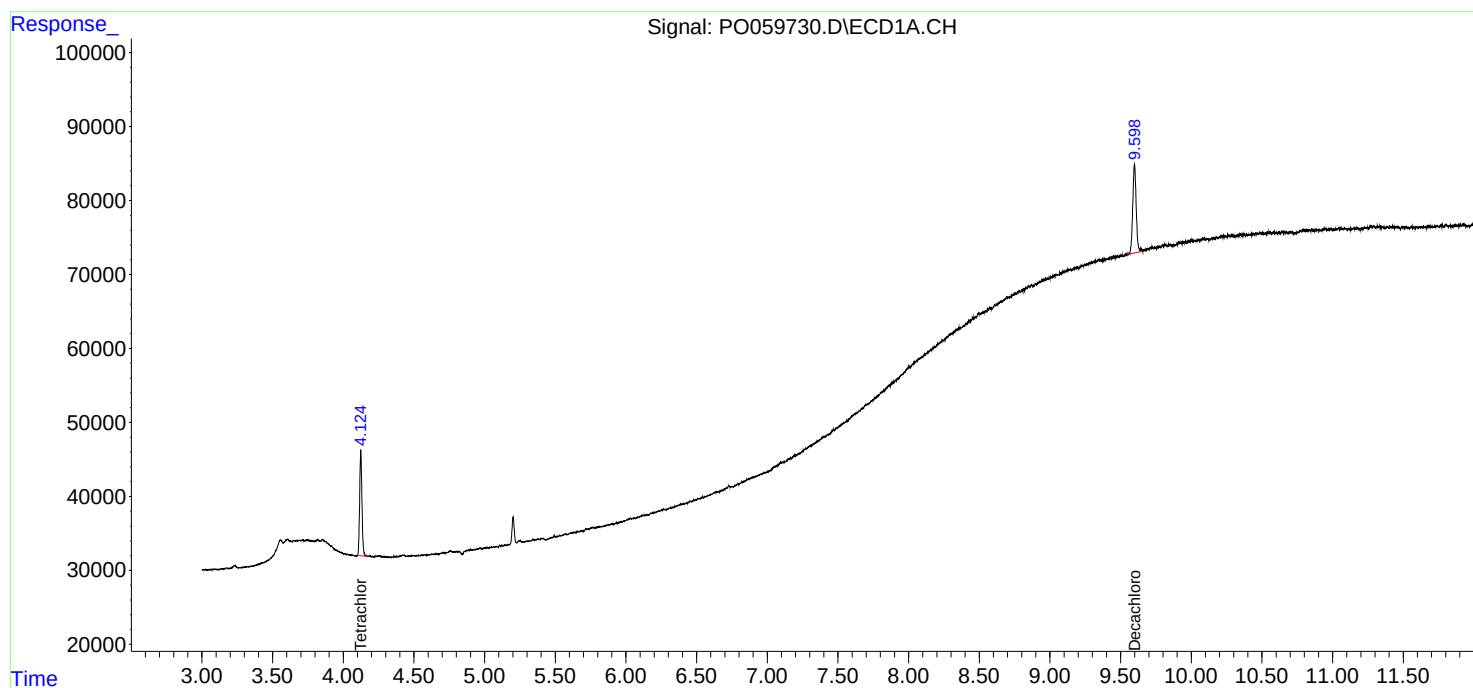

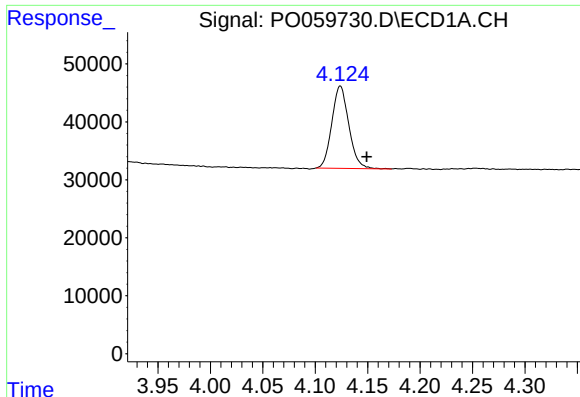


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.025 min
Response: 159993
Conc: 4.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
WEIR-TANK-082219-1


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:35 PM

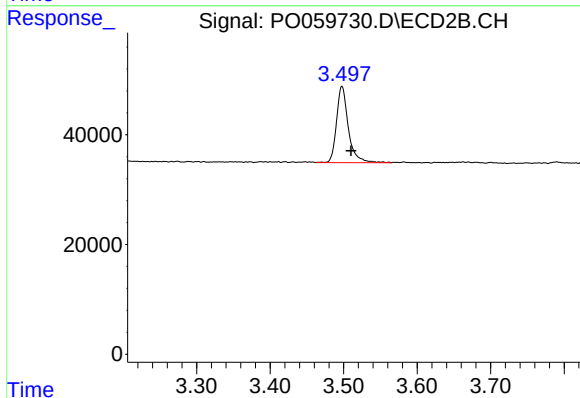


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.012 min
Response: 155067
Conc: 4.31 ng/ml

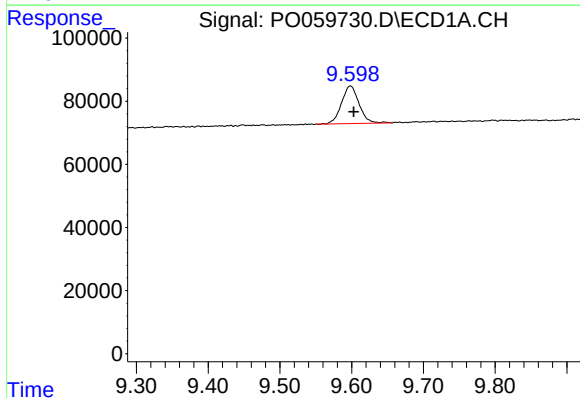

#2 Decachlorobiphenyl

R.T.: 9.598 min
Delta R.T.: -0.005 min
Response: 202781
Conc: 3.81 ng/ml

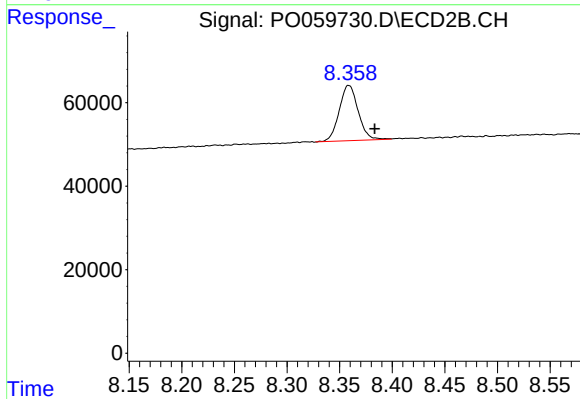

#2 Decachlorobiphenyl

R.T.: 8.358 min
Delta R.T.: -0.026 min
Response: 165682
Conc: 4.11 ng/ml m