

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
 Data File : P0059731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Aug 2019 11:32
 Operator : SM/AJ
 Sample : K4497-04 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WEIR-TANK-082219-2

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:10:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 12:31:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.125	3.498	189465	177481	5.411	4.931
2) SA Decachlor...	9.599	8.359	232218	193156	4.365	4.790m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
Data File : P0059731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Aug 2019 11:32
Operator : SM/AJ
Sample : K4497-04 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WEIR-TANK-082219-2


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 12:31:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

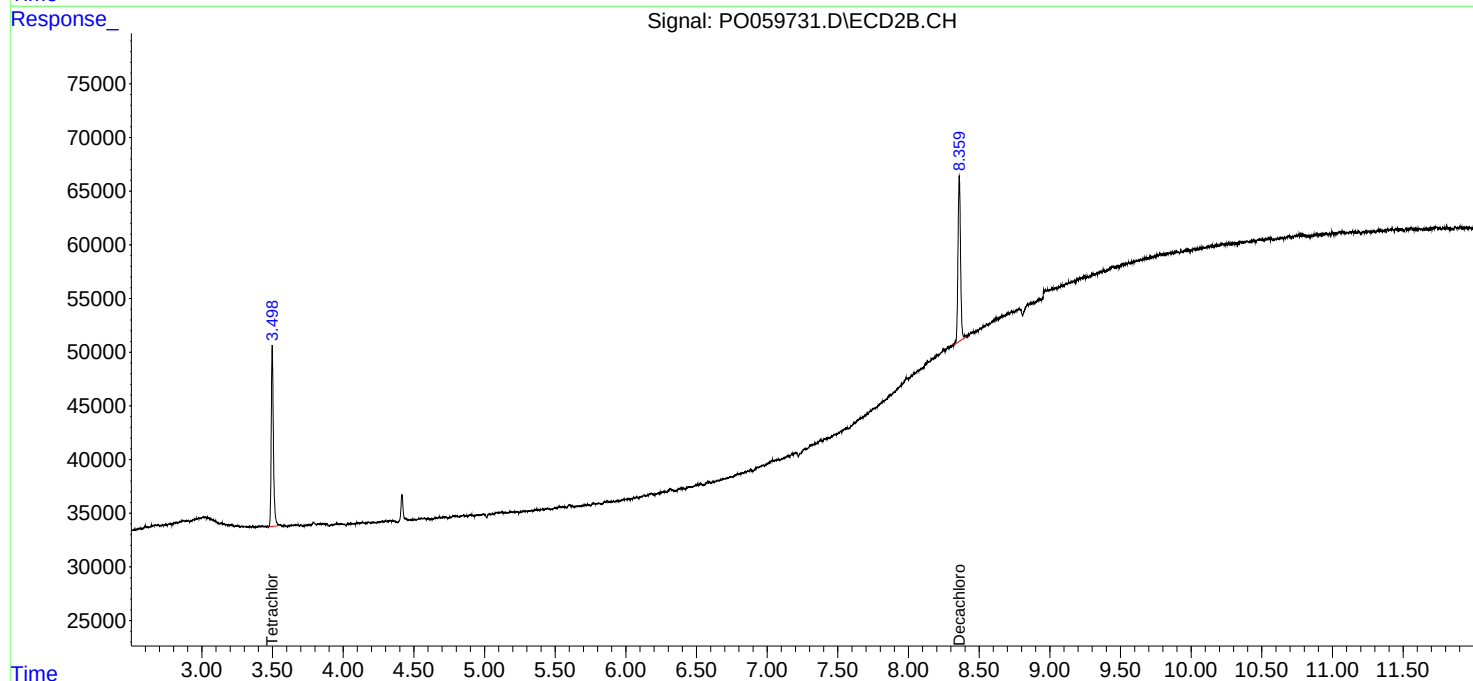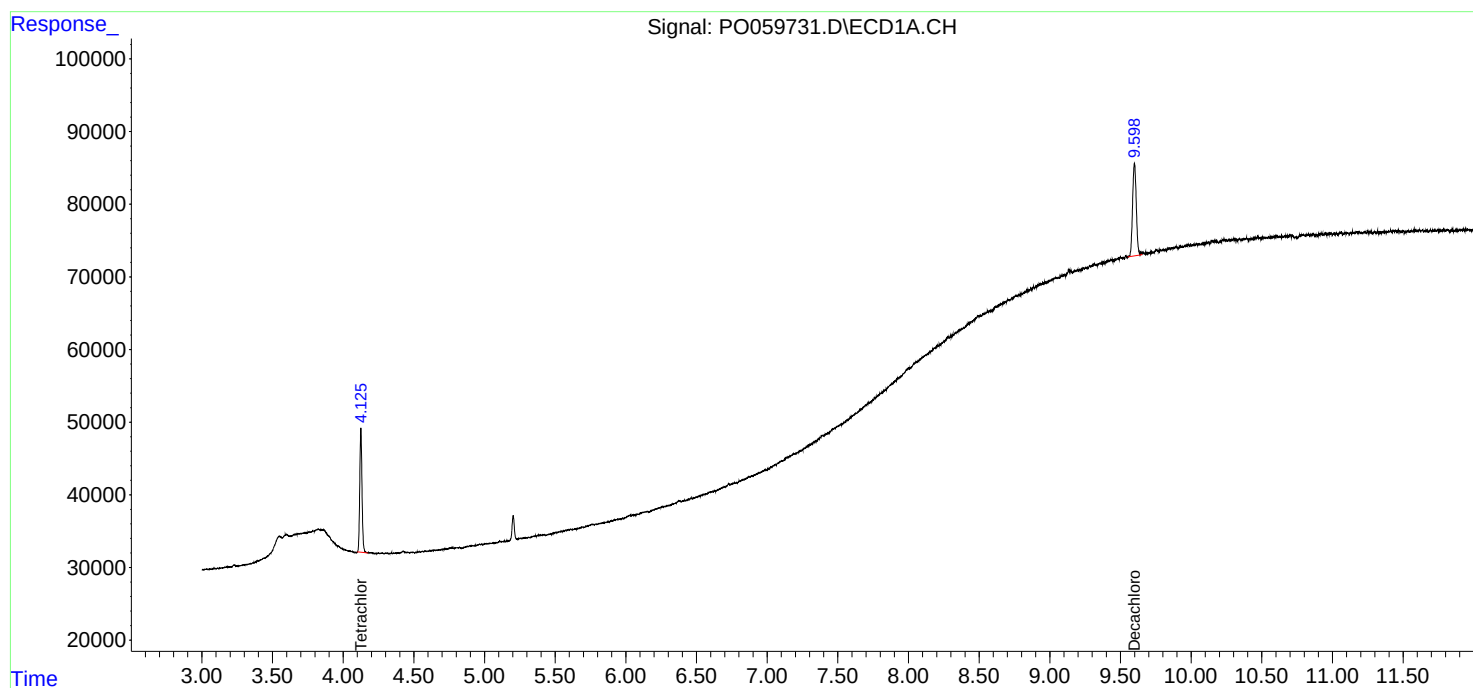

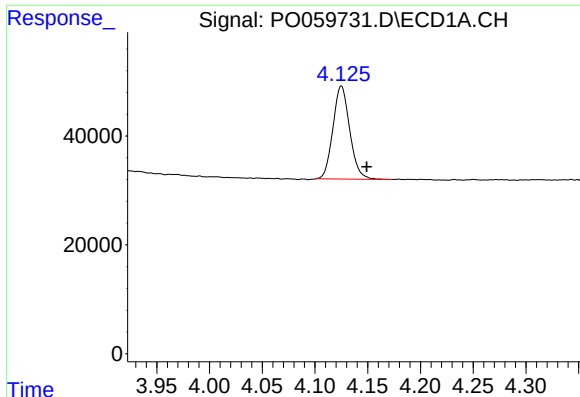


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: -0.024 min
Response: 189465
Conc: 5.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
WEIR-TANK-082219-2


Manual Integrations
APPROVED

Ankita
8/26/2019 3:10:36 PM

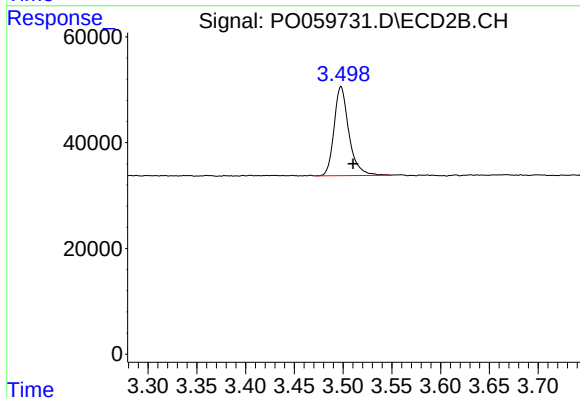


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.012 min
Response: 177481
Conc: 4.93 ng/ml

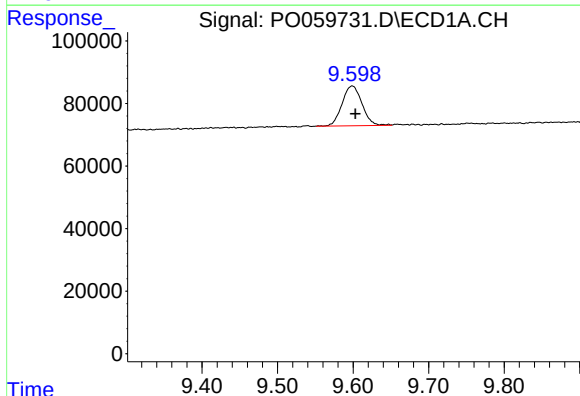

#2 Decachlorobiphenyl

R.T.: 9.599 min
Delta R.T.: -0.004 min
Response: 232218
Conc: 4.36 ng/ml

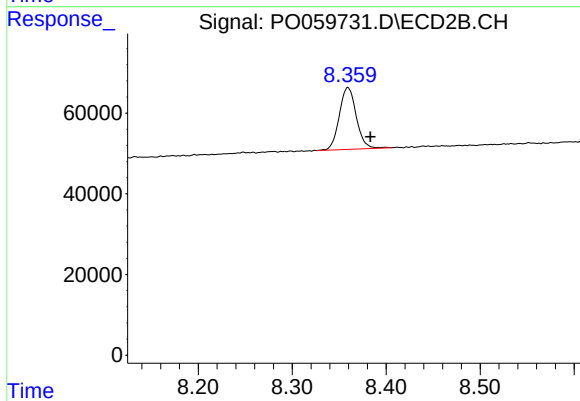

#2 Decachlorobiphenyl

R.T.: 8.359 min
Delta R.T.: -0.024 min
Response: 193156
Conc: 4.79 ng/ml m