

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
 Data File : P0059784.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2019 1:55
 Operator : SM/AJ
 Sample : K4496-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S600-M-1.0-1.5-082219

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:15:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 03:21:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.497	1114299	1019003	31.826m	28.309
2) SA Decachlor...	9.593	8.357	972109	799990	18.273	19.841

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
Data File : P0059784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2019 1:55
Operator : SM/AJ
Sample : K4496-01
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S600-M-1.0-1.5-082219


Manual Integrations
APPROVED

Ankita
8/26/2019 3:15:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 03:21:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

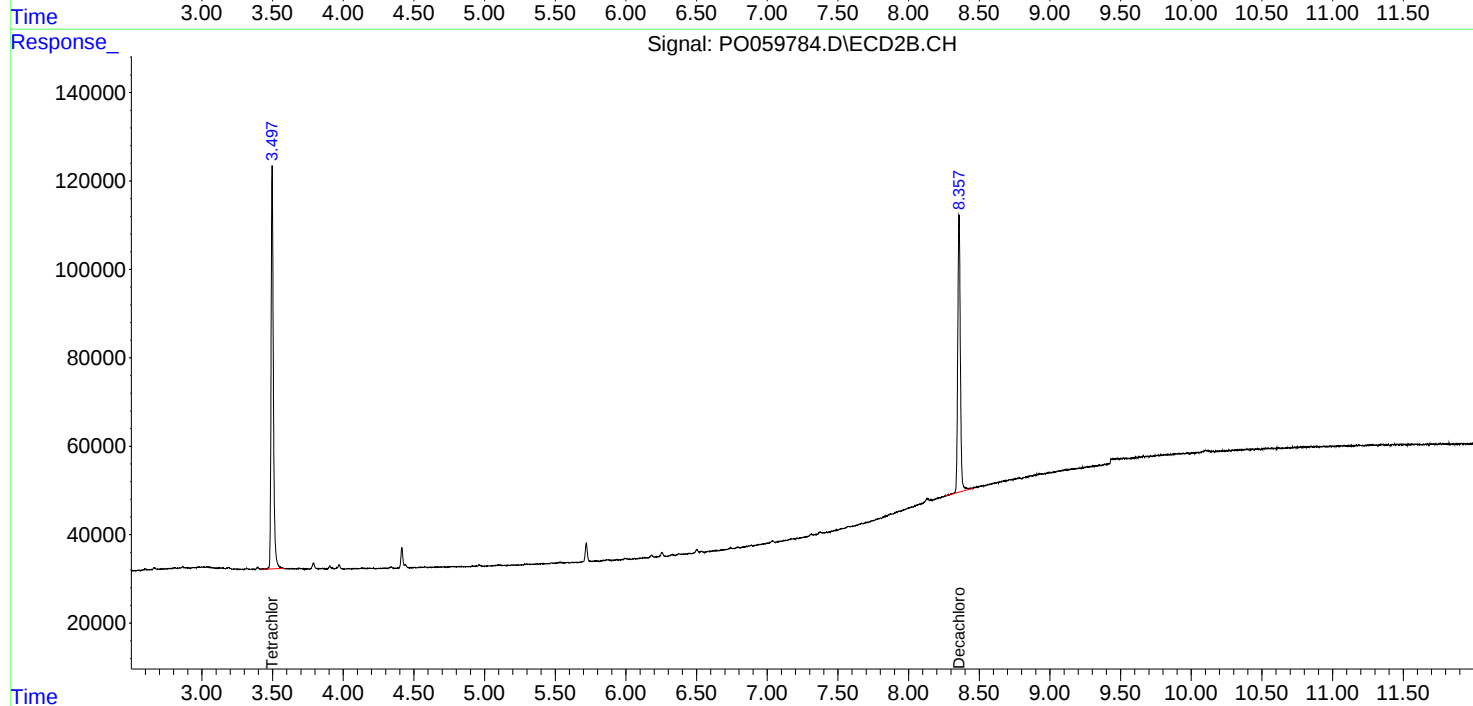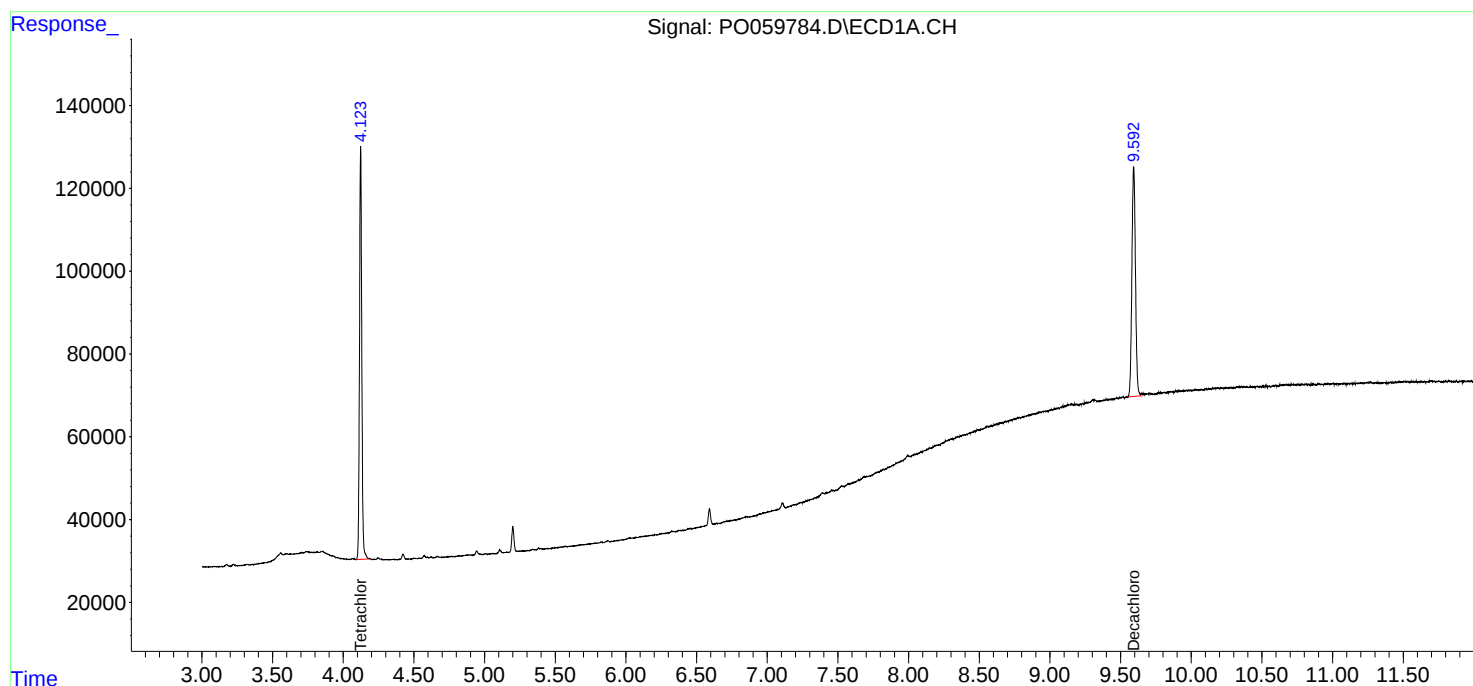

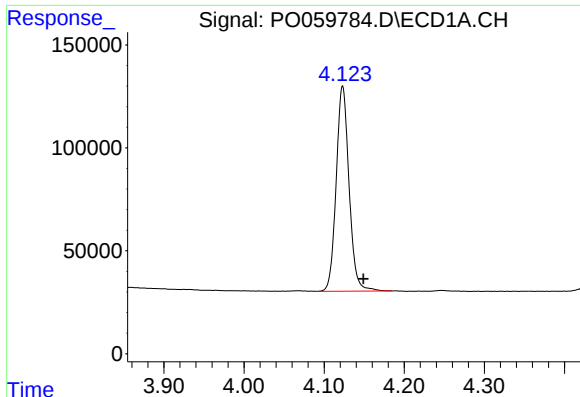


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: -0.026 min
Response: 1114299
Conc: 31.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S600-M-1.0-1.5-082219


Manual Integrations
APPROVED

Ankita
8/26/2019 3:15:47 PM

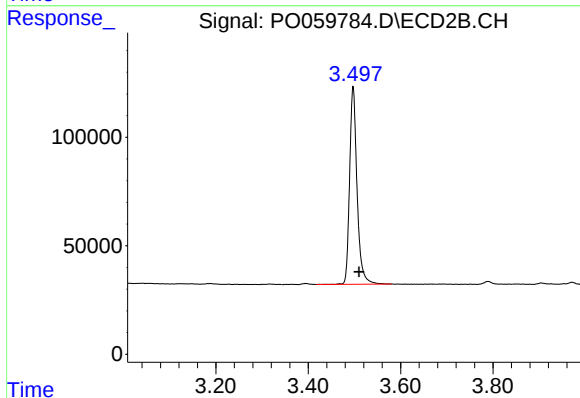


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.013 min
Response: 1019003
Conc: 28.31 ng/ml

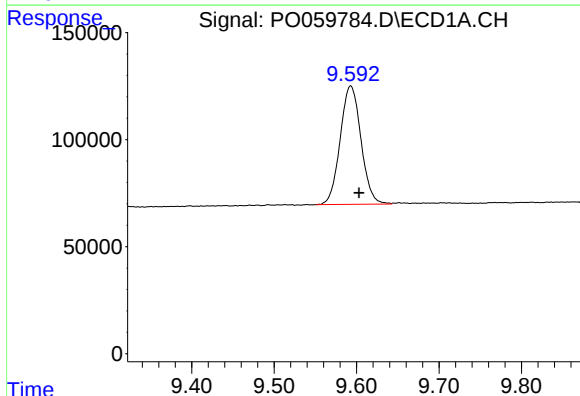

#2 Decachlorobiphenyl

R.T.: 9.593 min
Delta R.T.: -0.010 min
Response: 972109
Conc: 18.27 ng/ml

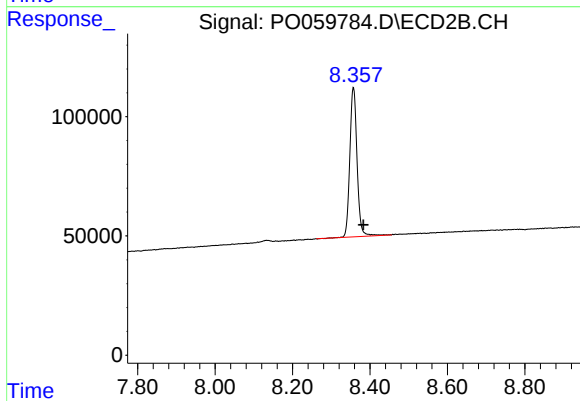

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.026 min
Response: 799990
Conc: 19.84 ng/ml