

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
 Data File : P0059788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2019 3:00
 Operator : SM/AJ
 Sample : K4496-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S601-M-1.0-1.5-082219

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:15:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 03:22:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.122	3.497	974519	880052	27.833m	24.449
2) SA Decachlor...	9.593	8.355	775985	641507	14.586	15.910

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082319\
Data File : P0059788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2019 3:00
Operator : SM/AJ
Sample : K4496-11
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S601-M-1.0-1.5-082219


Manual Integrations
APPROVED

Ankita
8/26/2019 3:15:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 03:22:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

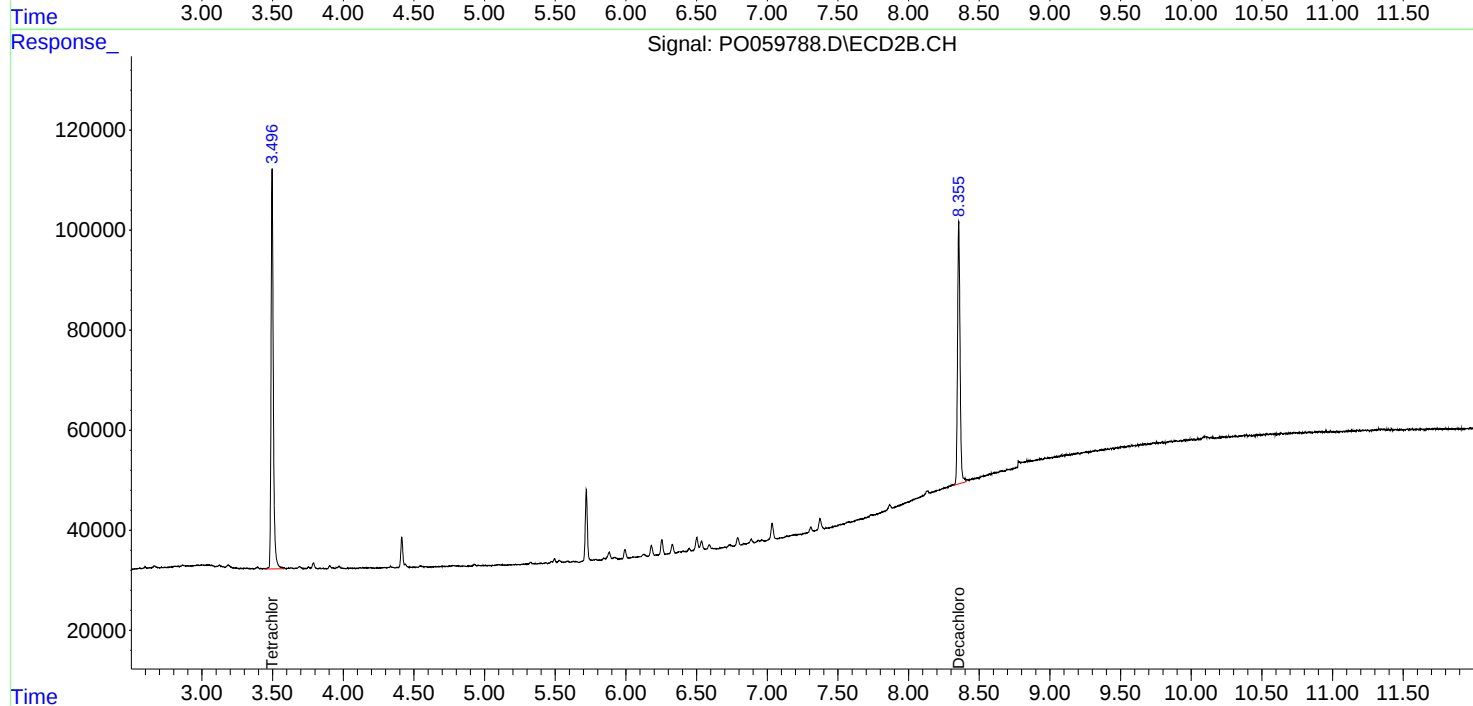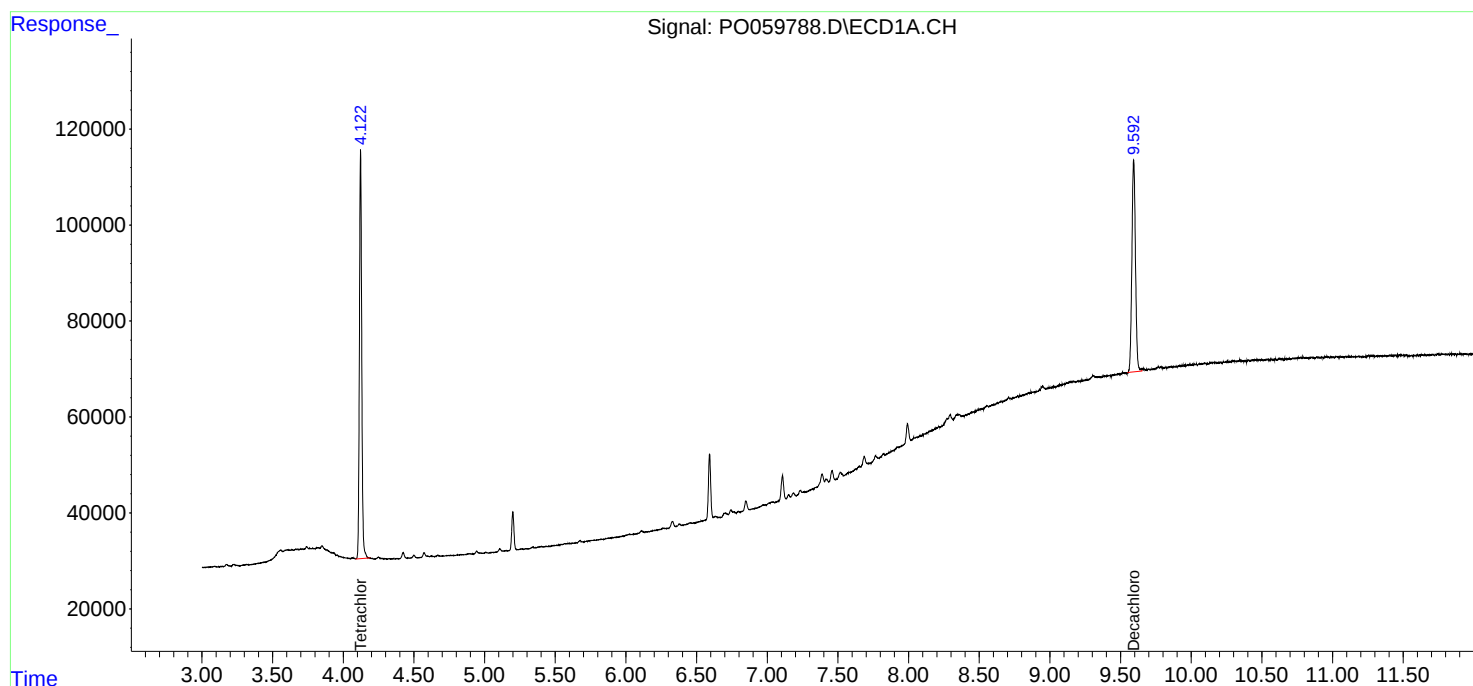

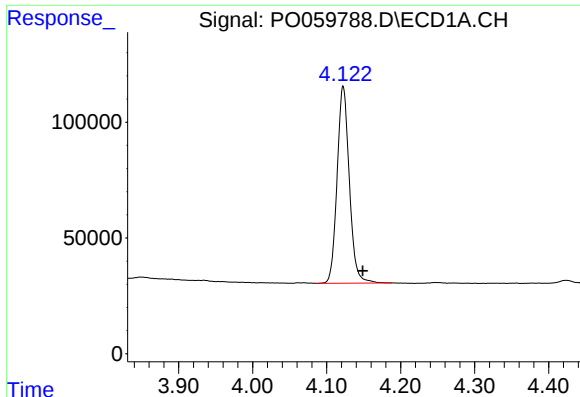


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: -0.027 min
Response: 974519
Conc: 27.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S601-M-1.0-1.5-082219


Manual Integrations
APPROVED

Ankita
8/26/2019 3:15:50 PM

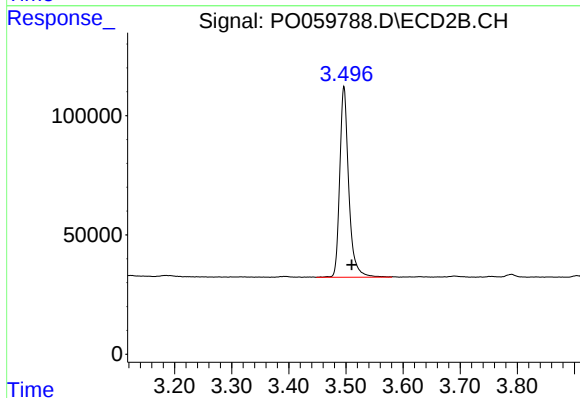


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.013 min
Response: 880052
Conc: 24.45 ng/ml

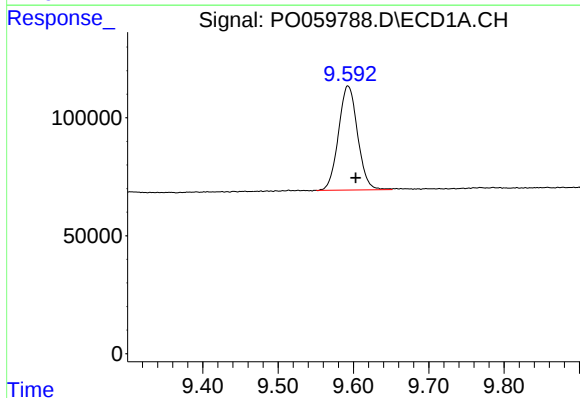

#2 Decachlorobiphenyl

R.T.: 9.593 min
Delta R.T.: -0.010 min
Response: 775985
Conc: 14.59 ng/ml

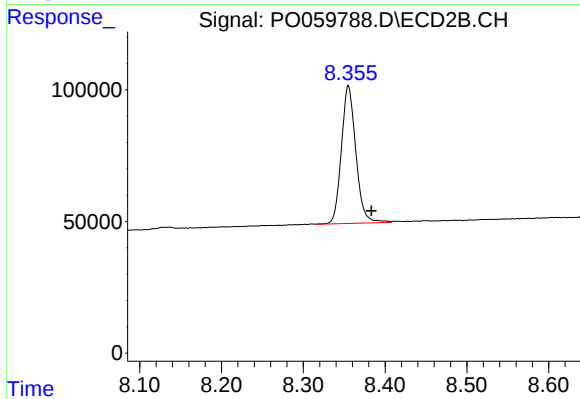

#2 Decachlorobiphenyl

R.T.: 8.355 min
Delta R.T.: -0.028 min
Response: 641507
Conc: 15.91 ng/ml