

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0082319\
 Data File : P0059795.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2019 9:50
 Operator : SM/AJ
 Sample : K4479-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU19-FLDDCAP1RE

Manual Integrations
 APPROVED

Ankita
 8/26/2019 3:16:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 09:27:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.127	3.497	781602	712836	22.323	19.803
2) SA Decachlor...	9.596	8.356	606603	446689	11.402	11.078m
Target Compounds						
31) L7 AR-1260-1	6.851	5.993	96501	69901	35.797	30.673
32) L7 AR-1260-2	7.107	6.181	125658	73302	33.866	25.019 #
33) L7 AR-1260-3	7.461	6.328	97106	60566	29.639	22.863
34) L7 AR-1260-4	7.687	6.791	71443	49816	23.261m	22.018
35) L7 AR-1260-5	7.995	7.035	132667	125926	18.736m	22.882

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082319\
Data File : PO059795.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2019 9:50
Operator : SM/AJ
Sample : K4479-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:16:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 09:27:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

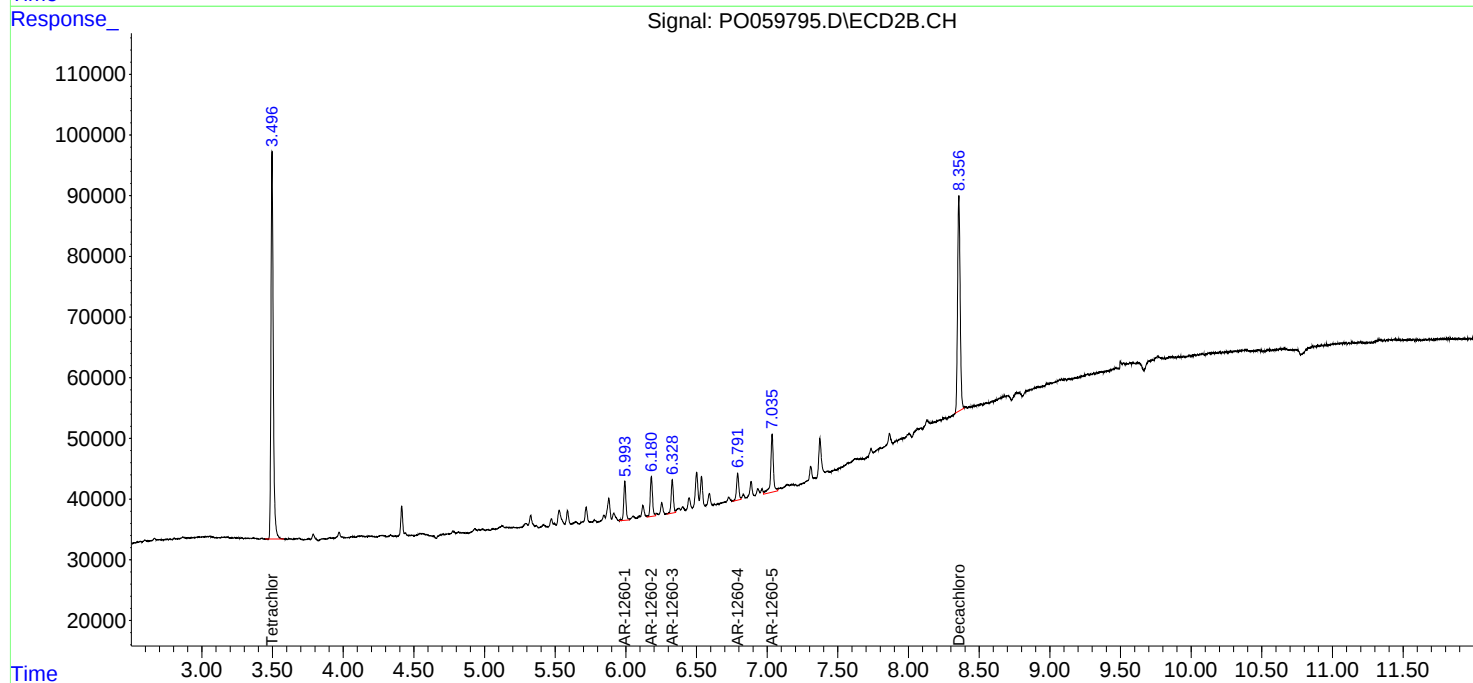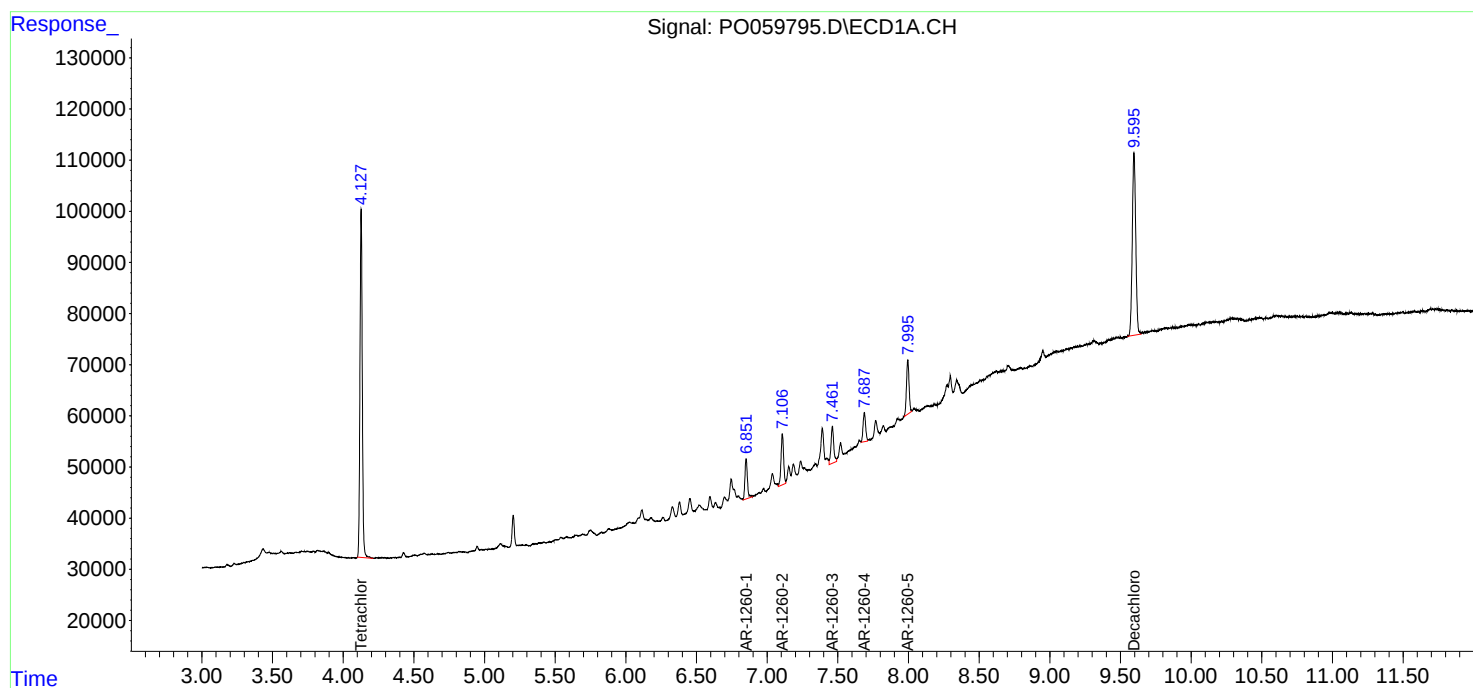

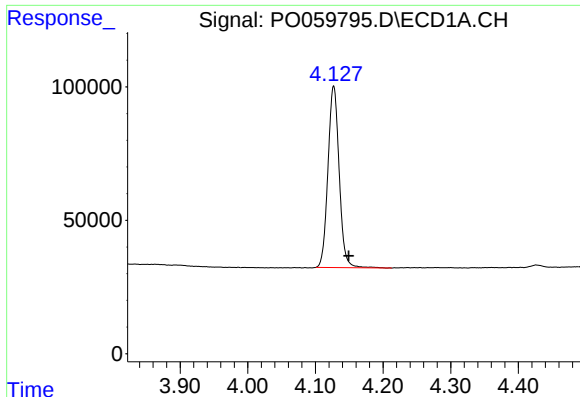


#1 Tetrachloro-m-xylene

R.T.: 4.127 min
Delta R.T.: -0.022 min
Response: 781602
Conc: 22.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:16:02 PM

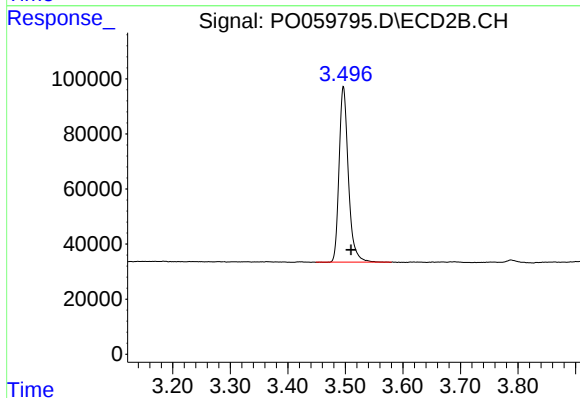


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: -0.013 min
Response: 712836
Conc: 19.80 ng/ml

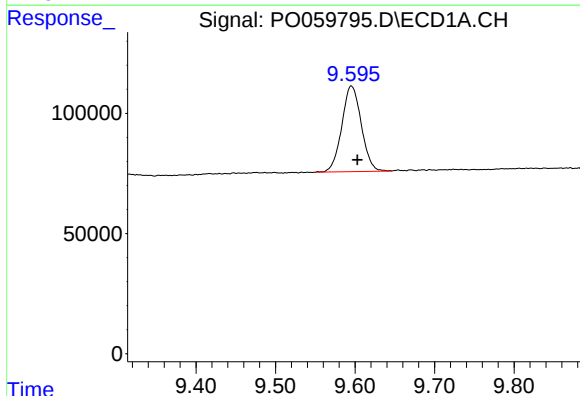


#2 Decachlorobiphenyl

R.T.: 9.596 min
Delta R.T.: -0.007 min
Response: 606603
Conc: 11.40 ng/ml

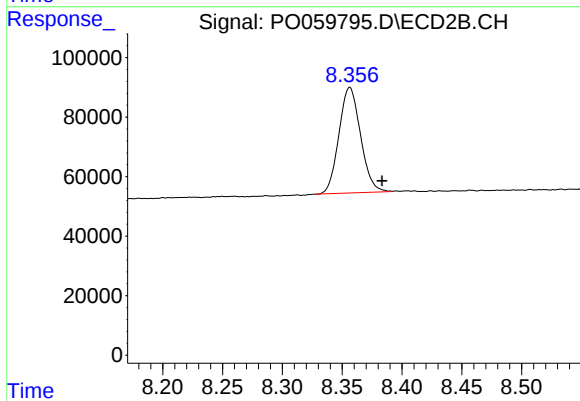

#2 Decachlorobiphenyl

R.T.: 8.356 min
Delta R.T.: -0.027 min
Response: 446689
Conc: 11.08 ng/ml m

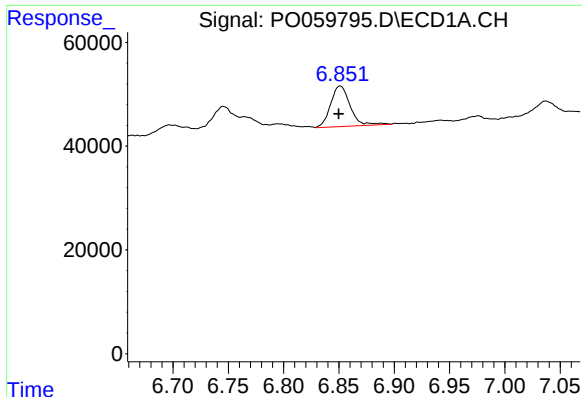


#31 AR-1260-1

R.T.: 6.851 min
Delta R.T.: 0.001 min
Response: 96501
Conc: 35.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:16:02 PM

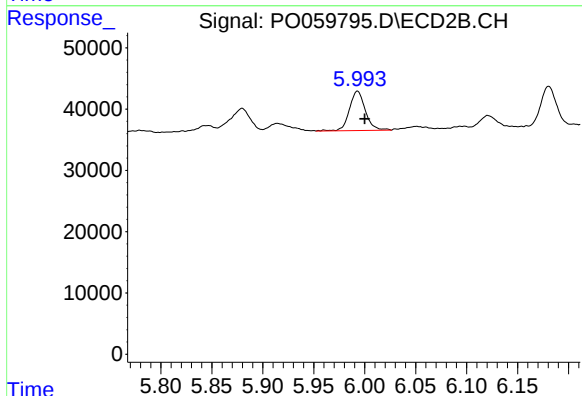


#31 AR-1260-1

R.T.: 5.993 min
Delta R.T.: -0.007 min
Response: 69901
Conc: 30.67 ng/ml

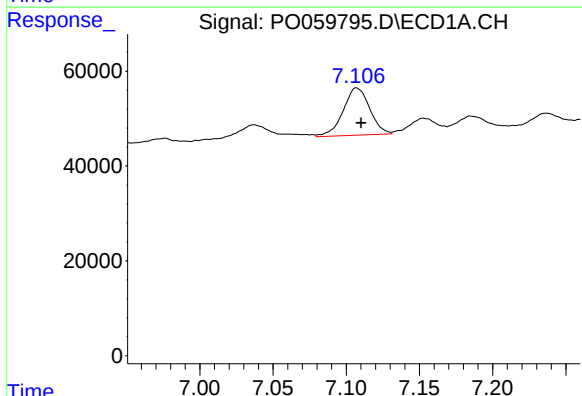


#32 AR-1260-2

R.T.: 7.107 min
Delta R.T.: -0.003 min
Response: 125658
Conc: 33.87 ng/ml

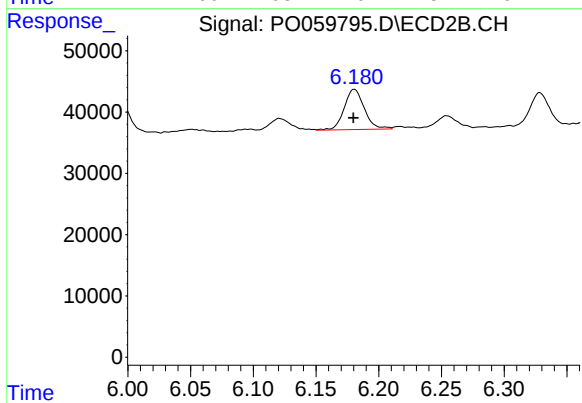

#32 AR-1260-2

R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 73302
Conc: 25.02 ng/ml

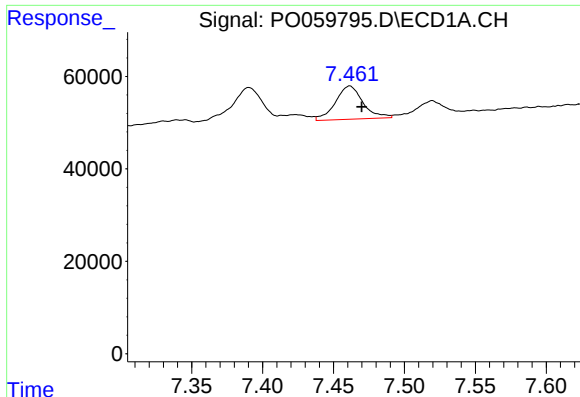


#33 AR-1260-3

R.T.: 7.461 min
Delta R.T.: -0.009 min
Response: 97106
Conc: 29.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE


Manual Integrations
APPROVED

Ankita
8/26/2019 3:16:02 PM

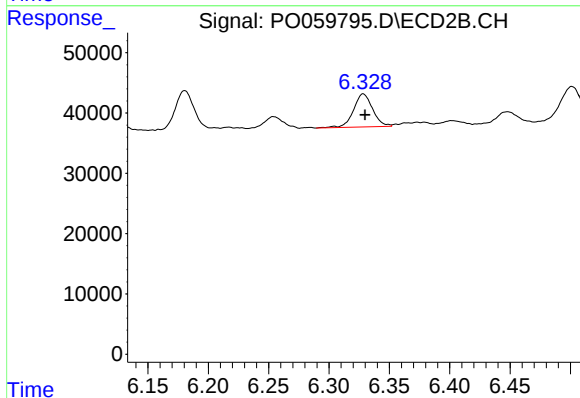


#33 AR-1260-3

R.T.: 6.328 min
Delta R.T.: -0.002 min
Response: 60566
Conc: 22.86 ng/ml

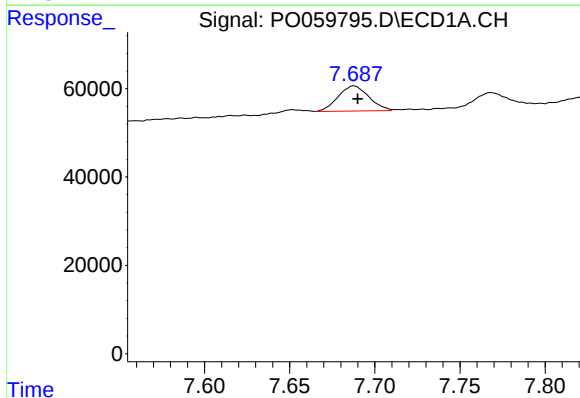


#34 AR-1260-4

R.T.: 7.687 min
Delta R.T.: -0.003 min
Response: 71443
Conc: 23.26 ng/ml m

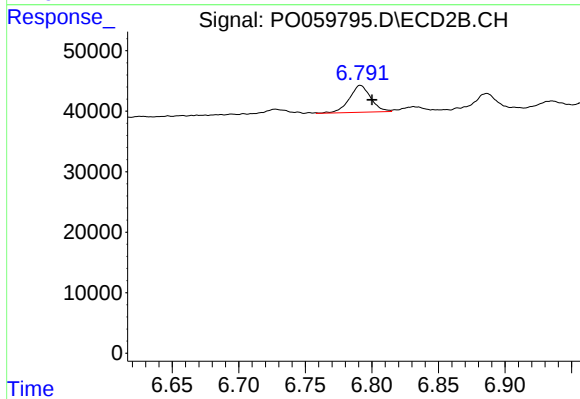

#34 AR-1260-4

R.T.: 6.791 min
Delta R.T.: -0.009 min
Response: 49816
Conc: 22.02 ng/ml

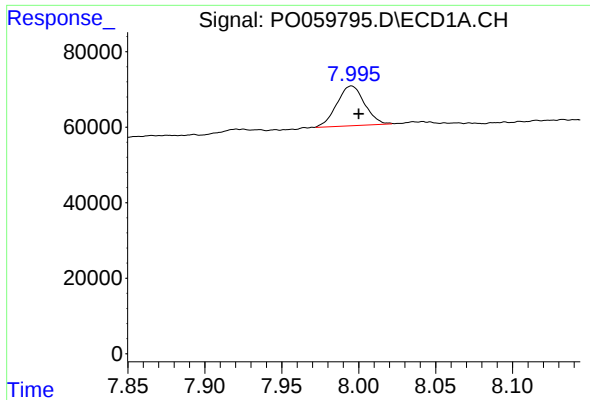


#35 AR-1260-5

R.T.: 7.995 min
Delta R.T.: -0.005 min
Response: 132667
Conc: 18.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU19-FLDDCAP1RE

Manual Integrations
APPROVED

Ankita
8/26/2019 3:16:02 PM

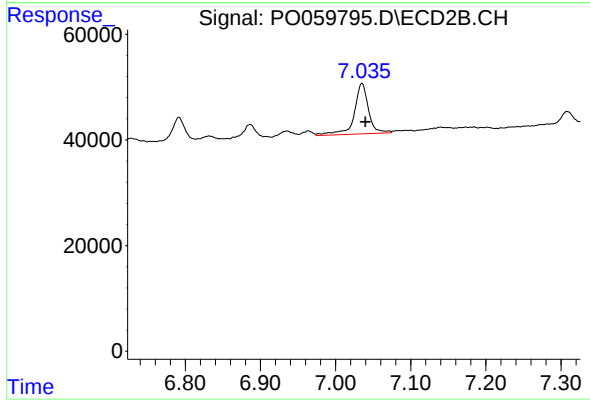

#35 AR-1260-5

R.T.: 7.035 min
Delta R.T.: -0.005 min
Response: 125926
Conc: 22.88 ng/ml