

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082324\
 Data File : P0105793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 17:08
 Operator : YP/AJ
 Sample : P3714-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-08222024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/26/2024
 Supervised By :Ankita Jodhani 08/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 08:21:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.453	3.723	160.1E6	49145856	17.128m	19.269
2) SA Decachlor...	10.191	8.758	111.2E6	37526162	19.159	19.015

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082324\
Data File : PO105793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 17:08
Operator : YP/AJ
Sample : P3714-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-01-08222024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2024
Supervised By :Ankita Jodhani 08/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 08:21:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

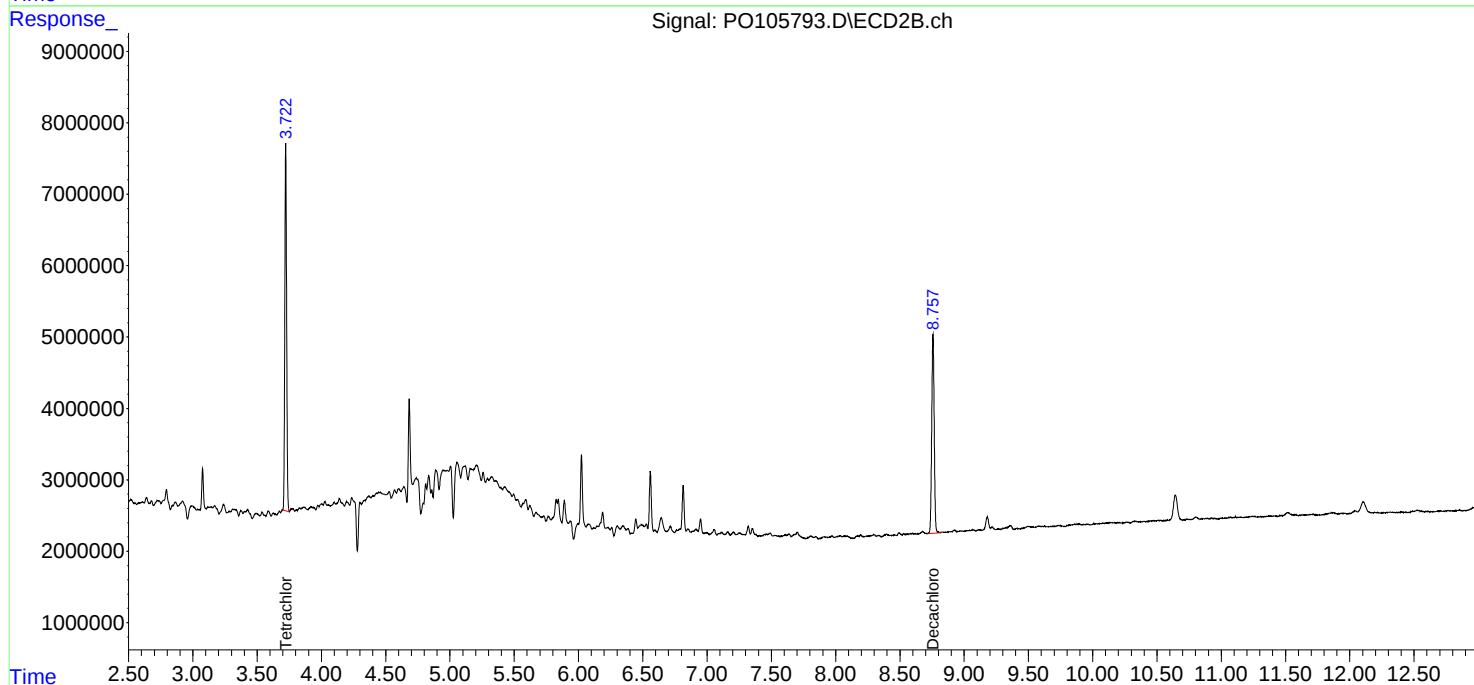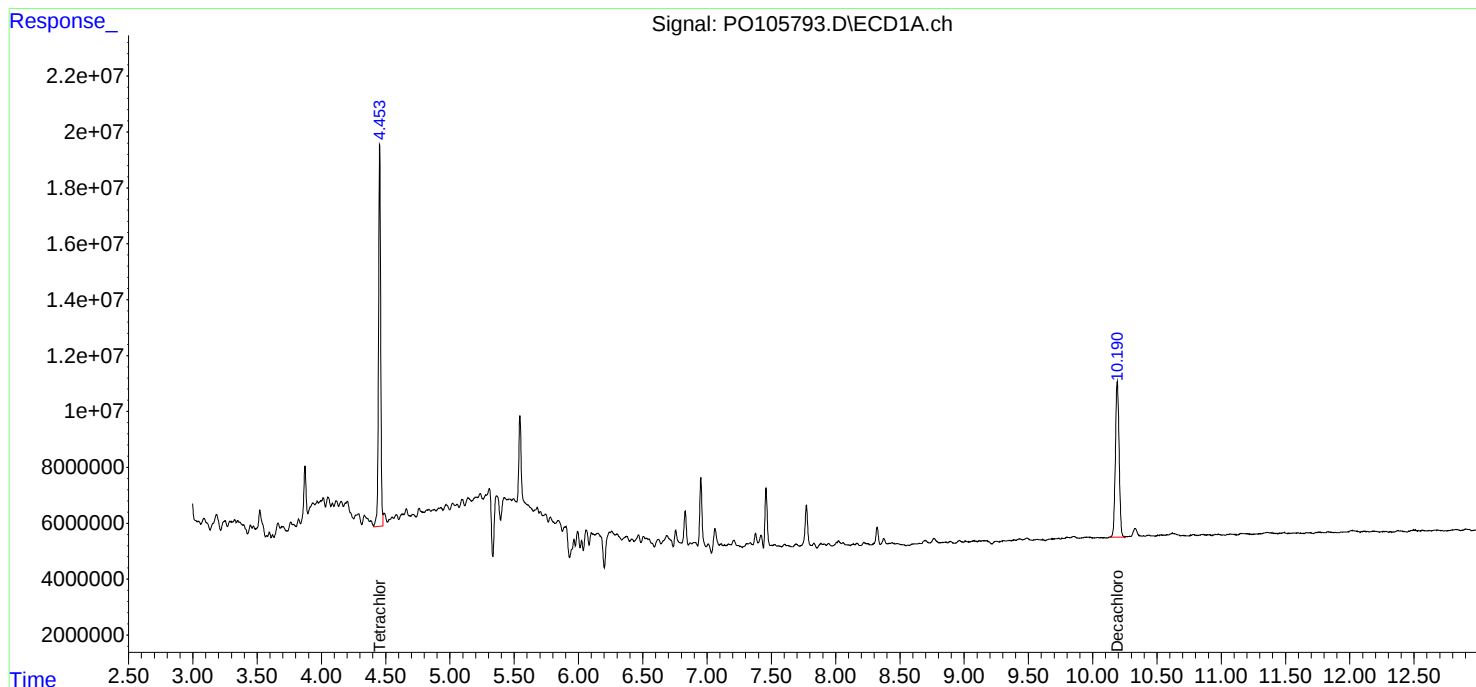

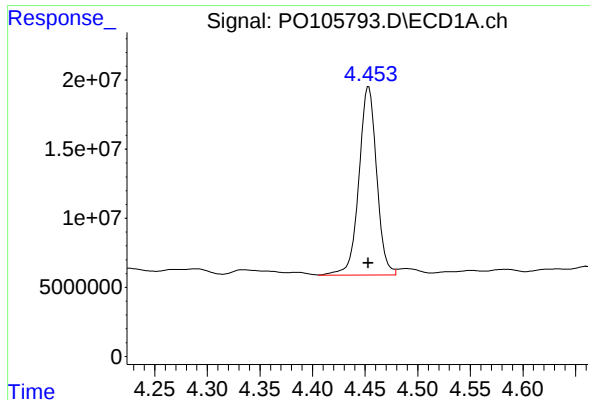


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.000 min
Response: 160132724
Conc: 17.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-01-08222024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2024
Supervised By :Ankita Jodhani 08/26/2024

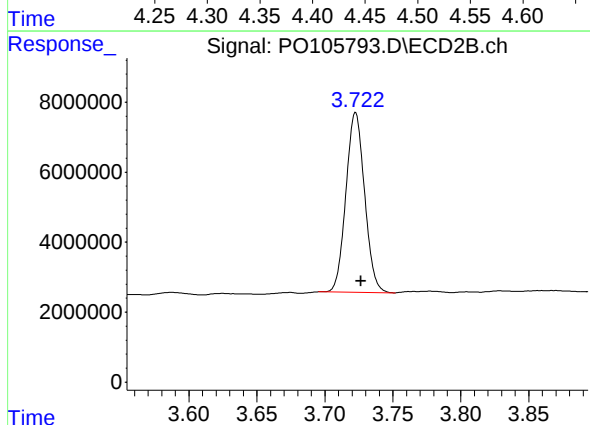


#1 Tetrachloro-m-xylene

R.T.: 3.723 min
Delta R.T.: -0.004 min
Response: 49145856
Conc: 19.27 ng/ml

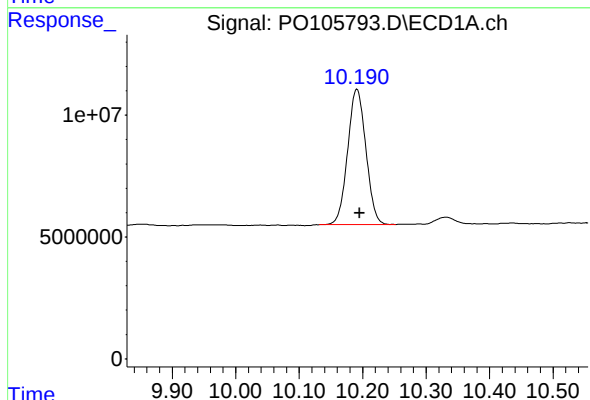

#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: -0.004 min
Response: 111213639
Conc: 19.16 ng/ml

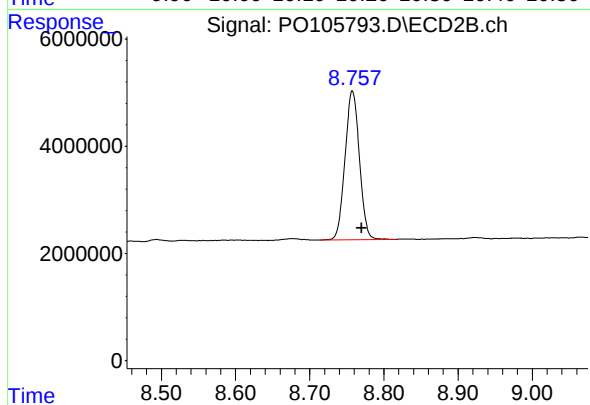

#2 Decachlorobiphenyl

R.T.: 8.758 min
Delta R.T.: -0.012 min
Response: 37526162
Conc: 19.02 ng/ml