

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082324\
 Data File : P0105797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2024 18:18
 Operator : YP/AJ
 Sample : P3718-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1803

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 08:27:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.454	3.723	125.5E6	44296050	13.429	17.367 #
2) SA Decachlor...	10.193	8.757	64354806	25075166	11.087	12.706

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082324\
Data File : PO105797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2024 18:18
Operator : YP/AJ
Sample : P3718-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1803

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 08:27:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

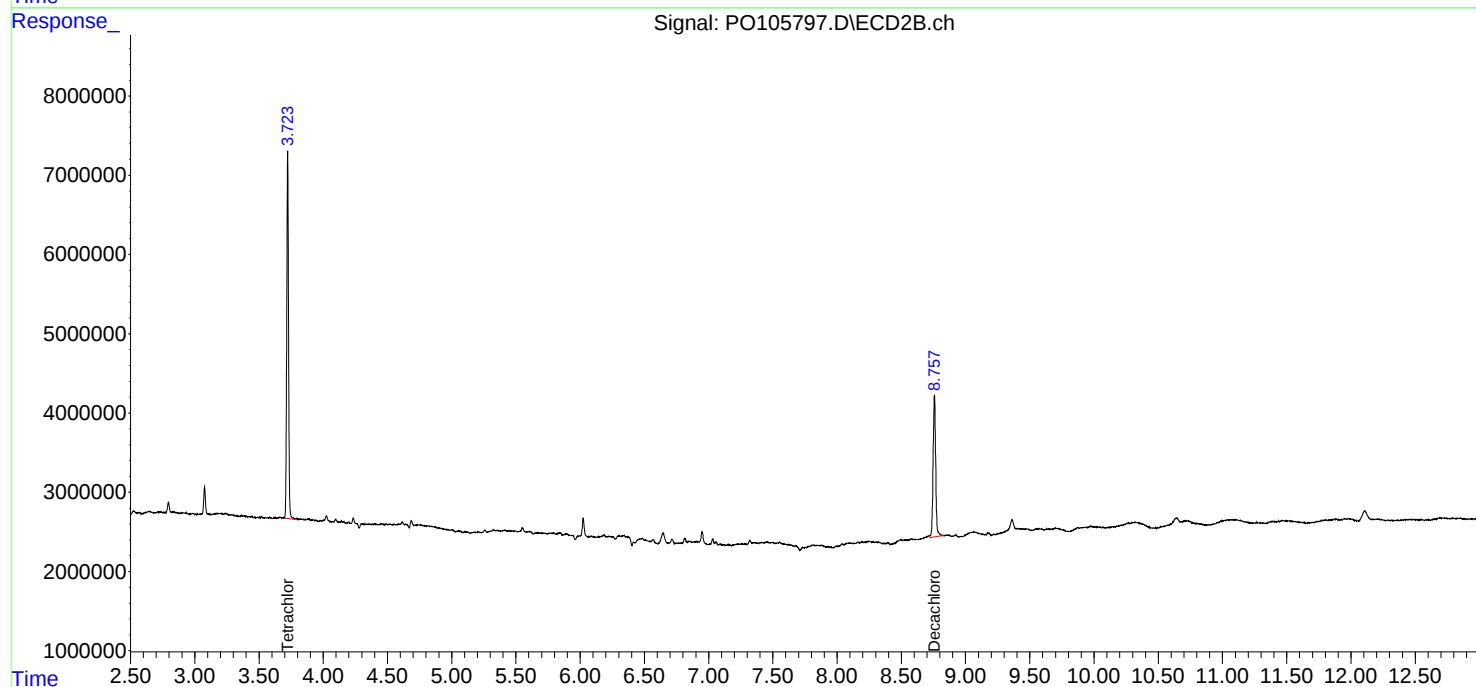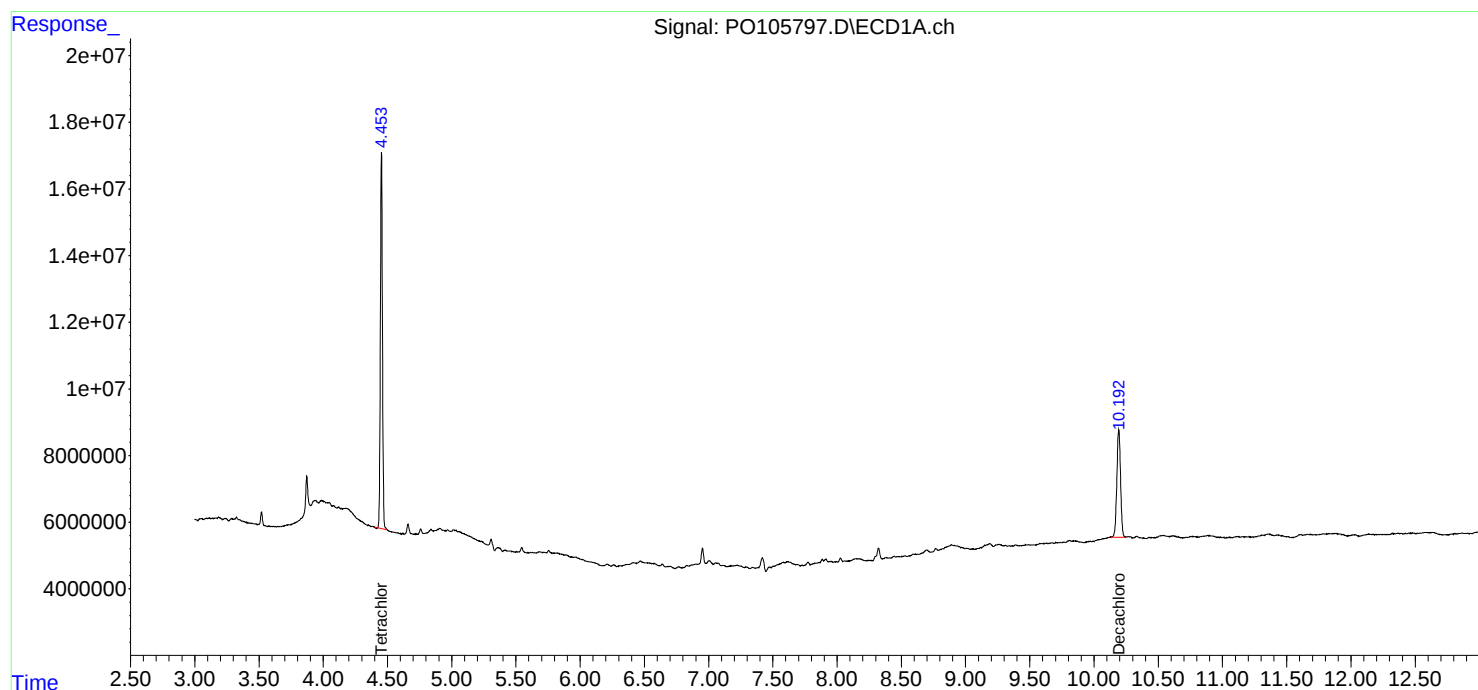


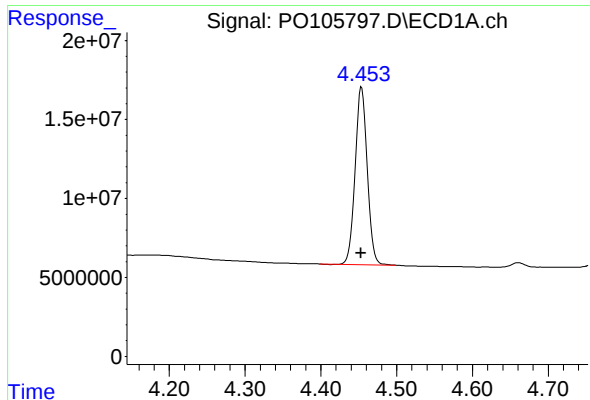

#1 Tetrachloro-m-xylene


R.T.: 4.454 min
Delta R.T.: 0.000 min
Response: 125549854
Conc: 13.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
1803

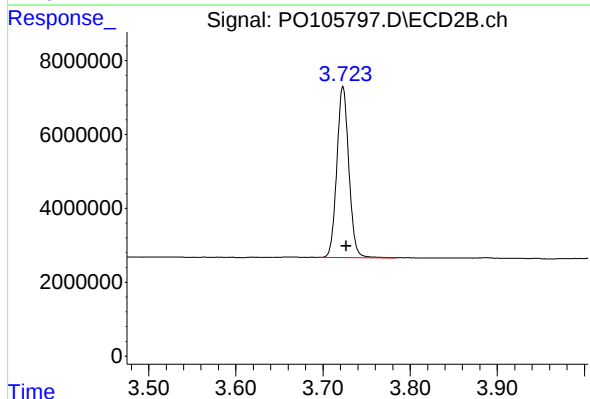


#1 Tetrachloro-m-xylene

R.T.: 3.723 min
Delta R.T.: -0.004 min
Response: 44296050
Conc: 17.37 ng/ml

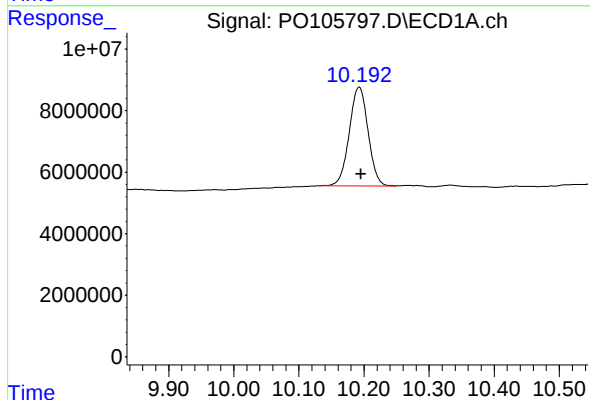

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.002 min
Response: 64354806
Conc: 11.09 ng/ml

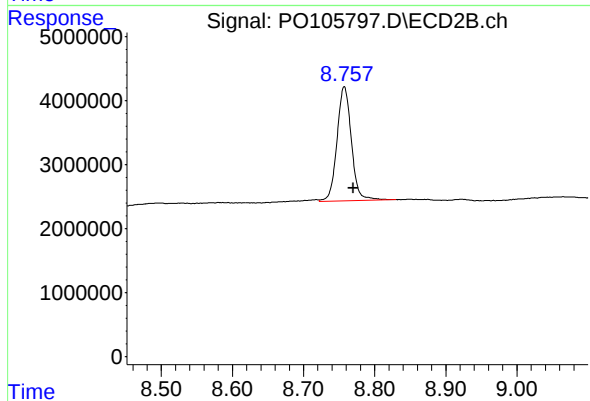

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.013 min
Response: 25075166
Conc: 12.71 ng/ml