

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082324\
 Data File : P0105821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Aug 2024 01:51
 Operator : YP/AJ
 Sample : P3725-01 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HIA-705Y-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/26/2024
 Supervised By :Ankita Jodhani 08/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 09:05:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 15 11:44:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.721	14926972	3966372	1.597	1.555
2) SA Decachlor...	10.190	8.756	10930596	2761421	1.883	1.399m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082324\
Data File : PO105821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Aug 2024 01:51
Operator : YP/AJ
Sample : P3725-01 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HIA-705Y-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2024
Supervised By :Ankita Jodhani 08/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 09:05:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 15 11:44:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

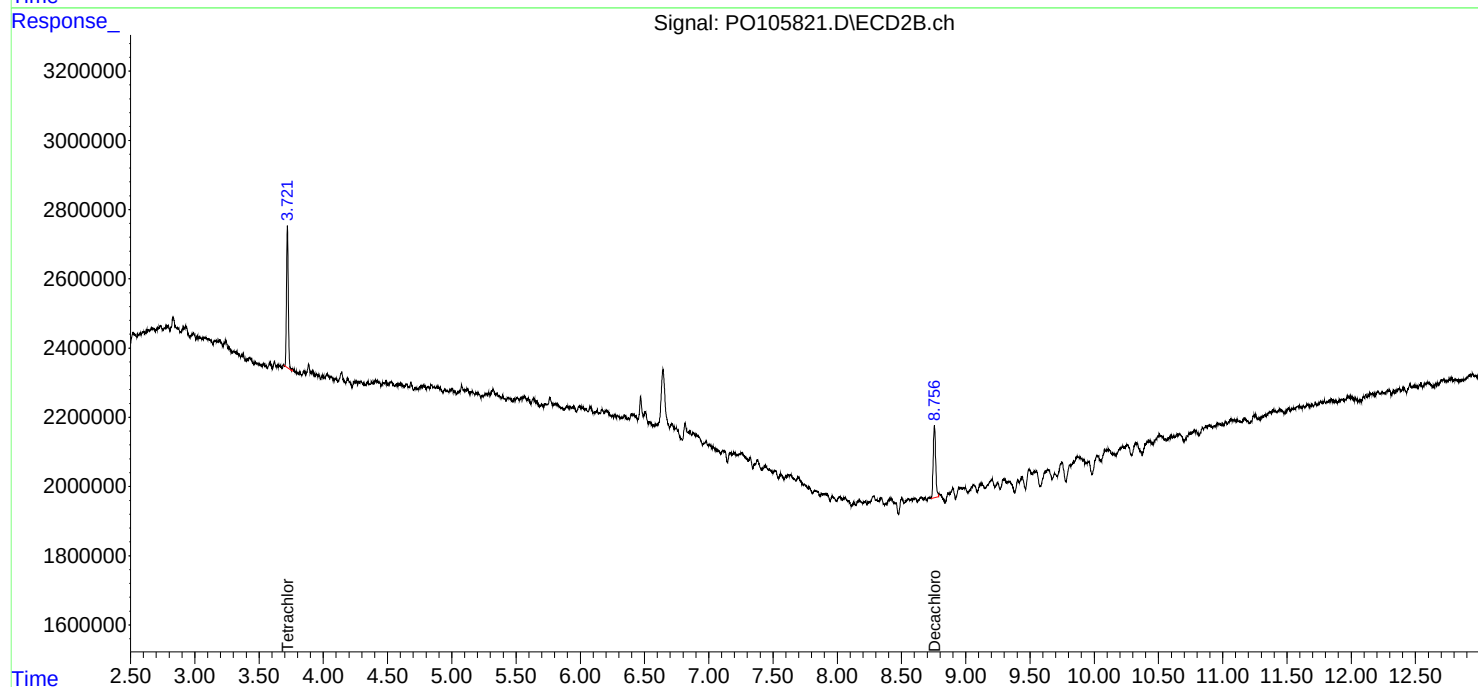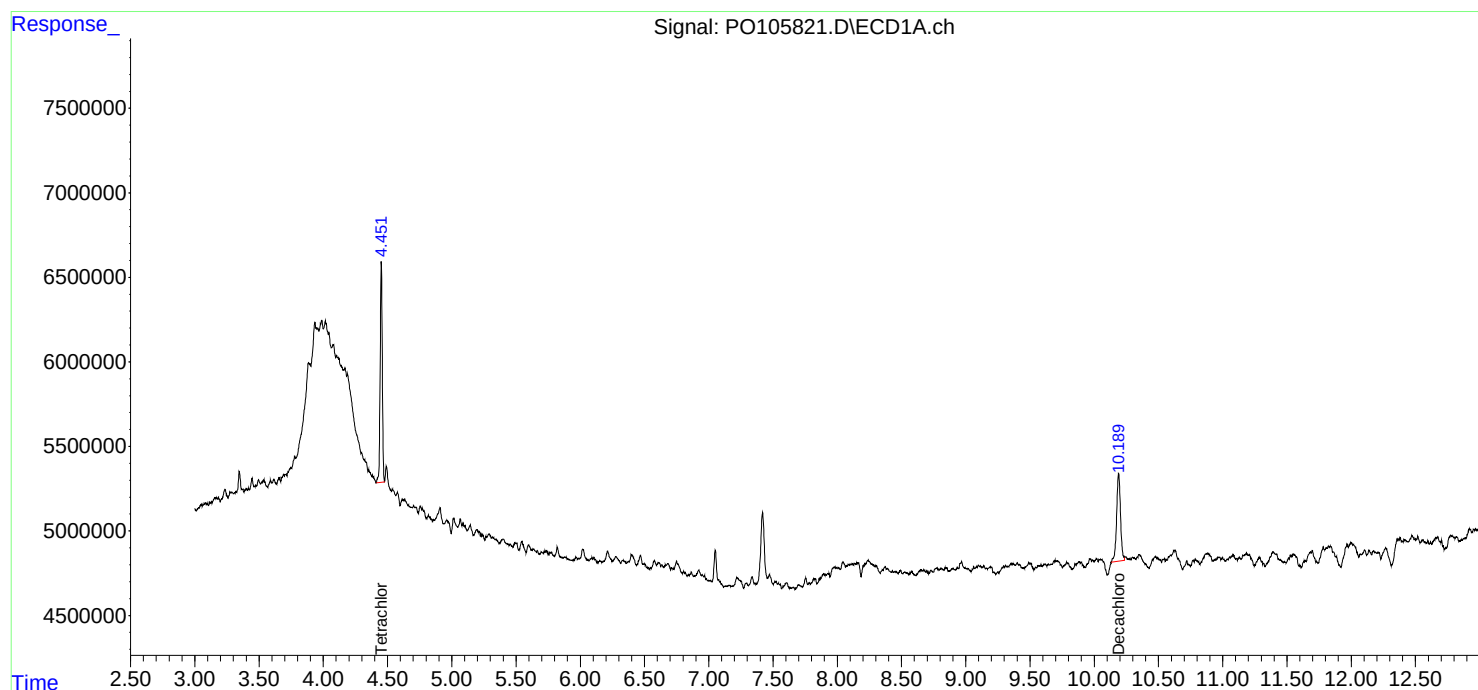

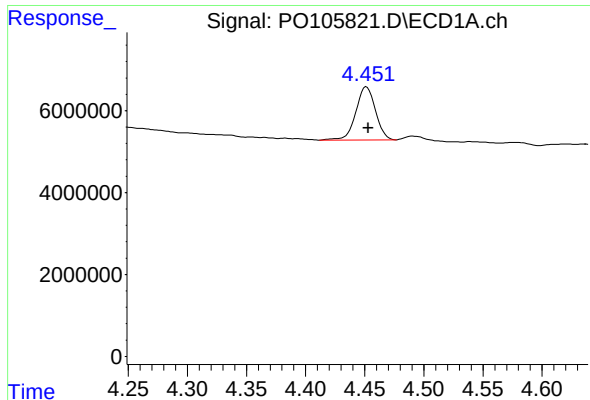


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: -0.001 min
Response: 14926972
Conc: 1.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
HIA-705Y-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2024
Supervised By :Ankita Jodhani 08/26/2024

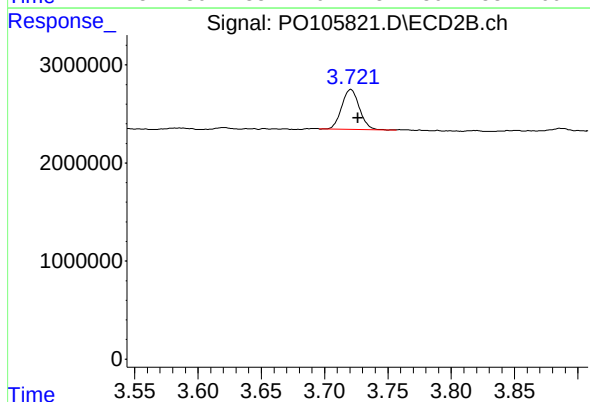


#1 Tetrachloro-m-xylene

R.T.: 3.721 min
Delta R.T.: -0.006 min
Response: 3966372
Conc: 1.56 ng/ml

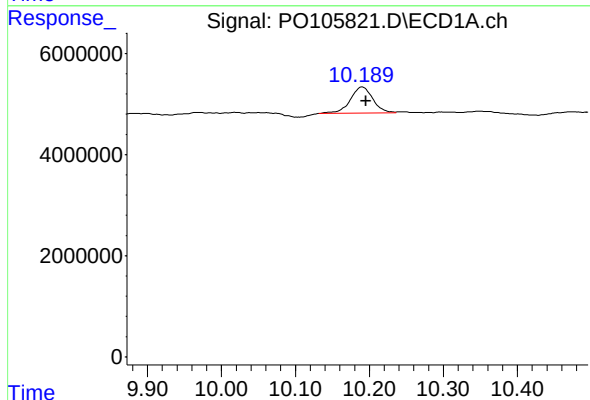

#2 Decachlorobiphenyl

R.T.: 10.190 min
Delta R.T.: -0.005 min
Response: 10930596
Conc: 1.88 ng/ml

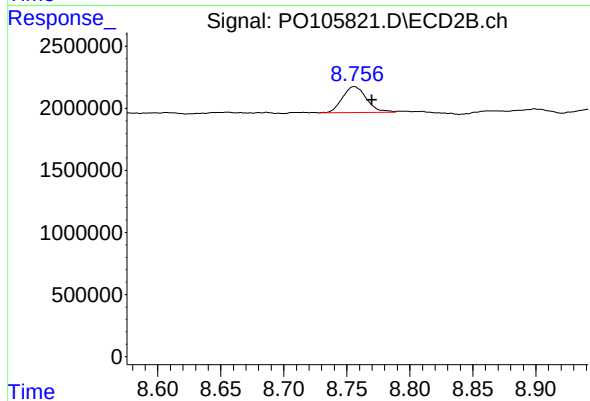

#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: -0.014 min
Response: 2761421
Conc: 1.40 ng/ml m