

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082420\
 Data File : P0070811.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2020 12:32
 Operator : DD\AJ
 Sample : L3772-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 349-346

Manual Integrations
 APPROVED

Ankita
 8/25/2020 2:43:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 13:37:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.555	1805570	1028355	25.919	25.545
2) SA Decachlor...	9.998	8.740	2117850	1354022	22.622	24.045
Target Compounds						
31) L7 AR-1260-1	7.332	6.343	539606	364031	130.898m	137.556m
32) L7 AR-1260-2	7.600	6.544	888768	528023	142.986	143.889
33) L7 AR-1260-3	7.956	6.691	1000120	379554	186.625	122.257 #
34) L7 AR-1260-4	8.183	7.166	840484	521337	165.093	186.962
35) L7 AR-1260-5	8.498	7.418	1928478	1309359	161.866	167.256

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082420\
Data File : PO070811.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2020 12:32
Operator : DD\AJ
Sample : L3772-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
349-346


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 13:37:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

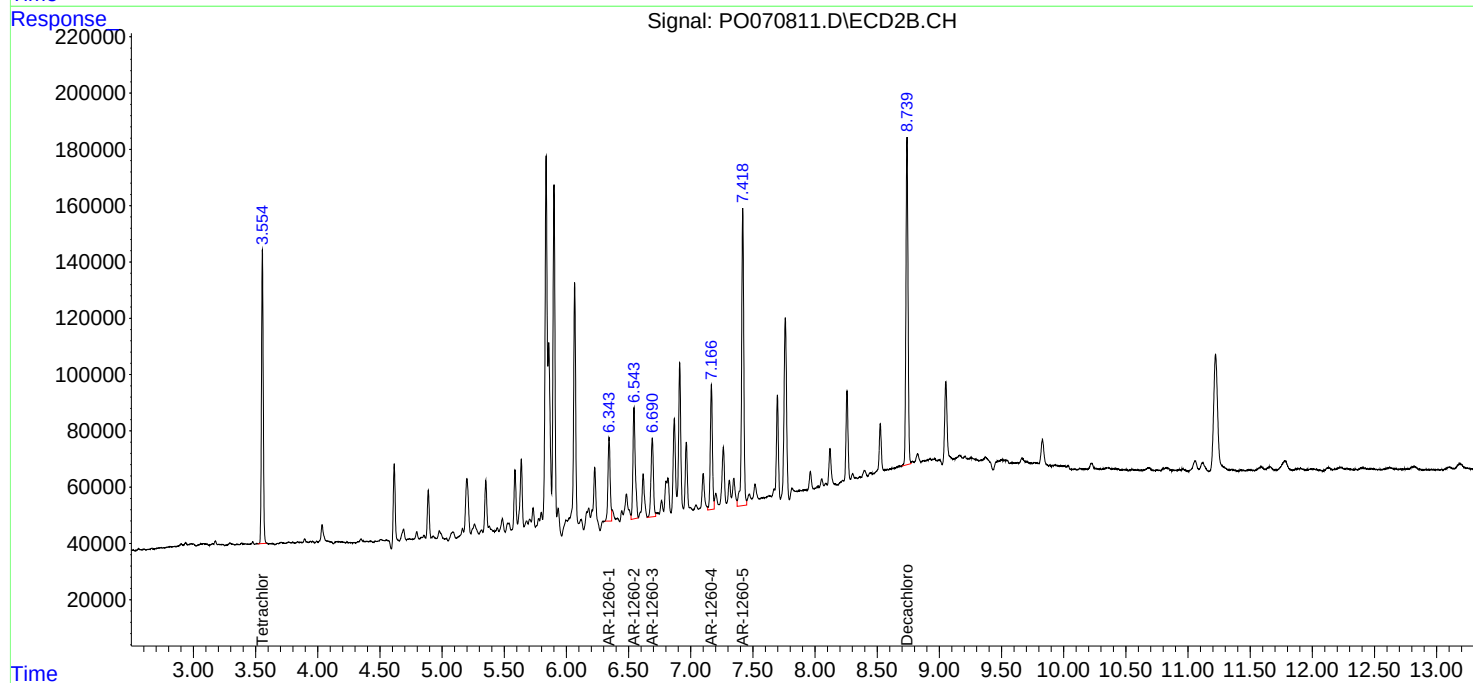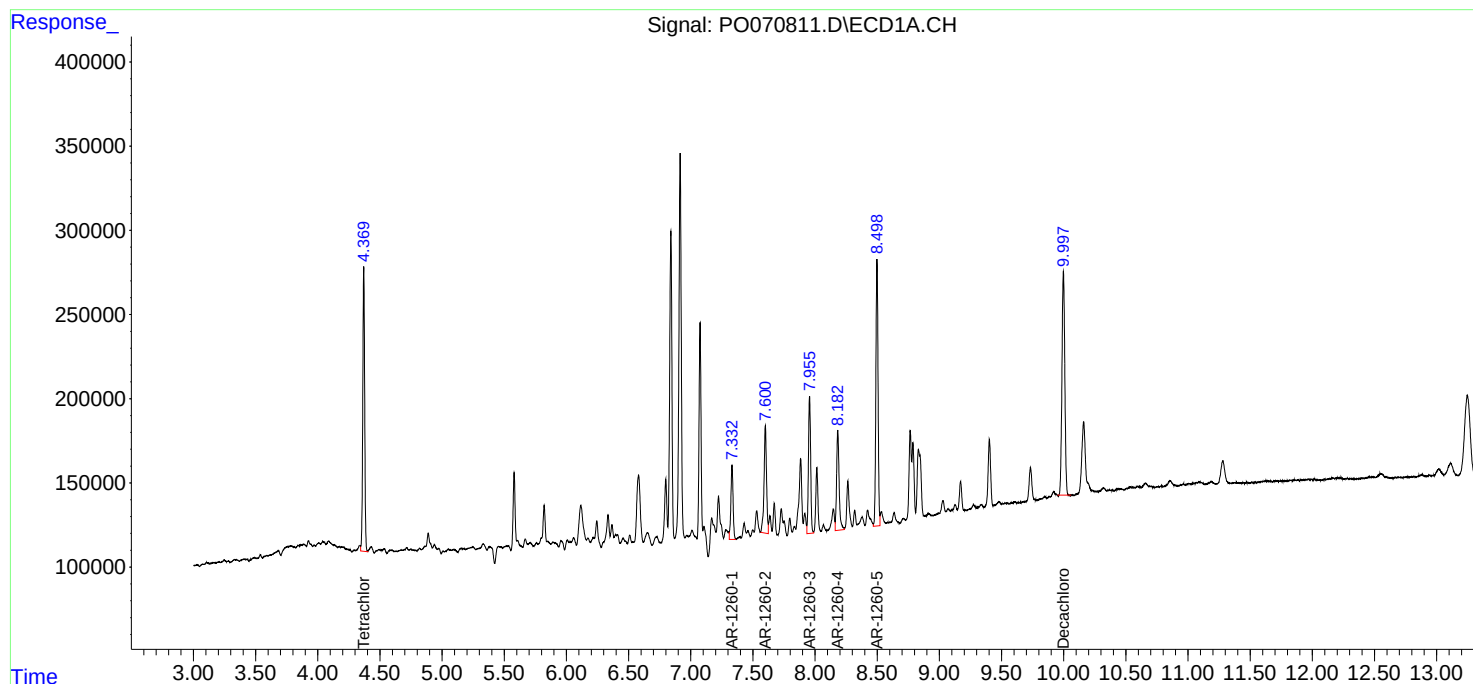

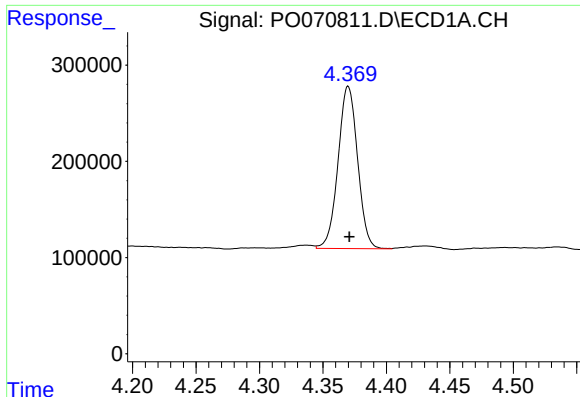


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: -0.001 min
Response: 1805570
Conc: 25.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
349-346


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:41 PM

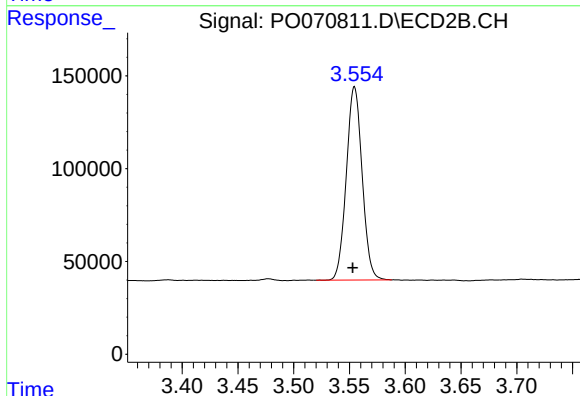


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.002 min
Response: 1028355
Conc: 25.54 ng/ml

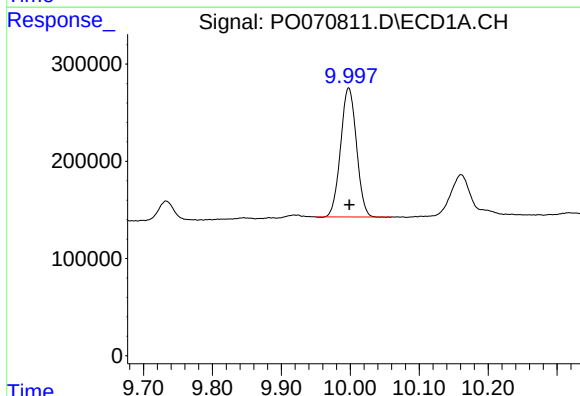


#2 Decachlorobiphenyl

R.T.: 9.998 min
Delta R.T.: -0.001 min
Response: 2117850
Conc: 22.62 ng/ml

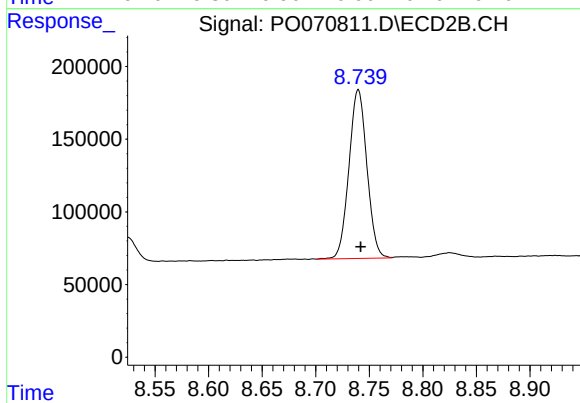

#2 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.002 min
Response: 1354022
Conc: 24.05 ng/ml

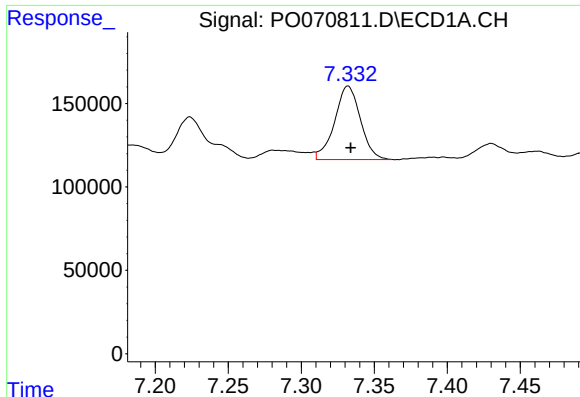


#31 AR-1260-1

R.T.: 7.332 min
Delta R.T.: -0.002 min
Response: 539606
Conc: 130.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
349-346


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:41 PM

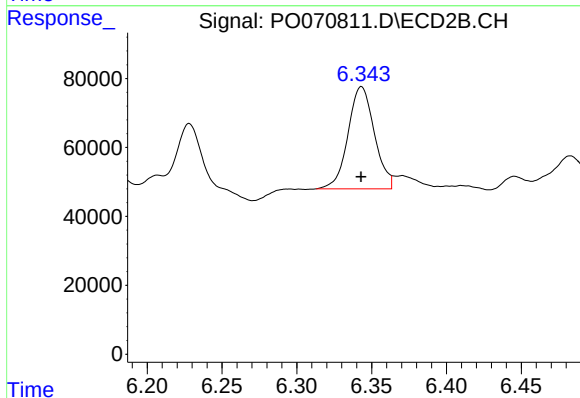


#31 AR-1260-1

R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 364031
Conc: 137.56 ng/ml m

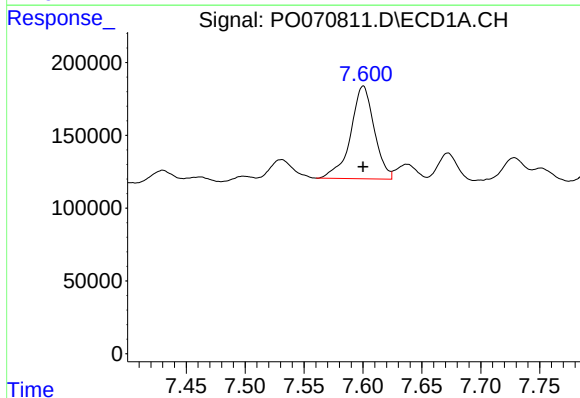


#32 AR-1260-2

R.T.: 7.600 min
Delta R.T.: 0.000 min
Response: 888768
Conc: 142.99 ng/ml

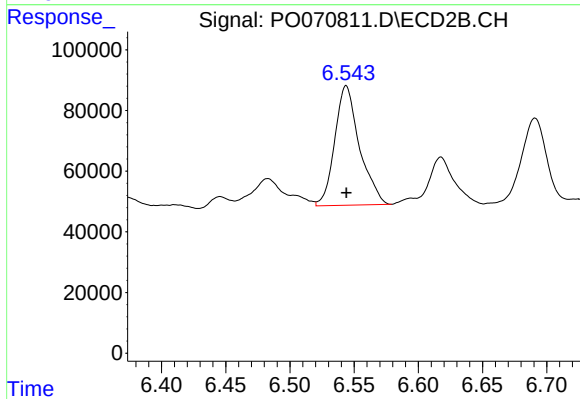

#32 AR-1260-2

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 528023
Conc: 143.89 ng/ml

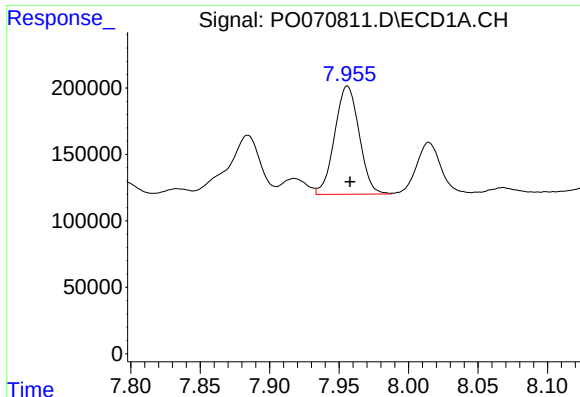


#33 AR-1260-3

R.T.: 7.956 min
Delta R.T.: -0.002 min
Response: 1000120
Conc: 186.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
349-346


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:41 PM

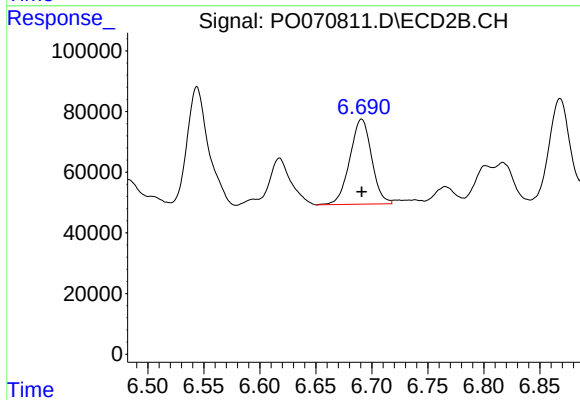


#33 AR-1260-3

R.T.: 6.691 min
Delta R.T.: 0.000 min
Response: 379554
Conc: 122.26 ng/ml

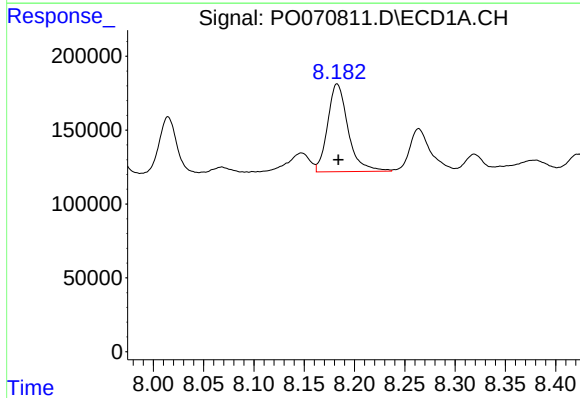


#34 AR-1260-4

R.T.: 8.183 min
Delta R.T.: -0.001 min
Response: 840484
Conc: 165.09 ng/ml

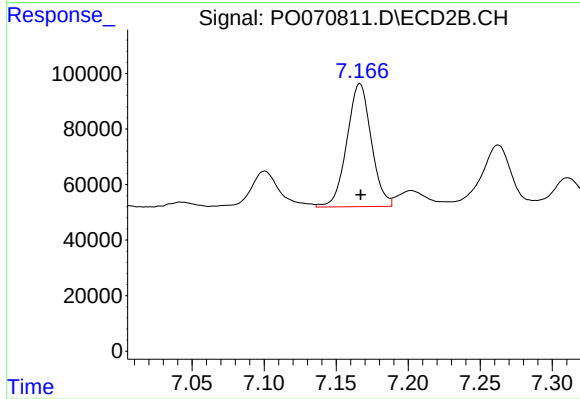

#34 AR-1260-4

R.T.: 7.166 min
Delta R.T.: 0.000 min
Response: 521337
Conc: 186.96 ng/ml

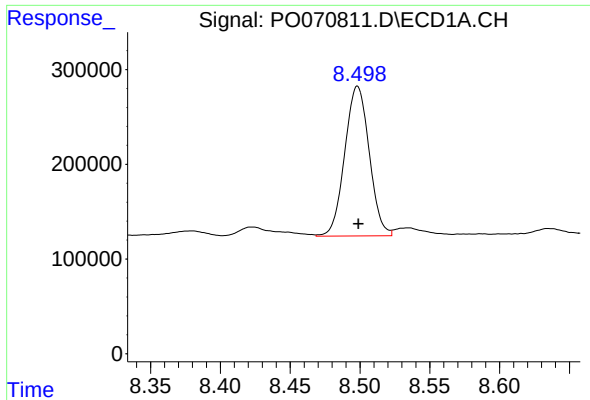


#35 AR-1260-5

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 1928478
Conc: 161.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
349-346

Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:41 PM

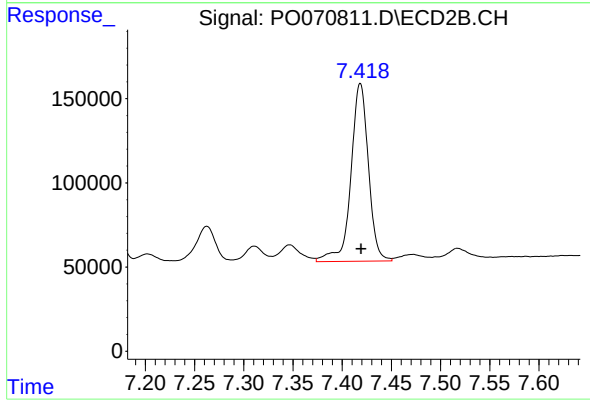

#35 AR-1260-5

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1309359
Conc: 167.26 ng/ml