

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082420\
 Data File : P0070820.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2020 15:05
 Operator : DD\AJ
 Sample : L3774-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-1-2

Manual Integrations
 APPROVED

Ankita
 8/25/2020 2:43:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 15:47:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.560	1394784	1575063	20.022	39.126 #
2) SA Decachlor...	10.030f	8.763f	3081774	2355128	32.918m	41.823m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082420\
Data File : PO070820.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2020 15:05
Operator : DD\AJ
Sample : L3774-09
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-1-2


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 15:47:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

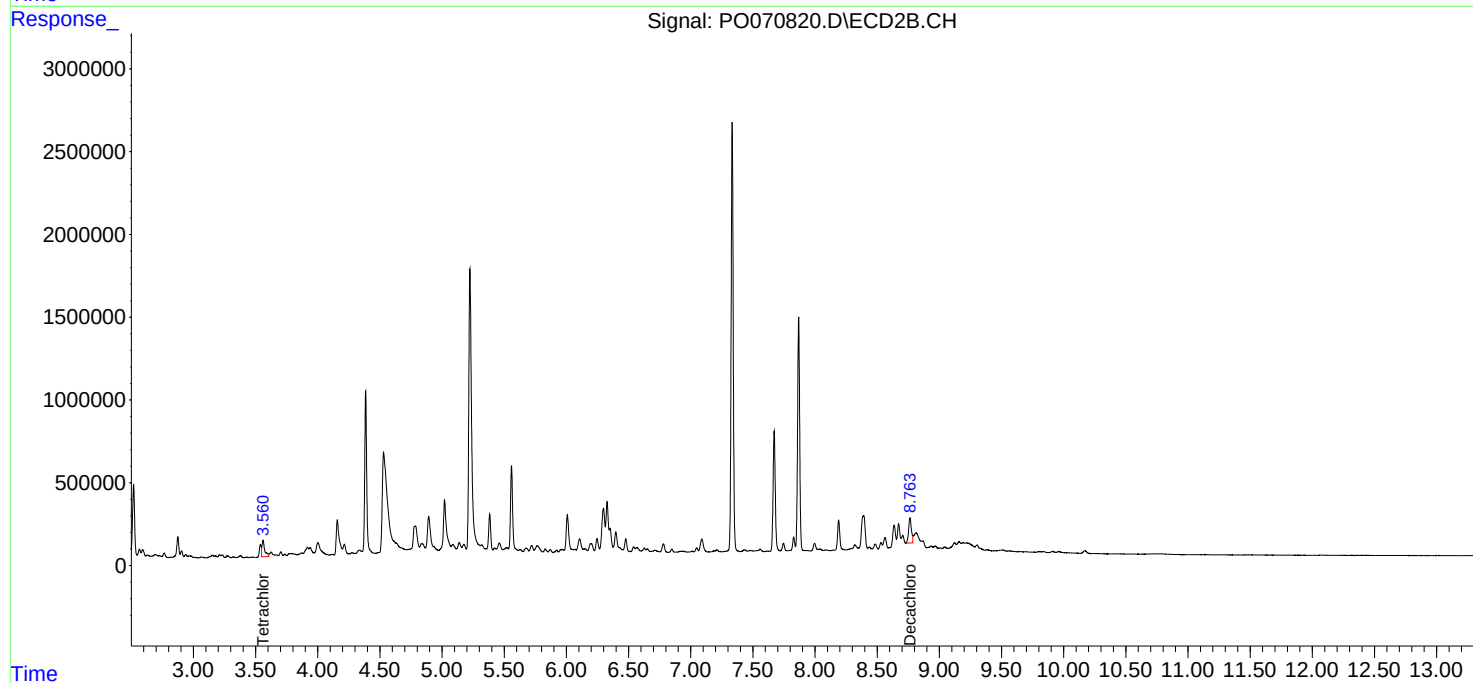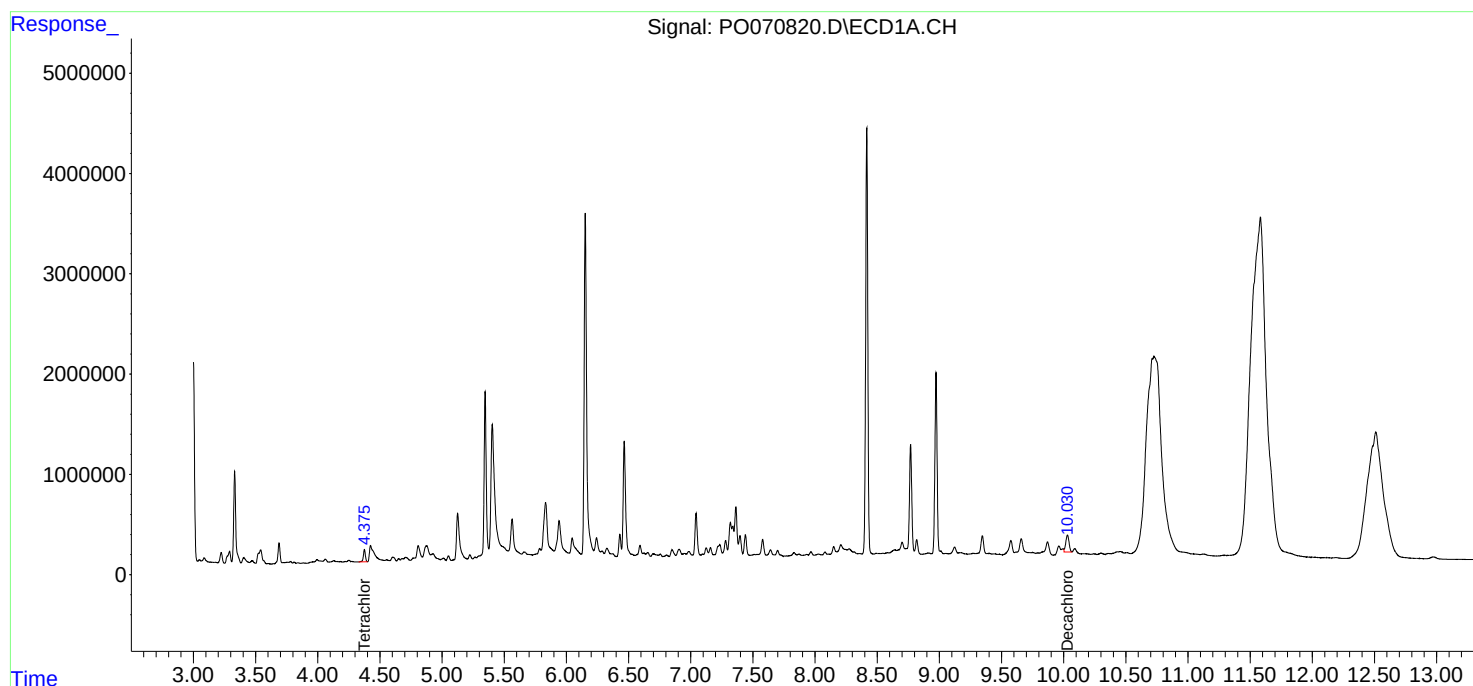

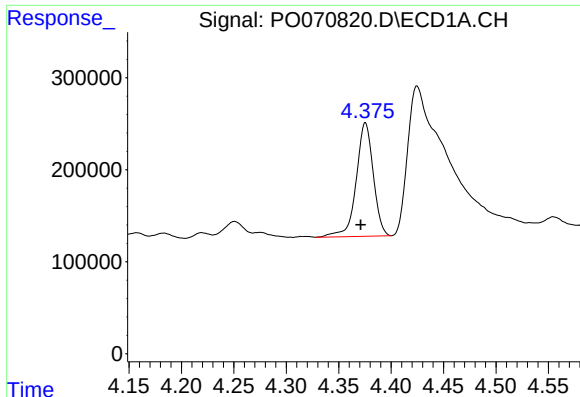


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: 0.004 min
Response: 1394784
Conc: 20.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-1-2


Manual Integrations
APPROVED

Ankita
8/25/2020 2:43:50 PM

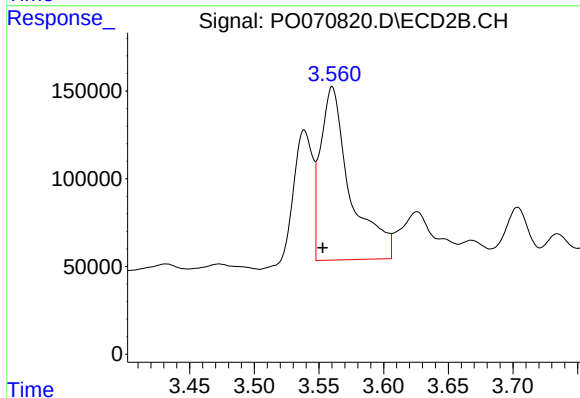


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.007 min
Response: 1575063
Conc: 39.13 ng/ml

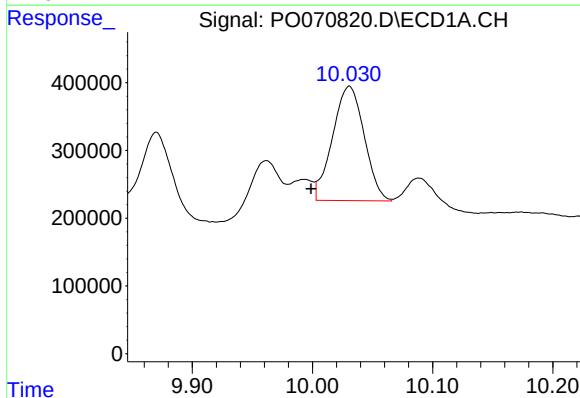

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: 0.031 min
Response: 3081774
Conc: 32.92 ng/ml m

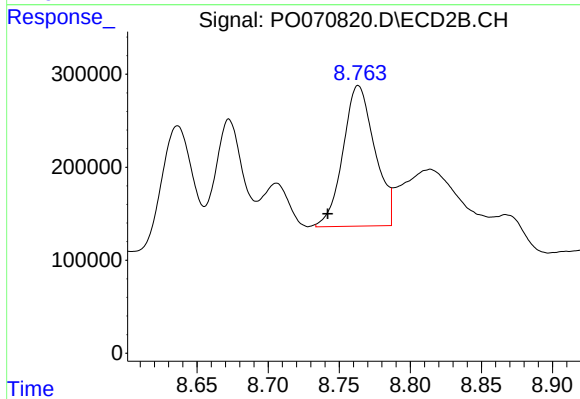

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: 0.021 min
Response: 2355128
Conc: 41.82 ng/ml m