

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082518\
Data File : P0048508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2018 17:01
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 23:14:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.384	3.627	5426266	7288009	28.645	26.920
2) SA Decachlor...	10.066	8.601	2906708	2629022	16.880	15.698

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082518\
Data File : P0048508.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2018 17:01
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 23:14:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

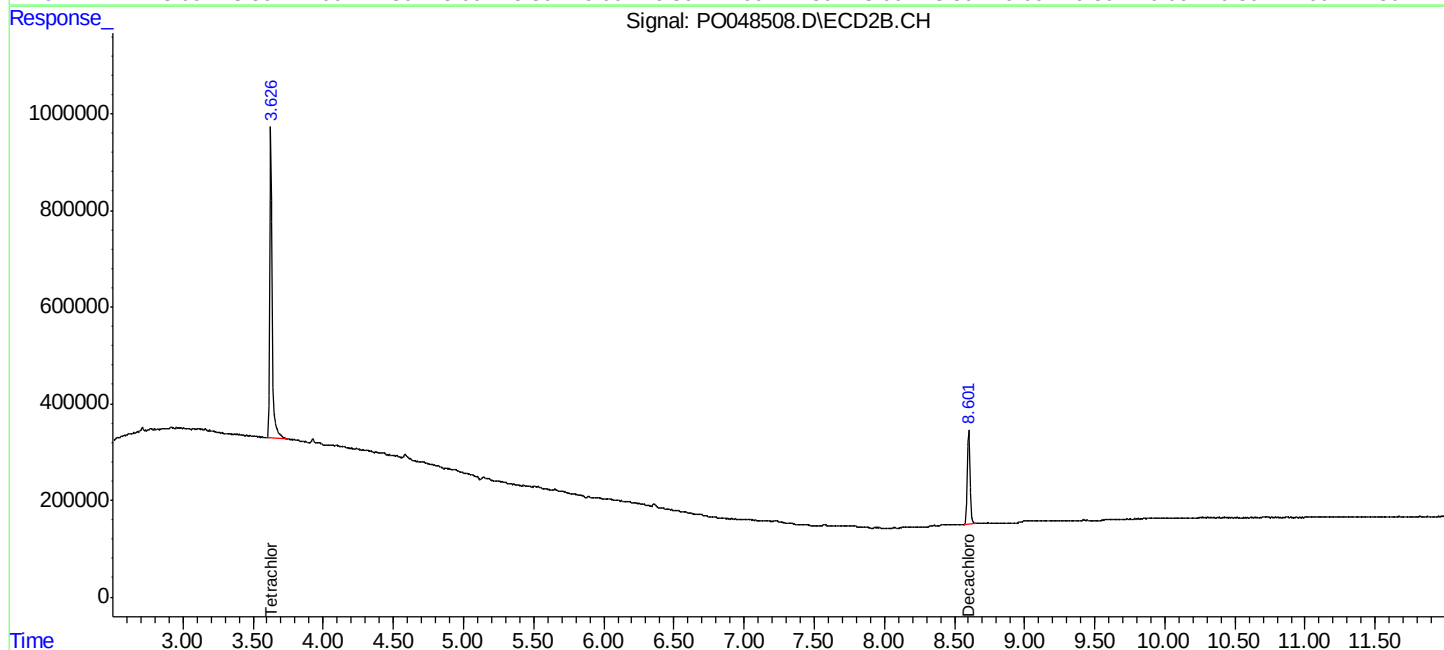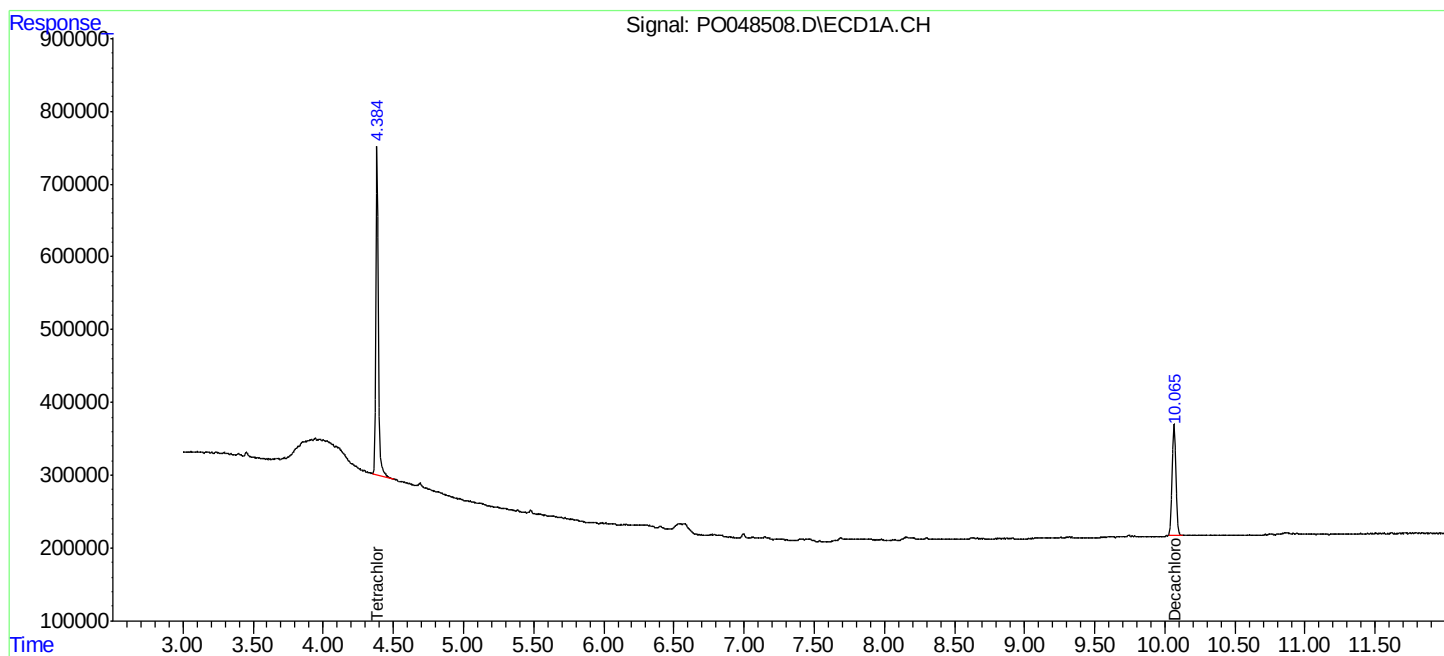


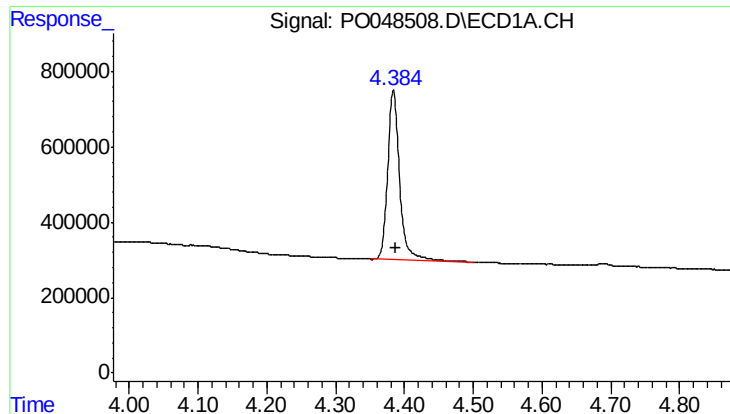

#1 Tetrachloro-m-xylene


R.T.: 4.384 min
Delta R.T.: -0.004 min
Response: 5426266
Conc: 28.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

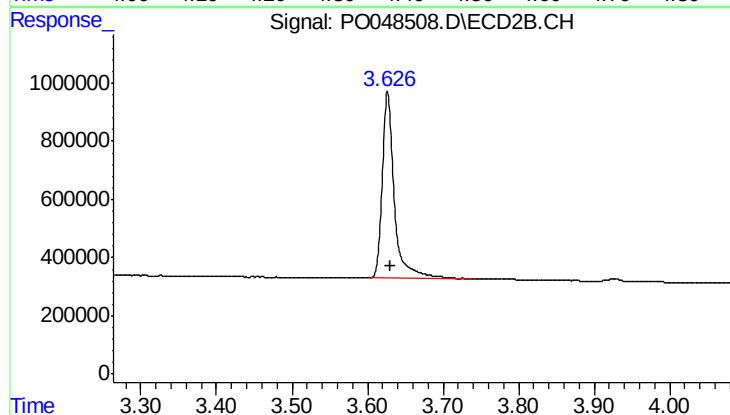


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: -0.003 min
Response: 7288009
Conc: 26.92 ng/ml

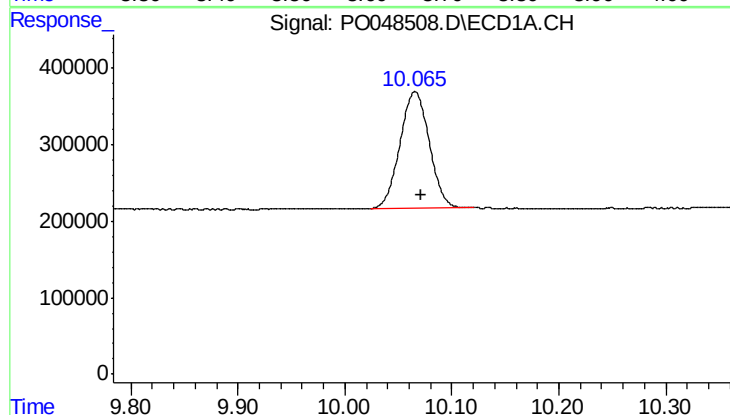

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.006 min
Response: 2906708
Conc: 16.88 ng/ml

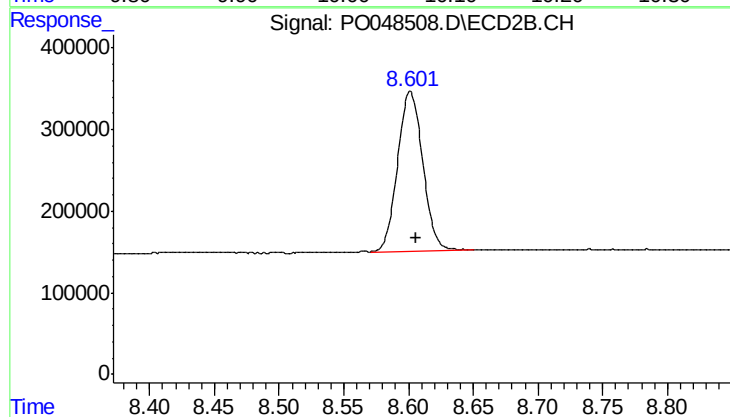

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: -0.005 min
Response: 2629022
Conc: 15.70 ng/ml