

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082518\
 Data File : P0048513.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Aug 2018 19:50
 Operator : SM/SJ
 Sample : J4621-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 9:44:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 05:12:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.623	4927878	6597695	26.014	24.370m
2) SA Decachlor...	10.062	8.598	2417407	2126657	14.038m	12.698

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082518\
Data File : P0048513.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Aug 2018 19:50
Operator : SM/SJ
Sample : J4621-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-2


Manual Integrations
APPROVED

Sohil
8/27/2018 9:44:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 05:12:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

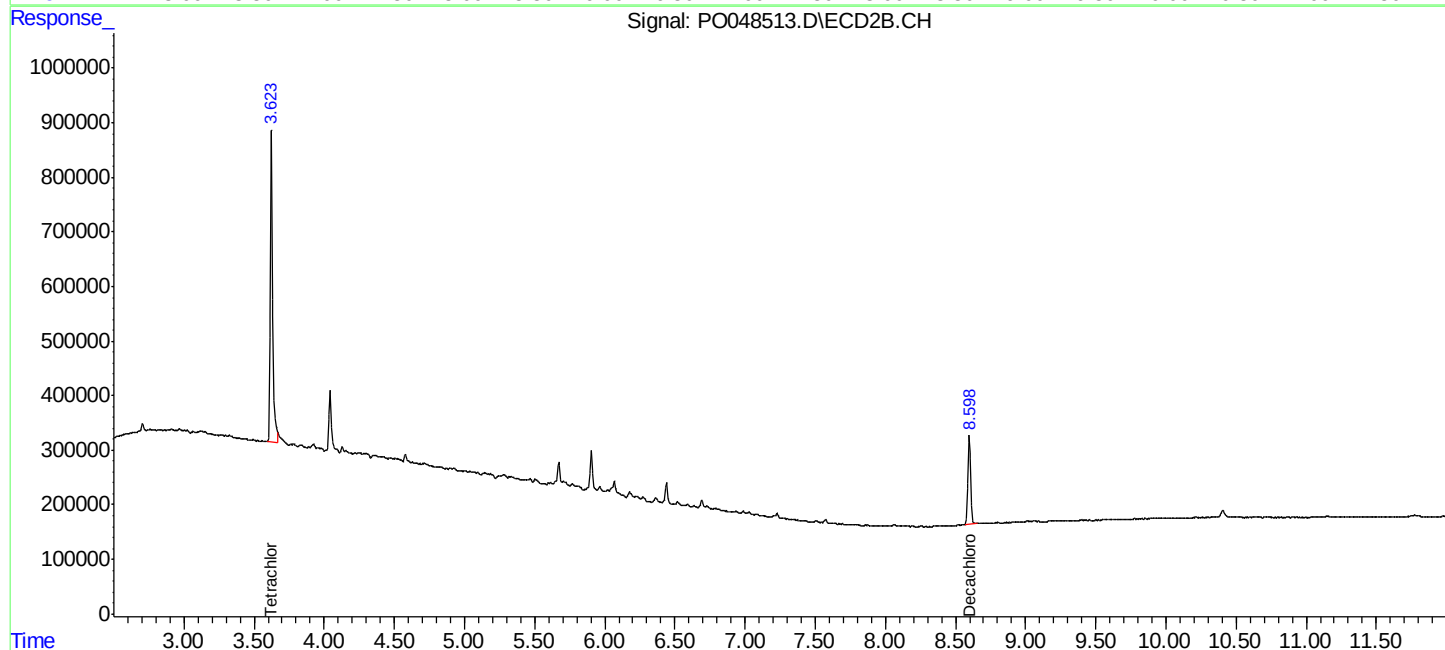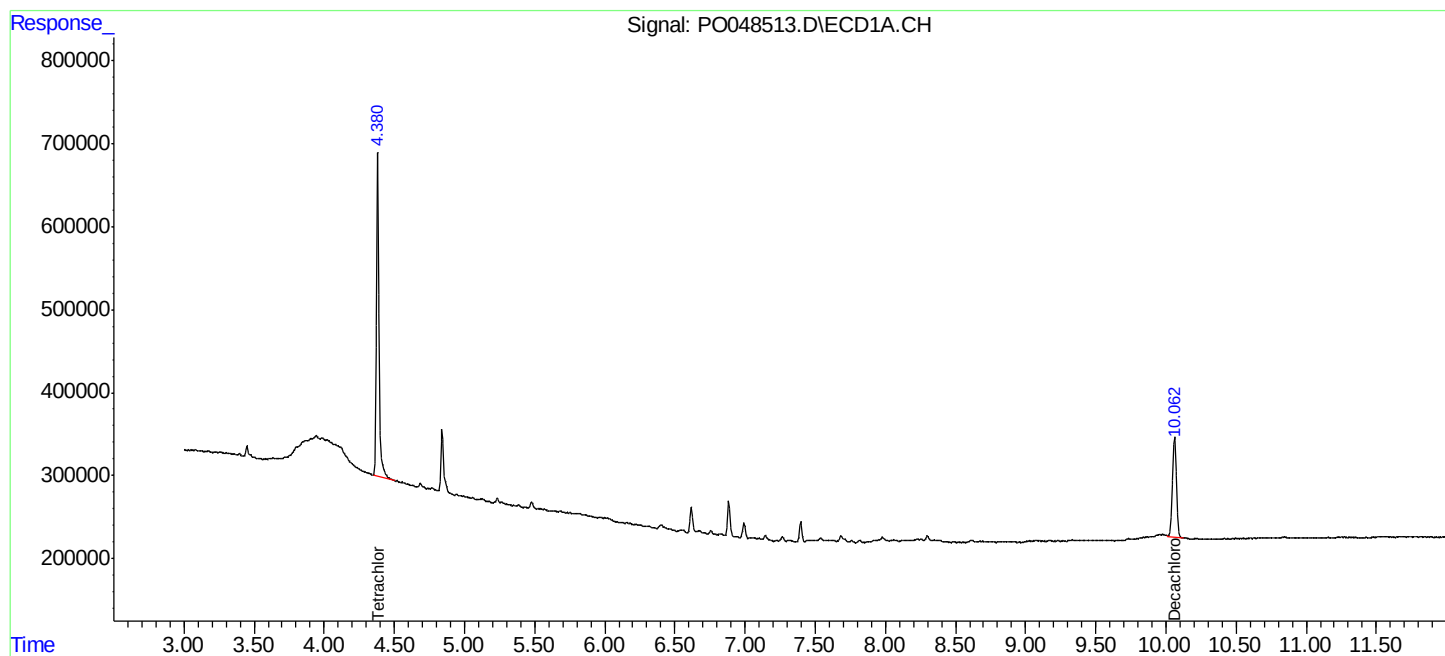

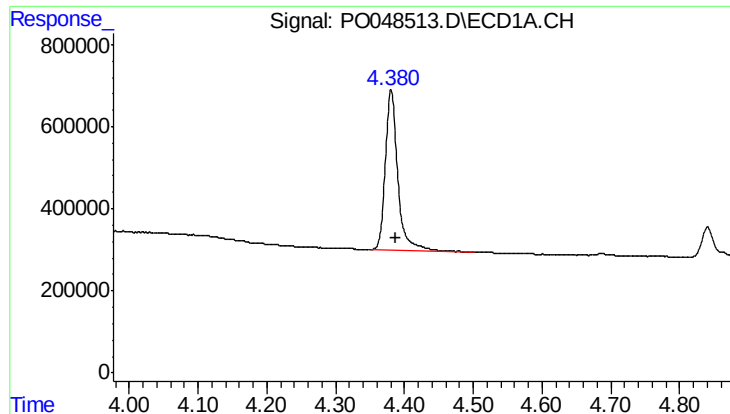


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: -0.007 min
Response: 4927878
Conc: 26.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-2


Manual Integrations
APPROVED

Sohil
8/27/2018 9:44:31 AM

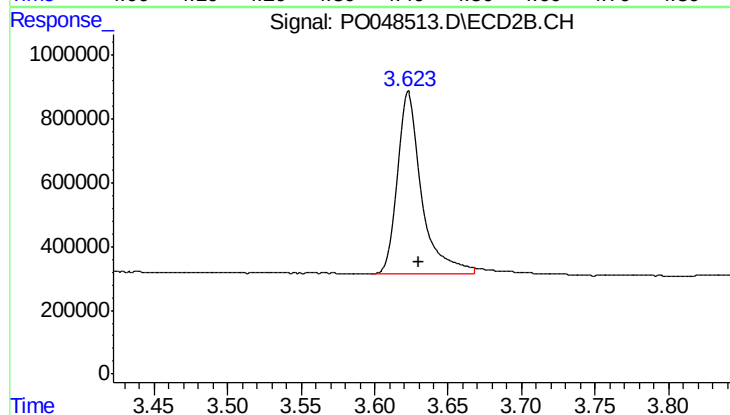


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.008 min
Response: 6597695
Conc: 24.37 ng/ml m

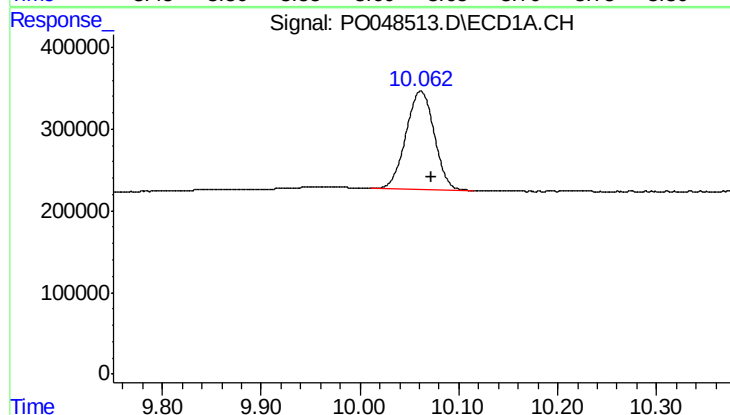

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.010 min
Response: 2417407
Conc: 14.04 ng/ml m

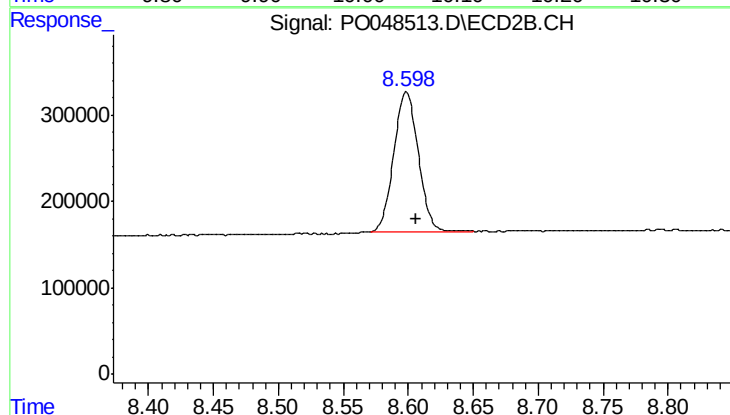

#2 Decachlorobiphenyl

R.T.: 8.598 min
Delta R.T.: -0.008 min
Response: 2126657
Conc: 12.70 ng/ml