

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
 Data File : P0070833.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2020 10:48
 Operator : DD\AJ
 Sample : L3774-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-1-1RE

Manual Integrations
 APPROVED

Ankita
 8/26/2020 11:46:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 14:46:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.560	1952925	999142	28.034	24.819m
2) SA Decachlor...	9.991	8.764f	556198	1996274	5.941m	35.450m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082520\
Data File : PO070833.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2020 10:48
Operator : DD\AJ
Sample : L3774-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-1-1RE


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 14:46:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

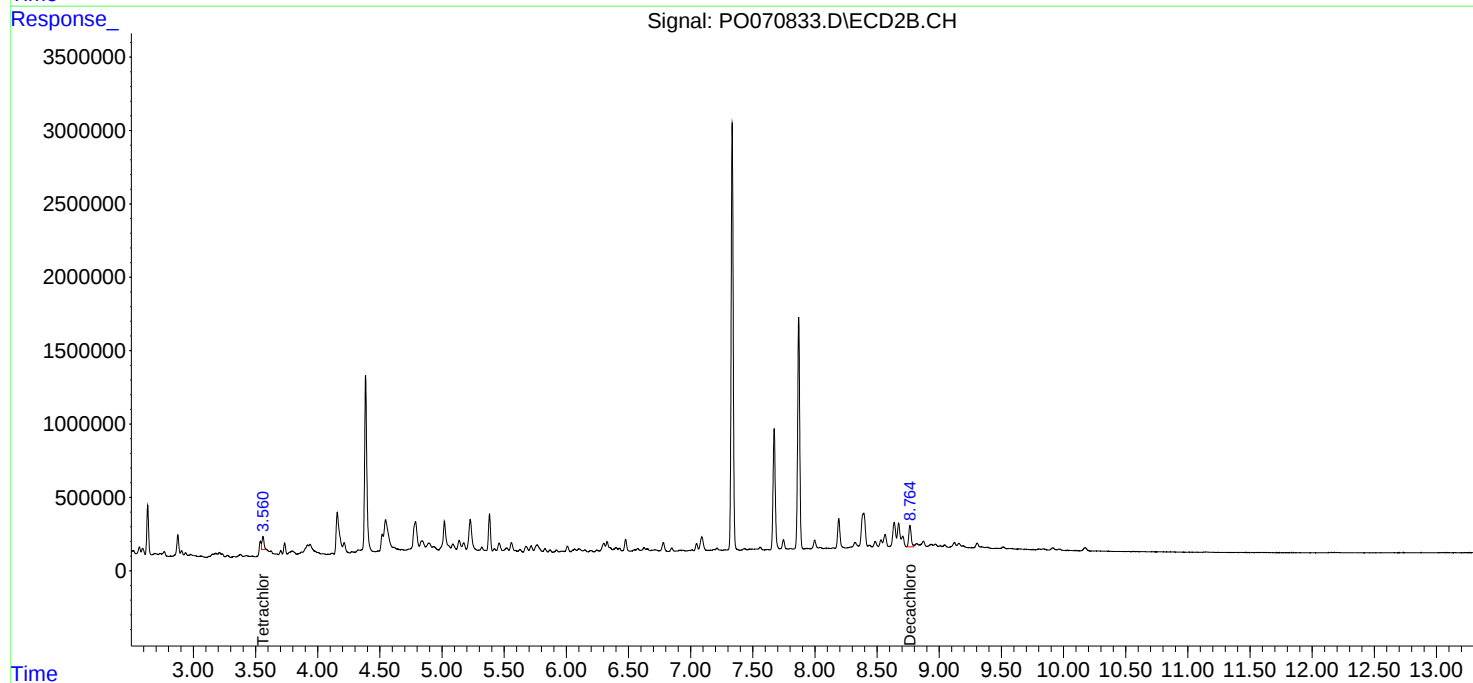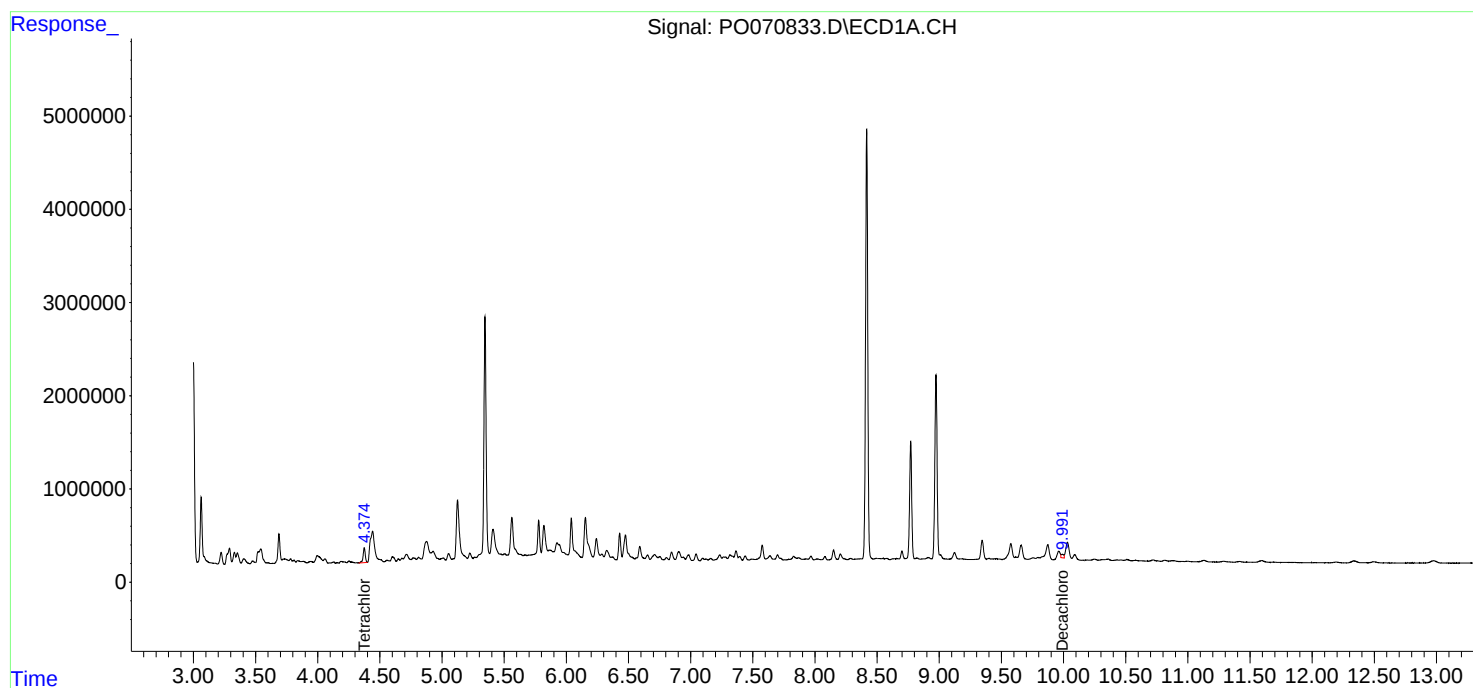

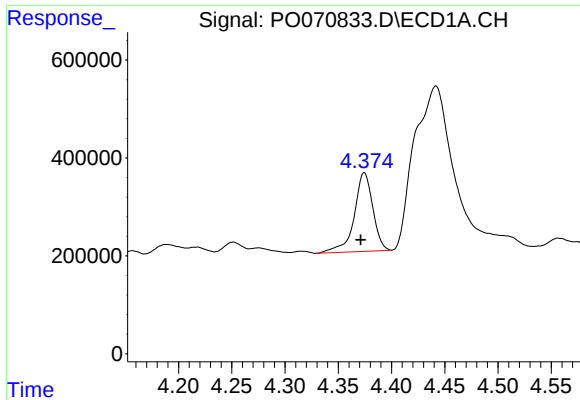


#1 Tetrachloro-m-xylene

R.T.: 4.374 min
Delta R.T.: 0.003 min
Response: 1952925
Conc: 28.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-1-1RE


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:25 AM

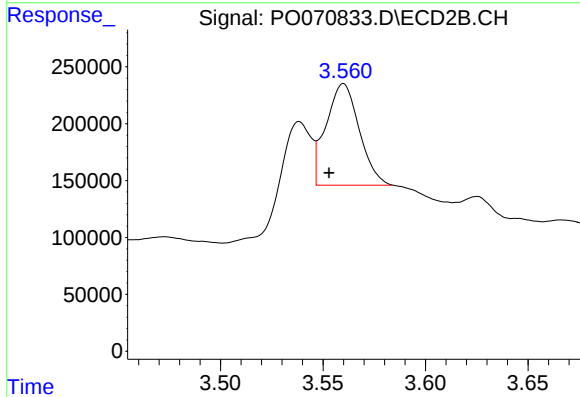


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.007 min
Response: 999142
Conc: 24.82 ng/ml m

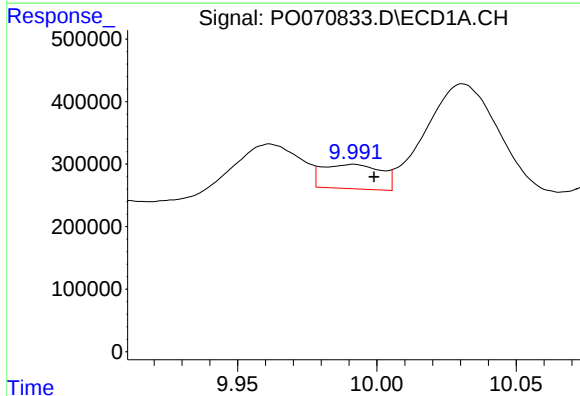

#2 Decachlorobiphenyl

R.T.: 9.991 min
Delta R.T.: -0.008 min
Response: 556198
Conc: 5.94 ng/ml m

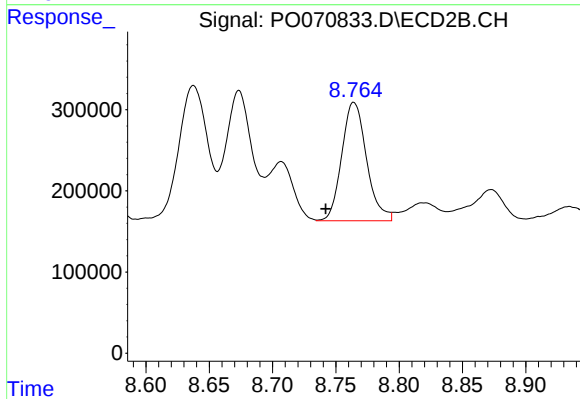

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.022 min
Response: 1996274
Conc: 35.45 ng/ml m