

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
 Data File : P0070834.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2020 11:05
 Operator : DD\AJ
 Sample : L3774-09RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-1-2RE

Manual Integrations
 APPROVED

Ankita
 8/26/2020 11:46:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 14:47:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.559	1616279	1616067	23.202	40.144m#
2) SA Decachlor...	10.005	8.762f	420814	2202777	4.495m	39.118m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082520\
Data File : PO070834.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2020 11:05
Operator : DD\AJ
Sample : L3774-09RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-1-2RE


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 14:47:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

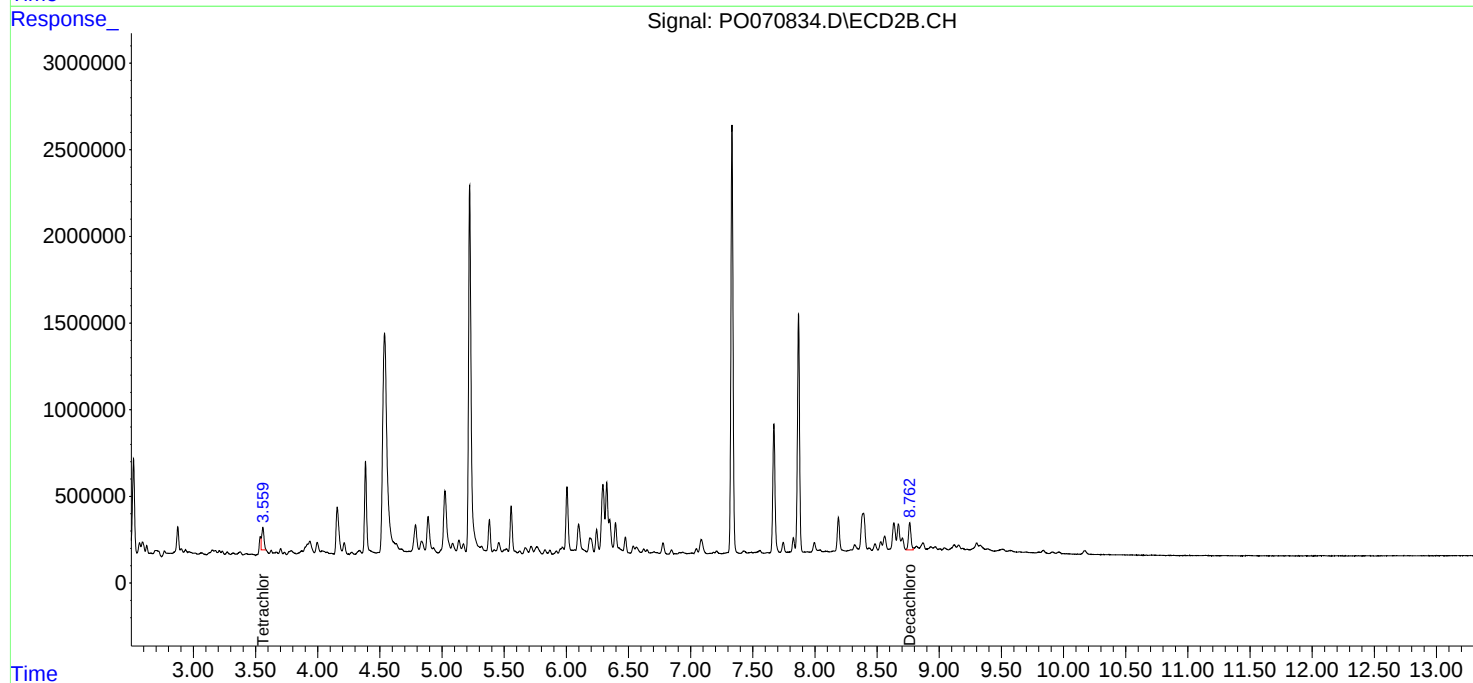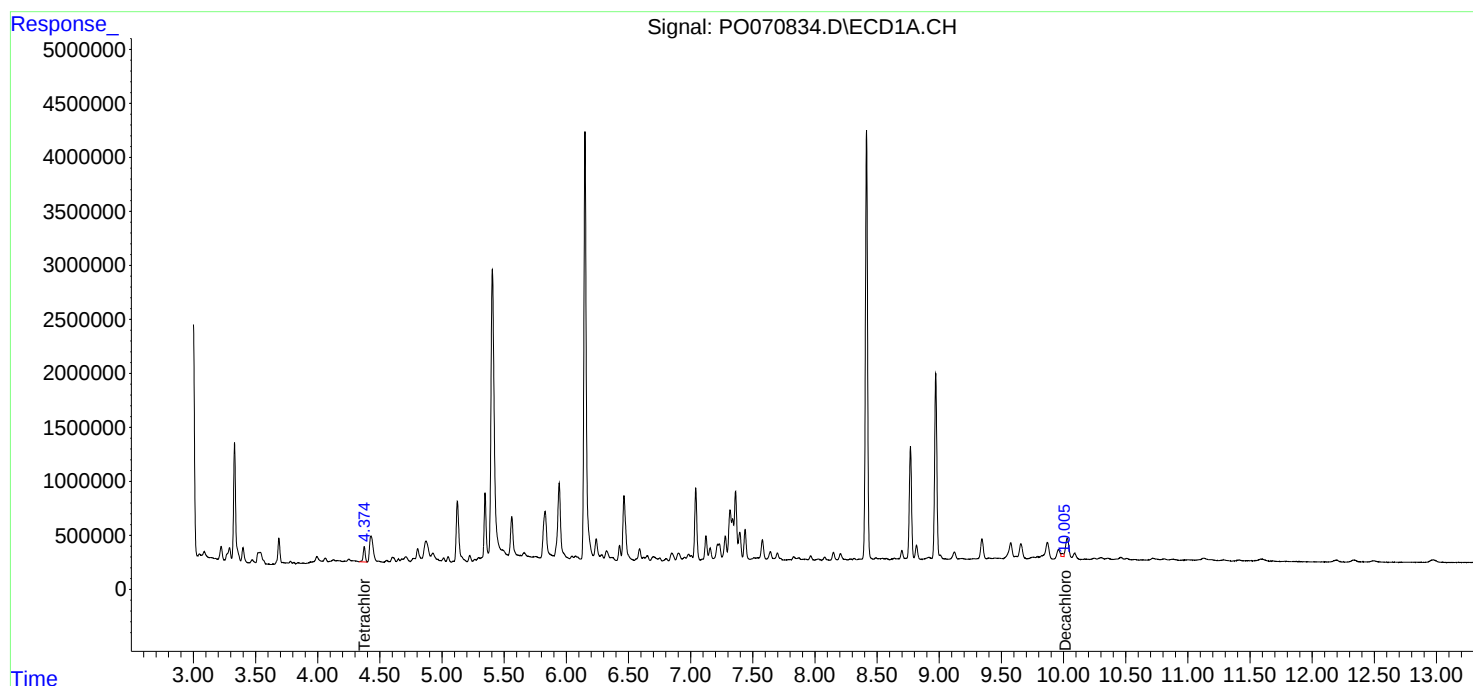

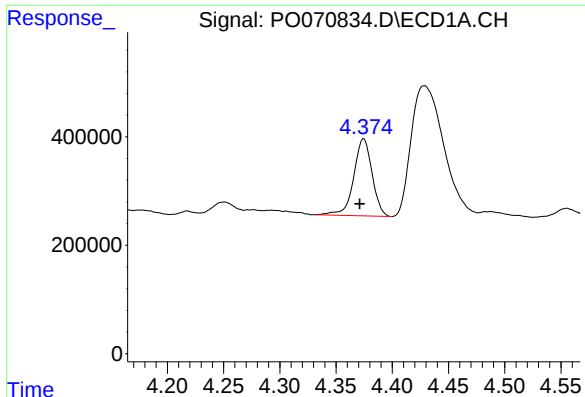


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: 0.004 min
Response: 1616279
Conc: 23.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-1-2RE


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:27 AM

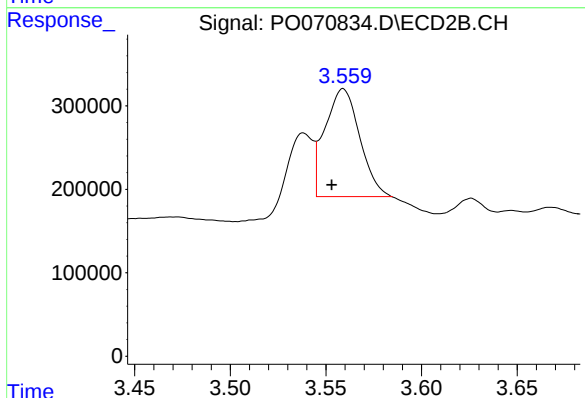


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: 0.006 min
Response: 1616067
Conc: 40.14 ng/ml m

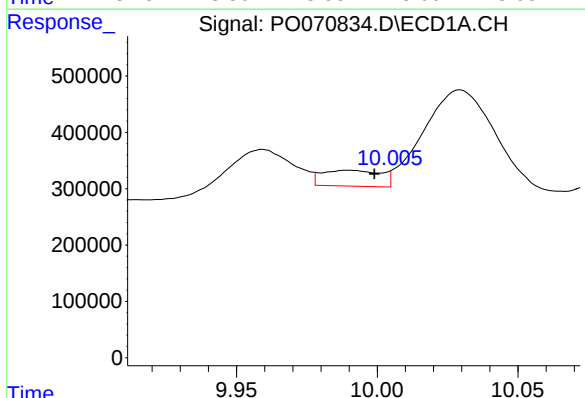

#2 Decachlorobiphenyl

R.T.: 10.005 min
Delta R.T.: 0.006 min
Response: 420814
Conc: 4.49 ng/ml m

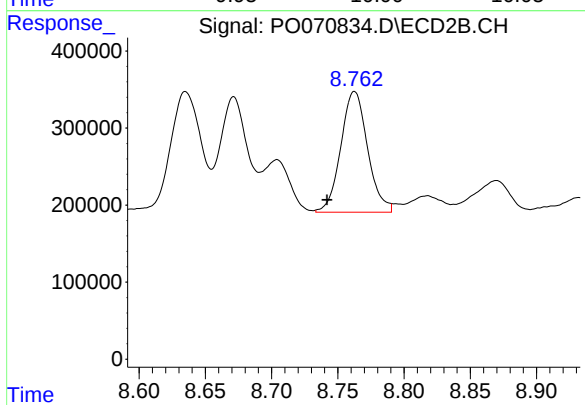

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.020 min
Response: 2202777
Conc: 39.12 ng/ml m