

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
 Data File : P0070840.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2020 15:23
 Operator : DD\AJ
 Sample : L3786-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 129

Manual Integrations
 APPROVED

Ankita
 8/26/2020 11:46:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 17:19:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.557	1306627	784406	18.757	19.485
2) SA Decachlor...	10.000	8.743	1198730	749288	12.804m	13.306

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082520\
Data File : PO070840.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2020 15:23
Operator : DD\AJ
Sample : L3786-06
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
129


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 17:19:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

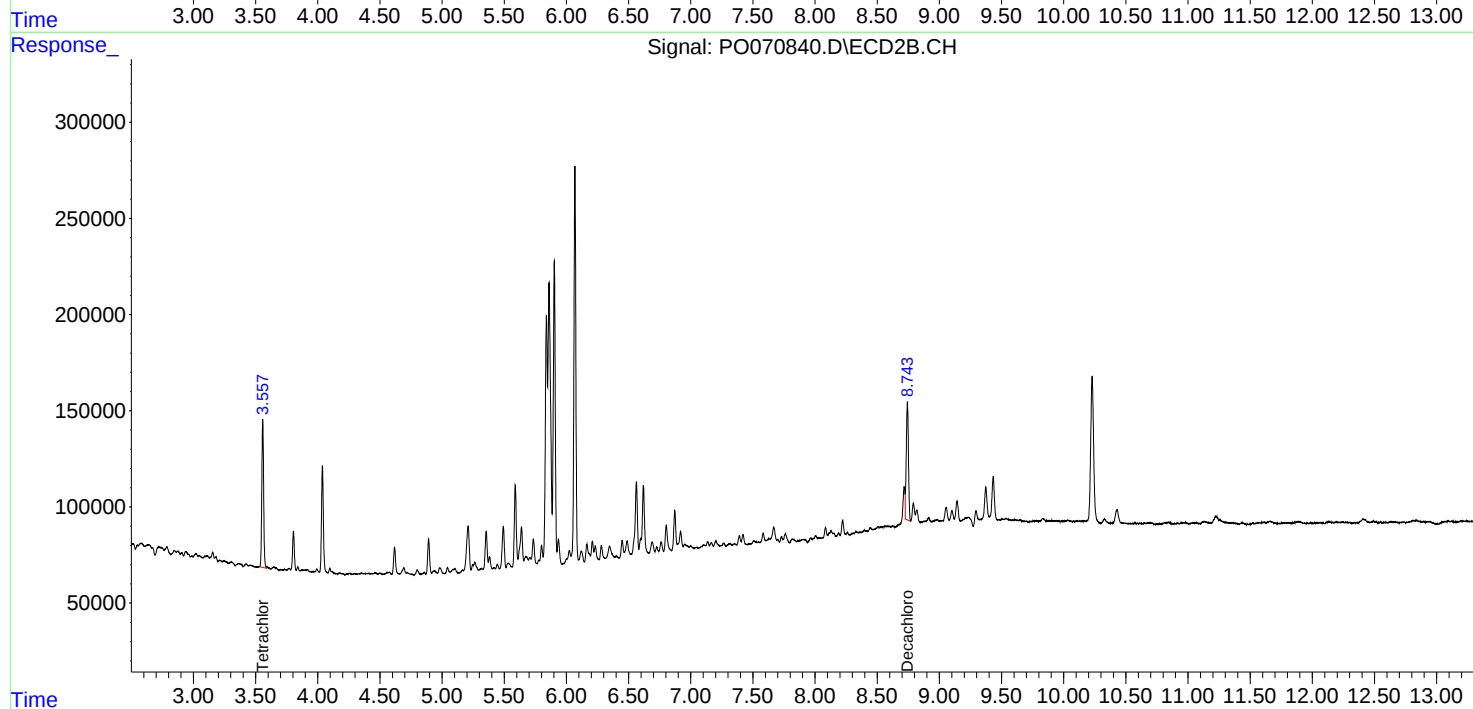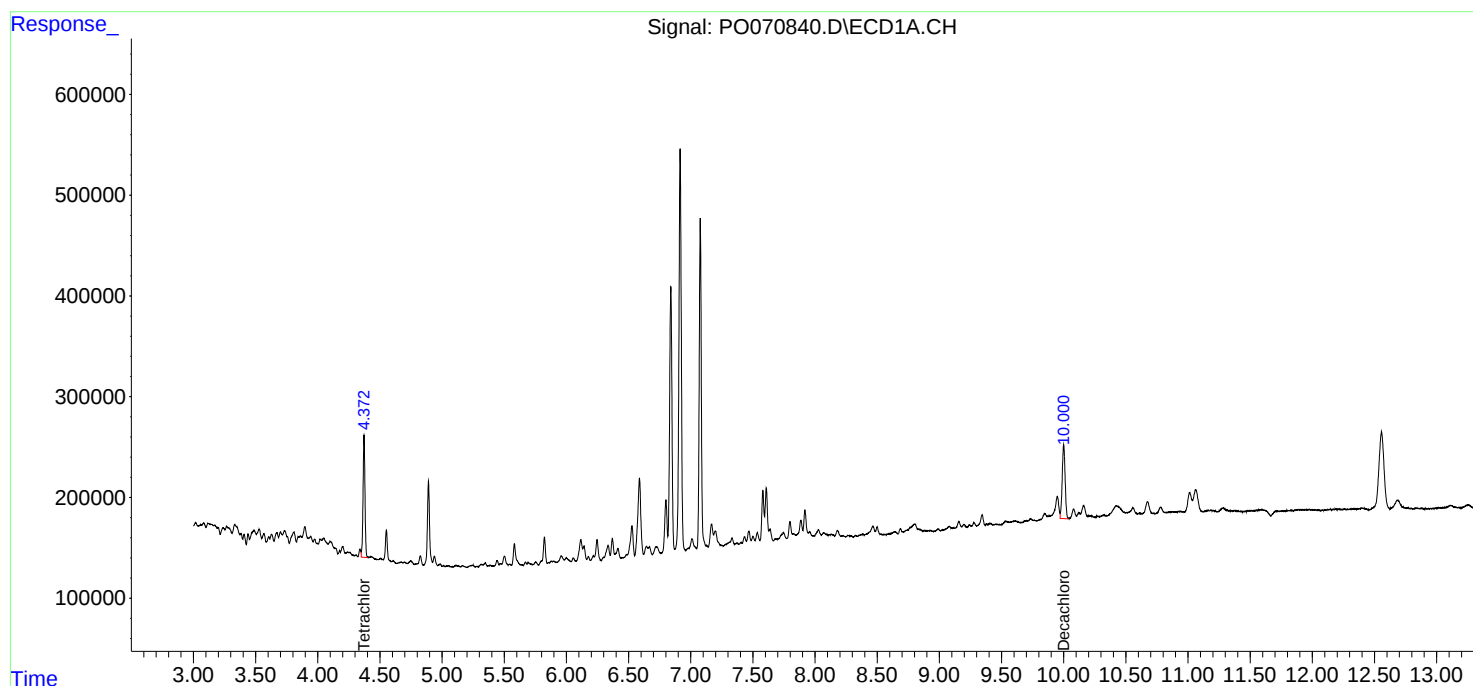

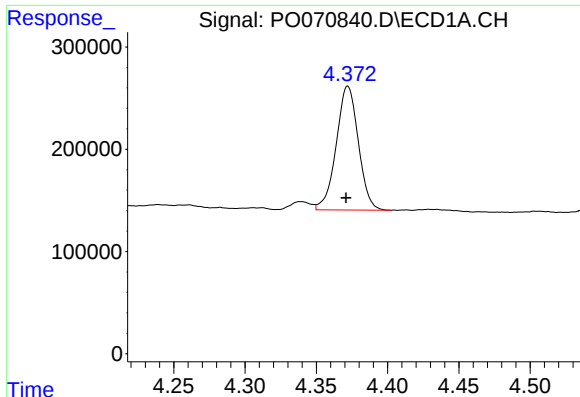


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.001 min
Response: 1306627
Conc: 18.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
129


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:31 AM

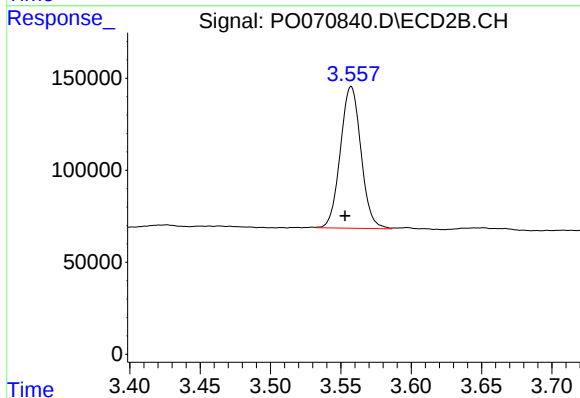


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.004 min
Response: 784406
Conc: 19.49 ng/ml

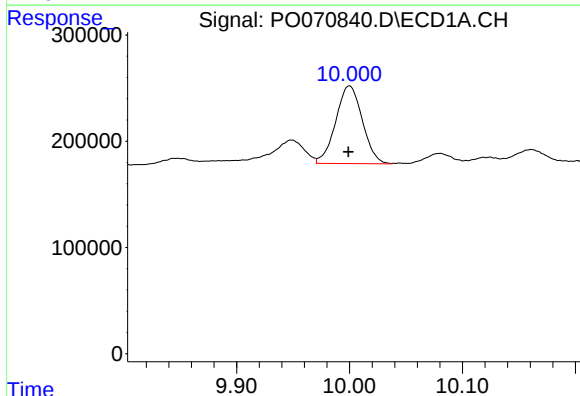

#2 Decachlorobiphenyl

R.T.: 10.000 min
Delta R.T.: 0.000 min
Response: 1198730
Conc: 12.80 ng/ml m

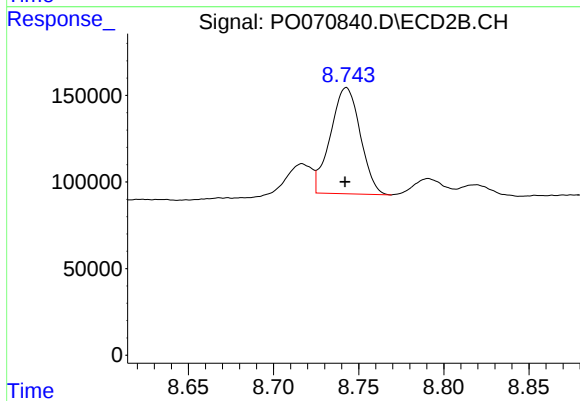

#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.000 min
Response: 749288
Conc: 13.31 ng/ml