

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
 Data File : P0070847.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2020 17:23
 Operator : DD\AJ
 Sample : L3784-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 17:44:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.556	1967739	1153955	28.247	28.665
2) SA Decachlor...	10.000	8.743	1721973	1104905	18.393	19.621

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082520\
Data File : PO070847.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2020 17:23
Operator : DD\AJ
Sample : L3784-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RO-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 17:44:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

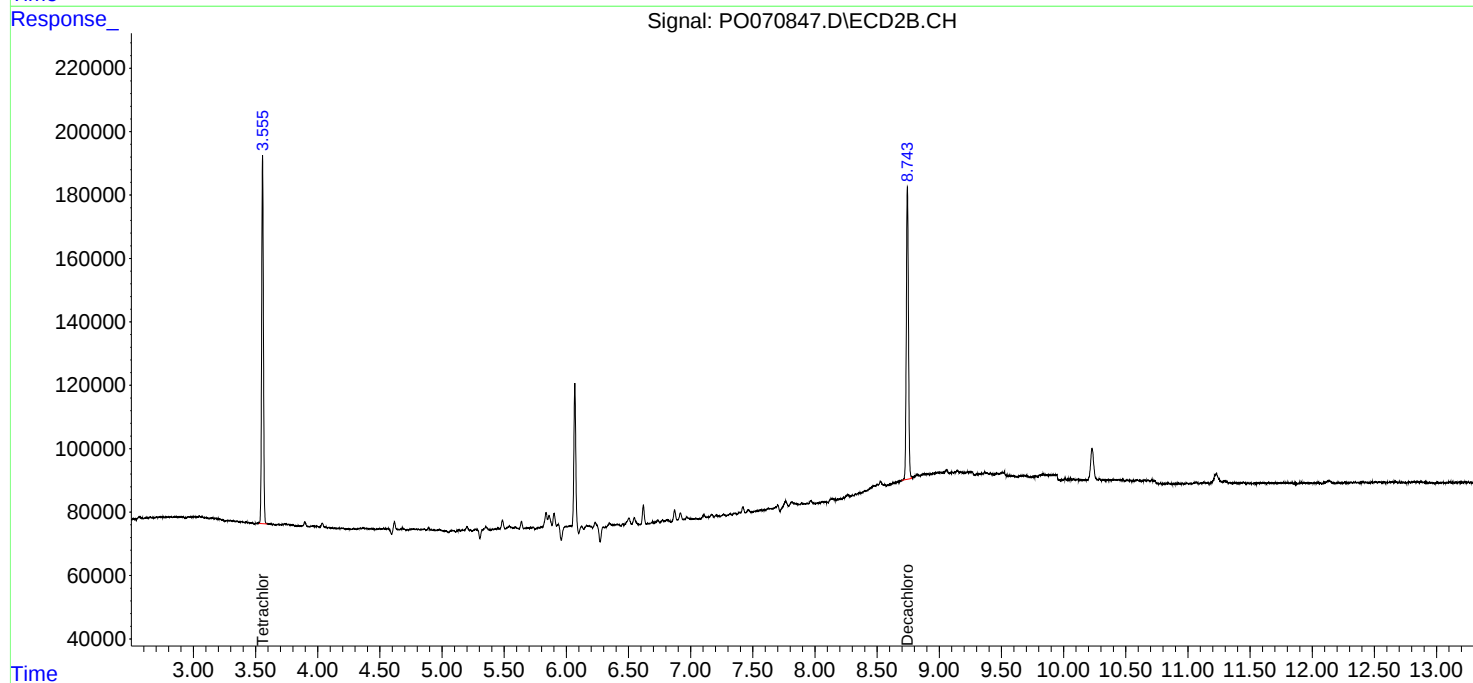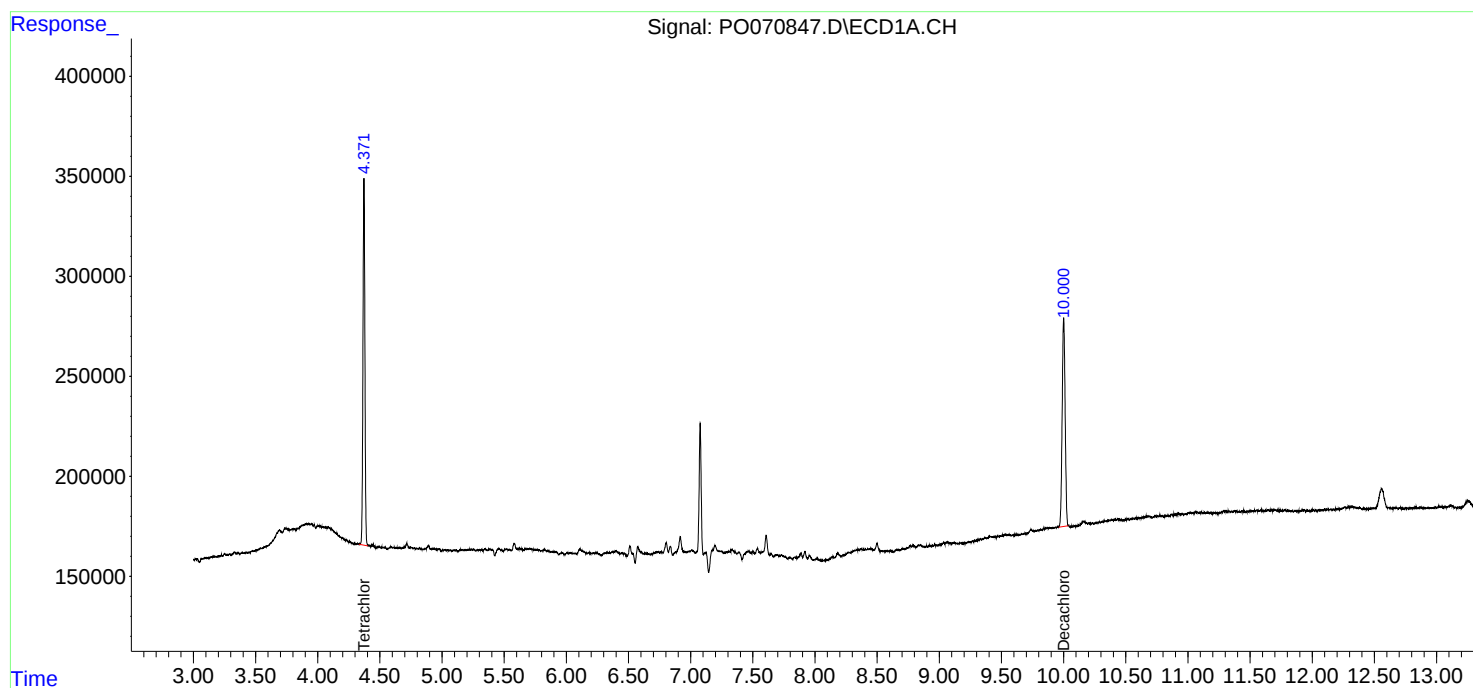


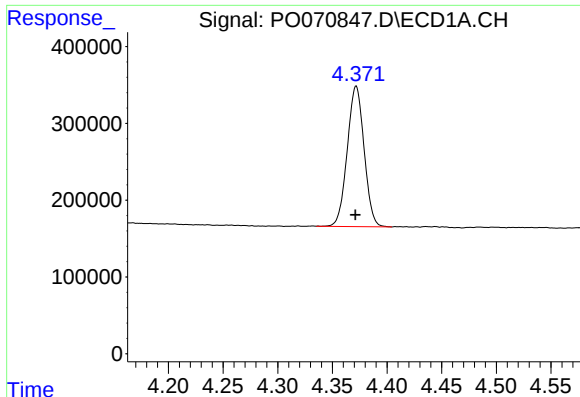

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 1967739
Conc: 28.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-23

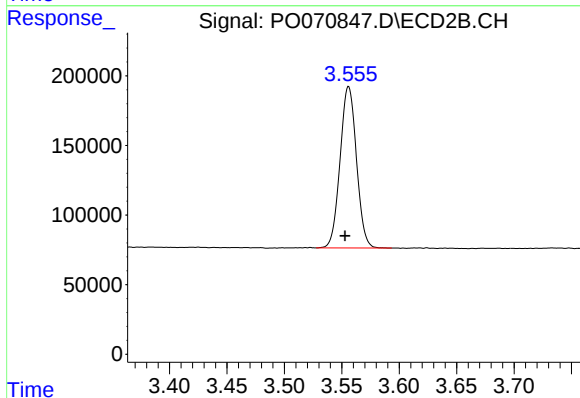


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: 0.003 min
Response: 1153955
Conc: 28.66 ng/ml

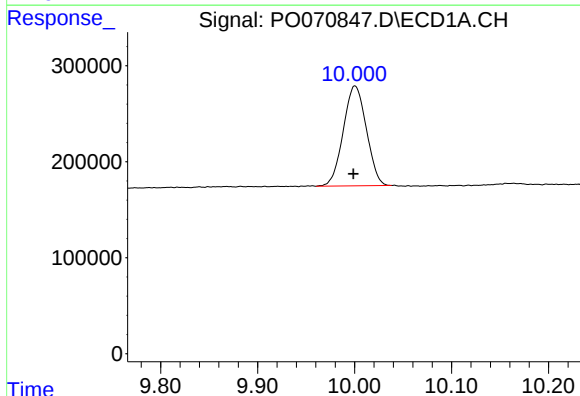

#2 Decachlorobiphenyl

R.T.: 10.000 min
Delta R.T.: 0.001 min
Response: 1721973
Conc: 18.39 ng/ml

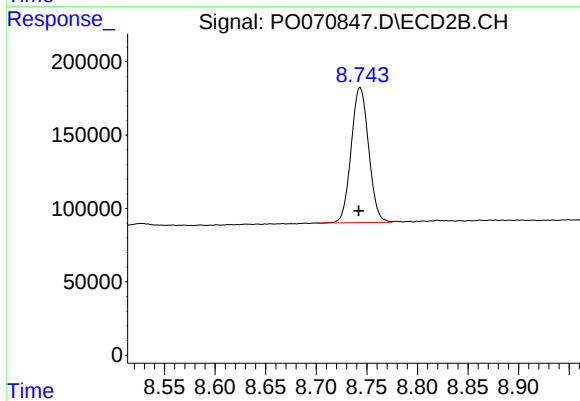

#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.001 min
Response: 1104905
Conc: 19.62 ng/ml