

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
 Data File : P0070849.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Aug 2020 17:57
 Operator : DD\AJ
 Sample : L3784-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-06

Manual Integrations
 APPROVED

Ankita
 8/26/2020 11:46:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 01:42:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.555	2001974	1159296	28.739	28.798
2) SA Decachlor...	9.999	8.743	1710250	1101497	18.268m	19.561

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082520\
Data File : P0070849.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Aug 2020 17:57
Operator : DD\AJ
Sample : L3784-13
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 01:42:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

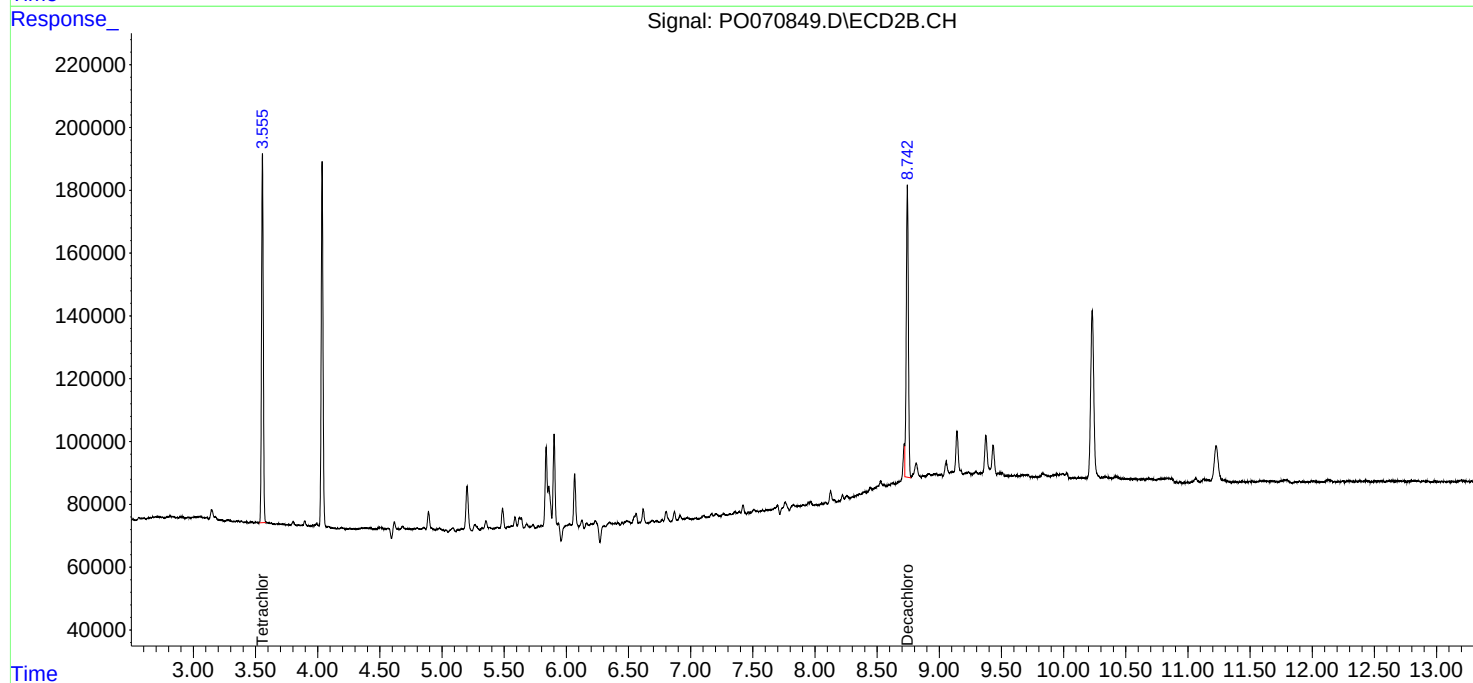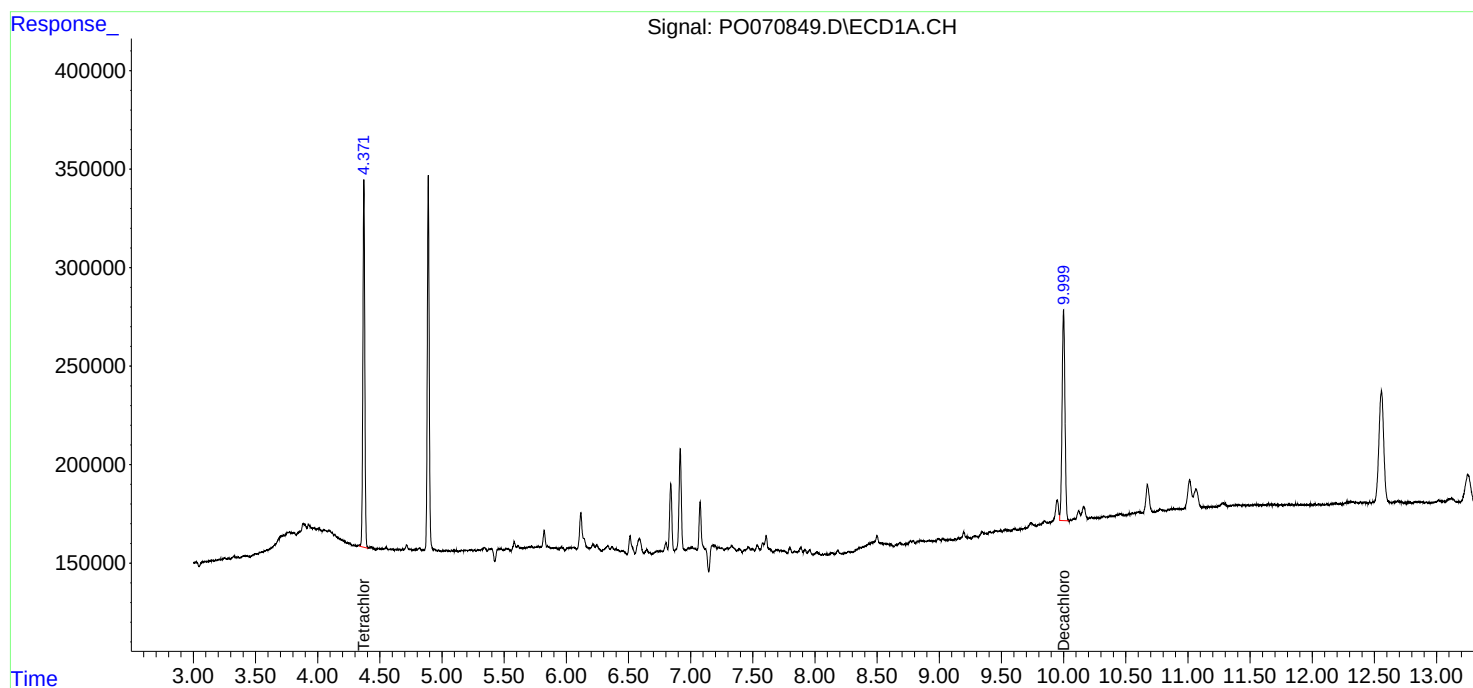

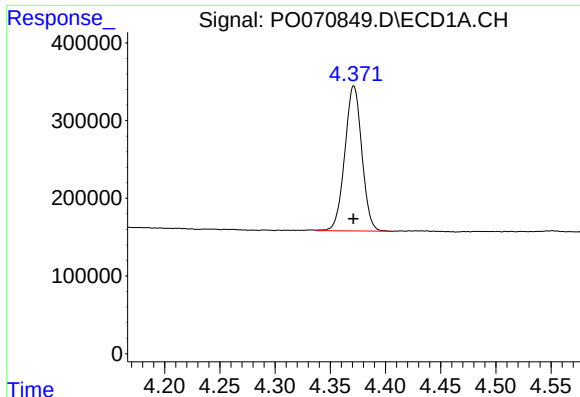


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 2001974
Conc: 28.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
8/26/2020 11:46:38 AM

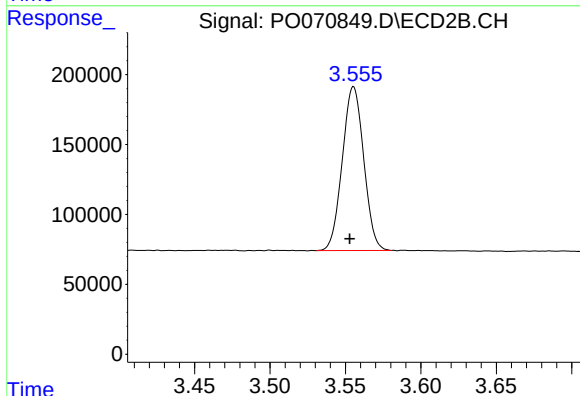


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.002 min
Response: 1159296
Conc: 28.80 ng/ml

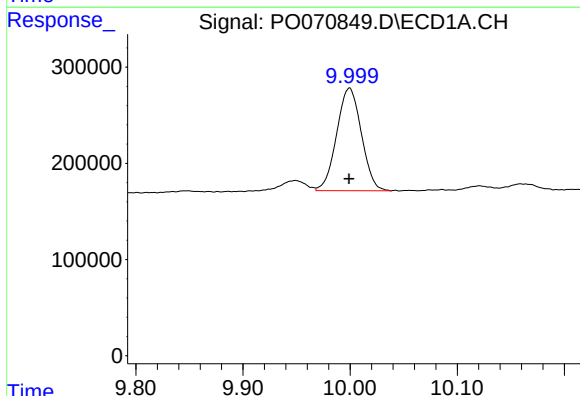

#2 Decachlorobiphenyl

R.T.: 9.999 min
Delta R.T.: 0.000 min
Response: 1710250
Conc: 18.27 ng/ml m

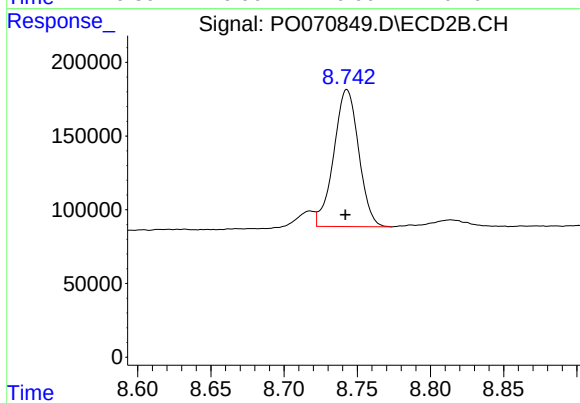

#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.000 min
Response: 1101497
Conc: 19.56 ng/ml