

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082525\
 Data File : P0113224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Aug 2025 14:35
 Operator : YP/AJ
 Sample : Q2948-03 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH590U-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/26/2025
 Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 14:49:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 19 06:08:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.659	3.652	9715902	6683930	1.187	1.321
2) SA Decachlor...	8.678	8.626	6810799	2095050	0.983m	1.106m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082525\
Data File : PO113224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Aug 2025 14:35
Operator : YP/AJ
Sample : Q2948-03 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH590U-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2025
Supervised By :mohammad ahmed 08/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 14:49:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 19 06:08:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

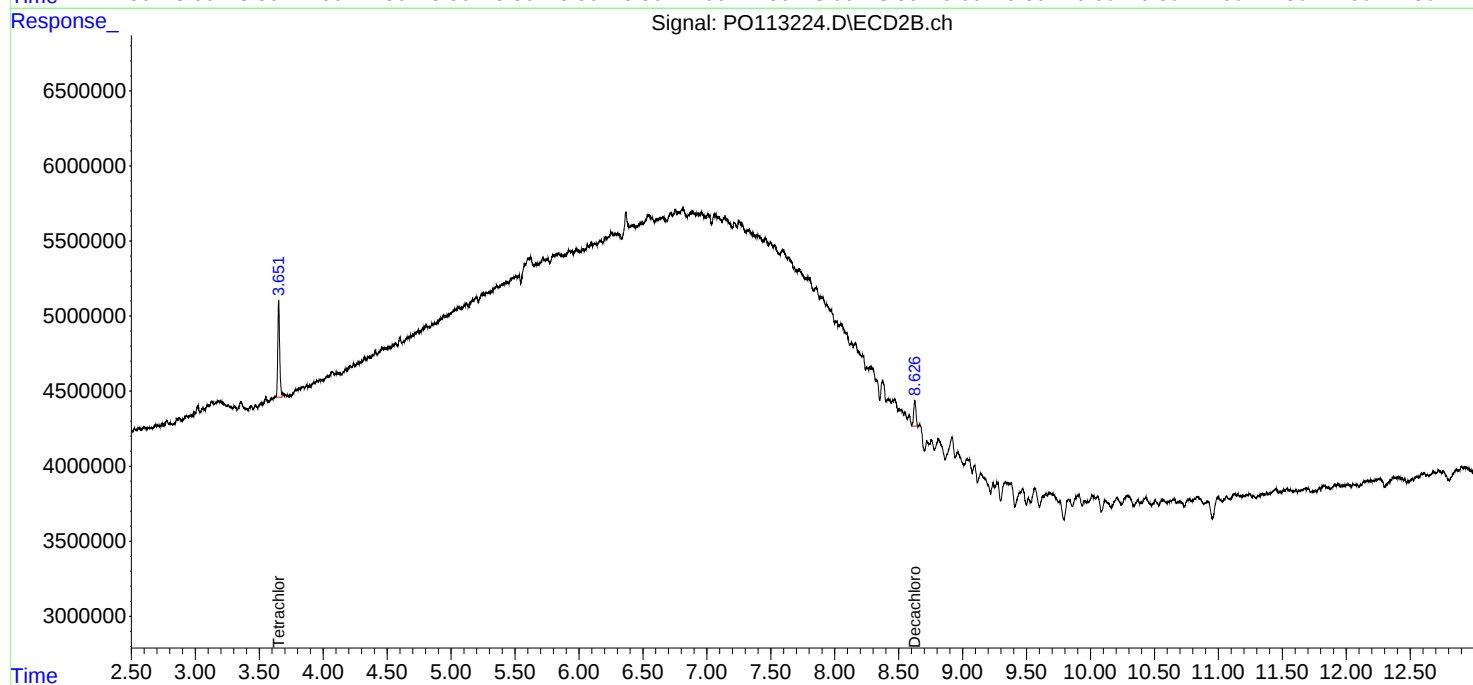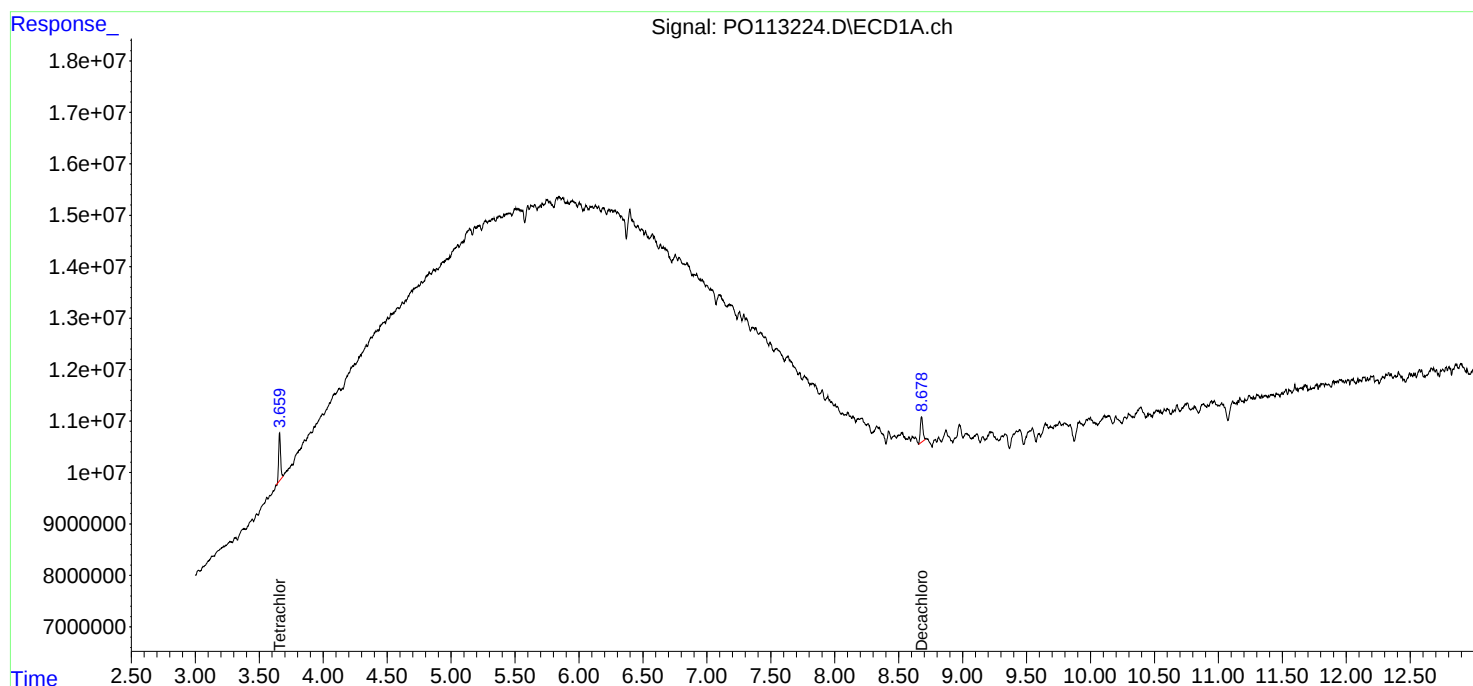

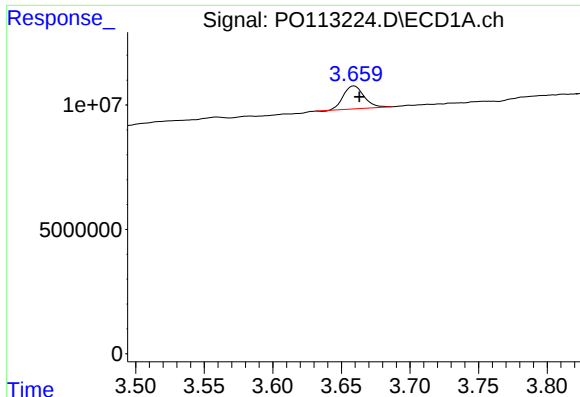


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.004 min
Response: 9715902
Conc: 1.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEH590U-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/26/2025
Supervised By :mohammad ahmed 08/27/2025

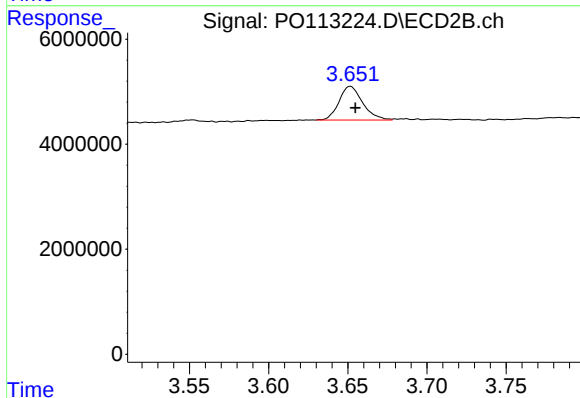


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.003 min
Response: 6683930
Conc: 1.32 ng/ml

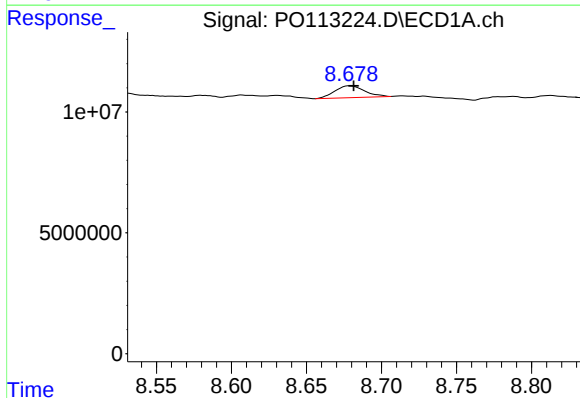

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.004 min
Response: 6810799
Conc: 0.98 ng/ml m

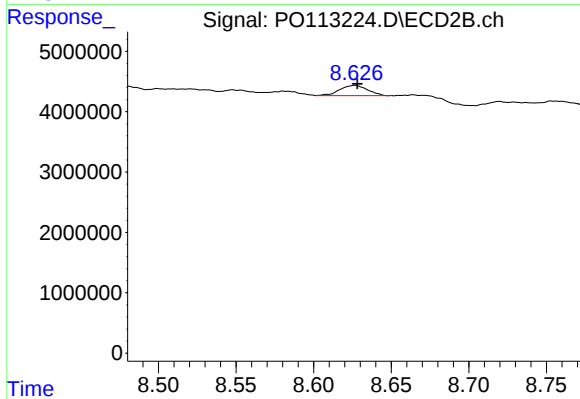

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.003 min
Response: 2095050
Conc: 1.11 ng/ml m