

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082619\
 Data File : P0059845.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Aug 2019 10:00
 Operator : SM/AJ
 Sample : K4490-02RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BRICKRE

Manual Integrations
 APPROVED

Ankita
 8/27/2019 2:47:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 26 14:33:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.118	3.494	1028595	954825	29.378m	26.526
2) SA Decachlor...	9.583	8.352	1448888	1137892	27.235m	28.221

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082619\
Data File : PO059845.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Aug 2019 10:00
Operator : SM/AJ
Sample : K4490-02RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BRICKRE


Manual Integrations
APPROVED

Ankita
8/27/2019 2:47:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 26 14:33:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

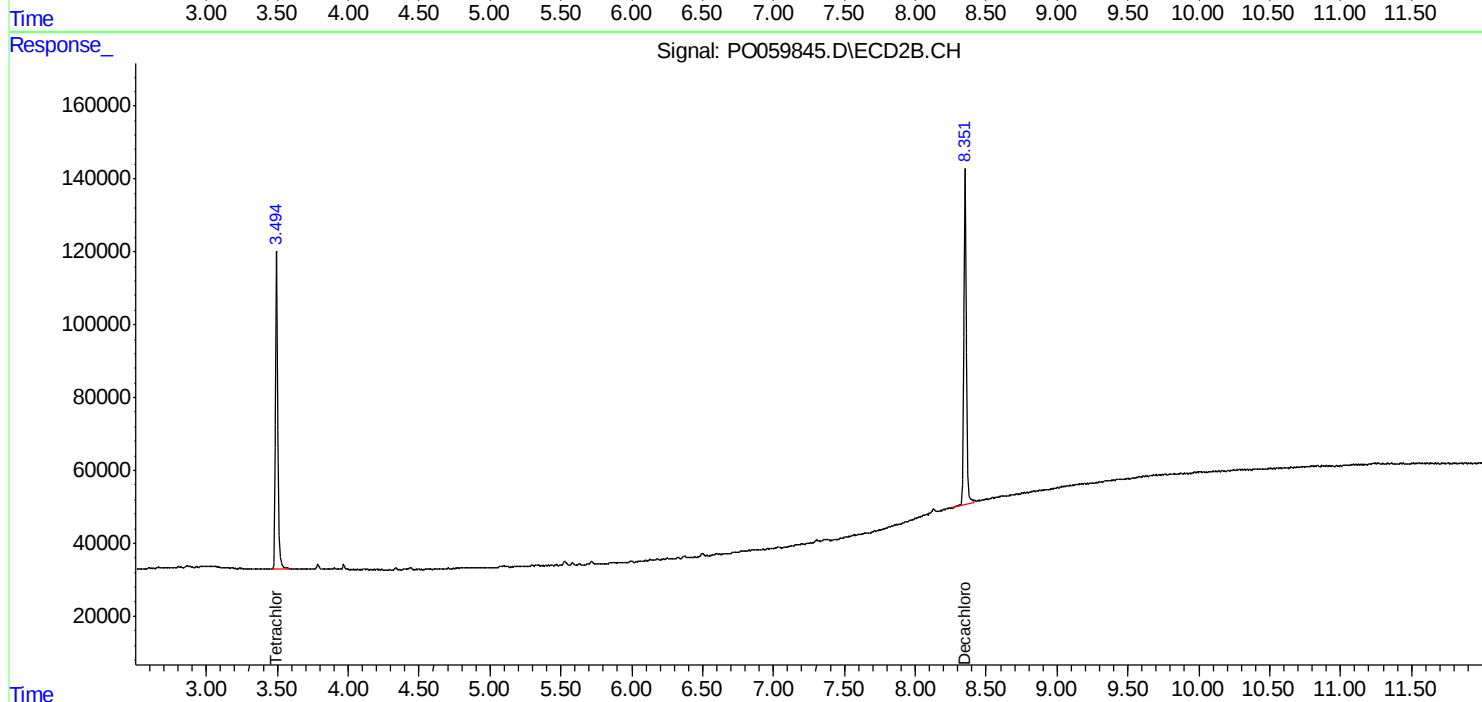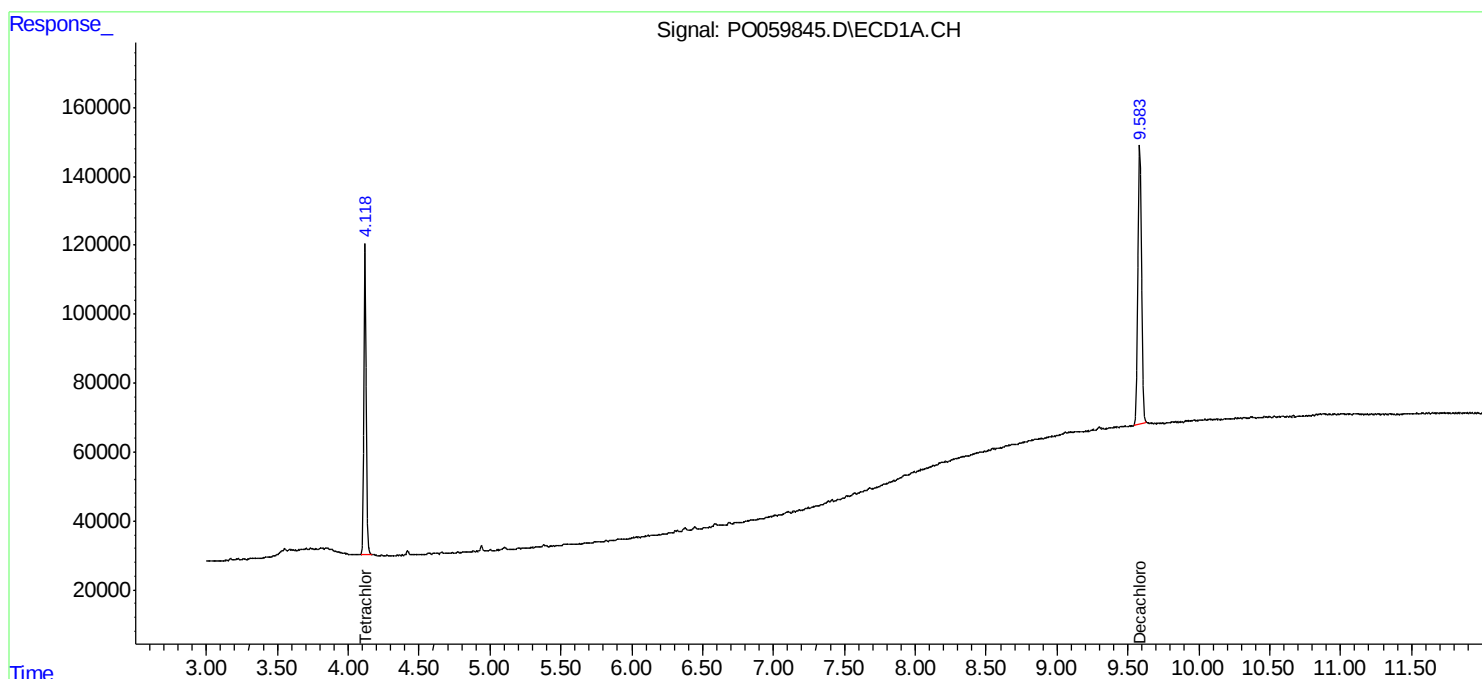

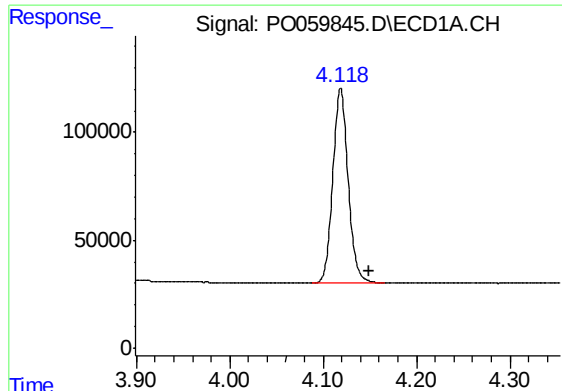


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: -0.031 min
Response: 1028595
Conc: 29.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BRICKRE


Manual Integrations
APPROVED

Ankita
8/27/2019 2:47:18 PM

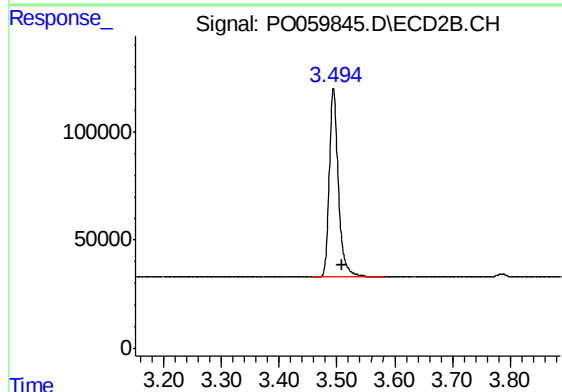


#1 Tetrachloro-m-xylene

R.T.: 3.494 min
Delta R.T.: -0.016 min
Response: 954825
Conc: 26.53 ng/ml

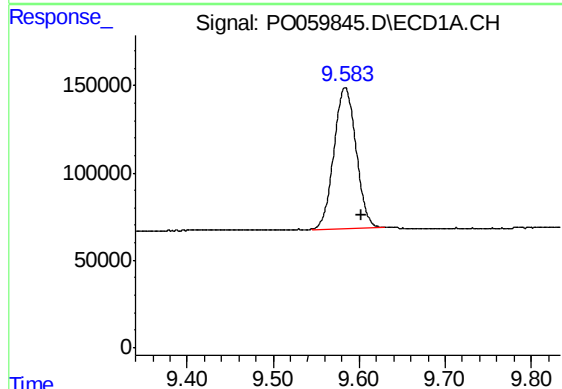

#2 Decachlorobiphenyl

R.T.: 9.583 min
Delta R.T.: -0.020 min
Response: 1448888
Conc: 27.23 ng/ml m

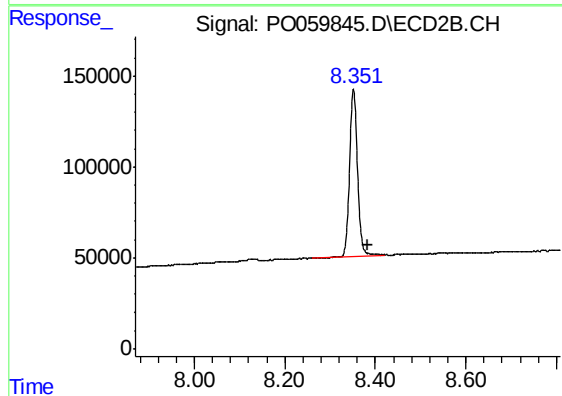

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: -0.032 min
Response: 1137892
Conc: 28.22 ng/ml