

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082619\
 Data File : P0059859.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Aug 2019 18:13
 Operator : SM/AJ
 Sample : PB122555BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB122555BL

Manual Integrations
 APPROVED

Ankita
 8/27/2019 3:13:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 02:27:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0081719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 17 03:09:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.124	3.496	1151902	991868	32.900	27.555
2)	SA Decachlor...	9.590	8.354	1691346	1051494	31.792m	26.078m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082619\
Data File : PO059859.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Aug 2019 18:13
Operator : SM/AJ
Sample : PB122555BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB122555BL


Manual Integrations
APPROVED

Ankita
8/27/2019 3:13:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 02:27:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO081719.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Aug 17 03:09:44 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

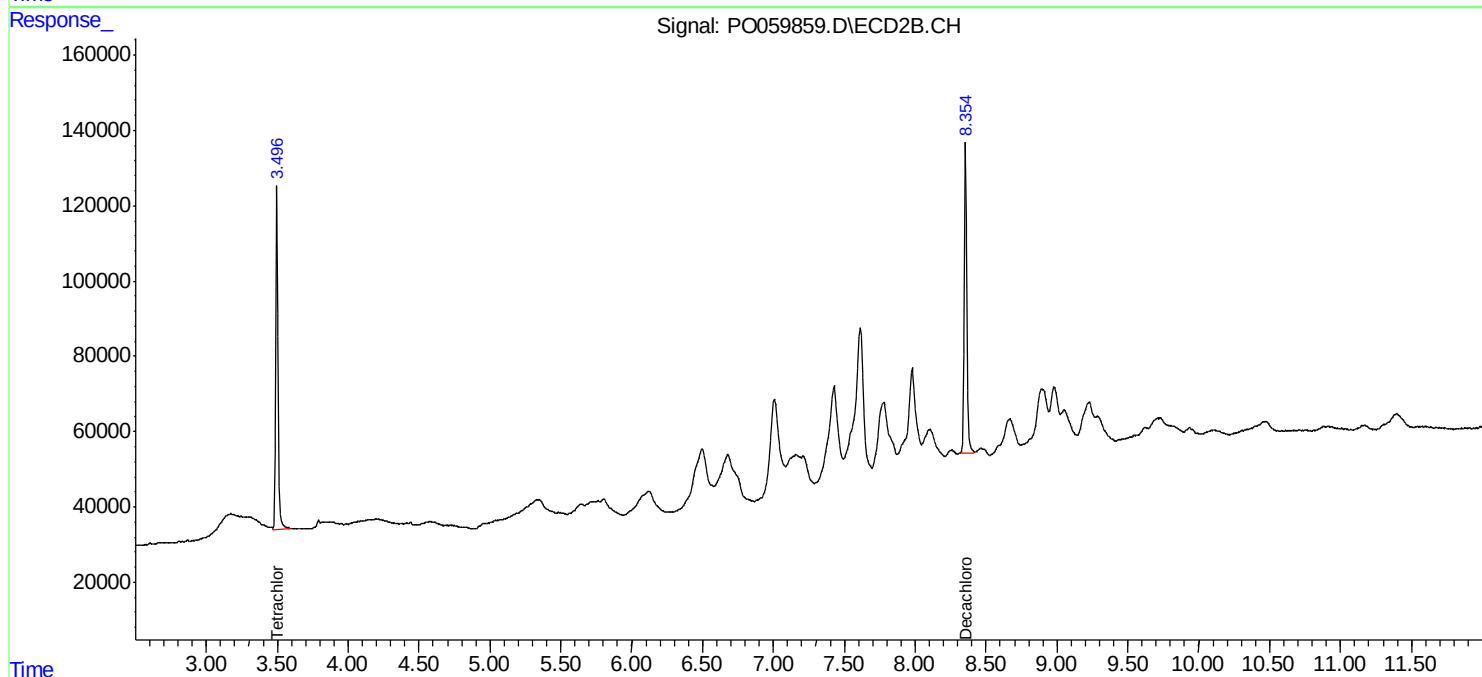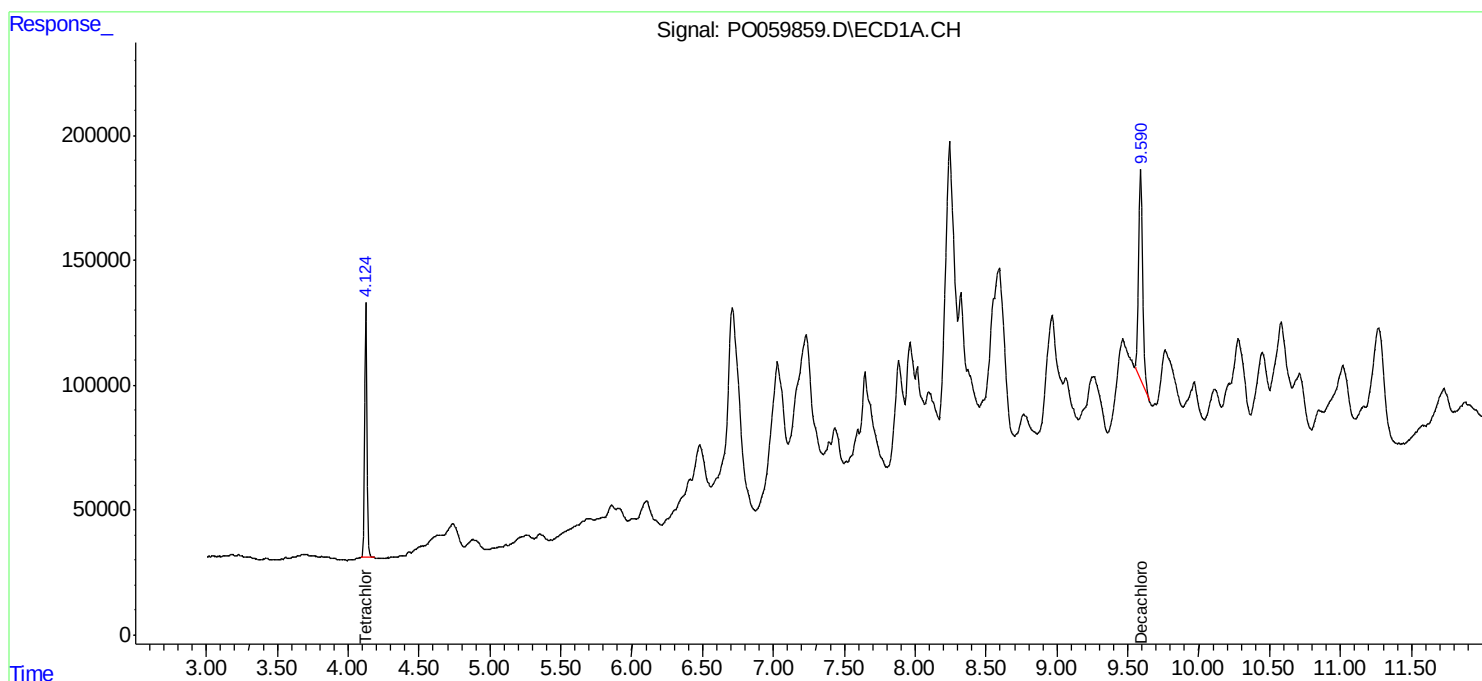

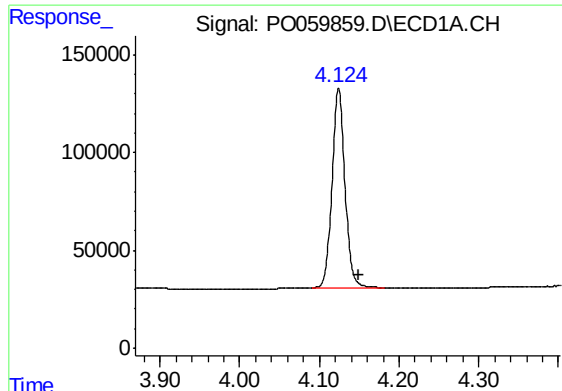


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.025 min
Response: 1151902
Conc: 32.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB122555BL


Manual Integrations
APPROVED

Ankita
8/27/2019 3:13:52 PM

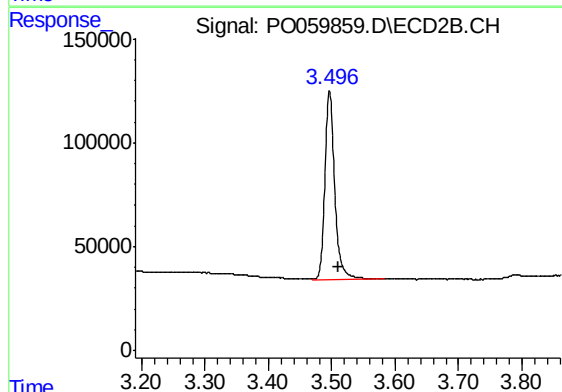


#1 Tetrachloro-m-xylene

R.T.: 3.496 min
Delta R.T.: -0.014 min
Response: 991868
Conc: 27.56 ng/ml

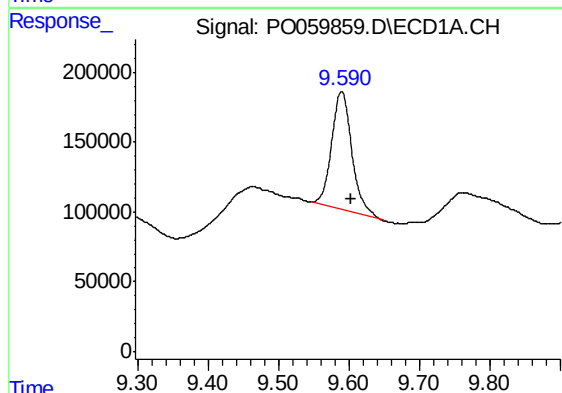

#2 Decachlorobiphenyl

R.T.: 9.590 min
Delta R.T.: -0.013 min
Response: 1691346
Conc: 31.79 ng/ml m

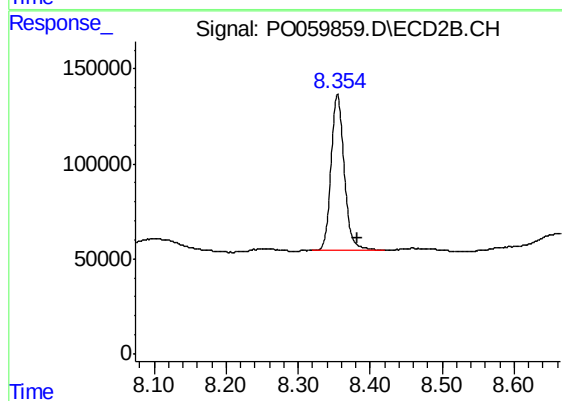

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: -0.029 min
Response: 1051494
Conc: 26.08 ng/ml m