

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082620\
 Data File : P0070895.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Aug 2020 18:10
 Operator : DD\AJ
 Sample : L3792-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Ankita
 8/27/2020 9:53:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 01:48:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 21 04:17:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.557	1242136	679574	17.831m	16.881
2) SA Decachlor...	9.998	8.741	1147735	649777	12.259	11.539

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082620\
Data File : PO070895.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Aug 2020 18:10
Operator : DD\AJ
Sample : L3792-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
8/27/2020 9:53:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 01:48:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 21 04:17:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

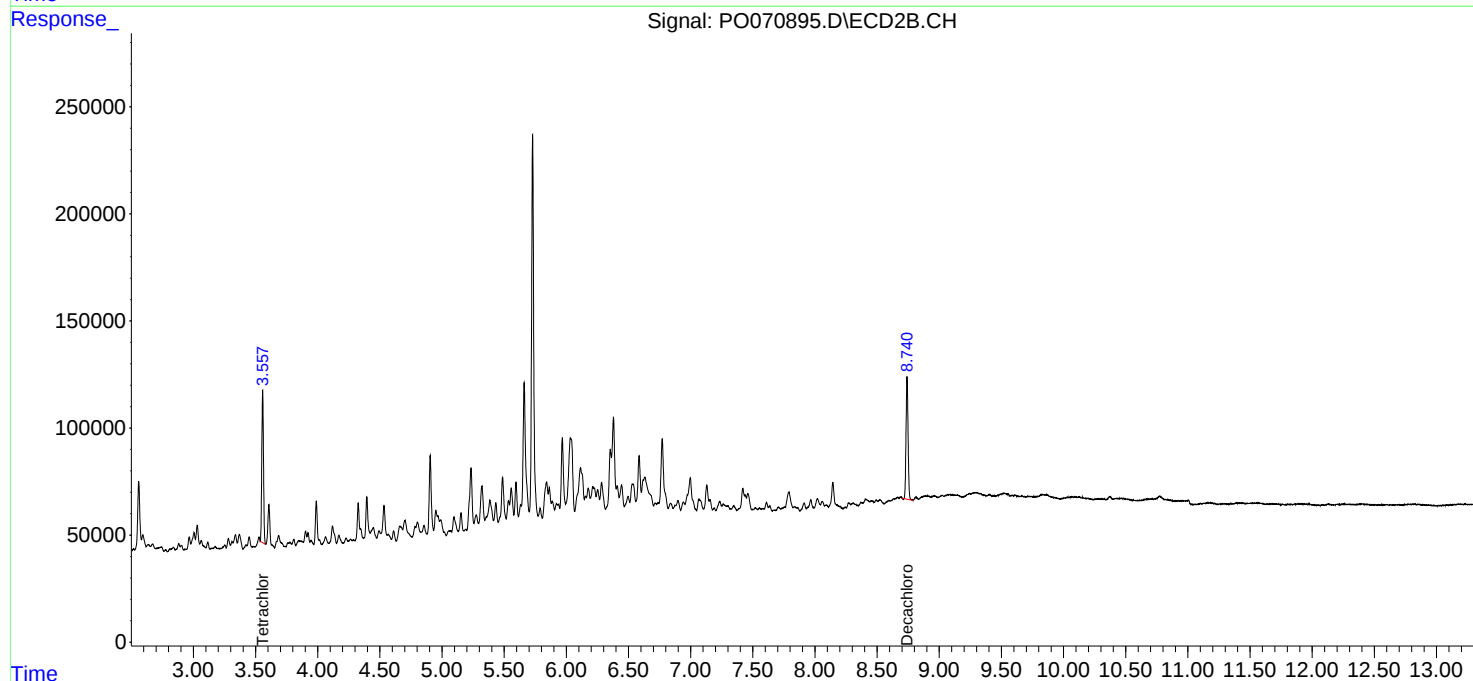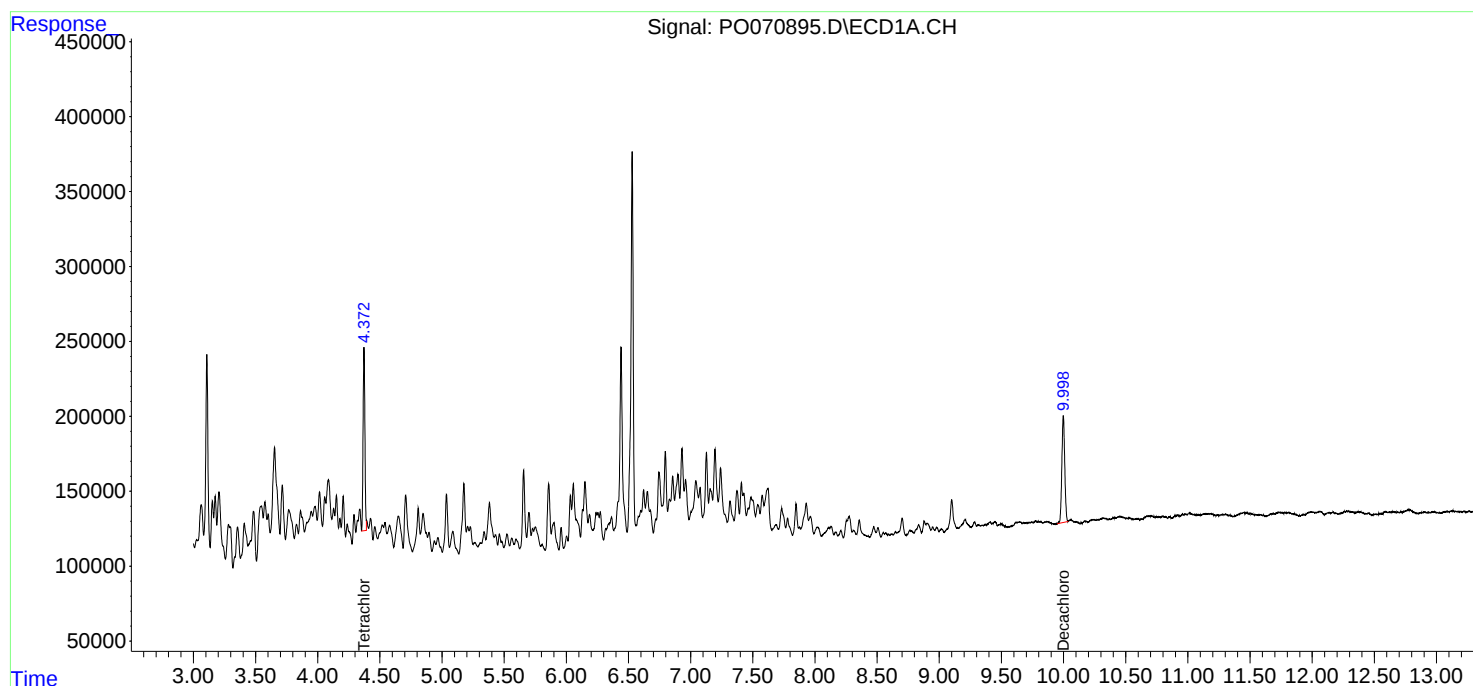

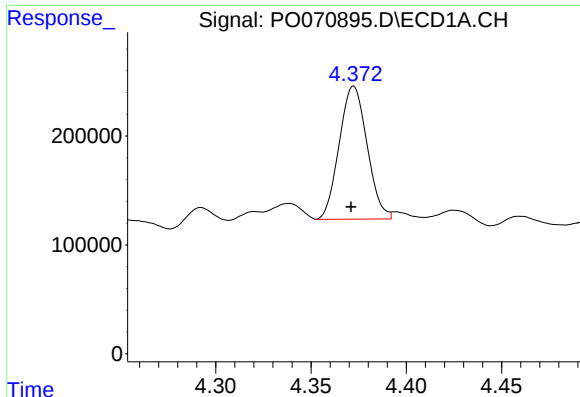


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 1242136
Conc: 17.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
8/27/2020 9:53:38 AM

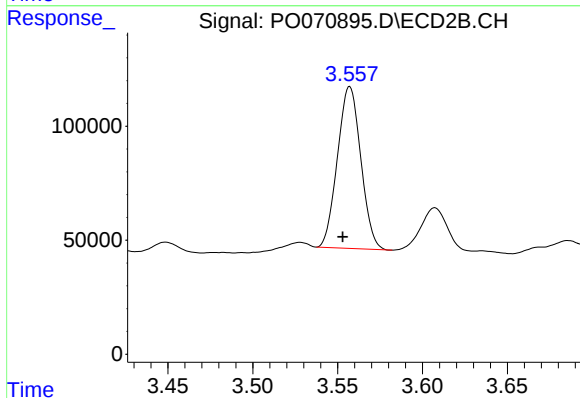


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.004 min
Response: 679574
Conc: 16.88 ng/ml

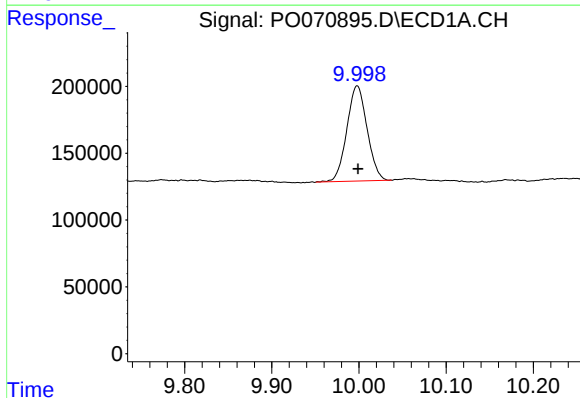

#2 Decachlorobiphenyl

R.T.: 9.998 min
Delta R.T.: -0.001 min
Response: 1147735
Conc: 12.26 ng/ml

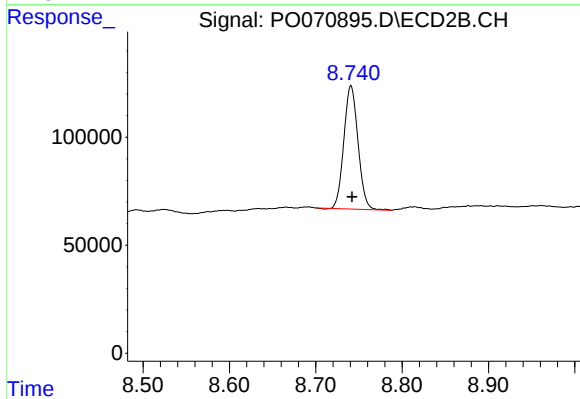

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: -0.001 min
Response: 649777
Conc: 11.54 ng/ml