

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0082624\
 Data File : P0105877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Aug 2024 00:41
 Operator : YP/AJ
 Sample : P3728-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-03-08232024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/28/2024
 Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 27 07:21:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0082624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 27 06:50:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.452	3.720	120.5E6	46974033	13.206m	17.386 #
2) SA Decachlor...	10.191	8.755	93256864	31946601	17.184	14.634

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO082624\
Data File : PO105877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Aug 2024 00:41
Operator : YP/AJ
Sample : P3728-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-03-08232024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 27 07:21:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO082624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 27 06:50:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

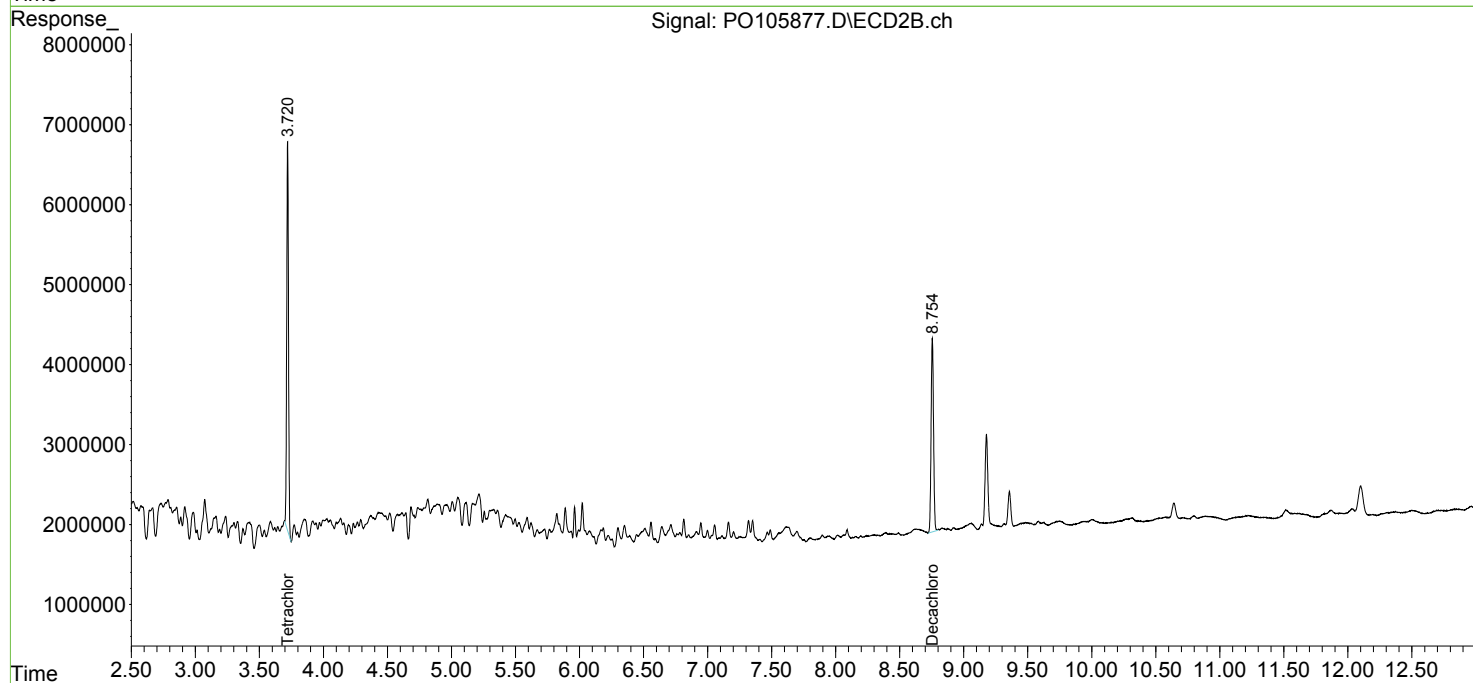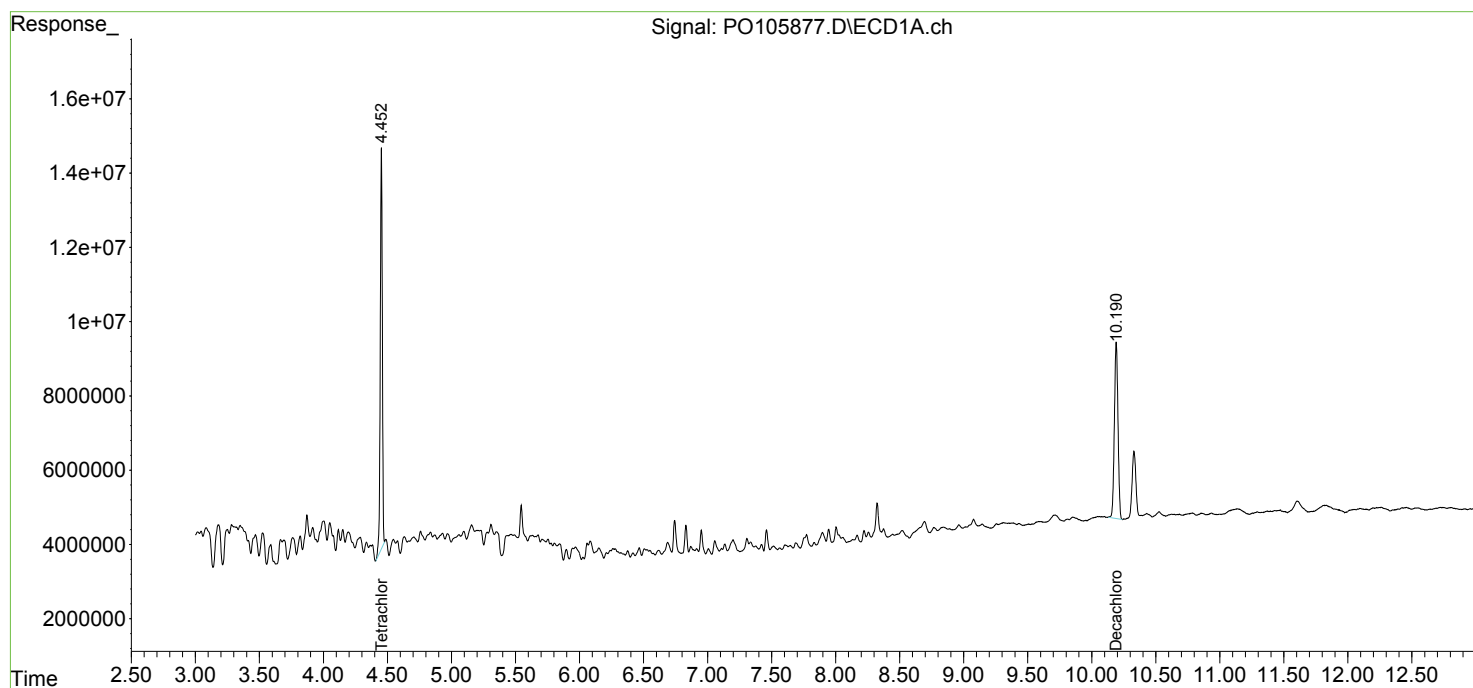

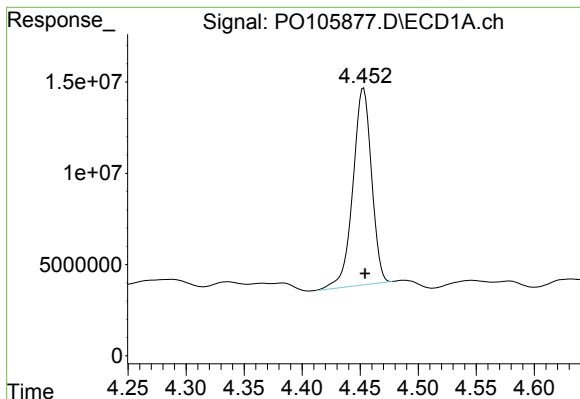


#1 Tetrachloro-m-xylene

R.T.: 4.452 min
Delta R.T.: -0.002 min
Response: 120485524
Conc: 13.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-03-08232024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/28/2024
Supervised By :Ankita Jodhani 08/28/2024

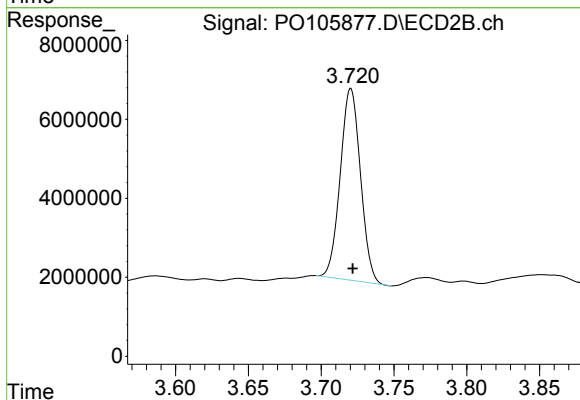


#1 Tetrachloro-m-xylene

R.T.: 3.720 min
Delta R.T.: -0.001 min
Response: 46974033
Conc: 17.39 ng/ml

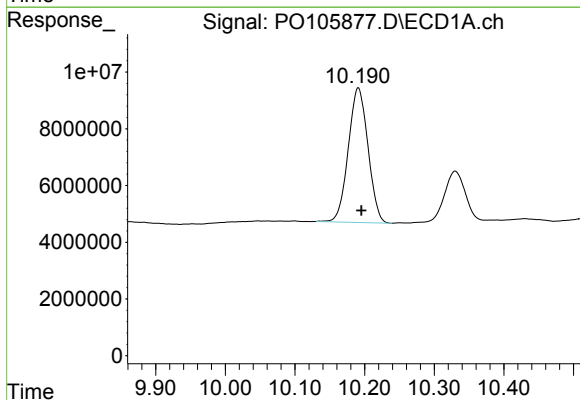

#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: -0.005 min
Response: 93256864
Conc: 17.18 ng/ml

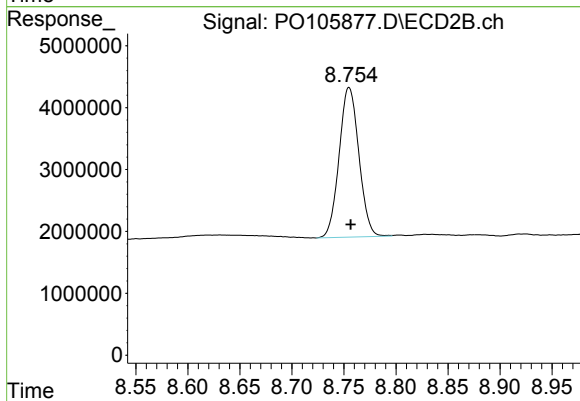

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.002 min
Response: 31946601
Conc: 14.63 ng/ml