

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
 Data File : P0048550.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Aug 2018 20:35
 Operator : SM/SJ
 Sample : J4659-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 082218-SIDI-E-U-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 28 07:01:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 24 08:17:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.625	4419027	4485255	23.328	16.567 #
2) SA Decachlor...	10.063	8.599	3255863	3063578	18.907	18.293

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0082718\
Data File : P0048550.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Aug 2018 20:35
Operator : SM/SJ
Sample : J4659-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
082218-SIDI-E-U-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 28 07:01:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0082418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 24 08:17:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

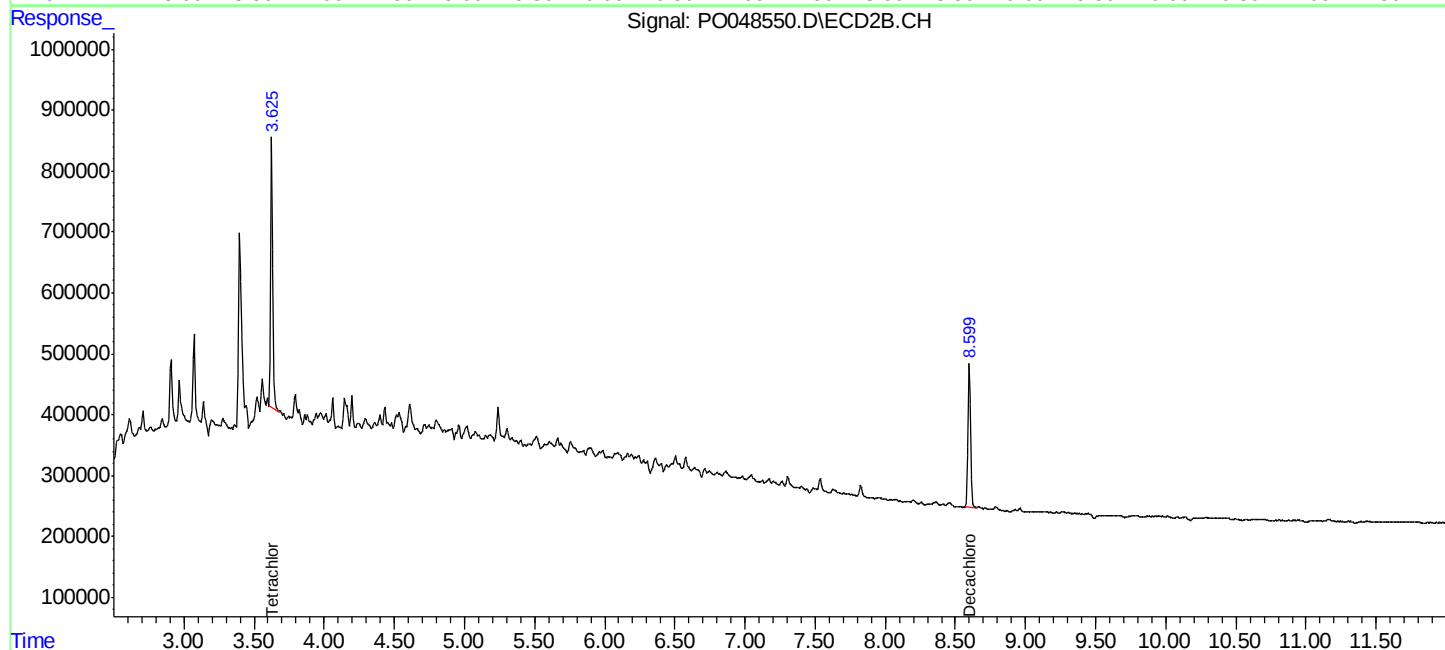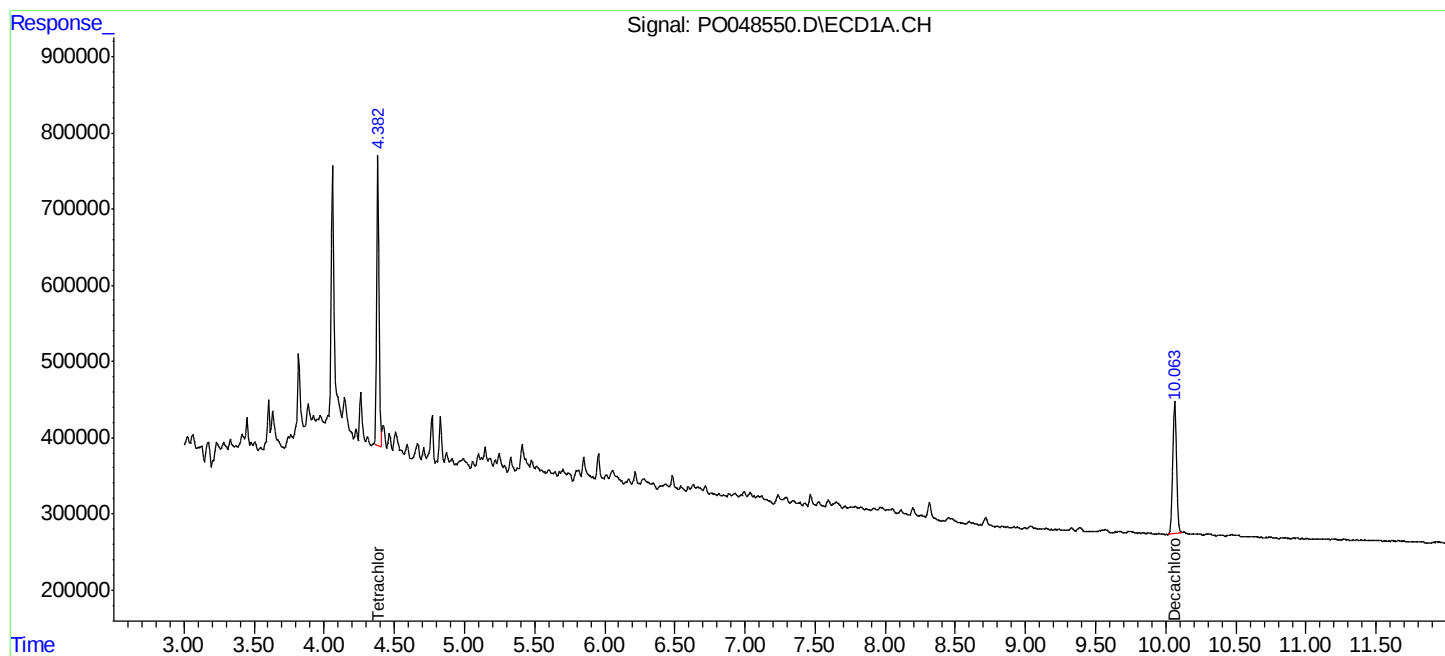


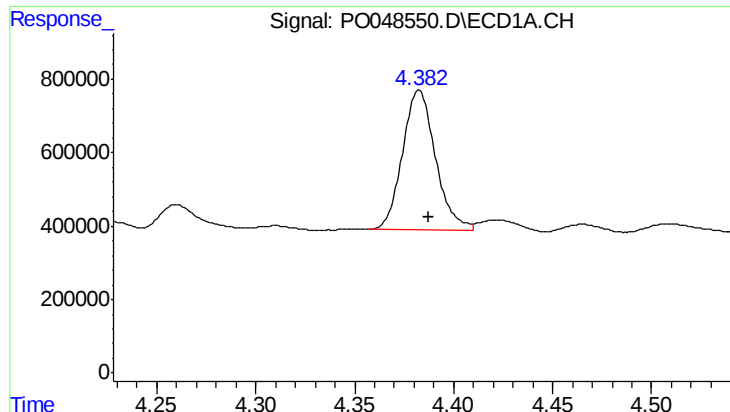

#1 Tetrachloro-m-xylene


R.T.: 4.383 min
Delta R.T.: -0.005 min
Response: 4419027
Conc: 23.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
082218-SIDI-E-U-S

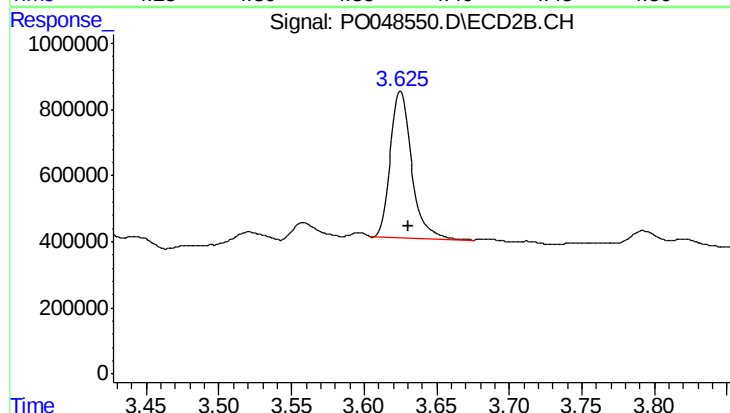


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.005 min
Response: 4485255
Conc: 16.57 ng/ml

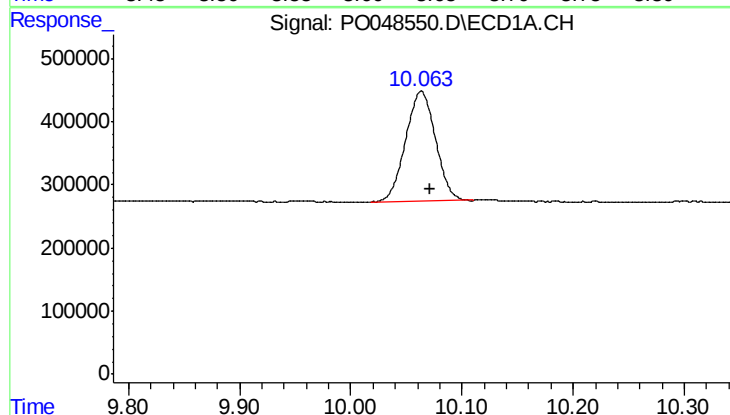

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.008 min
Response: 3255863
Conc: 18.91 ng/ml

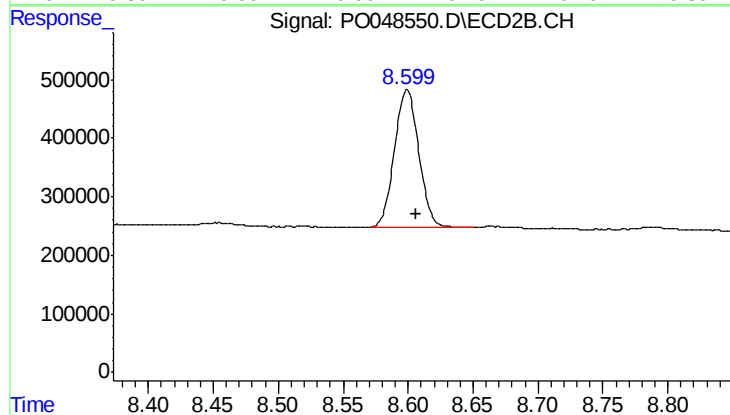

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: -0.007 min
Response: 3063578
Conc: 18.29 ng/ml